

9-1-2005

# Justification for Class III Permit Modification September 2005 DSS Site 1035 Operable Unit 1295 Building 6715 Septic System at Technical Area III

Sandia National Laboratories/NM

Follow this and additional works at: [https://digitalrepository.unm.edu/snl\\_complete](https://digitalrepository.unm.edu/snl_complete)

---

## Recommended Citation

Sandia National Laboratories/NM. "Justification for Class III Permit Modification September 2005 DSS Site 1035 Operable Unit 1295 Building 6715 Septic System at Technical Area III." (2005). [https://digitalrepository.unm.edu/snl\\_complete/241](https://digitalrepository.unm.edu/snl_complete/241)

This Technical Report is brought to you for free and open access by the Sandia National Labs/NM Technical Reports at UNM Digital Repository. It has been accepted for inclusion in Regulatorily Completed by an authorized administrator of UNM Digital Repository. For more information, please contact [disc@unm.edu](mailto:disc@unm.edu).




This work supported by the United States Department of Energy under contract DE-AC04-94185000.



# Drain and Septic Systems - Areas of Concern (AOCs)

276, 1004, 1031, 1034, 1035, 1036, 1052, 1078, 1079, 1080, 1081, 1084, 1087, 1092, 1098, 1102, 1104, 1113, and 1120 (Poster 1/2)



Environmental Restoration Project

## Site History

Drain and septic system site histories for the 19 AOCs are as follows:

AOC Number	Site Name	Location	Year Building and System Built	Year Drain or Septic System Abandoned	Years Septic Tank Effluent Sampled	Year Septic Tank Pumped For the last Time
276	Former Bldg 829X Silver Recovery Sump	TA-I	1948-1978	1994	No septic tank at this site	NA
1004	Bldg 6969 Septic System	Robotic Vehicle Range	1988	System is active	Periodically since 1992	Periodically
1031	Former Bldgs 6589 and 6600 Septic System	TA-III	1967	1991 (septic tank and seepage pit backfilled in 2002)	1990-1991, 1992, 1995	1996
1034	Bldg 6710 Septic System	TA-III	1958	Early 1990s	1990-1991, 1992, 1995	1996
1035	Bldg 6715 Septic System	TA-III	1962	Early 1990s	1990-1991, 1992, 1995	1996
1036	Bldg 6922 Septic System	TA-III	1955	1991	1990-1991, 1992, 1995, 2005	2005
1052	Bldg 803 Seepage Pit	TA-I	1957	Unknown	No septic tank at this site	NA
1078	Bldg 6640 Septic System	TA-III	1959	1991	1990-1991	Unknown (backfilled in 1991)
1079	Bldg 6643 Septic System	TA-III	1989	1991	1990-1991, 1992, 1995, 2005	2005
1080	Bldg 6644 Septic System	TA-III	1989	1991	1990-1991, 1992, 1995	1996
1081	Bldg 6650 Septic System	TA-III	1967 (southern system), Early 1960s (northern system)	1991	1990-1991, 1992, 1995	1996 (south septic tank), Unknown (north septic tank)
1084	Bldg 6505 Septic System	TA-III	1954	1991	1990-1991	Unknown (backfilled before 2002)
1087	Bldg 6743 Seepage Pit	TA-III	1967	2004-2005	No septic tank at this site	NA
1092	MO 228-230 Septic System	TA-III	1988	1991	1990-1991	Unknown (backfilled before 2002)
1098	TA-V Plenum Rooms Drywell	TA-V	1958	Late 1990s	No septic tank at this site	NA
1102	Former Bldg 889 Septic System	TA-I	Early 1950s	Early 1990s	1992-1995	Unknown (removed prior to 1999)
1104	Bldg 6595 Seepage Pit	TA-V	1966	Early 1990s	No septic tank at this site	NA
1113	Bldg 6597 Drywell	TA-V	1971	Prior to 2002	No septic tank at this site	NA
1120	Bldg 6643 Drywell	TA-III	1989	1991	No septic tank at this site	NA

## Depth to Groundwater

Depth to groundwater at these 19 AOCs is as follows:

AOC Number	Site Name	Location	Groundwater Depth (ft bgs)
276	Former Bldg 829X Silver Recovery Sump	TA-I	555
1004	Bldg 6969 Septic System	Robotic Vehicle Range	548
1031	Former Bldgs. 6589 and 6600 Septic System	TA-III	486
1034	Bldg 6710 Septic System	TA-III	470
1035	Bldg 6715 Septic System	TA-III	470
1036	Bldg 6922 Septic System	TA-III	490
1052	Bldg 803 Seepage Pit	TA-I	552
1078	Bldg 6640 Septic System	TA-III	476
1079	Bldg 6643 Septic System	TA-III	487
1080	Bldg 6644 Septic System	TA-III	480
1081	Bldg 6650 Septic System	TA-III	480
1084	Bldg 6505 Septic System	TA-III	508
1087	Bldg 6743 Seepage Pit	TA-III	461
1092	MO 228-230 Septic System	TA-III	488
1098	TA-V Plenum Rooms Drywell	TA-V	509
1104	Bldg 6595 Seepage Pit	TA-V	507
1113	Bldg 6597 Drywell	TA-V	515
1120	Bldg 6643 Drywell	TA-III	483

## Constituents of Concern

- VOCs
- SVOCs
- PCBs
- HE Compounds
- Metals
- Cyanide
- Radionuclides

## Investigations

- A backhoe was used to positively locate buried components (drainfield drain lines, drywells) for placement of soil vapor samplers, and soil borings.
- Ten of the 19 AOCs were selected by NMED for passive soil-vapor sampling to screen for VOCs; no significant VOC contamination was identified at any of the ten sites.
- Soil samples were collected from directly beneath drainfield drain lines, seepage pits, and drywells to determine if COCs were released to the environment from drain systems.
- Four of the sites were selected by NMED for active soil vapor sampling to screen for VOCs. Each of the active soil-vapor monitoring wells was 150 ft deep with vapor sampling ports at 5, 20, 70, 100, and 150-ft bgs. The VOC concentrations were significantly lower than the 10 ppmv action level established by NMED.

The years that site-specific characterization activities were conducted and soil sampling depths at each of these 19 AOC sites are as follows:

AOC Number	Site Name	Buried Components (Drain Lines, Drywells) Located With a Backhoe	Soil Sampling Beneath Drainlines, Seepage Pits, Drywells	Type(s) of Drain System, and Soil Sampling Depths (ft bgs)	Passive Soil Vapor Sampling	Active Soil Vapor Monitor Well Installation and Sampling
276	Former Bldg 829X Silver Recovery Sump	None	1994, 2002	Silver Recovery Sump 8, 13	2002	None
1004	Bldg 6969 Septic System	2002	2002	Drainfield 8, 13	2002	2003
1031	Former Bldgs 6589 and 6600 Septic System	2002	2002	Seepage Pits 15, 20	2002	None
1034	Bldg 6710 Septic System	None	2002	Seepage Pit 14, 19	2002	None
1035	Bldg 6715 Septic System	None	2002	Seepage Pit 11, 16	2002	None
1036	Bldg 6922 Septic System	1997	1998, 1999	Drainfield 5, 10	None	None
1052	Bldg 803 Seepage Pit	None	2002	Seepage Pit 27, 27	2002	2003
1078	Bldg 6640 Septic System	2002	2002	Drainfield 5, 10	None	None
1079	Bldg 6643 Septic System	2002	2002	Drainfield 11, 16	None	None
1080	Bldg 6644 Septic System	2002	2002	Drainfield Borehole 1 & 2 5, 10 Borehole 3 6, 11	None	None
1081	Bldg 6650 Septic System	2003 (north septic tank)	2002	South seepage pit 10, 12, 15, 17 North seepage pit 10, 12, 15, 17, 20, 24, 25	2002	2003
1084	Bldg 6505 Septic System	2002	2002	Drainfield 3, 8	2002	None
1087	Bldg 6743 Seepage Pit	None	2002	Seepage Pit 8, 13	2002	None
1092	MO 228-230 Septic System	2002-2003	2002	Drainfield 6, 11	None	2003
1098	TA-V Plenum Rooms Drywell	None	2002	Drywell 10, 15	None	None
1102	Former Bldg 889 Septic System	1999-2002	2002	Seepage Pit 25, 30	None	None
1104	Bldg 6595 Seepage Pit	None	2002	Seepage Pit 11, 16	None	None
1113	Bldg 6597 Drywell	2002	2002	Drywell 5, 10	None	None
1120	Bldg 6643 Drywell	2002	2002	Drywell 8, 13	2002	None

## For More Information Contact

U.S. Department of Energy  
Sandia Site Office  
Environmental Restoration  
Mr. John Gould  
Telephone (505) 845-6089

Sandia National Laboratories  
Environmental Restoration Project  
Task Leader: Mike Sanders  
Telephone (505) 284-2478




This work supported by the United States Department of Energy under contract DE-AC04-94-185000.



## Drain and Septic Systems - Areas of Concern (AOCs)

276, 1004, 1031, 1034, 1035, 1036, 1052, 1078, 1079, 1080, 1081, 1084, 1087, 1092, 1098, 1102, 1104, 1113, and 1120 (Poster 2/2)



Environmental Restoration Project

### Summary of Data Used for NFA Justification

- Soil samples were analyzed at on- and off-site laboratories for VOCs, SVOCs, PCBs, HE compounds, metals, cyanide, gross alpha/beta activity, and radionuclides by gamma spectroscopy.
- There were VOCs detected at the 19 sites, SVOCs were detected at 15 of the sites, PCBs were detected at 9 sites, and cyanide was identified at 14 of the sites. HE compounds were detected at one of the sites (AOC 1113).
- Barium was detected at concentrations above the background value at six sites. Chromium and arsenic were detected at concentrations above background values at five sites. Silver was detected at concentrations above the background value at three sites, lead was detected above the background value at two sites, and mercury was detected above the background value at one site. No other metals were detected above background concentrations.
- Uranium-235 was detected at an activity slightly above the background activity at 5 of the 19 sites and, although not detected, the MDA for U-235 exceeded the background activity at 14 sites and the MDA for U-238 exceeded the background activity at one site. Gross alpha activity was slightly above background activity at five of the 19 sites, and gross beta activity was above the background activity at one site.
- All confirmatory soil sample analytical results for each site were used for characterizing that site, for performing the risk screening assessment, and as justification for the NFA proposal for the site.

### Recommended Future Land Use

- Industrial land use was established for these 19 AOC sites.

### Results of Risk Analysis

- Risk assessment results for industrial and residential land-use scenarios are calculated per NMED risk assessment guidance as presented in "Supplemental Risk Document Supporting Class 3 Permit Modification Process."
- Because COCs were present in concentrations greater than background-screening levels or because constituents were present that did not have background-screening numbers, it was necessary to perform risk assessments for these all of these AOCs. The risk assessment analysis evaluated the potential for adverse health effects for industrial and residential land-use scenarios.
- The maximum concentration value for lead was 22.2 mg/kg at AOC 1081 and 11.9 mg/kg at AOC 1087; these exceed the background value of 11.8 mg/kg. The EPA intentionally does not provide any human health toxicological data on lead; therefore, no risk parameter values could be calculated. The NMED guidance for lead screening concentrations for construction and industrial land-use scenarios are 750 and 1,500 mg/kg, respectively. The EPA screening guidance value for a residential land-use scenario is 400 mg/kg. The maximum concentration for lead at these two sites are less than all the screening values; therefore, lead was eliminated from further consideration in the human health risk assessment for each site.
- The non-radiological total human health HIs for 18 of the 19 AOCs are below NMED guidelines for a residential land-use scenario.
- For four sites, the total estimated excess cancer risks are at or slightly above the residential land-use scenario guideline. However, the incremental excess cancer risk values for these four sites are below the NMED residential land-use scenario guideline.
- For one of the 19 sites (AOC 1081), the total HI and the estimated excess cancer risk are above the NMED guidelines for the residential land-use scenario due to elevated levels of arsenic and silver. However, the total HI and estimated excess cancer risk values are below the NMED guidelines for the industrial land-use scenario.
- The total human health TEDEs for industrial land-use scenarios ranged from 0.001 to 0.46 mrem/yr, all of which are substantially below the EPA numerical guideline of 15 mrem/yr. The total human health TEDEs for residential land-use scenarios ranged from 0.0052 to 0.12 mrem/yr, all of which are substantially below the EPA numerical guideline of 75 mrem/yr. Therefore, these AOCs are eligible for unrestricted radiological release.
- Using the SNL predictive ecological risk and scoping assessment methodologies, it was concluded that a complete ecological pathway for each of 18 of the sites was not associated with the respective COPELs for that site. Thus, a more detailed ecological risk assessment to predict the level of risk was not deemed necessary for these sites.
- Ecological risks associated with AOC 1084 were predicted incorporating potential receptors and site-specific COPELs. The HQ values predicted were less than one, with the exception of barium. For barium, the contribution from background concentrations accounts for the majority (52%) of the HQ values. Therefore, ecological risks associated with this site are expected to be low.
- In conclusion, human health and ecological risks are acceptable for 18 sites for a residential land-use scenario and for all 19 for an industrial land-use scenario per NMED guidance. Thus, 18 of these sites are proposed for CAC without institutional controls, and one site (AOC 1081) is proposed for CAC with institutional controls.

The total HIs and excess cancer risk values for the nonradiological COCs at the 19 AOCs are as follows:

The total HIs and excess cancer risk values for the nonradiological COCs at the 19 AOCs are as follows:

AOC Number	Site Name	Residential Land-Use Scenario	
		Total Hazard Index	Excess Cancer Risk
276	Former Bldg 829X Silver Recovery Sump	0.27	2E-5 Total <sup>a</sup> 3.95E-6 Incremental
1004	Bldg 6969 Septic System	0.08	2E-6 Total
1031	Former Bldgs. 6589 and 6600 Septic System	0.25	1E-5 Total <sup>a</sup> 2.55E-6 Incremental
1034	Bldg 6710 Septic System	0.00	2E-9 Total
1035	Bldg 6715 Septic System	0.04	3E-9 Total
1036	Bldg 6922 Septic System	0.26	1E-5 Total <sup>a</sup> 8.35E-7 Incremental
1052	Bldg 803 Seepage Pit	0.00	2E-6 Total
1078	Bldg 6640 Septic System	0.27	1E-5 Total <sup>a</sup> 3.72E-7 Incremental
1079	Bldg 6643 Septic System	0.00	3E-8 Total
1080	Bldg 6644 Septic System	0.00	4E-8 Total
1084	Bldg 6505 Septic System	0.08	None
1087	Bldg 6743 Seepage Pit	0.00	4E-9 Total
1092	MO 228-230 Septic System	0.06	None
1098	TA-V Plenum Rooms Drywell	0.03	3E-7 Total
1102	Former Bldg 889 Septic System	0.00	1E-10 Total
1104	Bldg 6595 Seepage Pit	0.00	2E-6 Total
1113	Bldg 6597 Drywell	0.14	1E-7 Total
1120	Bldg 6643 Drywell	0.12	1E-6 Total
<i>NMED Guidance for Residential Land Use</i>		< 1	<1E-5
AOC Number	Site Name	Industrial Land-Use Scenario	
		Total Hazard Index	Excess Cancer Risk
1081	Bldg 6650 Septic System	0.39	5E-6 Total
<i>NMED Guidance for Industrial Land Use</i>		< 1	<1E-5

<sup>a</sup>Maximum value exceeds NMED guidance for specified land-use scenario, therefore, incremental values are shown.

### For More Information Contact


U.S. Department of Energy  
Sandia Site Office  
Environmental Restoration  
Mr. John Gould  
Telephone (505) 845-6089

Sandia National Laboratories  
Environmental Restoration Project  
Task Leader: Mike Sanders  
Telephone (505) 284-2478







This work supported by the United States Department of Energy under contract DE-AC04-94185000.

# Drain and Septic Systems (DSS) Areas of Concern (AOCs) 276, 1004, 1031, 1034, 1035 1036, 1052






Environmental Restoration Project

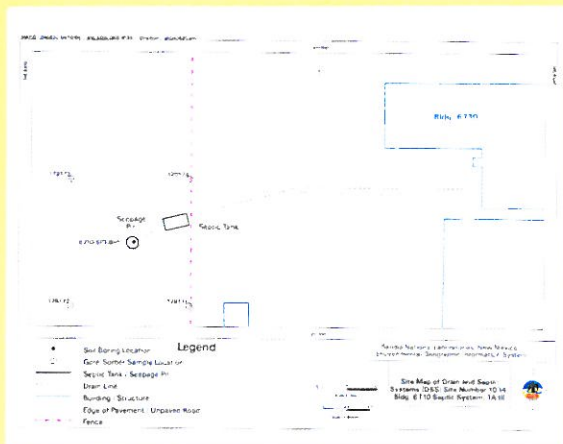

Septic system demolition and backfilling.




Three-foot long Geoprobe soil sampling device used to collect soil samples.

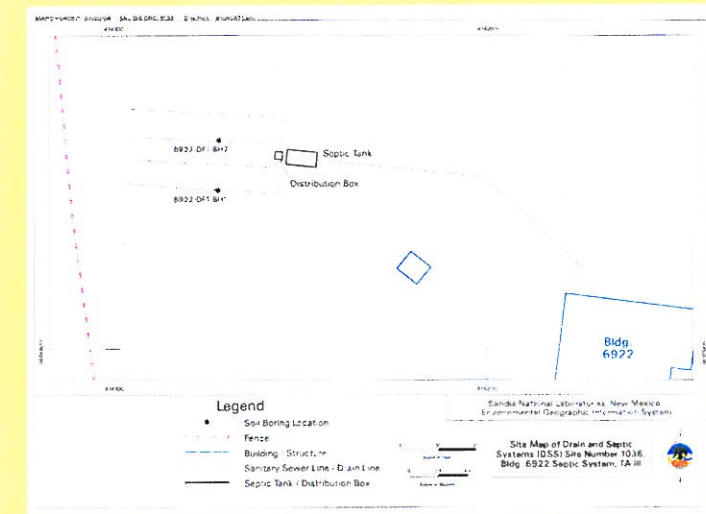

### For More Information Contact

U.S. Department of Energy  
Sandia Site Office  
Environmental Restoration  
Mr. John Gould  
Telephone (505) 845-6089

Sandia National Laboratories  
Environmental Restoration Project  
Task Leader: Mike Sanders  
Telephone (505) 284-2478



Sandia National Laboratories

---

Justification for Class III Permit Modification

September 2005

DSS Site 1035

Operable Unit 1295

Building 6715 Septic System at Technical  
Area III


**CAC (SWMU Assessment Report) Submitted September 2004**

**RSI Submitted April 2005**

Environmental  
Restoration  
Project



United States Department of Energy  
Sandia Site Office



**Sandia National Laboratories**

---

**Justification for Class III Permit Modification**

**September 2005**

**DSS Site 1035**

**Operable Unit 1295**

**Building 6715 Septic System at Technical  
Area III**

**CAC (SWMU Assessment Report) Submitted September 2004**

**RSI Submitted April 2005**

**Environmental  
Restoration  
Project**



**United States Department of Energy  
Sandia Site Office**

CAC



**National Nuclear Security Administration**

Sandia Site Office  
P.O. Box 5400  
Albuquerque, New Mexico 87185-5400



SEP 17 2004

**CERTIFIED MAIL-RETURN RECEIPT REQUESTED**

Mr. James Bearzi, Chief  
Hazardous Waste Bureau  
New Mexico Environment Department  
2905 Rodeo Park Road East, Building 1  
Santa Fe, NM 87505

Dear Mr. Bearzi:


On behalf of the Department of Energy (DOE) and Sandia Corporation, DOE is submitting the enclosed Solid Waste Management Unit (SWMU) Assessment Reports and Proposals for Corrective Action Complete for Drain and Septic Systems (DSS) Sites 1034, 1035, 1036, 1078, 1079, 1084, 1098, 1104, and 1120 at Sandia National Laboratories, New Mexico, EPA ID No. NM5890110518. These documents are compiled as DSS Round 6 and No Further Action (NFA) Batch 24.

This submittal includes descriptions of the site characterization work and risk assessments for the above referenced DSS Sites. The risk assessments conclude that for these sites: (1) there is no significant risk to human health under either the industrial or residential land-use scenarios; and (2) that there are no ecological risks associated with these sites.

Based on the information provided, DOE and Sandia are requesting a determination of Corrective Action Complete without controls for these DSS sites.

If you have any questions, please contact John Gould at (505) 845-6089.

Sincerely,

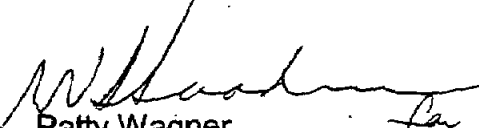  
Patty Wagner  
Manager

Enclosure



Mr. J. Bearzi

(2)

SEP 17 2004


cc w/enclosure:

L. King, EPA, Region 6 (Via Certified Mail)  
W. Moats, NMED-HWB (via Certified Mail)  
M. Gardipe, NNSA/SC/ERD  
C. Voorhees, NMED-OB

cc w/o enclosure:

K. Thomas, EPA, Region 6  
F. Nimick, SNL, MS 1089  
D. Stockham, SNL, MS 1087  
B. Langkopf, SNL, MS 1087  
M. Sanders, SNL, MS 1087  
R. Methvin, SNL MS 1087  
J. Pavletich, SNL MS 1087  
A. Villareal, SNL, MS 1035  
A. Blumberg, SNL, MS 0141  
M. J. Davis, SNL, MS 1089  
ESHSEC Records Center, MS 1087





Sandia National Laboratories/New Mexico  
Environmental Restoration Project

---

**SWMU ASSESSMENT REPORT AND  
PROPOSAL FOR  
CORRECTIVE ACTION COMPLETE  
DRAIN AND SEPTIC SYSTEMS SITE 1035,  
BUILDING 6715 SEPTIC SYSTEM**

**September 2004**



United States Department of Energy  
Sandia Site Office

---



## TABLE OF CONTENTS

LIST OF FIGURES .....	iii
LIST OF TABLES.....	v
LIST OF ANNEXES .....	vii
ACRONYMS AND ABBREVIATIONS.....	ix
1.0 PROJECT BACKGROUND.....	1-1
2.0 DSS SITE 1035: BUILDING 6715 SEPTIC SYSTEM.....	2-1
2.1 Summary .....	2-1
2.2 Site Description and Operational History.....	2-1
2.2.1 Site Description .....	2-1
2.2.2 Operational History.....	2-7
2.3 Land Use .....	2-7
2.3.1 Current Land Use .....	2-7
2.3.2 Future/Proposed Land Use .....	2-7
3.0 INVESTIGATORY ACTIVITIES .....	3-1
3.1 Summary .....	3-1
3.2 Investigation 1—Septic Tank Sampling.....	3-1
3.3 Investigation 2—Passive Soil-Vapor Sampling .....	3-1
3.3.1 Passive Soil-Vapor Sampling Methodology.....	3-2
3.3.2 Soil-Vapor Survey Results and Conclusions .....	3-2
3.4 Investigation 3—Soil Sampling.....	3-2
3.4.1 Soil Sampling Methodology .....	3-5
3.4.2 Soil Sampling Results and Conclusions .....	3-5
3.4.3 Soil Sampling Quality Assurance/Quality Control Samples and Data Validation Results .....	3-20
3.5 Site Sampling Data Gaps .....	3-20
4.0 CONCEPTUAL SITE MODEL.....	4-1
4.1 Nature and Extent of Contamination .....	4-1
4.2 Environmental Fate .....	4-1
4.3 Site Assessment.....	4-6
4.3.1 Summary .....	4-6
4.3.2 Risk Assessments .....	4-6

## TABLE OF CONTENTS (Concluded)

4.4	Baseline Risk Assessments .....	4-8
4.4.1	Human Health.....	4-8
4.4.2	Ecological .....	4-8
5.0	RECOMMENDATION FOR CORRECTIVE ACTION COMPLETE WITHOUT CONTROLS DETERMINATION .....	5-1
5.1	Rationale .....	5-1
5.2	Criterion.....	5-1
6.0	REFERENCES.....	6-1

## LIST OF FIGURES

### Figure

2.2.1-1	Location Map of Drain and Septic Systems (DSS) Site Number 1035, Bldg. 6715 Septic System, TA-III .....	2-3
2.2.1-2	Site Map of Drain and Septic Systems (DSS) Site Number 1035, Bldg. 6715 Septic System, TA-III .....	2-5
3.4-1	Collecting soil samples with the Geoprobe™ from the borehole drilled through the center of the seepage pit at DSS Site 1035, the Building 6715 Septic System. View to the southeast. September 12, 2002.....	3-3
4.2-1	Conceptual Site Model Flow Diagram for DSS Site 1035, Building 6715 Septic System .....	4-3

**This page intentionally left blank.**



## LIST OF TABLES

### Table

3.4-1	Summary of Area Sampled, Analytical Methods, and Laboratories Used for DSS Site 1035, Building 6715 Septic System Soil Samples.....	3-6
3.4.2-1	Summary of DSS Site 1035, Building 6715 Septic System, Confirmatory Soil Sampling, VOC Analytical Results, September 2002 (Off-Site Laboratory).....	3-7
3.4.2-2	Summary of DSS Site 1035, Building 6715 Septic System, Confirmatory Soil Sampling, VOC Analytical MDLs, September 2002 (Off-Site Laboratory).....	3-8
3.4.2-3	Summary of DSS Site 1035, Building 6715 Septic System, Confirmatory Soil Sampling, SVOC Analytical Results, September 2002 (Off-Site Laboratory).....	3-10
3.4.2-4	Summary of DSS Site 1035, Building 6715 Septic System, Confirmatory Soil Sampling, SVOC Analytical MDLs, September 2002 (Off-Site Laboratory).....	3-11
3.4.2-5	Summary of DSS Site 1035, Building 6715 Septic System, Confirmatory Soil Sampling, PCB Analytical Results, September 2002 (Off-Site Laboratory).....	3-13
3.4.2-6	Summary of DSS Site 1035, Building 6715 Septic System, Confirmatory Soil Sampling, PCB Analytical MDLs, September 2002 (Off-Site Laboratory).....	3-13
3.4.2-7	Summary of DSS Site 1035, Building 6715 Septic System, Confirmatory Soil Sampling, HE Compound Analytical Results, September 2002 (Off-Site Laboratory).....	3-14
3.4.2-8	Summary of DSS Site 1035, Building 6715 Septic System, Confirmatory Soil Sampling, HE Compound Analytical MDLs, September 2002 (Off-Site Laboratory).....	3-15
3.4.2-9	Summary of DSS Site 1035, Building 6715 Septic System, Confirmatory Soil Sampling, Metals Analytical Results, September 2002 (Off-Site Laboratory).....	3-16
3.4.2-10	Summary of DSS Site 1035, Building 6715 Septic System, Confirmatory Soil Sampling, Metals Analytical MDLs, September 2002 (Off-Site Laboratory).....	3-17

## LIST OF TABLES (Concluded)

### Table

3.4.2-11	Summary of DSS Site 1035, Building 6715 Septic System, Confirmatory Soil Sampling, Total Cyanide Analytical Results, September 2002 (Off-Site Laboratory).....	3-18
3.4.2-12	Summary of DSS Site 1035, Building 6715 Septic System, Confirmatory Soil Sampling, Total Cyanide Analytical MDLs, September 2002 (Off-Site Laboratory).....	3-18
3.4.2-13	Summary of DSS Site 1035, Building 6715 Septic System, Confirmatory Soil Sampling, Gamma Spectroscopy Analytical Results, September 2002 (On-Site Laboratory).....	3-19
3.4.2-14	Summary of DSS Site 1035, Building 6715 Septic System, Confirmatory Soil Sampling, Gross Alpha/Beta Activity Analytical Results, September 2002 (Off-Site Laboratory).....	3-21
4.2-1	Summary of Potential COCs for DSS Site 1035, Building 6715 Septic System .....	4-5
4.3.2-1	Summation of Incremental Radiological and Nonradiological Risks from DSS Site 1035, Building 6715 Septic System Carcinogens .....	4-7

## LIST OF ANNEXES

### Annex

- A DSS Site 1035 Septic Tank Sampling Results
- B DSS Site 1035 Gore-Sorber™ Passive Soil-Vapor Survey Analytical Results
- C DSS Site 1035 Soil Sample Data Validation Results
- D DSS Site 1035 Risk Assessment

**This page intentionally left blank.**

## ACRONYMS AND ABBREVIATIONS

AOP	Administrative Operating Procedure
BA	butyl acetate
bgs	below ground surface
CAC	Corrective Action Complete
COC	constituent of concern
DSS	Drain and Septic Systems
EB	equipment blank
EPA	U.S. Environmental Protection Agency
ER	Environmental Restoration
FIP	Field Implementation Plan
GS	Gore-Sorber™
HE	high explosive
HI	hazard index
HWB	Hazardous Waste Bureau
KAFB	Kirtland Air Force Base
MDA	minimum detectable activity
MDL	method detection limit
mrem	millirem
NFA	no further action
NMED	New Mexico Environment Department
OU	Operable Unit
PCB	polychlorinated biphenyl
RCRA	Resource Conservation and Recovery Act
RPSD	Radiation Protection Sample Diagnostics
SAP	Sampling and Analysis Plan
SNL/NM	Sandia National Laboratories/New Mexico
SVOC	semivolatile organic compound
SWMU	Solid Waste Management Unit
TA	Technical Area
TB	trip blank
TEDE	total effective dose equivalent
TOP	Technical Operating Procedure
VOC	volatile organic compound
yr	year

**This page intentionally left blank.**

## 1.0 PROJECT BACKGROUND

Environmental characterization of Sandia National Laboratories/New Mexico (SNL/NM) drain and septic systems (DSS) started in the early 1990s. These units consist of either septic systems (one or more septic tanks plumbed to either drainfields or seepage pits), or other types of miscellaneous drain units without septic tanks (including drywells or french drains, seepage pits, and surface outfalls). Initially, 23 of these sites were designated as Solid Waste Management Units (SWMUs) under Operable Unit (OU) 1295, Septic Tanks and Drainfields. Characterization work at 22 of these 23 SWMUs has taken place since 1994 as part of SNL/NM Environmental Restoration (ER) Project activities. The twenty-third site did not require any characterization, and an administrative proposal for no further action (NFA) was granted in July 1995.

Numerous other DSS sites that were not designated as SWMUs were also present throughout SNL/NM. An initial list of these non-SWMU sites was compiled and summarized in an SNL/NM document dated July 8, 1996; the list included a total of 101 sites, facilities, or systems (Bleakly July 1996). For tracking purposes, each of these 101 individual DSS sites was designated with a unique four-digit site identification number starting with 1001. This numbering scheme was devised to clearly differentiate these non-SWMU sites from existing SNL/NM SWMUs, which have been designated by one- to three-digit numbers. As work progressed on the DSS site evaluation project, it became apparent that the original 1996 list was in need of field verification and updating. This process included researching SNL/NM's extensive library of facilities engineering drawings and conducting field-verification inspections jointly with SNL/NM ER personnel and New Mexico Environment Department (NMED)/Hazardous Waste Bureau (HWB) regulatory staff from July 1999 through January 2000. The goals of this additional work included the following:

- Determine to the degree possible whether each of the 101 systems included on the 1996 list was still in existence, or had ever existed.
- For systems confirmed or believed to exist, determine the exact or apparent locations and components of those systems (septic tanks, drainfields, seepage pits, etc.).
- Identify which systems would, or would not, need initial shallow investigation work as required by the NMED.
- For systems requiring characterization, determine the specific types of shallow characterization work (including passive soil-vapor sampling and/or shallow soil borings) that would be required by the NMED.

A number of additional drain systems were identified from the engineering drawings and field inspection work. It was also determined that some of the sites on the 1996 list actually contained more than one individual drain or septic system that had been combined under one four-digit site number. In order to reduce confusion, a decision was made to assign each individual system its own unique four-digit number. A new site list containing a total of 121 individual DSS sites was generated in 2000. Of these 121 sites, the NMED required environmental assessment work at a total of 61. No characterization was required at the remaining 60 sites because the sites either were found not to exist, were the responsibility of

other non-SNL/NM organizations, were already designated as individual SWMUs, or were considered by the NMED to pose no threat to human health or the environment. Subsequent backhoe excavation at DSS Site 1091 confirmed that the system did not exist, which decreased the number of DSS sites requiring characterization to 60.

Concurrent with the field inspection and site identification work, NMED/HWB and SNL/NM ER Project technical personnel worked together to reach consensus on a staged approach and specific procedures that would be used to characterize the DSS sites, as well as the remaining OU 1295 Septic Tanks and Drainfield SWMUs that had not been approved for NFA. These procedures are described in detail in the "Sampling and Analysis Plan [SAP] for Characterizing and Assessing Potential Releases to the Environment From Septic and Other Miscellaneous Drain Systems at Sandia National Laboratories/New Mexico" (SNL/NM October 1999), which was approved by the NMED/HWB on January 28, 2000 (Bearzi January 2000). A follow-on document, "Field Implementation Plan [FIP], Characterization of Non-Environmental Restoration Drain and Septic Systems" (SNL/NM November 2001), was then written to formally document the updated DSS site list and the specific site characterization work required by the NMED for each of the 60 DSS sites. The FIP was approved by the NMED in February 2002 (Moats February 2002).



## **2.0 DSS SITE 1035: BUILDING 6715 SEPTIC SYSTEM**

### **2.1 Summary**

The SNL/NM ER Project conducted an assessment of DSS Site 1035, the Building 6715 Septic System. There are no known or specific environmental concerns at this site. The assessment was conducted to determine whether environmental contamination was released to the environment via the septic system present at the site. This report provides documentation that the site was specifically characterized, that no significant releases of contaminants to the environment occurred via the Building 6715 Septic System, and that it does not pose a threat to human health or the environment under either the industrial or residential land-use scenarios. Current operations at the site are conducted in accordance with applicable laws and regulations that are protective of the environment, and septic system discharges are now directed to the City of Albuquerque sewer system.

Review and analysis of all relevant data for DSS Site 1035 indicate that concentrations of constituents of concern (COCs) at this site were found to be below applicable risk assessment action levels. Thus, a determination of Corrective Action Complete (CAC) without controls (NMED April 2004) is recommended for DSS Site 1035 based upon sampling data demonstrating that COCs released from the site into the environment pose an acceptable level of risk.


### **2.2 Site Description and Operational History**

#### **2.2.1 Site Description**






DSS Site 1035 is located in SNL/NM Technical Area (TA)-III on federally owned land controlled by Kirtland Air Force Base (KAFB) and permitted to the U.S. Department of Energy (Figure 2.2.1-1). The site is located approximately 1,500 feet southwest of the entrance to TA-III (Figure 2.2.1-2). The abandoned septic system consisted of a 750-gallon septic tank that emptied to a single seepage pit (Figure 2.2.1-2). Construction details are based upon engineering drawings (SNL/NM November 1976) and site inspections. The system received discharges from Building 6715, approximately 90 feet to the east.

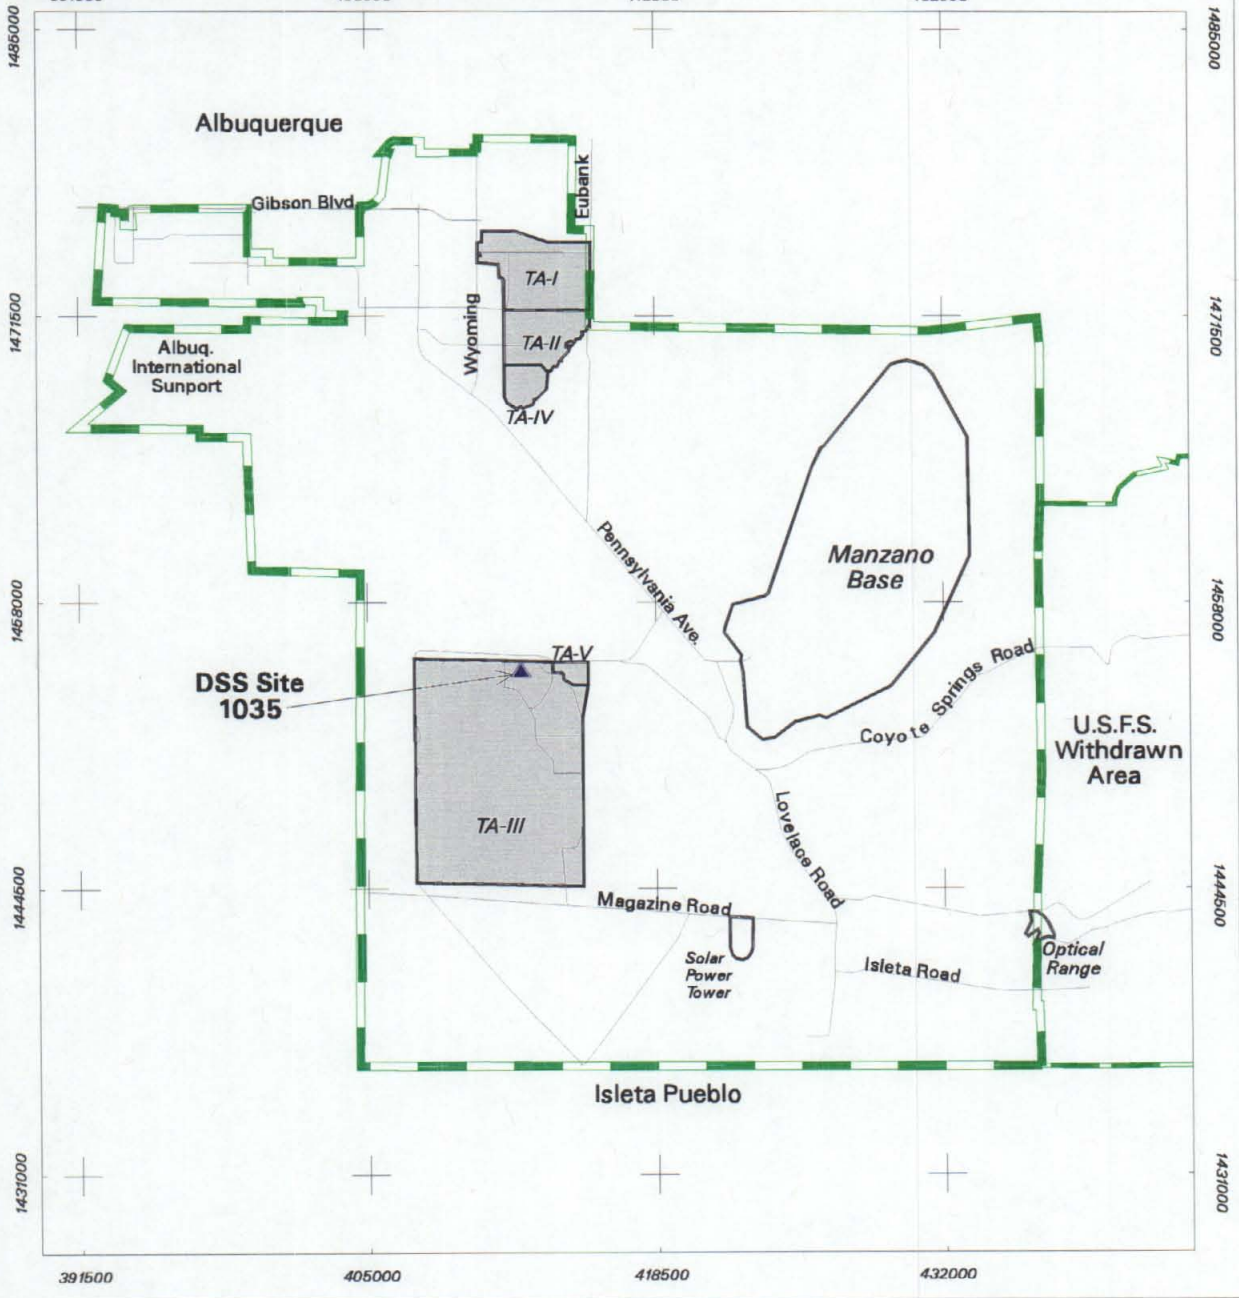The surface geology at DSS Site 1035 is characterized by a veneer of aeolian sediments underlain by Upper Santa Fe Group alluvial fan deposits that interfinger with sediments of the ancestral Rio Grande west of the site. These deposits extend to, and probably far below, the water table at this site. The alluvial fan materials originated in the Manzanita Mountains east of DSS Site 1035, and typically consist of a mixture of silts, sands, and gravels that are poorly sorted, and exhibit moderately connected lenticular bedding. Individual beds range from 1 to 5 feet in thickness with a preferred east-west orientation and have moderate to low hydraulic conductivities (SNL/NM March 1996). Site vegetation primarily consists of desert grasses, shrubs, and cacti.


**This page intentionally left blank.**




**Legend**

-  DSS Site 1035
-  Major Road
-  KAFB Boundary
-  USFS Withdrawn Area Boundary
-  SNL Technical Area

**Figure 2.2.1-1**  
**Location Map of Drain and Septic**  
**Systems (DSS) Site Number 1035,**  
**Bldg. 6715 Septic System, TA-III**





Sandia National Laboratories, New Mexico  
 Environmental Geographic Information System

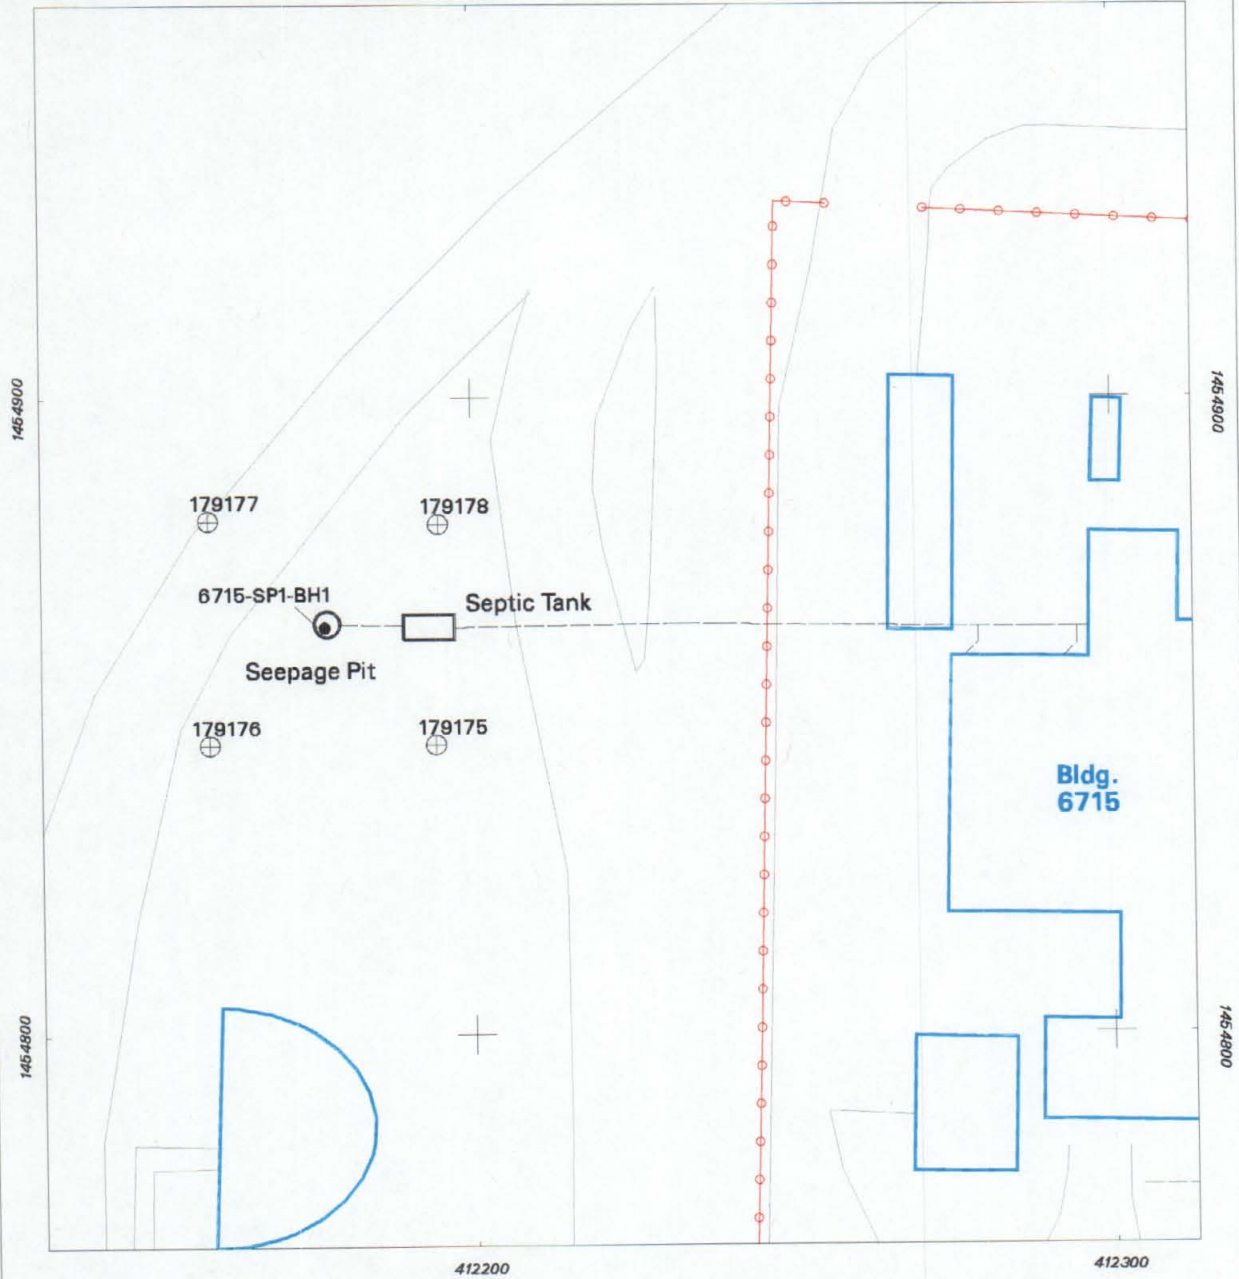

### Legend

- Soil Boring Location
- ⊕ Gore-Sorber Sample Location
- ▭ Septic Tank / Seepage Pit
- Fence
- Road
- ▭ Building / Structure
- - - Septic Drain Line

**Figure 2.2.1-2**  
**Site Map of Drain and Septic**  
**Systems (DSS) Site Number 1035,**  
**Bldg. 6715 Septic System, TA-III**



Sandia National Laboratories, New Mexico  
Environmental Geographic Information System

The ground surface in the vicinity of the site is flat to very slightly sloping to the west. The closest major drainage is the Arroyo del Coyote, located approximately 1.1 miles northeast of the site. No perennial surface-water bodies are present in the vicinity of the site. Average annual rainfall in the SNL/NM and KAFB area, as measured at Albuquerque International Sunport, is 8.1 inches (NOAA 1990). Infiltration of precipitation is almost nonexistent as virtually all of the moisture subsequently undergoes evapotranspiration. The estimates of evapotranspiration rates for the KAFB area range from 95 to 99 percent of the annual rainfall (SNL/NM March 1996).

The site lies at an average elevation of approximately 5,390 feet above mean sea level (SNL/NM April 2003). Depth to groundwater is approximately 470 feet below ground surface (bgs) at the site. Groundwater flow is thought to be generally to the west in this area (SNL/NM March 2002). The nearest production wells to DSS Site 1035 are KAFB-4, approximately 2.7 miles to the northwest, and KAFB-11, approximately 3.2 miles to the northeast. The nearest groundwater monitoring well is TAV-MW5, approximately 1,000 feet northeast of the site.

## 2.2.2 Operational History

Available information indicates that Building 6715, currently known as the Explosive Test Facility, was constructed in 1962 (SNL/NM March 2003), and it is assumed the septic system was constructed at the same time. Because operational records are not available, the site investigation was planned to be consistent with other DSS site investigations and to sample for the possible COCs that may have been released during facility operations.

In the early 1990s, Building 6715 was connected to an extension of the City of Albuquerque sanitary sewer system (Jones June 1991). The old septic system line was disconnected and capped, and the system was abandoned in place concurrent with this change (Romero September 2003).

## 2.3 Land Use

### 2.3.1 Current Land Use

The current land use for DSS Site 1035 is industrial.

### 2.3.2 Future/Proposed Land Use

The projected future land use for DSS Site 1035 is industrial (DOE et al. September 1995).

**This page intentionally left blank.**

## **3.0 INVESTIGATORY ACTIVITIES**

### **3.1 Summary**

Three assessment investigations have been conducted at this site. In late 1990 or early 1991, 1992, and 1995, waste characterization samples were collected from the septic tank (Investigation 1). In late April and early May 2002, a passive soil-vapor survey was conducted to determine whether areas of significant volatile organic compound (VOC) contamination were present in the soil around the seepage pit (Investigation 2). In September 2002, subsurface soil samples were collected from one boring drilled through the center of, and beneath, the seepage pit (Investigation 3). Investigations 2 and 3 were required by the NMED/HWB to adequately characterize the site and were conducted in accordance with procedures presented in the SAP (SNL/NM October 1999) and FIP (SNL/NM November 2001) described in Chapter 1.0. These investigations are discussed in the following sections.

### **3.2 Investigation 1—Septic Tank Sampling**

Investigation 1 consisted of sampling efforts to characterize the waste contents of all SNL/NM septic tanks for chemical and radiological contamination. The primary goal of the sampling was to identify types and concentrations of potential contaminants in the waste within the tanks so that the appropriate waste disposal and remedial activities could be planned.

In late 1990 or early 1991, August 1992, and July 1995, as part of the SNL/NM Septic System Monitoring Program, aqueous and sludge samples were collected from the Building 6715 septic tank (SNL/NM April 1991, SNL/NM June 1993, and SNL/NM December 1995). In late 1990 or early 1991, an aqueous sample was analyzed at an off-site laboratory for VOCs, oil and grease, total cyanide, nitrate, phenolics, total metals, and gross alpha/beta activity. On August 18, 1992, a sludge sample was collected and analyzed at an off-site laboratory for gross alpha/beta activity, tritium, and radionuclides by gamma spectroscopy. On July 12, 1995, an aqueous sample and a sludge sample were collected and analyzed at an off-site laboratory. The aqueous sample was analyzed for VOCs, semivolatile organic compounds (SVOCs), pesticides and polychlorinated biphenyls (PCBs), total metals, pH, formaldehyde, fluoride, nitrate plus nitrite, oil and grease, total phenols, gross alpha/beta activity, tritium, and radionuclides by gamma spectroscopy. The sludge sample was analyzed for VOCs, SVOCs, pesticides and PCBs, total metals, and radionuclides by isotopic analysis and gamma spectroscopy. The analytical results are presented in Annex A. A fraction of each sample was also submitted to the SNL/NM Radiation Protection Sample Diagnostics (RPSD) Laboratory for gamma spectroscopy analysis prior to off-site release.

On March 27, 1996, the residual contents, approximately 615 gallons of waste and added water, were pumped out and managed according to SNL/NM policy (Shain August 1996).

### **3.3 Investigation 2—Passive Soil-Vapor Sampling**

In late April and early May 2002, a passive soil-vapor survey was conducted in the Building 6715 Septic System area. This survey was required at this site by NMED/HWB

regulators and was conducted to determine whether significant VOC contamination was present in the soil at the site.

### 3.3.1 Passive Soil-Vapor Sampling Methodology

A Gore-Sorber™ (GS) passive soil-vapor survey is a qualitative screening procedure that can be used to identify many VOCs present in the vapor phase in soil. The technique is highly sensitive to organic vapors, and the result produces a qualitative measure of organic soil vapor chemistry over a two- to three-week period rather than at one point in time.

Each GS soil-vapor sampler consists of a 1-foot-long, 0.25-inch-diameter tube of waterproof, vapor-permeable fabric containing 40 milligrams of absorbent material. At each sampling location, a 3-foot-deep by 1.5-inch-diameter borehole was drilled with the Geoprobe™. A sample identification tag and location string were attached to the GS sampler and lowered into the open borehole to a depth of 1 to 2 feet bgs. The location string was attached to a numbered pin flag at the surface. A cork was placed in the borehole above the sampler as a seal, and the upper 1 foot of the borehole, from the cork to the ground surface, was backfilled with site soil.

The vapor samplers were left in the ground for approximately two weeks before retrieval. After retrieval, each sampler was individually placed into a pre-cleaned jar, sealed, and sent to W.L. Gore and Associates for analysis by thermal desorption and gas chromatography using a modified U.S. Environmental Protection Agency (EPA) Method 8260. Analytical results for the VOCs of interest are reported as mass (expressed in micrograms) of the individual VOCs absorbed by the sampler while it was in the ground (Gore June 2002). All samples were documented and handled in accordance with applicable SNL/NM operating procedures.

### 3.3.2 Soil-Vapor Survey Results and Conclusions

A total of four GS passive soil-vapor samplers were placed in the seepage pit area of the site (Figure 2.2.1-2). Samplers were installed at the site on April 29, 2002, and were retrieved on May 14, 2002. Sample locations are designated by the same six-digit sample number both on Figure 2.2.1-2 and in the analytical results tables presented in Annex B.

As shown in the analytical results tables in Annex B, the GS samplers were analyzed for a total of 30 individual or groups of VOCs, including trichloroethene, tetrachloroethene, cis- and trans-dichloroethene, and benzene/toluene/ethylbenzene/xylene. Low to trace-level (but quantifiable) amounts of 18 individual or groups of VOCs were detected in the GS samplers installed at this site. The analytical results indicated there were no areas of significant VOC contamination at the site that would require additional characterization.

## 3.4 Investigation 3—Soil Sampling

Soil sampling beneath the seepage pit was conducted in accordance with the rationale and procedures in the SAP (SNL/NM October 1999) approved by the NMED. On September 12, 2002, soil samples were collected from one seepage pit borehole. The soil boring location is shown on Figure 2.2.1-2. Figure 3.4-1 shows soil samples being collected at DSS Site 1035.





Figure 3.4-1  
Collecting soil samples with the Geoprobe™ from the  
borehole drilled through the center of the seepage pit at DSS Site 1035,  
the Building 6715 Septic System. View to the southeast. September 12, 2002

A summary of the borehole, sample depths, sample analyses, analytical methods, laboratories, and sample date is presented in Table 3.4-1.

### 3.4.1 Soil Sampling Methodology

An auger drill rig was used to sample the borehole at two depth intervals. In the borehole drilled through the center of the seepage pit, the shallow sample interval started at the estimated base of the gravel aggregate in the seepage pit bottom, and the lower (deep) interval started 5 feet below the top of the upper interval. Once the auger rig had reached the top of the sampling interval, a 3- or 4-foot-long by 1.5-inch inside diameter Geoprobe™ sampling tube lined with a butyl acetate (BA) sampling sleeve was inserted into the borehole and hydraulically driven downward 3 or 4 feet to fill the tube with soil.

Once the sample tube was retrieved from the borehole, the sample for VOC analysis was immediately collected by slicing off a 3- to 4-inch section from the lower end of the BA sleeve and capping the section ends with Teflon® film, then a rubber end cap, and finally sealing the tube with tape.

For the non-VOC analyses, the soil remaining in the BA liner was emptied into a decontaminated mixing bowl, and aliquots of soil were transferred into appropriate sample containers for analysis. On occasion, the amount of soil recovered in the first sampling run was insufficient for sample volume requirements. In this case, additional sampling runs were completed until an adequate soil volume was recovered. Soil recovered from these additional runs was emptied into the mixing bowl and blended with the soil already collected. Aliquots of the blended soil were then transferred into sample containers and submitted for analysis.

All samples were documented and handled in accordance with applicable SNL/NM operating procedures and transported to on- and off-site laboratories for analysis.

### 3.4.2 Soil Sampling Results and Conclusions

Analytical results for the soil samples collected at DSS Site 1035 are presented and discussed in this section.

#### VOCs

VOC analytical results for the two soil samples collected from the seepage pit borehole are summarized in Table 3.4.2-1. Method detection limits (MDLs) for the VOC soil analyses are presented in Table 3.4.2-2. Acetone was detected in the 11-foot-bgs sample, and 2-butanone was detected in the 16-foot-bgs sample. These compounds were not detected in the associated trip blank (TB) but they are common laboratory contaminants and these detections may not indicate soil contamination at this site.

Table 3.4-1  
 Summary of Area Sampled, Analytical Methods, and Laboratories Used for  
 DSS Site 1035, Building 6715 Septic System Soil Samples

Sampling Area	Number of Borehole Locations	Top of Sampling Intervals in Each Borehole (ft. bgs)	Total Number of Soil Samples	Analytical Parameters and EPA Methods <sup>a</sup>	Analytical Laboratory	Date Samples Collected
Seepage Pit	1	11, 16	2	VOCs EPA Method 8260	GEL	09-12-02
	1	11, 16	2	SVOCs EPA Method 8270	GEL	09-12-02
	1	11, 16	2	PCBs EPA Method 8082	GEL	09-12-02
	1	11, 16	2	HE Compounds EPA Method 8330	GEL	09-12-02
	1	11, 16	2	RCRA Metals EPA Methods 6000/7000	GEL	09-12-02
	1	11, 16	2	Hexavalent Chromium EPA Method 7196A	GEL	09-12-02
	1	11, 16	2	Total Cyanide EPA Method 9012A	GEL	09-12-02
	1	11, 16	2	Gamma Spectroscopy Radionuclides EPA Method 901.1	RPSD	09-12-02
	1	11, 16	2	Gross Alpha/Beta Activity EPA Method 900.0	GEL	09-12-02

<sup>a</sup>EPA November 1986.

- bgs = Below ground surface.
- DSS = Drain and Septic Systems.
- EPA = U. S. Environmental Protection Agency.
- ft = Foot (feet).
- GEL = General Engineering Laboratories, Inc.
- HE = High explosive(s).
- PCB = Polychlorinated biphenyl.
- RCRA = Resource Conservation and Recovery Act.
- RPSD = Radiation Protection Sample Diagnostics Laboratory.
- SVOC = Semivolatile organic compound.
- VOC = Volatile organic compound.

Table 3.4.2-1  
 Summary of DSS Site 1035, Building 6715 Septic System  
 Confirmatory Soil Sampling, VOC Analytical Results  
 September 2002  
 (Off-Site Laboratory)

Sample Attributes			VOCs (EPA Method 8260 <sup>a</sup> ) (µg/kg)	
Record Number <sup>b</sup>	ER Sample ID	Sample Depth (ft)	Acetone	2-Butanone
605672	6715-SP1-BH1-11-S	11	<b>4.17 J (5)</b>	ND (3.74)
605672	6715-SP1-BH1-16-S	16	ND (3.52)	<b>6.74</b>
Quality Assurance/Quality Control Sample (µg/L)				
605672	6715-SP1-TB <sup>c</sup>	NA	ND (4.5)	ND (2.31)

Note: Values in **bold** represent detected analytes.

<sup>a</sup>EPA November 1986.

<sup>b</sup>Analysis request/chain-of-custody record.

<sup>c</sup>ER sample ID reflects the final site for VOC samples included in this shipment.

BH = Borehole.

DSS = Drain and Septic Systems.

EPA = U.S. Environmental Protection Agency.

ER = Environmental Restoration.

ft = Foot (feet).

ID = Identification.

J ( ) = The reported value is greater than or equal to the MDL but is less than the practical quantitation limit, shown in parentheses.

MDL = Method detection limit.

µg/kg = Microgram(s) per kilogram.

µg/L = Microgram(s) per liter.

NA = Not applicable.

ND ( ) = Not detected above the MDL, shown in parentheses.

S = Soil sample.

SP = Seepage pit.

TB = Trip blank.

VOC = Volatile organic compound.

Table 3.4.2-2  
 Summary of DSS Site 1035, Building 6715 Septic System  
 Confirmatory Soil Sampling, VOC Analytical MDLs  
 September 2002  
 (Off-Site Laboratory)

Analyte	EPA Method 8260 <sup>a</sup> Detection Limit ( $\mu\text{g}/\text{kg}$ )
Acetone	3.45–3.59
Benzene	0.441–0.459
Bromodichloromethane	0.48–0.5
Bromoform	0.48–0.5
Bromomethane	0.49–0.51
2-Butanone	3.67–3.82
Carbon disulfide	2.31–2.41
Carbon tetrachloride	0.48–0.5
Chlorobenzene	0.402–0.418
Chloroethane	0.794–0.827
Chloroform	0.51–0.531
Chloromethane	0.363–0.378
Dibromochloromethane	0.49–0.51
1,1-Dichloroethane	0.461–0.48
1,2-Dichloroethane	0.422–0.439
1,1-Dichloroethene	0.49–0.51
cis-1,2-Dichloroethene	0.461–0.48
trans-1,2-Dichloroethene	0.52–0.541
1,2-Dichloropropane	0.471–0.49
cis-1,3-Dichloropropene	0.422–0.439
trans-1,3-Dichloropropene	0.245–0.255
Ethylbenzene	0.373–0.388
2-Hexanone	3.7–3.85
Methylene chloride	1.32–1.38
4-Methyl-2-pentanone	3.95–4.11
Styrene	0.382–0.398
1,1,2,2-Tetrachloroethane	0.892–0.929
Tetrachloroethene	0.373–0.388
Toluene	0.333–0.347
1,1,1-Trichloroethane	0.52–0.541
1,1,2-Trichloroethane	0.529–0.551
Trichloroethene	0.441–0.459
Vinyl acetate	1.75–1.82
Vinyl chloride	0.549–0.571
Xylene	0.382–0.398

<sup>a</sup>EPA November 1986.

DSS = Drain and Septic Systems.

EPA = U.S. Environmental Protection Agency.

MDL = Method detection limit.

$\mu\text{g}/\text{kg}$  = Microgram(s) per kilogram.

VOC = Volatile organic compound.

### SVOCs

SVOC analytical results for the two soil samples collected from the seepage pit borehole are summarized in Table 3.4.2-3. MDLs for the SVOC soil analyses are presented in Table 3.4.2-4. One SVOC, bis(2-ethylhexyl) phthalate, was detected in both the 11- and 16-foot-bgs samples collected from the borehole. This compound is a common component in plastics and may not indicate soil contamination at this site.

### PCBs

PCB analytical results for the two soil samples collected from the seepage pit borehole are summarized in Table 3.4.2-5. MDLs for the PCB soil analyses are presented in Table 3.4.2-6. No PCBs were detected in either of the soil samples collected from the borehole.

### HE Compounds

High explosive (HE) compound analytical results for the two soil samples collected from the seepage pit borehole are summarized in Table 3.4.2-7. MDLs for the HE soil analyses are presented in Table 3.4.2-8. No HE compounds were detected in the samples collected from the borehole.

### RCRA Metals and Hexavalent Chromium

Resource Conservation and Recovery Act (RCRA) metals and hexavalent chromium analytical results for the two soil samples collected from the seepage pit borehole are summarized in Table 3.4.2-9. MDLs for the metals in soil analyses are presented in Table 3.4.2-10. Barium was detected above the NMED-approved background in only the 16-foot-bgs sample from the borehole. All other metal concentrations were below the NMED-approved background concentrations.

### Total Cyanide

Total cyanide analytical results for the two soil samples collected from the seepage pit borehole are summarized in Table 3.4.2-11. MDLs for the cyanide soil analyses are presented in Table 3.4.2-12. Cyanide was detected in both the 11- and 16-foot-bgs samples from the borehole. All other metal concentrations were below the NMED-approved background concentrations.

### Radionuclides

Analytical results for the gamma spectroscopy analysis of the two soil samples collected from the seepage pit borehole are summarized in Table 3.4.2-13. No activities above NMED-approved background levels were detected in any sample analyzed. However, although not detected, the minimum detectable activity (MDA) for one uranium-235 analysis exceeded the background activity because the standard gamma spectroscopy count time for soil samples (6,000 seconds) was not sufficient to reach the NMED-approved background activity

Table 3.4.2-3  
 Summary of DSS Site 1035, Building 6715 Septic System  
 Confirmatory Soil Sampling, SVOC Analytical Results  
 September 2002  
 (Off-Site Laboratory)

Sample Attributes			SVOCs (EPA Method 8270 <sup>a</sup> ) ( $\mu\text{g}/\text{kg}$ )
Record Number <sup>b</sup>	ER Sample ID	Sample Depth (ft)	bis(2-Ethylhexyl) phthalate
605672	6715-SP1-BH1-11-S	11	<b>142 J (333)</b>
605672	6715-SP1-BH1-16-S	16	<b>102 J (333)</b>

Note: Values in **bold** represent detected analytes.

<sup>a</sup>EPA November 1986.

<sup>b</sup>Analysis request/chain-of-custody record.

BH = Borehole.

DSS = Drain and Septic Systems.

EPA = U.S. Environmental Protection Agency.

ER = Environmental Restoration.

ft = Foot (feet).

ID = Identification.

J ( ) = The reported value is greater than or equal to the MDL but is less than the practical quantitation limit, shown in parentheses.

MDL = Method detection limit.

$\mu\text{g}/\text{kg}$  = Microgram(s) per kilogram.

S = Soil sample.

SP = Seepage pit.

SVOC = Semivolatile organic compound.

Table 3.4.2-4  
 Summary of DSS Site 1035, Building 6715 Septic System  
 Confirmatory Soil Sampling, SVOC Analytical MDLs  
 September 2002  
 (Off-Site Laboratory)

Analyte	EPA Method 8270 <sup>a</sup> Detection Limit (µg/kg)
Acenaphthene	8
Acenaphthylene	16.7
Anthracene	16.7
Benzo(a)anthracene	16.7
Benzo(a)pyrene	16.7
Benzo(b)fluoranthene	16.7
Benzo(g,h,i)perylene	16.7
Benzo(k)fluoranthene	16.7
4-Bromophenyl phenyl ether	34
Butylbenzyl phthalate	28.7
Carbazole	16.7
4-Chlorobenzenamine	167
bis(2-Chloroethoxy)methane	12.3
bis(2-Chloroethyl)ether	37.3
bis-Chloroisopropyl ether	11
4-Chloro-3-methylphenol	167
2-Chloronaphthalene	13.7
2-Chlorophenol	15.3
4-Chlorophenyl phenyl ether	19.7
Chrysene	16.7
o-Cresol	26
Dibenz[a,h]anthracene	16.7
Dibenzofuran	17
1,2-Dichlorobenzene	10
1,3-Dichlorobenzene	11.3
1,4-Dichlorobenzene	15.7
3,3'-Dichlorobenzidine	167
2,4-Dichlorophenol	20.7
Diethylphthalate	17.7
2,4-Dimethylphenol	167
Dimethylphthalate	18.3
Di-n-butyl phthalate	24
Dinitro-o-cresol	167
2,4-Dinitrophenol	167
2,4-Dinitrotoluene	25.3
2,6-Dinitrotoluene	33.3
Di-n-octyl phthalate	30.3
Diphenyl amine	22.3
bis(2-Ethylhexyl) phthalate	30
Fluoranthene	16.7
Fluorene	4
Hexachlorobenzene	20

Refer to footnotes at end of table.



Table 3.4.2-4 (Concluded)  
 Summary of DSS Site 1035, Building 6715 Septic System  
 Confirmatory Soil Sampling, SVOC Analytical MDLs  
 September 2002  
 (Off-Site Laboratory)

Analyte	EPA Method 8270 <sup>a</sup> Detection Limit ( $\mu\text{g}/\text{kg}$ )
Hexachlorobutadiene	12.7
Hexachlorocyclopentadiene	167
Hexachloroethane	22
Indeno(1,2,3-cd)pyrene	16.7
Isophorone	16
2-Methylnaphthalene	16.7
4-Methylphenol	33.3
Naphthalene	16.7
2-Nitroaniline	167
3-Nitroaniline	167
4-Nitroaniline	37
Nitrobenzene	20.3
2-Nitrophenol	17
4-Nitrophenol	167
n-Nitrosodipropylamine	22.7
Pentachlorophenol	167
Phenanthrene	16.7
Phenol	12.7
Pyrene	16.7
1,2,4-Trichlorobenzene	12.7
2,4,5-Trichlorophenol	17.3
2,4,6-Trichlorophenol	27.3

<sup>a</sup>EPA November 1986.

DSS = Drain and Septic Systems.

EPA = U.S. Environmental Protection Agency.

MDL = Method detection limit.

$\mu\text{g}/\text{kg}$  = Microgram(s) per kilogram.

SVOC = Semivolatile organic compound.

Table 3.4.2-5  
 Summary of DSS Site 1035, Building 6715 Septic System  
 Confirmatory Soil Sampling, PCB Analytical Results  
 September 2002  
 (Off-Site Laboratory)

Sample Attributes			PCBs (EPA Method 8082 <sup>a</sup> ) (µg/kg)
Record Number <sup>b</sup>	ER Sample ID	Sample Depth (ft)	
605672	6715-SP1-BH1-11-S	11	ND
605672	6715-SP1-BH1-16-S	16	ND

<sup>a</sup>EPA November 1986.

<sup>b</sup>Analysis request/chain-of-custody record.

BH = Borehole.

DSS = Drain and Septic Systems.

EPA = U.S. Environmental Protection Agency.

ER = Environmental Restoration.

ft = Foot (feet).

ID = Identification.

µg/kg = Microgram(s) per kilogram.

ND = Not detected.

PCB = Polychlorinated biphenyl.

S = Soil sample.

SP = Seepage pit.

Table 3.4.2-6  
 Summary of DSS Site 1035, Building 6715 Septic System  
 Confirmatory Soil Sampling, PCB Analytical MDLs  
 September 2002  
 (Off-Site Laboratory)

Analyte	EPA Method 8082 <sup>a</sup> Detection Limit (µg/kg)
Aroclor-1016	1
Aroclor-1221	2.82
Aroclor-1232	1.67
Aroclor-1242	1.67
Aroclor-1248	1
Aroclor-1254	0.5
Aroclor-1260	1

<sup>a</sup>EPA November 1986.

DSS = Drain and Septic Systems.

EPA = U.S. Environmental Protection Agency.

MDL = Method detection limit.

µg/kg = Microgram(s) per kilogram.

PCB = Polychlorinated biphenyl.

Table 3.4.2-7  
 Summary of DSS Site 1035, Building 6715 Septic System  
 Confirmatory Soil Sampling, HE Compound Analytical Results  
 September 2002  
 (Off-Site Laboratory)

Sample Attributes			HE (EPA Method 8330 <sup>a</sup> ) (µg/kg)
Record Number <sup>b</sup>	ER Sample ID	Sample Depth (ft)	
605672	6715-SP1-BH1-11-S	11	ND
605672	6715-SP1-BH1-16-S	16	ND

<sup>a</sup>EPA November 1986.

<sup>b</sup>Analysis request/chain-of-custody record.

BH = Borehole.

DSS = Drain and Septic Systems.

EPA = U.S. Environmental Protection Agency.

ER = Environmental Restoration.

ft = Foot (feet).

HE = High explosive(s).

ID = Identification.

µg/kg = Microgram(s) per kilogram.

ND = Not detected.

S = Soil sample.

SP = Seepage pit.

Table 3.4.2-8  
 Summary of DSS Site 1035, Building 6715 Septic System  
 Confirmatory Soil Sampling, HE Compound Analytical MDLs  
 September 2002  
 (Off-Site Laboratory)

Analyte	EPA Method 8330 <sup>a</sup> Detection Limit (µg/kg)
2-Amino-4,6-dinitrotoluene	18.1
4-Amino-2,6-dinitrotoluene	34.1
1,3-Dinitrobenzene	34.1
2,4-Dinitrotoluene	55
2,6-Dinitrotoluene	48
HMX	48
Nitrobenzene	48
2-Nitrotoluene	24
3-Nitrotoluene	24
4-Nitrotoluene	24
RDX	48
Tetryl	22.1
1,3,5-Trinitrobenzene	29
2,4,6-Trinitrotoluene	48

<sup>a</sup>EPA November 1986.

DSS = Drain and Septic Systems.

EPA = U.S. Environmental Protection Agency.

HE = High Explosive(s).

HMX = Octahydro-1,3,5,7-tetranitro-1,3,5,7-tetrazocine.

MDL = Method detection limit.

µg/kg = Microgram(s) per kilogram.

RDX = Hexahydro-1,3,5-trinitro-1,3,5-triazine.

Tetryl = Methyl-2,4,6-trinitrophenylnitramine.

Table 3.4.2-9  
 Summary of DSS Site 1035, Building 6715 Septic System  
 Confirmatory Soil Sampling, Metals Analytical Results  
 September 2002  
 (Off-Site Laboratory)

Sample Attributes			Metals (EPA Methods 6000/7000/ 7196 <sup>a</sup> ) (mg/kg)									
Record Number <sup>b</sup>	ER Sample ID	Sample Depth (ft)	Arsenic	Barium	Cadmium	Chromium	Chromium (VI)	Lead	Mercury	Selenium	Silver	
605672	6715-SP1-BH1-11-S	11	3.79 J	83.2	0.213 J (0.455)	11.2	ND (0.0522)	6.26	0.00605 J (0.00938)	0.361 J (0.455)	ND (0.082)	
605672	6715-SP1-BH1-16-S	16	3.91 J	<b>232</b>	0.208 J (0.5)	10.9	ND (0.0519)	5.82	0.00424 J (0.00872)	ND (0.162 J)	ND (0.0902)	
Background Concentration—Southwest Area Supergroup <sup>c</sup>			4.4	214	0.9	15.9	1	11.8	<0.1	<1	<1	

Note: Values in **bold** exceed background soil concentrations.

<sup>a</sup>EPA November 1986.

<sup>b</sup>Analysis request/chain-of-custody record.

<sup>c</sup>Dirwiddie September 1997.

BH = Borehole.

DSS = Drain and Septic Systems.

EPA = U.S. Environmental Protection Agency.

ER = Environmental Restoration.

ft = Foot (feet).

ID = Identification.

J = Analytical result was qualified as an estimated value.

J ( ) = The reported value is greater than or equal to the MDL but is less than the practical quantitation limit, shown in parentheses.

MDL = Method detection limit.

mg/kg = Milligram(s) per kilogram.

ND ( ) = Not detected above the MDL, shown in parentheses.

S = Soil sample.

SP = Seepage pit.

Table 3.4.2-10  
 Summary of DSS Site 1035, Building 6715 Septic System  
 Confirmatory Soil Sampling, Metals Analytical MDLs  
 September 2002  
 (Off-Site Laboratory)

Analyte	EPA Method 6000/7000/7196 <sup>a</sup> Detection Limit (mg/kg)
Arsenic	0.188-0.206
Barium	0.0606-0.0667
Cadmium	0.0435-0.0478
Chromium	0.146-0.161
Chromium (VI)	0.0519-0.0522
Lead	0.258-0.284
Mercury	0.000857-0.000922
Selenium	0.147-0.162
Silver	0.082-0.0902

<sup>a</sup>EPA November 1986.

DSS = Drain and Septic Systems.

EPA = U.S. Environmental Protection Agency.

MDL = Method detection limit.

mg/kg = Milligram(s) per kilogram.

Table 3.4.2-11  
 Summary of DSS Site 1035, Building 6715 Septic System  
 Confirmatory Soil Sampling, Total Cyanide Analytical Results  
 September 2002  
 (Off-Site Laboratory)

Sample Attributes			Total Cyanide (EPA Method 9012A <sup>a</sup> ) (mg/kg)
Record Number <sup>b</sup>	ER Sample ID	Sample Depth (ft)	Total Cyanide
605672	6715-SP1-BH1-11-S	11	<b>0.0462 J (0.227)</b>
605672	6715-SP1-BH1-16-S	16	<b>0.0457 J (0.25)</b>

Note: Values in **bold** represent detected analytes.

<sup>a</sup>EPA November 1986.

<sup>b</sup>Analysis request/chain-of-custody record.

BH = Borehole.

DSS = Drain and Septic Systems.

EPA = U.S. Environmental Protection Agency.

ER = Environmental Restoration.

ft = Foot (feet).

ID = Identification.

J ( ) = The reported value is greater than or equal to the MDL but is less than the practical quantitation limit, shown in parentheses.

MDL = Method detection limit.

mg/kg = Milligram(s) per kilogram.

S = Soil sample.

SP = Seepage pit.

Table 3.4.2-12  
 Summary of DSS Site 1035, Building 6715 Septic System  
 Confirmatory Soil Sampling, Total Cyanide Analytical MDLs  
 September 2002  
 (Off-Site Laboratory)

Analyte	EPA Method 9012A <sup>a</sup> Detection Limit (mg/kg)
Total Cyanide	0.0381–0.0419

<sup>a</sup>EPA November 1986.

DSS = Drain and Septic Systems.

EPA = U.S. Environmental Protection Agency.

MDL = Method detection limit.

mg/kg = Milligram(s) per kilogram.

Table 3.4.2-13  
 Summary of DSS Site 1035, Building 6715 Septic System  
 Confirmatory Soil Sampling, Gamma Spectroscopy Analytical Results  
 September 2002  
 (On-Site Laboratory)

Sample Attributes		Activity (EPA Method 901.1 <sup>a</sup> )(pCi/g)									
Record Number <sup>b</sup>	ER Sample ID	Sample Depth (ft)	Cesium-137		Thorium-232		Uranium-235		Uranium-238		
			Result	Error <sup>c</sup>	Result	Error <sup>c</sup>	Result	Error <sup>c</sup>	Result	Error <sup>c</sup>	
605732	6715-SP1-BH1-11-S	11	ND (0.0319)	--	0.696	0.338	0.0948	0.169	ND (0.487)	--	
605732	6715-SP1-BH1-16-S	16	ND (0.0344)	--	0.794	0.381	<b>ND (0.199)</b>	--	ND (0.516)	--	
Background Activity—Southwest Area			0.079	NA	1.01	NA	0.16	NA	1.4	NA	
Supergroup <sup>d</sup>											

Note: Values in **bold** exceed background soil activities.

<sup>a</sup>EPA November 1986.

<sup>b</sup>Analysis request/chain-of-custody record.

<sup>c</sup>Two standard deviations about the mean detected activity.

<sup>d</sup>Dinwiddie September 1997.

BH = Borehole.

DSS = Drain and Septic Systems.

EPA = U.S. Environmental Protection Agency.

ER = Environmental Restoration.

ft = Foot (feet).

ID = Identification.

MDA = Minimum detectable activity.

NA = Not applicable.

ND ( ) = Not detected above the MDA, shown in parentheses.

**ND ( )** = Not detected, but the MDA (shown in parentheses) exceeds background activity.

pCi/g = Picocurie(s) per gram.

S = Soil sample.

SP = Seepage pit.

-- = Error not calculated for nondetect results.



established for SNL/NM soil. Even though the MDA may be slightly elevated, it is still very low, and the risk assessment outcome for the site is not significantly impacted by its use.

### Gross Alpha/Beta Activity

Gross alpha/beta activity analytical results for the two soil samples collected from the seepage pit borehole are summarized in Table 3.4.2-14. No gross alpha or beta activity was detected above the New Mexico-established background levels (Miller September 2003) in any of the samples. These results indicate no significant levels of radioactive material are present in the soil at the site.

### 3.4.3 Soil Sampling Quality Assurance/Quality Control Samples and Data Validation Results

Throughout the DSS Project, quality assurance/quality control samples were collected at an approximate frequency of 1 per 20 field samples. These included duplicate, equipment blank (EB), and TB samples. Typically, samples were shipped to the laboratory in batches of up to 20 samples, so that any one shipment might contain samples from several sites. Aqueous EB samples were collected at an approximate frequency of 1 per 20 site samples. The EB samples were analyzed for the same analytical suite as the soil samples in that shipment. The analytical results for the EB samples appear only on the data tables for the site where they were collected. However, the results were used in the data validation process for all the samples in that batch.

Aqueous TB samples, for VOC analysis only, were included in every sample cooler containing VOC soil samples. The analytical results for the TB samples appear on the VOC data tables for the sites in that shipment. The results were used in the data validation process for all the samples in that batch. No VOCs were detected in the TB for DSS Site 1035 (Table 3.4.2-1).

No duplicate samples were collected at this site.

All laboratory data were reviewed and verified/validated according to "Verification and Validation of Chemical and Radiochemical Data," Technical Operating Procedure (TOP) 94-03, Rev. 0 (SNL/NM July 1994) or SNL/NM ER Project "Data Validation Procedure for Chemical and Radiochemical Data," Administrative Operating Procedure (AOP) 00-03 (SNL/NM December 1999). In addition, SNL/NM Department 7713 (RPSD Laboratory) reviewed all gamma spectroscopy results according to "Laboratory Data Review Guidelines," Procedure No. RPSD-02-11, Issue No. 2 (SNL/NM July 1996). Annex C contains the data validation reports for the samples collected at this site. The data are acceptable for use in this request for a determination of CAC without controls.

## 3.5 Site Sampling Data Gaps

Analytical data from the site assessment were sufficient for characterizing the nature and extent of possible COC releases. There are no further data gaps regarding characterization of DSS Site 1035.

Table 3.4.2-14  
 Summary of DSS Site 1035, Building 6715 Septic System  
 Confirmatory Soil Sampling, Gross Alpha/Beta Activity Analytical Results  
 September 2002  
 (Off-Site Laboratory)

Sample Attributes			Activity (EPA Method 900.0 <sup>a</sup> )(pCi/g)			
Record Number <sup>b</sup>	ER Sample ID	Sample Depth (ft)	Gross Alpha		Gross Beta	
			Result	Error <sup>c</sup>	Result	Error <sup>c</sup>
605672	6715-SP1-BH1-11-S	11	12	2.85	19.3	1.81
605672	6715-SP1-BH1-16-S	16	12.5	2.88	18.4	1.97
Background Activity <sup>d</sup>			17.4	NA	35.4	NA

<sup>a</sup>EPA November 1986.

<sup>b</sup>Analysis request/chain-of-custody record.

<sup>c</sup>Two standard deviations about the mean detected activity.

<sup>d</sup>Miller September 2003.

BH = Borehole.

DSS = Drain and Septic Systems.

EPA = U.S. Environmental Protection Agency.

ER = Environmental Restoration.

ft = Foot (feet).

ID = Identification.

NA = Not applicable.

pCi/g = Picocurie(s) per gram.

S = Soil sample.

SP = Seepage pit.

**This page intentionally left blank.**

## 4.0 CONCEPTUAL SITE MODEL

The conceptual site model for DSS Site 1035, the Building 6715 Septic System, is based upon the COCs identified in the soil samples collected from beneath the seepage pit at this site. This section summarizes the nature and extent of contamination and the environmental fate of the COCs.

### 4.1 Nature and Extent of Contamination

Potential COCs at DSS Site 1035 are VOCs, SVOCs, PCBs, HE compounds, cyanide, RCRA metals, hexavalent chromium, and radionuclides. No PCBs, HE compounds, or hexavalent chromium were detected in any of the soil samples collected at this site. The VOCs acetone and 2-butanone were detected in soil samples collected from the site. The SVOC bis(2-ethylhexyl) phthalate was detected in both samples collected from the borehole. Barium was detected above the NMED-approved maximum background concentration for SNL/NM Southwest Area Supergroup soils (Dinwiddie September 1997). Cyanide was detected in both soil samples. But since it does not have a quantified background screening concentration, it is unknown if this COC exceeds background. When a metal concentration exceeded its maximum background screening value, it was considered further in the risk assessment process. None of the four representative gamma spectroscopy radionuclides were detected at activities exceeding the corresponding background levels. However, the MDA value for one of the uranium-235 analyses exceeded the corresponding background activity. Finally, no gross alpha/beta activity was detected above the New Mexico-established background levels.

### 4.2 Environmental Fate

Potential COCs may have been released into the vadose zone via aqueous effluent discharged from the septic system seepage pit. Possible secondary release mechanisms include the uptake of COCs that may have been released into the soil beneath the seepage pit (Figure 4.2-1). The depth to groundwater at the site (approximately 470 feet bgs) most likely precludes migration of potential COCs into the groundwater system. The potential pathways to receptors include soil ingestion, dermal contact, and inhalation, which could occur as a result of receptor exposure to contaminated subsurface soil at the site. No intake routes through plant, meat, or milk ingestion are considered appropriate for either the industrial or residential land-use scenarios. Annex D provides additional discussion on the fate and transport of COCs at DSS Site 1035.

Table 4.2-1 summarizes the potential COCs for DSS Site 1035. All potential COCs were retained in the conceptual model and were evaluated in both the human health and ecological risk assessments. The current and future land use for DSS Site 1035 is industrial (DOE et al. September 1995).

The potential human receptors at the site are considered to be an industrial worker and resident. The exposure routes for the receptors are dermal contact and ingestion/inhalation; however, these are realistic possibilities only if contaminated soil is excavated at the site. The

**This page intentionally left blank.**

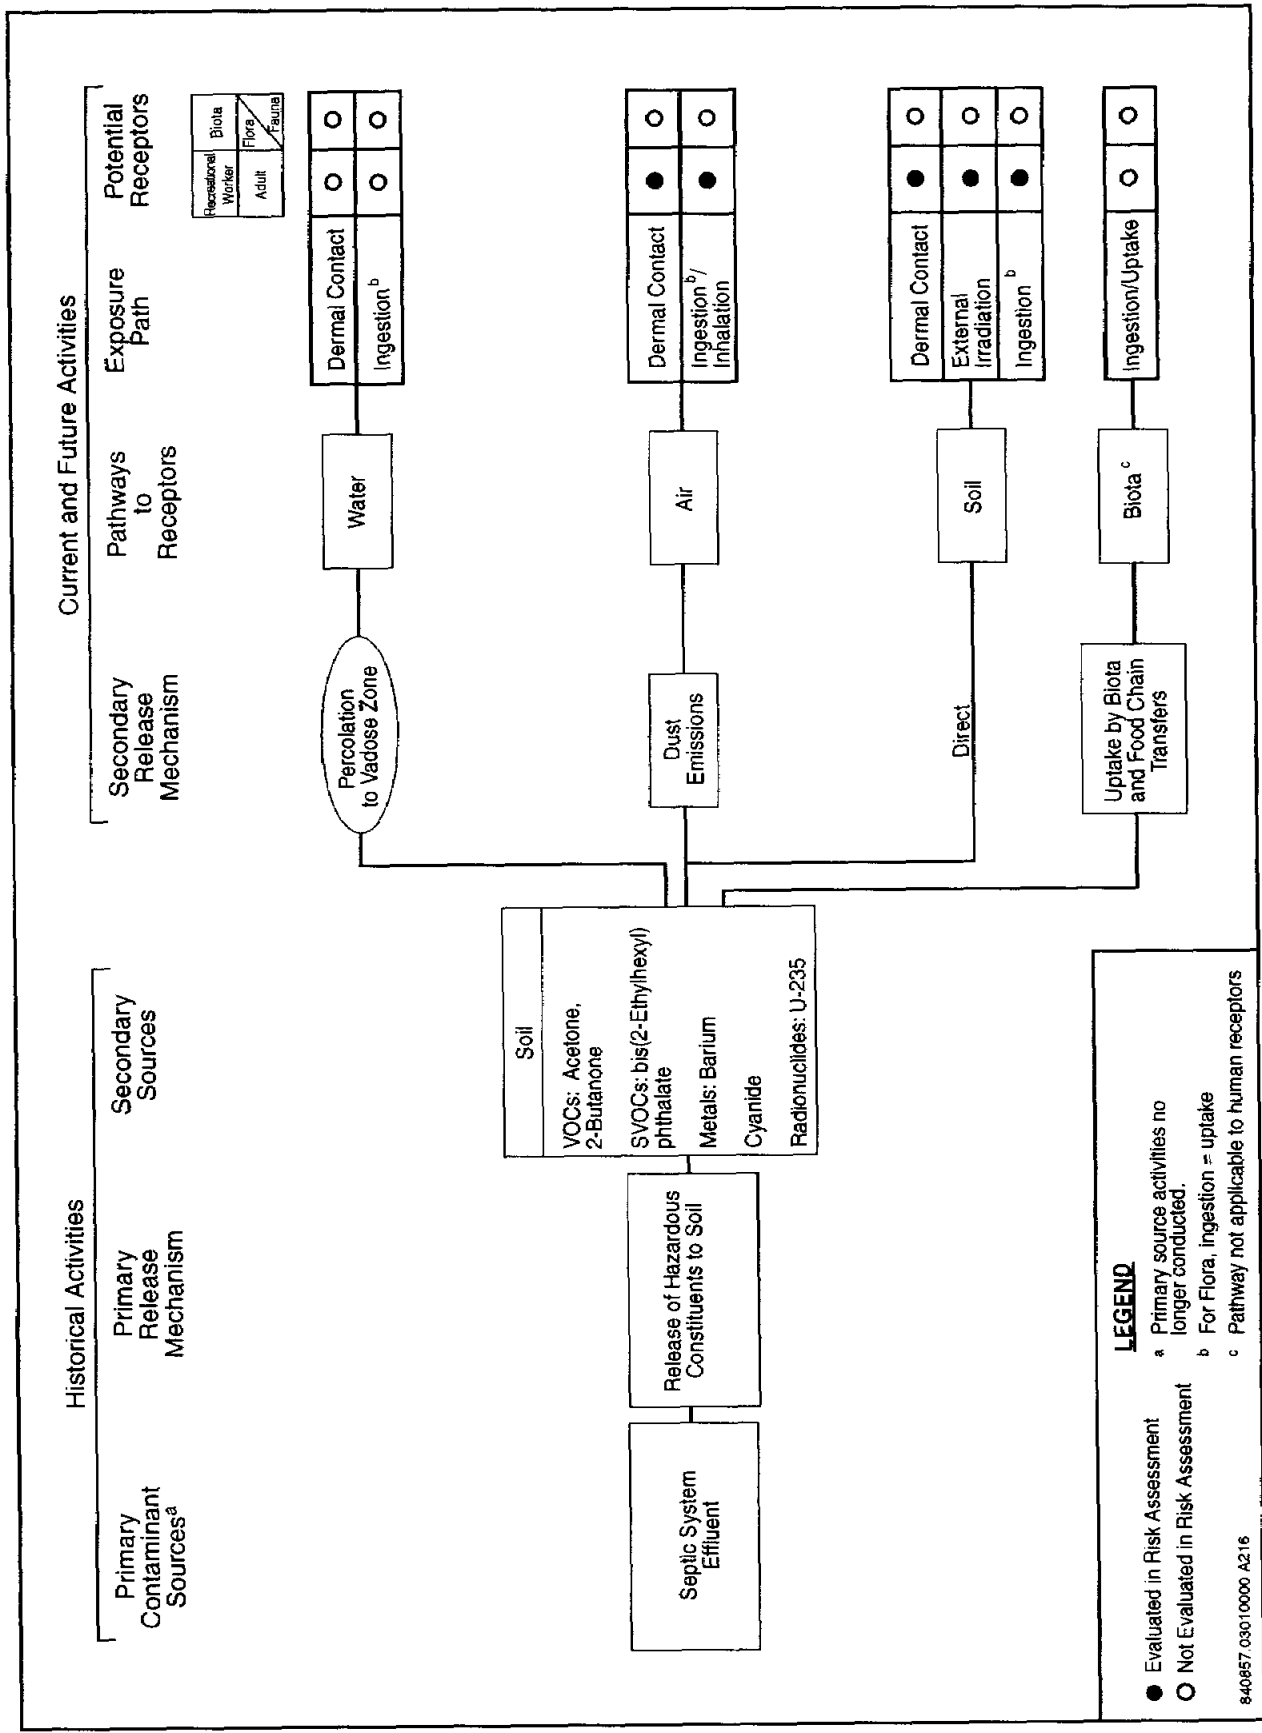


Figure 4.2-1  
 Conceptual Site Model Flow Diagram for DSS Site 1035, Building 6715 Septic System



Table 4.2-1  
Summary of Potential COCs for DSS Site 1035, Building 6715 Septic System

COC Type	Number of Samples <sup>a</sup>	COCs Detected or with Concentrations Greater than Background or Nonquantified Background	Maximum Background Limit/Southwest Area Supergroup <sup>b</sup> (mg/kg)	Maximum Concentration <sup>c</sup> (All Samples) (mg/kg)	Average Concentration <sup>d</sup> (mg/kg)	Number of Samples Where COCs Detected with Concentrations Greater than Background or Nonquantified Background <sup>e</sup>
VOCs	2	Acetone	NA	0.0042 J	0.0030	1
	2	2-Butanone	NA	0.0067	0.0043	1
SVOCs	2	bis(2-Ethylhexyl) phthalate	NA	0.142 J	0.122	2
	2	None	NA	NA	NA	None
PCBs	2	None	NA	NA	NA	None
HE Compounds	2	None	NA	NA	NA	None
RCRA Metals	2	Barium	214	232	157	1
	2	None	NA	NA	NA	None
Hexavalent Chromium	2	None	NA	0.0462 J	0.0460	2
Cyanide	2	None	0.16	ND (0.199)	NC <sup>f</sup>	1
Radionuclides (pCi/g)	2	Uranium-235	NA	NA	NA	None
	2	None	NA	NA	NA	None
Gamma Spectroscopy	2	None	NA	NA	NA	None
	2	None	NA	NA	NA	None

<sup>a</sup>Number of samples includes duplicates and splits.

<sup>b</sup>Dinwiddie September 1997.

<sup>c</sup>Maximum concentration is either the maximum amount detected, or for radionuclides, the greater of either the maximum detection or the maximum MDA above background.

<sup>d</sup>Average concentration includes all samples except blanks. The average is calculated as the sum of detected amounts and one-half of the MDLs for nondetect results, divided by the number of samples.

<sup>e</sup>See appropriate data table for sample locations.

<sup>f</sup>An average MDA is not calculated because of the variability in instrument counting error and the number of reported nondetect activities for gamma spectroscopy. COC = Constituent of concern.

DSS = Drain and Septic Systems.

HE = High explosive(s).

J = Analytical result was qualified as an estimated value.

MDA = Minimum detectable activity.

MDL = Method detection limit.

mg/kg = Milligram(s) per kilogram.

NA = Not applicable.

NC

NC = Not calculated.

ND ( )

ND ( ) = Not detected above the MDA, shown in parentheses.

PCB = Polychlorinated biphenyl.

pCi/g = Picocurie(s) per gram.

RCRA = Resource Conservation and Recovery Act.

SVOC = Semivolatile organic compound.

VOC = Volatile organic compound.



major exposure route modeled in the human health risk assessment is soil ingestion for COCs. The inhalation pathway is included because of the potential to inhale dust and volatiles. The dermal pathway is included because of the potential for receptors to be exposed to the contaminated soil.

No pathways to groundwater and no intake routes through flora or fauna are considered appropriate for either the industrial or residential land-use scenarios. Annex D provides additional discussion of the exposure routes and receptors at DSS Site 1035.

### **4.3 Site Assessment**

Site assessment at DSS Site 1035 included risk assessments for both human health and ecological risk. This section briefly summarizes the site assessment results, and Annex D discusses the risk assessment performed for DSS Site 1035 in more detail.

#### **4.3.1 Summary**

The site assessment concluded that DSS Site 1035 poses no significant threat to human health under either the industrial or residential land-use scenarios.

Ecological risks were found to be insignificant because no pathways exist.

#### **4.3.2 Risk Assessments**

Risk assessments were performed for both human health and ecological risk at DSS Site 1035. This section summarizes the results.

##### **4.3.2.1 Human Health**

DSS Site 1035 has been recommended for an industrial land-use scenario (DOE et al. September 1995). Because acetone, 2-butanone, bis(2-ethylhexyl) phthalate, barium, cyanide, and uranium-235 were detected, are present above background levels, have nonquantified background levels, or have MDA values above background levels, it was necessary to perform a human health risk assessment analysis for the site, which included these COCs. Annex D provides a complete discussion of the risk assessment process, results, and uncertainties. The risk assessment process provides a quantitative evaluation of the potential adverse human health effects from constituents in the site's soil by calculating the hazard index (HI) and excess cancer risk for both industrial and residential land-use scenarios.

The HI calculated for the COCs at DSS Site 1035 is 0.00 for the industrial land-use scenario, which is less than the numerical standard of 1.0 suggested by risk assessment guidance (EPA 1989). The incremental HI risk, determined by subtracting risk associated with background from potential nonradiological COC risk (without rounding), is 0.00. The excess cancer risk for DSS Site 1035 COCs is  $7E-10$  for an industrial land-use scenario. NMED guidance states that cumulative excess lifetime cancer risk must be less than  $1E-5$  (Bearzi January 2001); thus the excess cancer risk for this site is below the suggested acceptable risk value. The incremental

excess cancer risk is 7.41E-10. Both the incremental HI and excess cancer risk are below NMED guidelines.

The HI calculated for the COCs at DSS Site 1035 is 0.04 for the residential land-use scenario, which is less than the numerical standard of 1.0 suggested by risk assessment guidance (EPA 1989). The incremental HI risk, determined by subtracting risk associated with background from potential nonradiological COC risk (without rounding), is 0.00. The excess cancer risk for DSS Site 1035 COCs is 3E-9 for a residential land-use scenario. NMED guidance states that cumulative excess lifetime cancer risk must be less than 1E-5 (Bearzi January 2001); thus the excess cancer risk for this site is below the suggested acceptable risk value. The incremental excess cancer risk is 3.21E-9. Both the incremental HI and incremental excess cancer risk are below NMED guidelines.

For the radiological COCs, one of the constituents (uranium-235) had an MDA value greater than the corresponding background level. The incremental total effective dose equivalent (TEDE) and corresponding estimated cancer risk from the radiological COC are much lower than the EPA guidance values. The estimated TEDE is 4.3E-3 millirem (mrem)/year (yr) for the industrial land-use scenario, which is much lower than the EPA's numerical guidance of 15 mrem/yr (EPA 1997a). The corresponding incremental estimated cancer risk value is 5.0E-8 for the industrial land-use scenario. Furthermore, the incremental TEDE for the residential land-use scenario that results from a complete loss of institutional control is 1.1E-2 mrem/yr with an associated incremental estimated cancer risk of 1.5E-7. The guideline for this scenario is 75 mrem/yr (SNL/NM February 1998). Therefore, DSS Site 1035 is eligible for unrestricted radiological release.

The incremental radiological and nonradiological carcinogenic risks are tabulated and summed in Table 4.3.2-1.

Table 4.3.2-1  
Summation of Incremental Radiological and Nonradiological Risks from  
DSS Site 1035, Building 6715 Septic System Carcinogens

Scenario	Nonradiological Risk	Radiological Risk	Total Risk
Industrial	7.41E-10	5.0E-8	5.0E-8
Residential	3.21E-9	1.5E-7	1.5E-7

DSS = Drain and Septic Systems.

Uncertainties associated with the calculations are considered small relative to the conservatism of the risk assessment analysis. Therefore, it is concluded that this site poses insignificant risk to human health under both the industrial and residential land-use scenarios.

#### 4.3.2.2 Ecological

An ecological assessment that corresponds with the procedures in the EPA's Ecological Risk Assessment Guidance for Superfund (EPA 1997b) also was performed as set forth by the NMED Risk-Based Decision Tree in the "RPMP [RCRA Permits Management Program] Document Requirement Guide" (NMED March 1998). An early step in the evaluation compared COC concentrations and identified potentially bioaccumulative constituents (see Annex D,

Sections IV and VII.2). This methodology also required developing a site conceptual model and a food web model, as well as selecting ecological receptors, as presented in "Predictive Ecological Risk Assessment Methodology, Environmental Restoration Program, Sandia National Laboratories, New Mexico" (IT July 1998). The risk assessment also includes the estimation of exposure and ecological risk.

All COCs at DSS Site 1035 are located at depths greater than 5 feet bgs. Therefore, no complete ecological pathways exist at this site, and a more detailed ecological risk assessment is not necessary.

#### **4.4 Baseline Risk Assessments**

This section discusses the baseline risk assessments for human health and ecological risk.

##### **4.4.1 Human Health**

Because the results of the human health risk assessment summarized in Section 4.3.2.1 indicate that DSS Site 1035 poses insignificant risk to human health under both the industrial and residential land-use scenarios, a baseline human health risk assessment is not required for this site.

##### **4.4.2 Ecological**

Because the results of the ecological risk assessment summarized in Section 4.3.2.2 indicate that no complete pathways exist at DSS Site 1035, a baseline ecological risk assessment is not required for the site.

## **5.0 RECOMMENDATION FOR CORRECTIVE ACTION COMPLETE WITHOUT CONTROLS DETERMINATION**

### **5.1 Rationale**

Based upon field investigation data and the human health and ecological risk assessment analyses, a determination of CAC without controls is recommended for DSS Site 1035 for the following reasons:

- The soil has been sampled for all potential COCs.
- No COCs are present in the soil at levels considered hazardous to human health for either an industrial or residential land-use scenario.
- None of the COCs warrant ecological concern because no complete pathways exist at the site.

### **5.2 Criterion**

Based upon the evidence provided in Section 5.1, a determination of CAC without controls (NMED April 2004) is recommended for DSS Site 1035. This is consistent with the NMED's NFA Criterion 5, which states, "the SWMU/AOC [Area of Concern] has been characterized or remediated in accordance with current applicable state or federal regulations, and the available data indicate that contaminants pose an acceptable level of risk under current and projected future land use" (NMED March 1998).

**This page intentionally left blank.**

## 6.0 REFERENCES

Bearzi, J. (New Mexico Environment Department/Hazardous Waste Bureau), January 2000. Letter to M.J. Zamorski (U.S. Department of Energy) and L. Shephard (Sandia National Laboratories/New Mexico) approving the "Sampling and Analysis Plan for Characterizing and Assessing Potential Releases to the Environment for Septic and Other Miscellaneous Drain Systems at Sandia National Laboratories/New Mexico." January 28, 2000.

Bearzi, J.P. (New Mexico Environment Department), January 2001. Memorandum to RCRA-Regulated Facilities, "Risk-Based Screening Levels for RCRA Corrective Action Sites in New Mexico," Hazardous Waste Bureau, New Mexico Environment Department, Santa Fe, New Mexico. January 23, 2001.

Bleakly, D. (Sandia National Laboratories/New Mexico), July 1996. Memorandum, "List of Non-ER Septic/Drain Systems for the Sites Identified Through the Septic System Inventory Program." July 8, 1996.

Dinwiddie, R.S. (New Mexico Environment Department), September 1997. Letter to M.J. Zamorski (U.S. Department of Energy), Request for Supplemental Information: Background Concentrations Report, SNL/KAFB, September 24, 1997.

DOE, see U.S. Department of Energy.

EPA, see U.S. Environmental Protection Agency.

Gore, see Gore, W.L. and Associates.

Gore, W.L. and Associates (Gore), June 2002. "Gore-Sorber Screening Survey Final Report, Non-ER Drain and Septic, Kirtland AFB, NM," W.L. Gore Production Order Number 10960025, Sandia National Laboratories/New Mexico, June 6, 2002

IT, see IT Corporation.

IT Corporation (IT), July 1998. "Predictive Ecological Risk Assessment Methodology, Environmental Restoration Program, Sandia National Laboratories, New Mexico," IT Corporation, Albuquerque, New Mexico.

Jones, J. (Sandia National Laboratories/New Mexico), June 1991. Internal Memorandum to D. Dionne listing the septic tanks that were removed from service with the construction of the Area III sanitary sewer system. June 21, 1991.

Miller, M. (Sandia National Laboratories/New Mexico), September 2003. Memorandum to F.B. Nimick (Sandia National Laboratories/New Mexico), regarding "State of New Mexico Background for Gross Alpha/Beta Assays in Soil Samples." September 12, 2003.

Moats, W. (New Mexico Environment Department/Hazardous Waste Bureau), February 2002. Letter to M.J. Zamorski (U.S. Department of Energy) and P. Davies (Sandia National Laboratories/New Mexico) approving the "Field Implementation Plan, Characterization of Non-Environmental Restoration Drain and Septic Systems." February 21, 2002.

National Oceanic and Atmospheric Administration (NOAA), 1990. "Local Climatological Data, Annual Summary with Comparative Data," Albuquerque, New Mexico.

New Mexico Environment Department (NMED) March 1998. "RPMP Document Requirement Guide," RCRA Permits Management Program, Hazardous and Radioactive Materials Bureau, New Mexico Environment Department, Santa Fe, New Mexico.

New Mexico Environment Department (NMED) April 2004. "Compliance Order on Consent Pursuant to New Mexico Hazardous Waste Act § 74-4-10," New Mexico Environment Department, Santa Fe, New Mexico. April 29, 2004.

NMED, see New Mexico Environment Department.

NOAA, see National Oceanic and Atmospheric Administration.

Romero, T. (Sandia National Laboratories/New Mexico), September 2003. Internal communication to M. Sanders stating that during the connection of septic systems to the new City of Albuquerque sewer system, the old systems were disconnected and the lines capped. September 16, 2003.

Sandia National Laboratories/New Mexico (SNL/NM), November 1976. SNL/NM Facilities Engineering Drawing 87174 M1 showing the Building 6715 Septic System, Sandia National Laboratories, Albuquerque, New Mexico.

Sandia National Laboratories/New Mexico (SNL/NM), April 1991. "Sandia National Laboratories Septic Tank Characterization Summary Tables of Analytical Results for Detected Parameters, Technical Area III and Coyote Canyon Test Field, April 1991," Sandia National Laboratories, Albuquerque, New Mexico.

Sandia National Laboratories/New Mexico (SNL/NM), June 1993. "Sandia National Laboratories/New Mexico Septic Tank Monitoring Report, 1992 Report," Sandia National Laboratories, Albuquerque, New Mexico.

Sandia National Laboratories/New Mexico (SNL/NM), July 1994. "Verification and Validation of Chemical and Radiochemical Data," Technical Operating Procedure (TOP) 94-03, Rev. 0, Sandia National Laboratories, Albuquerque, New Mexico.

Sandia National Laboratories/New Mexico (SNL/NM), December 1995. "Sandia National Laboratories Septic Tank Characterization Summary Tables of Analytical Reports, December 1995," Sandia National Laboratories, Albuquerque, New Mexico.

Sandia National Laboratories/New Mexico (SNL/NM), March 1996. "Site-Wide Hydrogeologic Characterization Project, Calendar Year 1995 Annual Report," Environmental Restoration Project, Sandia National Laboratories, Albuquerque, New Mexico.

Sandia National Laboratories/New Mexico (SNL/NM), July 1996. "Laboratory Data Review Guidelines," Radiation Protection Diagnostics Procedure No. RPSD-02-11, Issue No. 2, Sandia National Laboratories, Albuquerque, New Mexico.

Sandia National Laboratories/New Mexico (SNL/NM), February 1998. "RESRAD Input Parameter Assumptions and Justification," Environmental Restoration Project, Sandia National Laboratories, Albuquerque, New Mexico.

Sandia National Laboratories/New Mexico (SNL/NM), October 1999. "Sampling and Analysis Plan for Characterizing and Assessing Potential Releases to the Environment From Septic and Other Miscellaneous Drain Systems at Sandia National Laboratories/New Mexico," Sandia National Laboratories, Albuquerque, New Mexico. October 19, 1999.

Sandia National Laboratories/New Mexico (SNL/NM), December 1999. "Data Validation Procedure for Chemical and Radiochemical Data," Administrative Operating Procedure (AOP) 00-03, Environmental Restoration Project, Sandia National Laboratories, Albuquerque, New Mexico.

Sandia National Laboratories/New Mexico (SNL/NM), November 2001. "Field Implementation Plan, Characterization of Non-Environmental Restoration Drain and Septic Systems," Sandia National Laboratories, Albuquerque, New Mexico.

Sandia National Laboratories/New Mexico (SNL/NM), March 2002. "Annual Groundwater Monitoring Report, Fiscal Year 2001," Sandia National Laboratories, Albuquerque, New Mexico.

Sandia National Laboratories/New Mexico (SNL/NM), March 2003. Database printout provided by SNL/NM Facilities Engineering showing the year that numerous SNL/NM buildings were constructed, Sandia National Laboratories, Albuquerque, New Mexico.

Sandia National Laboratories/New Mexico (SNL/NM), April 2003. "DSS Sites Mean Elevation Report," GIS Group, Environmental Restoration Department, Sandia National Laboratories, Albuquerque, New Mexico.

Shain, M. (IT Corporation), August 1996. Memorandum and spreadsheet to J. Jones (Sandia National Laboratories/New Mexico) summarizing dates, locations, and volume of effluent pumped from numerous Sandia National Laboratories/New Mexico septic tanks at Sandia National Laboratories, Albuquerque, New Mexico. August 23, 1996.

SNL/NM, see Sandia National Laboratories/New Mexico.

U.S. Department of Energy (DOE), U.S. Air Force, and U.S. Forest Service, September 1995. "Workbook: Future Use Management Area 2," prepared by Future Use Logistics and Support Working Group in cooperation with Department of Energy Affiliates, the U.S. Air Force, and the U.S. Forest Service.

U.S. Environmental Protection Agency (EPA), November 1986. "Test Methods for Evaluating Solid Waste," 3rd ed., Update 3, SW-846, Office of Solid Waste and Emergency Response, U.S. Environmental Protection Agency, Washington D.C.

U.S. Environmental Protection Agency (EPA), 1989. "Risk Assessment Guidance for Superfund, Vol. 1: Human Health Evaluation Manual," EPA/540/1-89/002, Office of Emergency and Remedial Response, U.S. Environmental Protection Agency, Washington, D.C.

U.S. Environmental Protection Agency (EPA), 1997a. "Establishment of Cleanup Levels for CERCLA Sites with Radioactive Contamination," OSWER Directive No. 9200.4-18, Office of Solid Waste and Emergency Response, U.S. Environmental Protection Agency, Washington, D.C.



U.S. Environmental Protection Agency (EPA), 1997b. "Ecological Risk Assessment Guidance for Superfund: Process for Designing and Conducting Ecological Risks," Interim Final, U.S. Environmental Protection Agency, Washington, D.C.





**ANNEX A**  
**DSS Site 1035**  
**Septic Tank Sampling Results**



4-17-91

Results of septic tank sampling  
conducted between 12/18/90 and  
1/8/91 for buildings noted.

DB Dionne

4-17-91

Nick Durand,

For your information.

David Dionne

TABLE 19

**SUMMARY OF ANALYTICAL RESULTS FOR DETECTED PARAMETERS  
TECHNICAL AREA III AND COYOTE CANYON TEST FIELD  
SEPTIC TANK SAMPLING**

BUILDING 6715

SAMPLE NUMBERS SNLA004837, SNLA004859, SNLA004838

Parameter	Results	Units
<b>VOLATILE ORGANICS</b>		
Acetone*	0.047	mg/l
Carbon Disulfide*	0.003	mg/l
Toluene	0.004	mg/l
<b>INORGANICS</b>		
Oil and Grease	1000	mg/l
Cyanide, Total	0.01	mg/l
Nitrate as N	0.09	mg/l
Phenolics	0.23	mg/l
<b>METALS</b>		
Arsenic	0.010	mg/l
Barium	0.80	mg/l
Cadmium	0.027	mg/l
Chromium	0.02	mg/l
Copper	0.90	mg/l
Lead	0.11	mg/l
Manganese	0.13	mg/l
Mercury	0.0352	mg/l
Selenium	0.17	mg/l
Silver	0.40	mg/l
Zinc	2.9	mg/l
<b>RADIOLOGICAL</b>		
Gross Alpha	180	pCi/l
Gross Beta	470	pCi/l

\*Not on total toxic organics list







**Building 6715  
Area 3  
Sample ID No. SNLA008594  
Tank ID No. AD89015R**

On August 18, 1992, a sludge sample was collected from the septic tank serving Building 6715. During review of the radiological data, no parameters were detected that exceed U.S. Department of Energy (DOE) derived concentration guideline (DCG) limits or the investigation levels (IL) established during this investigation.

Results of Septic Tank Analyses (Sludge Sample)			
Building No./Area:	6715 A-3		
Tank ID No.:	AD89015R		
Date Sampled:	8/18/92		
Sample ID No.:	SNLA008594		
Analytical Parameter	Measured Concentration	+ 2 Sigma Uncertainty	Units
Gross Alpha	2E+1	2E+1	pCi/g
Gross Beta	1E+1	3E+1	pCi/g
Gross Alpha	1E+1	2E+1	pCi/g
Gross Beta	2E+1	3E+1	pCi/g
Gross Alpha	1E+1	2E+1	pCi/g
Gross Beta	1E+1	3E+1	pCi/g
Gross Alpha	2E+1	2E+1	pCi/g
Gross Beta	1E+1	3E+1	pCi/g
Tritium	2E+02	3E+02	pCi/L
Bismuth-214	<0.0302	NA	pCi/mL
Cesium-137	0.00568	0.00325	pCi/mL
Potassium-40	0.503	0.0615	pCi/mL
Lead-212	0.0192	0.00653	pCi/mL
Lead-214	0.0219	0.00787	pCi/mL
Radium-226	0.179	0.0813	pCi/mL
Thorium-234	0.416	0.0987	pCi/mL
Thallium-208	0.00754	0.00351	pCi/mL

ND = Not Detected  
NA = Not Applicable





**RESULTS OF SEPTIC TANK SAMPLING  
CHEMICAL ANALYSES OF AQUEOUS SAMPLE**

Building ID: \_\_\_\_\_ Bldg 6715  
 Sample ID Number: \_\_\_\_\_ 024403  
 Date Sampled: \_\_\_\_\_ 7-12-95

Parameter (Method)	Result	Detection Limit (DL)	NM Discharge Limit <sup>a</sup>	COA Discharge Limit <sup>b</sup>	Comments
<i>Volatile Organics (8260)</i>	(mg/L)	(mg/L)	(mg/L)	(mg/L)	
None detected above DL	ND	various	various	TTO = 5.0	
<i>Semivolatile Organics (8270)</i>	(mg/L)	(mg/L)	(mg/L)	(mg/L)	
bis(2-Ethylhexyl)Phthalate	0.002J	0.010	NR	TTO = 5.0	
<i>Pesticides/PCBs (8080)</i>	(mg/L)	(mg/L)	(mg/L)	(mg/L)	
None detected above DL	ND	various	NR / PCBs = 0.001	TTO = 5.0	
<i>Metals (6010/7470)</i>	(mg/L)	(mg/L)	(mg/L)	(mg/L)	
Arsenic	ND	0.010	0.1	2.0	
Barium	0.113J	0.200	1.0	20.0	
Cadmium	ND	0.005	0.01	2.8	
Chromium	ND	0.020	0.05	20.0	
Copper	0.0164J	0.025	1.0	16.5	
Lead	ND	0.003	0.05	3.2	
Manganese	0.0277	0.015	0.2	20.0	
Nickel	0.025J	0.040	0.2	12.0	
Selenium	ND	0.005	0.05	2.0	
Silver	ND	0.010	0.05	5.0	
Thallium	ND	0.010	NR	NR	
Zinc	0.0459	0.020	10.0	28.0	
Mercury	ND	0.0002	0.002	0.1	
<i>Miscellaneous Analyses</i>	(mg/L)	(mg/L)	(mg/L)	(mg/L)	
Field pH	7.7 pH units	0 - 14 pH units	6 - 9 pH units	5 - 11 pH units	
Formaldehyde (NIOSH 3500)	0.31	0.25	NR	260.0	
Fluoride (300.0)	ND	0.10	1.6	180.0	
Nitrate + Nitrite (353.1)	6.740	1.000	10.0	NR	

Refer to footnotes at end of table.

**RESULTS OF SEPTIC TANK SAMPLING  
CHEMICAL ANALYSES OF AQUEOUS SAMPLE**

Building ID: Bldg 6715  
 Sample ID Number: 024403  
 Date Sampled: 7-12-95

Parameter (Method)	Result	Detection Limit (DL)	NM Discharge Limit <sup>a</sup>	COA Discharge Limit <sup>b</sup>	Comments
<i>Miscellaneous Analyses</i>	<i>(mg/L)</i>	<i>(mg/L)</i>	<i>(mg/L)</i>	<i>(mg/L)</i>	
Oil + Grease (9070)	5.60	1.00	NR	150.0	
Total Phenol (9066)	ND	0.050	0.005	4.0	

**Notes:**

<sup>a</sup> New Mexico Water Quality Control Commission Regulations (1990), Section 3-103.

<sup>b</sup> City of Albuquerque Sewer Use and Wastewater Control Ordinance (1993), Section 8-9-3 M - maximum allowable concentration for grab sample.

DL = Detection limit indicated on laboratory report.

IDL = Instrument detection limit.

J = Estimated concentration of analyte, between DL and IDL.

ND = Not detected above DL indicated.

NR = Not regulated.

TTO = Total toxic organics.

**RESULTS OF SEPTIC TANK SAMPLING  
RADIOLOGICAL ANALYSES OF AQUEOUS SAMPLE**

Building ID: Bldg 6715  
 Sample ID Number: 024403  
 Date Sampled: 7-12-95

Parameter (Method)	Result	MDA	Critical Level	NM Discharge Limit*	Comments
<i>Radiological Analyses</i>	<i>(pCi/L ± 2-σ)</i>	<i>(pCi/L)</i>	<i>(pCi/L)</i>	<i>(pCi/L)</i>	
Gross Alpha (9310)	925 ± 93	5	2.24	NR	
Gross Beta (9310)	43.6 ± 4.6	3.4	1.66	NR	
<i>Isotopic Analyses</i>	<i>(pCi/L ± 2-σ)</i>	<i>(pCi/L)</i>	<i>(pCi/L)</i>	<i>(pCi/L)</i>	
Tritium (906.0)	-29.0 ± 48.8	83.5	41.3	NR	
<i>Gamma Spectroscopy<sup>2</sup></i>	<i>(pCi/mL ± 2-σ)</i>	<i>(pCi/mL)</i>	<i>(pCi/L)</i>	<i>(pCi/L)</i>	
None detected above MDA	ND	various	NL	NR	

**Notes:**  
 \* New Mexico Water Quality Control Commission Regulations (1990), Section 3-103.  
<sup>2</sup> Analyzed in-house by SNL/NM Department 7715.  
 MDA = Minimum detectable activity.  
 ND = Not detected above MDA indicated.  
 NL = Not listed.  
 NR = Not regulated.



**RESULTS OF SEPTIC TANK SAMPLING  
CHEMICAL ANALYSES OF SLUDGE SAMPLE**

Building ID: Bldg 6715  
 Sample ID Number: 024403  
 Date Sampled: 7-12-95  
 Percent Moisture: Not Reported

Parameter (Method)	Result	Detection Limit (DL)	NM Discharge Limit <sup>a</sup>	COA Discharge Limit <sup>b</sup>	Comments
<i>Volatile Organics (8260)</i>	<i>(µg/kg)</i>	<i>(µg/kg)</i>	<i>(mg/L)</i>	<i>(mg/L)</i>	
Acetone	860B	140	NR	NR	
Trichloroethene	19J	140	NR	TTO = 5.0	
Benzene	110J	140	0.01	TTO = 5.0	
Toluene	390	140	0.75	TTO = 5.0	
Ethylbenzene	160	140	0.75	TTO = 5.0	
<i>Semivolatile Organics (8270)</i>	<i>(µg/kg)</i>	<i>(µg/kg)</i>	<i>(mg/L)</i>	<i>(mg/L)</i>	
1,2-Dichlorobenzene	420J	4700	NR	TTO = 5.0	
Napthalene	590J	4700	NR	TTO = 5.0	
Fluorene	680J	4700	NR	TTO = 5.0	
Phenanthrene	2200J	4700	NR	TTO = 5.0	
Fluoranthene	810J	4700	NR	TTO = 5.0	
Pyrene	2300J	4700	NR	TTO = 5.0	
Benzo(a)Anthracene	540J	4700	NR	TTO = 5.0	
bis(2-Ethylhexyl)Phthalate	2700J	4700	NR	TTO = 5.0	
<i>Pesticides/PCBs (6080)</i>	<i>(µg/kg)</i>	<i>(µg/kg)</i>	<i>(mg/L)</i>	<i>(mg/L)</i>	
beta-BHC	52	23	NR	TTO = 5.0	
4,4'-DDE	150	46	NR	TTO = 5.0	
Endosulfan Sulfate	200	46	NR	TTO = 5.0	
4,4'-DDT	370	46	NR	TTO = 5.0	
<i>Metals (6010/7470)</i>	<i>(mg/kg)</i>	<i>(mg/kg)</i>	<i>(mg/L)</i>	<i>(mg/L)</i>	
Arsenic	11.1J	13.8	0.1	2.0	
Barium	4230	276	1.0	20.0	
Cadmium	18.3	6.9	0.01	2.8	
Chromium	130	27.6	0.05	20.0	

Refer to footnotes at end of table.

**RESULTS OF SEPTIC TANK SAMPLING  
CHEMICAL ANALYSES OF SLUDGE SAMPLE**

Building ID: \_\_\_\_\_ Bldg 6715  
 Sample ID Number: \_\_\_\_\_ 024403  
 Date Sampled: \_\_\_\_\_ 7-12-95  
 Percent Moisture: \_\_\_\_\_ Not Reported

Parameter (Method)	Result	Detection Limit (DL)	NM Discharge Limit <sup>a</sup>	COA Discharge Limit <sup>b</sup>	Comments
<i>Metals (6010/7470)</i>	<i>(mg/kg)</i>	<i>(mg/kg)</i>	<i>(mg/L)</i>	<i>(mg/L)</i>	
Copper	3340	34.5	1.0	16.5	
Lead	379	4.1	0.05	3.2	
Manganese	66.3	20.7	0.2	20.0	
Nickel	49.0J	55.3	0.2	12.0	
Selenium	7.0	6.9	0.05	2.0	
Silver	304	13.8	0.05	5.0	
Thallium	ND	13.8	NR	NR	
Zinc	3260	27.6	10.0	28.0	
Mercury	20.7	1.4	0.002	0.1	

**Notes:**  
<sup>a</sup> New Mexico Water Quality Control Commission Regulations (1990), Section 3-103.  
<sup>b</sup> City of Albuquerque Sewer Use and Wastewater Control Ordinance (1993), Section 8-9-3 M – maximum allowable concentration for grab sample.  
 B = Analyte detected in method blank.  
 DL = Detection limit indicated on laboratory report.  
 IDL = Instrument detection limit.  
 J = Estimated concentration of analyte, between DL and IDL.  
 ND = Not detected above DL indicated.  
 NR = Not regulated.  
 TTO = Total toxic organics.

Refer to footnotes at end of table.

**RESULTS OF SEPTIC TANK SAMPLING  
RADIOLOGICAL ANALYSES OF SLUDGE SAMPLE**

Building ID: Bldg 6715  
 Sample ID Number: 024403  
 Date Sampled: 7-12-95  
 Percent Moisture: Not Reported

Parameter (Method)	Result	MDA	Critical Level	NM Discharge Limit*	Comments
<i>Isotopic Analyses<sup>b</sup></i>	<i>(pCi/g ± 2-σ)</i>	<i>(pCi/g)</i>	<i>(pCi/g)</i>	<i>(pCi/g)</i>	
Plutonium-239/240	0.080 ± 0.035	0.029	0.019	NR	
Plutonium-238	-0.0006 ± 0.0089	0.030	0.019	NR	
Strontium-90	0.06 ± 0.01	0.56	0.27	NR	
Thorium-232	0.059 ± 0.029	0.019	0.014	NR	
Thorium-230	0.14 ± 0.05	0.021	0.015	NR	
Thorium-228	0.14 ± 0.05	0.028	0.018	NR	
Uranium-238	7.01 ± 2.92	0.82	0.624	NR	
Uranium-235/236	3.98 ± 2.12	1.16	0.846	NR	
Uranium-234	12.4 ± 4.5	0.94	0.686	NR	
<i>Dry Gamma Spectroscopy<sup>c</sup></i>	<i>(pCi/g ± 2-σ)</i>	<i>(pCi/g)</i>	<i>(pCi/g)</i>	<i>(pCi/g)</i>	
Cesium-137	0.14 ± 0.03	0.02	0.012	NR	
Cesium-134	ND	0.024	0.012	NR	
Potassium-40	5.37 ± 0.71	0.27	0.13	NR	
Chromium-51	ND	0.28	0.13	NR	
Iron-59	ND	0.076	0.036	NR	
Cobalt-60	ND	0.035	0.017	NR	
Zirconium-95	ND	0.060	0.029	NR	
Ruthenium-103	ND	0.031	0.015	NR	
Ruthenium-106	ND	0.24	0.11	NR	
Cerium-144	ND	0.11	0.053	NR	
Thallium-208	0.18 ± 0.04	0.03	NL	NR	
Lead-210	1.75 ± 0.54	0.53	NL	NR	
Lead-212	0.64 ± 0.06	0.03	0.014	NR	
Lead-214	0.46 ± 0.06	0.05	0.026	NR	
Bismuth-212	0.37 ± 0.21	0.23	NL	NR	
Bismuth-214	0.40 ± 0.07	0.06	NL	NR	

Refer to footnotes at end of table.

**RESULTS OF SEPTIC TANK SAMPLING  
RADIOLOGICAL ANALYSES OF SLUDGE SAMPLE**

Building ID: Bldg 6715  
 Sample ID Number: 024403  
 Date Sampled: 7-12-95  
 Percent Moisture: Not Reported

Parameter (Method)	Result	MDA	Critical Level	NM Discharge Limit <sup>a</sup>	Comments
<i>Dry Gamma Spectroscopy<sup>f</sup></i>	<i>(pCi/g ± 2-σ)</i>	<i>(pCi/g)</i>	<i>(pCi/g)</i>	<i>(pCi/g)</i>	
Radium-224	1.59 ± 0.43	0.40	NL	NR	
Radium-226	0.43 ± 0.05	0.06	0.028	30.0 <sup>d</sup>	
Radium-228	0.47 ± 0.08	0.11	0.051	30.0 <sup>d</sup>	
Actinium-228	0.47 ± 0.08	0.11	0.051	NR	
Thorium-231	ND	0.62	0.30	NR	
Thorium-232	0.47 ± 0.08	0.11	0.051	NR	
Thorium-234	6.21 ± 0.73	0.23	0.11	NR	
Uranium-235	0.39 ± 0.04	0.12	0.057	NR	
Uranium-238	6.21 ± 0.73	0.23	0.11	NR	
Americium-241	ND	0.039	0.019	NR	

**Notes:**

- <sup>a</sup> New Mexico Water Quality Control Commission Regulations (1990), Section 3-103.
- <sup>b</sup> Isotopic uranium analyzed by NAS-NS-3050; plutonium by SL13028/SL13033; strontium by 7500-SR; thorium by NAS-NS-3004.
- <sup>c</sup> Analyzed by method HASL 300 at Quanterra, St. Louis.
- <sup>d</sup> NMWQCCR standard for Ra-226 + Ra-228 combined in pCi/L.
- MDA = Minimum detectable activity.
- ND = Not detected above MDA indicated.
- NR = Not regulated.
- NL = Not listed.







**ANNEX B**  
**DSS Site 1035**  
**Gore-Sorber™ Passive Soil-Vapor Survey Analytical Results**







# W. L. GORE & ASSOCIATES, INC.

100 CHESAPEAKE BLVD., P.O. BOX 10 • ELKTON, MARYLAND 21922-0010 • PHONE: 410/392-7600  
FAX: 410/506-4780

GORE-SORBER® EXPLORATION SURVEY  
GORE-SORBER® SCREENING SURVEY

1 of 6

## GORE-SORBER® Screening Survey Final Report

Non-ER Drain & Septic  
Kirtland AFB, NM

June 6, 2002

Prepared For:  
Sandia National Laboratories  
Mail Stop 0719, 1515 Eubank, SE  
Albuquerque, NM 87123

W.L. Gore & Associates, Inc.

Written/Submitted by:  
Jay W. Hodny, Ph.D., Project Manager

Reviewed/Approved by:  
Jim E. Whetzel, Project Manager

Analytical Data Reviewed by:  
Jim E. Whetzel, Chemist

I:\MAPPING\PROJECTS\10960025\020606R.DOC

*This document shall not be reproduced, except in full, without written approval of W.L. Gore & Associates*

**GORE-SORBER® Screening Survey  
Final Report**

**REPORT DATE:** June 6, 2002

**AUTHOR:** JWH

**SITE INFORMATION**

**Site Reference:** Non-ER Drain & Septic, Kirtland AFB, NM

**Customer Purchase Order Number:** 28518

**Gore Production Order Number:** 10960025

**Gore Site Code:** CCT, CCX

**FIELD PROCEDURES**

**# Modules shipped:** 142

**Installation Date(s):** 4/23,24,25,26,29,30/2002; 5/1,6/2002

**# Modules Installed:** 135

**Field work performed by:** Sandia National Laboratories

**Retrieval date(s):** 5/8,9,10,14,15,16,21/2002

**# Modules Retrieved:** 131

**# Modules Lost in Field:** 4

**# Modules Not Returned:** 1

**Exposure Time:** ~15 [days]

**# Trip Blanks Returned:** 3

**# Unused Modules Returned:** 3

**Date/Time Received by Gore:** 5/17/2002 @ 2:00 PM; 5/24/2002@1:30PM      **By:** MM

**Chain of Custody Form attached:** √

**Chain of Custody discrepancies:** None

**Comments:**

Modules #179227, -228, and -229 were identified as trip blanks.

Modules #179137, -138, -140, and -141 were not retrieved and considered lost from the field.

Module #179231 was not returned.

Modules #179230, 232, and -233 were returned unused.

**GORE-SORBER® Screening Survey  
Final Report**

**ANALYTICAL PROCEDURES**

W.L. Gore & Associates' Screening Module Laboratory operates under the guidelines of its Quality Assurance Manual, Operating Procedures and Methods. The quality assurance program is consistent with Good Laboratory Practices (GLP) and ISO Guide 25, "General Requirements for the Competence of Calibration and Testing Laboratories", third edition, 1990.

Instrumentation consists of state of the art gas chromatographs equipped with mass selective detectors, coupled with automated thermal desorption units. Sample preparation simply involves cutting the tip off the bottom of the sample module and transferring one or more exposed sorbent containers (sorbent, each containing 40mg of a suitable granular adsorbent) to a thermal desorption tube for analysis. Sorbent containers remain clean and protected from dirt, soil, and ground water by the insertion/retrieval cord, and require no further sample preparation.

**Analytical Method Quality Assurance:**

The analytical method employed is a modified EPA method 8260/8270. Before each run sequence, two instrument blanks, a sorbent containing 5µg BFB (Bromofluorobenzene), and a method blank are analyzed. The BFB mass spectra must meet the criteria set forth in the method before samples can be analyzed. A method blank and a sorbent containing BFB is also analyzed after every 30 samples and/or trip blanks. Standards containing the selected target compounds at three calibration levels of 5, 20, and 50µg are analyzed at the beginning of each run. The criterion for each target compound is less than 35% RSD (relative standard deviation). If this criterion is not met for any target compound, the analyst has the option of generating second- or third-order standard curves, as appropriate. A second-source reference standard, at a level of 10µg per target compound, is analyzed after every ten samples and/or trip blanks, and at the end of the run sequence. Positive identification of target compounds is determined by 1) the presence of the target ion and at least two secondary ions; 2) retention time versus reference standard; and, 3) the analyst's judgment.

**NOTE:** All data have been archived. Any replicate sorbents not used in the initial analysis will be discarded fifteen (15) days from the date of analysis.

**Laboratory analysis:** thermal desorption, gas chromatography, mass selective detection

**Instrument ID:** # 2 **Chemist:** JW

**Compounds/mixtures requested:** Gore Standard VOC/SVOC Target Compounds (A1)

**Deviations from Standard Method:** None

**Comments:** Soil vapor analytes and abbreviations are tabulated in the Data Table Key (page 6). Module #179091 was returned and noted as damaged, no carbonaceous sorbent; therefore, target compound masses reported in data table cannot be compared to the mass data from the other modules directly.

Module #179101, no identification tag was returned with this module.

**GORE-SORBER® Screening Survey  
Final Report**

**DATA TABULATION**

**# CONTOUR MAPS ENCLOSED:** No contour maps were generated.

**NOTE:** All data values presented in Appendix A represent masses of compound(s) desorbed from the GORE-SORBER Screening Modules received and analyzed by W.L. Gore & Associates, Inc., as identified in the Chain of Custody (Appendix A). The measurement traceability and instrument performance are reproducible and accurate for the measurement process documented. Semi-quantitation of the compound mass is based on either a single-level (QA Level 1) or three-level (QA Level 2) standard calibration.

**General Comments:**

- This survey reports soil gas mass levels present in the vapor phase. Vapors are subject to a variety of attenuation factors during migration away from the source concentration to the module. Thus, mass levels reported from the module will often be less than concentrations reported in soil and groundwater matrix data. In most instances, the soil gas masses reported on the modules compare favorably with concentrations reported in the soil or groundwater (e.g., where soil gas levels are reported at greater levels relative to other sampled locations on the site, matrix data should reveal the same pattern, and vice versa). However, due to a variety of factors, a perfect comparison between matrix data and soil gas levels can rarely be achieved.
- Soil gas signals reported by this method cannot be identified specifically to soil adsorbed, groundwater, and/or free-product contamination. The soil gas signal reported from each module can evolve from all of these sources. Differentiation between soil and groundwater contamination can only be achieved with prior knowledge of the site history (i.e., the site is known to have groundwater contamination only).
- QA/QC trip blank modules were provided to document potential exposures that were not part of the soil gas signal of interest (i.e., impact during module shipment, installation and retrieval, and storage). The trip blanks are identically manufactured and packaged soil gas modules to those modules placed in the subsurface. However, the trip blanks remain unopened during all phases of the soil gas survey. Levels reported on the trip blanks may indicate potential impact to modules other than the contaminant source of interest.

**GORE-SORBER® Screening Survey  
Final Report**

- Unresolved peak envelopes (UPEs) are represented as a series of compound peaks clustered together around a central gas chromatograph elution time in the total ion chromatogram. Typically, UPEs are indicative of complex fluid mixtures that are present in the subsurface. UPEs observed early in the chromatogram are considered to indicate the presence of more volatile fluids, while UPEs observed later in the chromatogram may indicate the presence of less volatile fluids. Multiple UPEs may indicate the presence of multiple complex fluids.

**Project Specific Comments:**

- Stacked total ion chromatograms (TICs) are included in Appendix A. The six-digit serial number of each module is incorporated into the TIC identification (e.g.: 123456S.D represents module #123456).
- No target compounds were detected on the trip blanks and/or the method blanks. Thus, target analyte levels reported for the field-installed modules that exceed trip and method blank levels, and the analyte method detection limit, have a high probability of originating from on-site sources.
- A small subset of modules was placed at each of several site locations; therefore no contour mapping was performed. Larger and more comprehensive soil gas surveys may be warranted at the individual sites where elevated soil gas levels were observed.

**GORE-SORBER® Screening Survey  
Final Report**

**KEY TO DATA TABLE  
Non-ER Drain & Septic, Kirtland AFB, NM**

**UNITS**

µg	micrograms (per sorber), reported for compounds
MDL	method detection limit
bdl	below detection limit
nd	non-detect

**ANALYTES**

<b>BTEX</b>	<i>combined masses of benzene, toluene, ethylbenzene and total xylenes (Gasoline Range Aromatics)</i>
BENZ	benzene
TOL	toluene
EtBENZ	ethylbenzene
mpXYL	m-, p-xylene
oXYL	o-xylene
C11,C13&C15	<i>combined masses of undecane, tridecane, and pentadecane (C11+C13+C15) (Diesel Range Alkanes)</i>
UNDEC	undecane
TRIDEC	tridecane
PENTADEC	pentadecane
TMBs	<i>combined masses of 1,3,5-trimethylbenzene and 1,2,4-trimethylbenzene</i>
135TMB	1,3,5-trimethylbenzene
124TMB	1,2,4-trimethylbenzene
ct12DCE	cis- & trans-1,2-dichloroethene
t12DCE	trans-1,2-dichloroethene
c12DCE	cis-1,2-dichloroethene
NAPH&2-MN	<i>combined masses of naphthalene and 2-methyl naphthalene</i>
NAPH	naphthalene
2MeNAPH	2-methyl naphthalene
MTBE	methyl t-butyl ether
11DCA	1,1-dichloroethane
CHCl <sub>3</sub>	chloroform
111TCA	1,1,1-trichloroethane
12DCA	1,2-dichloroethane
CCl <sub>4</sub>	carbon tetrachloride
TCE	trichloroethene
OCT	octane
PCE	tetrachloroethene
CIBENZ	chlorobenzene
14DCB	1,4-dichlorobenzene

**BLANKS**

TBn	unexposed trip blanks, travels with the exposed modules
method blank	QA/QC module, documents analytical conditions during analysis

## **APPENDIX A:**

1. CHAIN OF CUSTODY
2. DATA TABLE





# GORE-SORBER® Screening Survey Chain of Custody

For W.L. Gore & Associates use only  
Production Order # 10960025



**W. L. Gore & Associates, Inc., Survey Products Group**

100 Chesapeake Boulevard • Elkton, Maryland 21921 • Tel: (410) 392-7600 • Fax (410) 506-4780

*Instructions: Customer must complete ALL shaded cells*

Customer Name: <u>SANDIA NATIONAL LABS</u>			Site Name: <u>NON-ER DRAIN+ SEPTIC</u>		
Address: <u>ACCOUNTS PAYABLE MS0154</u>			Site Address: <u>KIVL 2ND AFB, NM</u>		
<u>P.O. BOX 5130</u>			<u>KIRTLAND</u>		
<u>ALBUQUERQUE NM 87185 U.S.A.</u>			Project Manager: <u>MIKE SANDERS</u>		
Phone: <u>505-284-3303</u>			Customer Project No.: _____		
FAX: <u>505-284-2616</u>			Customer P.O. #: <u>28518</u> Quote #: <u>211946</u>		
Serial # of Modules Shipped			# of Modules for Installation <u>135</u> # of Trip Blanks <u>7</u>		
# 179087 - # 179144	# <del>179087</del> - # <del>179134</del>	Total Modules Shipped: <u>142</u> Pieces			
# 179150 - # 179233	# <del>179135</del> - # <del>179136</del>	Total Modules Received: <u>142</u> Pieces			
# - #	# <del>179139</del> - #	Total Modules Installed: <u>135</u> Pieces			
# - #	# <del>179142</del> - # <del>179144</del>	Serial # of Trip Blanks (Client Decides)	#		
# - #	# <del>179150</del> - # <del>179151</del>	# <u>179227</u>	#		
# - #	# - #	#	#		
# - #	# - #	#	#		
# - #	# - #	#	#		
# - #	# - #	#	#		
# - #	# - #	#	#		
# - #	# - #	#	#		
Prepared By: <u><i>Chunara</i></u>			#	#	#
Verified By: <u><i>Mary Ann Murphy</i></u>			#	#	#
Installation Performed By:			Installation Method(s) (circle those that apply):		
Name (please print): <u>GILBERT QUINTANA</u>			Slide Hammer Hammer Drill Auger		
Company/Affiliation: <u>SNL/NM</u>			Other: <u>GEPRBE</u>		
Installation Start Date and Time: <u>4/23/02 10:15</u>			: <u>AM</u> PM		
Installation Complete Date and Time: <u>5/6/02 10:40</u>			: <u>AM</u> PM		
Retrieval Performed By:			Total Modules Retrieved: _____ Pieces		
Name (please print): <u>GILBERT QUINTANA</u>			Total Modules Lost in Field: _____ Pieces		
Company/Affiliation: <u>SNL/NM</u>			Total Unused Modules Returned: _____ Pieces		
Retrieval Start Date and Time: <u>5/8/02 1 1</u>			: AM PM		
Retrieval Complete Date and Time: _____			: AM PM		
Relinquished By: <u><i>W.L. Gore</i></u>	Date: <u>3-4-02</u>	Time: <u>12:00</u>	Received By: <u>Mike Sanders</u>	Date: <u>3-6-02</u>	Time: _____
Affiliation: <u>W.L. Gore &amp; Associates, Inc.</u>			Affiliation: <u>Sandia/ER</u>		
Relinquished By: <u><i>William J. Kelly</i></u>	Date: <u>5-14-02</u>	Time: <u>12:58</u>	Received By: _____	Date: _____	Time: _____
Affiliation: <u>6135</u>			Affiliation: _____		
Relinquished By: _____	Date: _____	Time: _____	Received By: <u><i>Mary Ann Murphy</i></u>	Date: _____	Time: _____
Affiliation: _____			Affiliation: <u>W.L. Gore &amp; Associates, Inc.</u>	<u>5/17/02</u>	<u>14:00</u>

# GORE-SORBER® Screening Survey Chain of Custody

For W.L. Gore & Associates use only  
Production Order # 10960025



**W. L. Gore & Associates, Inc., Survey Products Group**

100 Chesapeake Boulevard • Elkton, Maryland 21921 • Tel: (410) 392-7600 • Fax (410) 506-4780

**Instructions: Customer must complete ALL shaded cells**

Customer Name: <u>SANDIA NATIONAL LABS</u>			Site Name: <u>NON-ER DUAIN+ SEPTIC</u>		
Address: <u>ACCOUNTS PAYABLE MS0154</u>			Site Address: <u>KIVL 2ND AFB, NM</u>		
<u>P.O. BOX 5130</u>			<u>KIPTLAND</u>		
<u>ALBUQUERQUE NM 87185 U.S.A.</u>			Project Manager: <u>MIKE SANDERS</u>		
Phone: <u>505-284-3303</u>			Customer Project No.: _____		
FAX: <u>505-284-2616</u>			Customer P.O. #: <u>28518</u> Quote #: <u>211946</u>		
Serial # of Modules Shipped			# of Modules for Installation <u>135</u> # of Trip Blanks <u>7</u>		
# 179087 - # 179144	# <del>179152</del> - # <del>179187</del>	Total Modules Shipped:	<u>142</u>	Pieces	
# 179150 - # 179233	# <del>179188</del> - # <del>179216</del>	Total Modules Received:	<u>142</u>	Pieces	
# - #	# - #	Total Modules Installed:	<u>135</u>	Pieces	
# - #	# - #	Serial # of Trip Blanks (Client Decides)	#	#	
# - #	# - #	# <del>179228</del>	#	#	
# - #	# - #	# <del>179229</del>	#	#	
# - #	# - #	#	#	#	
# - #	# - #	#	#	#	
# - #	# - #	#	#	#	
# - #	# - #	#	#	#	
Prepared By: <u><i>William J. Fisher</i></u>	#	#	#	#	
Verified By: <u><i>Mary Anne Murphy</i></u>	#	#	#	#	
Installation Performed By:			Installation Method(s) (circle those that apply):		
Name (please print): <u>GILBERT QUINTANA</u>			Slide Hammer    Hammer Drill    Auger		
Company/Affiliation: <u>SNL/NM</u>			Other: <u>GEOPROBE</u>		
Installation Start Date and Time: <u>4/23/02 10:15</u>			: <u>AM</u> PM		
Installation Complete Date and Time: <u>5/6/02 10:40</u>			: <u>AM</u> PM		
Retrieval Performed By:			Total Modules Retrieved: <u>74</u> Pieces		
Name (please print): <u>GILBERT QUINTANA</u>			Total Modules Lost in Field: <u>4</u> Pieces		
Company/Affiliation: <u>SNL/NM</u>			Total Unused Modules Returned: <u>3</u> Pieces		
Retrieval Start Date and Time: <u>5/8/02 1 1</u>			: AM PM		
Retrieval Complete Date and Time: <u>1 1</u>			: AM PM		
Relinquished By: <u><i>William J. Fisher</i></u>	Date	Time	Received By: <u><i>Mike Sanders</i></u>	Date	Time
Affiliation: <u>W.L. Gore &amp; Associates, Inc.</u>	<u>3-4-02</u>	<u>12:00</u>	Affiliation: <u>Sandia, 6133</u>	<u>3-7-02</u>	
Relinquished By: <u><i>William J. Fisher</i></u>	Date	Time	Received By: _____	Date	Time
Affiliation: <u>Sandia N.L., 6135</u>	<u>5-21-02</u>	<u>0935</u>	Affiliation: _____		
Relinquished By: _____	Date	Time	Received By: <u><i>Mary Anne Murphy</i></u>	Date	Time
Affiliation: _____			Affiliation: <u>W.L. Gore &amp; Associates, Inc.</u>	<u>5-24-02</u>	<u>13:30</u>

# GORE-SORBER® Screening Survey Installation and Retrieval Log

SITE NAME & LOCATION

1 of 4

LINE #	MODULE #	INSTALLATION DATE/TIME	RETRIEVAL DATE/TIME	EVIDENCE OF LIQUID HYDROCARBONS (LPH) or HYDROCARBON ODOR (Check as appropriate)			MODULE IN WATER (check one)		COMMENTS
				LPH	ODOR	NONE	YES	NO	
1.	179087	4/23/02, 0815	05-08-02, 0800					✓	1001/898-GS-5
2.	179088	0822							GS-3
3.	179089	0830							GS-2
4.	179090	0840							GS-1
5.	179091	0852						✓	GS-4
6.	179092	0952	0830					✓	1052/903-GS-1
7.	179093	1000							-4
8.	179094	1010							-3
9.	179095	1018						✓	-2
10.	179096	1135	0900						1030/6587-
11.	179097	1151							-5
12.	179098	1238							-6
13.	179099	1247							-4
14.	179100	1254							-3
15.	179101	1304							-2
16.	179102	1347	0920						-1
	179103	1355							1082/6620-
18.	179104	1404							-4
19.	179105	1431							-5
20.	179106	1440							-3
21.	179107	4/24/02, 0848	5-9-02, 0930						1108/6531-
22.	179108	0853							-5
23.	179109	0900							-6
24.	179110	0907							-4
25.	179111	0916							-2
26.	179112	0936							-3
27.	179113	4/25/02, 0746	5-10-02, 0812						1027/6530-
28.	179114	0754							-5
29.	179115	0800							-2
30.	179116	0810							-3
31.	179117	0818	0917						-4
32.	179118	0915	5-10-02, 0925						-1
33.	179119	0922							1010/6536-
34.	179120	0931							5
35.	179121	0942							6
36.	179122	0947							4
37.	179123	0956	1002						2
38.	179124	1026	5-10-02, 1013						1
39.	179125	1043							1028/6560-
40.	179126	1052							1
41.	179127	1103	1041						4
42.	179128	1420	5-10-02, 1045						3
									2
									1026/6501-✓ 2

**GORE-SORBER® Screening Survey  
Installation and Retrieval Log**

**SITE NAME & LOCATION**

2 of 4

LINE #	MODULE #	INSTALLATION DATE/TIME	RETRIEVAL DATE/TIME	EVIDENCE OF LIQUID HYDROCARBONS (LPH) or HYDROCARBON ODOR (Check as appropriate)			MODULE IN WATER (check one)		COMMENTS
				LPH	ODOR	NONE	YES	NO	
43.	179129	4/25/02, 1428	5-10-02, 10:47						1026/654-65-3
44.	179130	1437	5-10-02, 10:51						↓ 1
45.	179131	1442	5-10-02, 10:53						1025/650- 1
46.	179132	1446	↓						2
47.	179133	↓ 1504	5-10-02, 11:06						↓ 3
48.	179134	4/26/02, 0905	5-10-02, 12:47						1093/6504- 1
49.	179135	0914	↓ 12:54						4
50.	179136	0930	5-10-02, 13:05						2
51.	179137	0938	Lost						3
52.	179138	0948	Lost						5
53.	179139	1018	5-10-02, 13:22						↓ 2
54.	179140	1026	Lost						3
55.	179141	1030	Lost						4
56.	179142	1038	5-10-02, 13:43						↓ 1
57.	179143	1136	5-10-02, 11:36						276/829X- 2
	179144	1142	↓						3
	179150	1150	↓						
60.	179151	↓ 1155	5-10-02, 11:54						↓ 1
61.	179152	4/29/02, 0814	5-14-02, 09:42						1089/6505- 1
62.	179153	0822	↓						5
63.	179154	0829	↓						3
64.	179155	0903	↓						2
65.	179156	0845	5-14-02, 10:21						↓ 4
66.	179157	0930	05-14-02, 09:19						1083/6570- 4
67.	179158	0934	↓						1
68.	179159	0940	↓						2
69.	179160	0948	↓ 0940						↓ 3
70.	179161	1050	05-14-02, 10:26						1032/6610- 1
71.	179162	1100	↓						2
72.	179163	1110	↓						4
73.	179164	1114	↓						3
74.	179165	1120	↓						5
75.	179166	1126	05-14-02, 11:03						↓ 6
76.	179167	1222	05-14-02, 11:06						1120/6643- 2
77.	179168	1230	↓						3
78.	179169	1237	↓						4
79.	179170	1242	05-14-02, 11:32						↓ 1
80.	179171	1320	5-14-02, 08:44						1034/6710- 4
	179172	1325	↓ 09:02						3
82.	179173	1332	↓ 08:51						
83.	179174	1340	↓ 08:55						↓
5 1039 84.	179175	↓ 1423	5-14-02, 08:14						1035/6715- ↓ 4

**GORE-SORBER® Screening Survey  
Installation and Retrieval Log**

**SITE NAME & LOCATION**

3 of 4

SS  
35

LINE #	MODULE #	INSTALLATION DATE/TIME	RETRIEVAL DATE/TIME	EVIDENCE OF LIQUID HYDROCARBONS (LPH) or HYDROCARBON ODOR (Check as appropriate)			MODULE IN WATER (check one)		COMMENTS
				LPH	ODOR	NONE	YES	NO	
85.	179176	4/29/02, 1431							
86.	179177	1440							1035/6715-65-3
87.	179178	1445	5-14-02 0837						2
88.	179179	4/30/02, 0910	5-15-02 0842						1003/915- 1
89.	179180	0919							3
90.	179181	0926							2
91.	179182	0937							1
92.	179183	0943							4
93.	179184	0947	5-15-02, 0912						5
94.	179185	1108	5-15-02, 1146						6
95.	179186	1113							1007/6730- 4
96.	179187	1119							3
97.	179188	1132							2
98.	179189	1140	5-15-02 1213						5
99.	179190	1238	5-15-02 10:09						1
100.	179191	1250							1029/6584W- 1
	179192	1300							-2
102.	179193	1313							-3
103.	179194	1318	5-15-02, 1032						-5
104.	179195	1445	5-15-02, 14:05						-4
105.	179196	1450							1006/6741- 5
106.	179197	1455							3
107.	179198	1502							4
108.	179199	1508	5-15-02, 1143						2
109.	179200	1525	5-15-02, 1039						1087/6743- 1
110.	179201	1530							2
111.	179202	1534							3
112.	179203	1540	5-15-02, 1059						4
113.	179204	5/1/02, 0822	5-16-02, 0801						1
114.	179205	0835							1008/6750 3
115.	179206	0843							4
116.	179207	0851	5-16-02, 0832						1
117.	179208	0944	5-16-02, 0841						2
118.	179209	0952							1004/6969- 2
119.	179210	1000							4
120.	179211	1009							3
121.	179212	1016	5-16-02, 0907						5
122.	179213	1110	5-16-02, 1105						1
123.	179214	1116							1095/9935- 3
124.	179215	1122	5-16-02, 11:21						2
125.	179216	1205	5-16-02-0931						1
126.	179217	1218	5-16-02-0935						1094/6969- 2

<b>GORE-SORBER® Screening Survey</b> <b>Installation and Retrieval Log</b>	<b>SITE NAME &amp; LOCATION</b>
---	---------------------------------

4. of 4.

LINE #	MODULE #	INSTALLATION DATE/TIME	RETRIEVAL DATE/TIME	EVIDENCE OF LIQUID HYDROCARBONS (LPH) or HYDROCARBON ODOR (Check as appropriate)			MODULE IN WATER (check one)		COMMENTS
				LPH	ODOR	NONE	YES	NO	
				127.	179218	5/1/02, 1225	5-16-02, 0942		
128.	179219	1231	5-16-02, 0950						1094/LAR-GS-3
129.	179220	5/6/02, 0850	5-21-01 07:57						↓ -4
130.	179221	0857							1081/6650 -1
131.	179222	0909							-3
132.	179223	0918							-2
133.	179224	0926							-4
134.	179225	0933	↓						-6
135.	179226	√ 0940	5-21-01, 0851						√ -5
136.	179227								√ -7
137.	179228								
138.	179229								
139.	179230								
140.	179231								
141.	179232								
142.	179233								
143.									
144.									
145.									
146.									
147.									
148.									
149.									
150.									
151.									
152.									
153.									
154.									
155.									
156.									
157.									
158.									
159.									
160.									
161.									
162.									
163.									
164.									
165.									
166.									
167.									
168.									

GORE SORBER SCREENING SURVEY ANALYTICAL RESULTS  
 SANDIA NATIONAL LABS, ALBUQUERQUE, NM  
 GORE STANDARD TARGET VOCs/SVOCs (A1)  
 NON-ER DRAIN AND SEPTIC, KIRTLAND AFB, NM  
 SITES CCT AND CCX - PRODUCTION ORDER #10960025

DATE ANALYZED	SAMPLE NAME	BTEX, ug	BENZ, ug	TOL, ug	EtBENZ, ug	mpXYL, ug	oXYL, ug	C11, C13, & C15, ug	UNDEC, ug	TRIDEC, ug	PENTADEC, ug	TMBS, ug
	MDL=	0.03	0.02	0.01	0.01	0.01	0.01	0.05	0.02	0.01	0.02	0.02
5/28/2002	179172	nd	nd	nd	nd	nd	nd	0.05	0.03	0.02	bdl	nd
5/29/2002	179173	0.39	0.09	0.18	nd	0.09	0.03	0.19	0.10	0.04	0.05	0.09
5/29/2002	179174	0.03	nd	nd	nd	0.03	nd	0.00	bdl	bdl	bdl	0.00
5/29/2002	179175	nd	nd	nd	nd	nd	nd	0.05	0.05	bdl	bdl	nd
5/29/2002	179176	0.19	0.08	0.10	nd	0.02	nd	1.20	1.12	0.06	0.03	0.04
5/29/2002	179177	0.34	0.14	0.11	nd	0.07	0.03	0.10	0.08	0.02	bdl	0.14
5/29/2002	179178	0.08	nd	0.05	0.01	0.02	nd	0.14	0.06	0.03	0.05	0.00
5/29/2002	179179	0.03	nd	0.03	nd	nd	nd	0.07	0.03	0.02	0.02	0.04
5/29/2002	179180	nd	nd	nd	nd	nd	nd	0.04	0.02	0.01	bdl	0.00
5/29/2002	179181	0.00	nd	nd	nd	bdl	nd	0.10	0.03	0.02	0.05	0.00
5/29/2002	179182	0.09	nd	0.08	nd	0.01	nd	0.08	0.03	0.02	0.03	0.00
5/29/2002	179183	nd	nd	nd	nd	nd	nd	0.08	0.04	bdl	0.04	0.00
5/29/2002	179184	nd	nd	nd	nd	nd	nd	0.09	0.03	0.02	0.04	0.00
5/29/2002	179185	nd	nd	nd	nd	nd	nd	0.05	bdl	0.01	0.04	nd
5/29/2002	179186	nd	nd	nd	nd	nd	nd	0.05	0.03	bdl	0.03	0.04
5/29/2002	179187	0.60	0.18	0.30	0.03	0.06	0.03	0.15	0.05	0.05	0.05	0.11
5/29/2002	179188	0.02	nd	nd	nd	0.02	nd	0.10	bdl	0.02	0.07	0.00
5/29/2002	179189	0.02	nd	nd	nd	0.02	nd	0.07	0.04	0.03	bdl	0.00
5/29/2002	179190	0.06	nd	0.03	nd	0.03	nd	0.11	0.05	0.03	0.04	0.00
5/29/2002	179191	0.10	nd	0.04	nd	0.05	nd	0.08	0.02	0.01	0.05	0.00
5/29/2002	179192	0.01	nd	nd	nd	0.01	nd	0.11	0.04	0.02	0.05	0.00
5/29/2002	179193	nd	nd	nd	nd	nd	nd	0.07	0.03	0.01	0.02	0.00
5/29/2002	179194	0.04	nd	nd	nd	0.04	nd	0.08	0.04	bdl	0.04	0.00
5/29/2002	179195	0.04	nd	nd	nd	0.04	nd	0.08	0.04	0.02	0.02	0.00
5/29/2002	179196	0.02	nd	nd	nd	0.02	nd	0.09	0.04	0.02	0.03	0.00
5/29/2002	179197	0.03	nd	nd	nd	0.03	nd	0.15	0.05	0.04	0.06	0.04
5/29/2002	179198	0.07	nd	0.04	nd	0.03	nd	0.09	0.04	0.03	0.03	nd
5/29/2002	179199	nd	nd	nd	nd	nd	nd	0.05	0.03	0.01	bdl	0.00
5/29/2002	179200	0.00	nd	nd	nd	bdl	nd	0.08	0.03	0.02	0.03	0.00
5/29/2002	179201	0.02	nd	nd	nd	0.02	nd	0.04	0.04	bdl	bdl	0.00
5/29/2002	179202	0.02	nd	nd	nd	0.02	nd	0.04	0.03	0.01	bdl	0.00
5/29/2002	179203	0.04	nd	0.04	nd	nd	nd	0.06	0.04	0.02	bdl	0.03
5/29/2002	179204	0.27	nd	0.22	nd	0.03	0.02	0.29	0.06	0.14	0.09	0.00
5/29/2002	179205	0.12	nd	0.09	nd	0.03	bdl	1.28	1.13	0.08	0.07	0.03
5/29/2002	179206	nd	nd	nd	nd	nd	nd	0.02	0.02	bdl	bdl	nd
5/29/2002	179207	0.03	nd	nd	nd	0.03	nd	0.04	0.04	bdl	bdl	0.00
5/29/2002	179208	0.06	nd	0.04	nd	0.02	nd	0.09	0.04	0.03	0.03	0.00
5/29/2002	179209	0.07	nd	0.04	nd	0.03	nd	0.01	bdl	0.01	bdl	0.00

No mdl is available for summed combinations of analytes. In summed columns (eg., BTEX), the reported values should be considered ESTIMATED if any of the individual compounds were reported as bdl.

DSS  
 1035



GORE SORBER SCREENING SURVEY ANALYTICAL RESULTS  
 SANDIA NATIONAL LABS, ALBUQUERQUE, NM  
 GORE STANDARD TARGET VOCs/SVOCs (A1)  
 NON-ER DRAIN AND SEPTIC, KIRTLAND AFB, NM  
 SITES CCT AND CCX - PRODUCTION ORDER #10960025

SAMPLE NAME	124TMB, ug	135TMB, ug	ct12DCE, ug	12DCE, ug	ct12DCE, ug	NAPH&2-MN, ug	NAPH, ug	2MeNAPH, ug	MTBE, ug	11DCA, ug	111TCA, ug	12DCA, ug
MDL=	0.03	0.02	0.14	0.03	0.03	0.01	0.02	0.04	0.04	0.04	0.02	0.02
179172	nd	nd	nd	0.00	0.09	0.03	0.06	nd	nd	nd	nd	nd
179173	0.06	0.03	nd	0.00	0.00	nd	bdl	nd	nd	nd	nd	nd
179174	bdl	bdl	nd	0.00	0.05	0.02	0.02	0.02	0.02	0.04	0.02	0.02
179175	nd	nd	nd	0.10	0.06	0.02	0.03	0.03	0.03	0.04	0.02	0.02
179176	0.04	0.04	nd	0.06	0.06	0.02	0.04	0.04	0.04	0.05	0.02	0.02
179177	bdl	bdl	nd	0.00	0.00	nd	bdl	nd	nd	nd	nd	nd
179178	0.04	bdl	nd	0.00	0.00	nd	bdl	nd	nd	nd	nd	nd
179179	bdl	bdl	nd	0.00	0.00	nd	bdl	nd	nd	nd	nd	nd
179180	bdl	bdl	nd	0.00	0.00	nd	bdl	nd	nd	nd	nd	nd
179181	bdl	bdl	nd	0.00	0.00	nd	bdl	nd	nd	nd	nd	nd
179182	bdl	bdl	nd	0.00	0.00	nd	bdl	nd	nd	nd	nd	nd
179183	bdl	bdl	nd	0.02	0.02	0.02	0.02	0.02	0.02	0.02	0.02	0.02
179184	bdl	bdl	nd	0.05	0.05	0.02	0.03	0.03	0.03	0.03	0.03	0.03
179185	nd	nd	nd	0.00	0.00	nd	bdl	nd	nd	nd	nd	nd
179186	0.04	0.02	nd	0.00	0.00	nd	bdl	nd	nd	nd	nd	nd
179187	0.09	0.02	nd	0.00	0.00	nd	bdl	nd	nd	nd	nd	nd
179188	bdl	nd	nd	0.00	0.00	nd	bdl	nd	nd	nd	nd	nd
179189	bdl	bdl	nd	0.00	0.00	nd	bdl	nd	nd	nd	nd	nd
179190	bdl	bdl	nd	0.00	0.00	nd	bdl	nd	nd	nd	nd	nd
179191	bdl	bdl	nd	0.00	0.00	nd	bdl	nd	nd	nd	nd	nd
179192	bdl	bdl	nd	0.00	0.00	nd	bdl	nd	nd	nd	nd	nd
179193	bdl	bdl	nd	0.00	0.00	nd	bdl	nd	nd	nd	nd	nd
179194	bdl	bdl	nd	0.02	0.02	0.02	0.02	0.02	0.02	0.02	0.02	0.02
179195	bdl	bdl	nd	0.10	0.10	0.03	0.07	0.07	0.07	0.07	0.07	0.07
179196	bdl	bdl	nd	0.05	0.05	0.02	0.02	0.02	0.02	0.02	0.02	0.02
179197	0.04	bdl	nd	0.11	0.11	0.04	0.07	0.07	0.07	0.07	0.07	0.07
179198	nd	nd	nd	0.00	0.00	nd	bdl	nd	nd	nd	nd	nd
179199	bdl	nd	nd	0.00	0.00	nd	bdl	nd	nd	nd	nd	nd
179200	bdl	nd	nd	0.02	0.02	nd	bdl	nd	nd	nd	nd	nd
179201	bdl	nd	nd	0.00	0.00	nd	bdl	nd	nd	nd	nd	nd
179202	bdl	nd	nd	0.00	0.00	nd	bdl	nd	nd	nd	nd	nd
179203	0.03	bdl	nd	0.03	0.03	0.03	0.03	0.03	0.03	0.03	0.03	0.03
179204	bdl	bdl	nd	0.11	0.11	0.04	0.07	0.07	0.07	0.07	0.07	0.07
179205	0.03	bdl	nd	0.13	0.13	0.05	0.07	0.07	0.07	0.07	0.07	0.07
179206	nd	nd	nd	0.03	0.03	nd	bdl	nd	nd	nd	nd	nd
179207	bdl	bdl	nd	0.00	0.00	nd	bdl	nd	nd	nd	nd	nd
179208	bdl	bdl	nd	0.00	0.00	nd	bdl	nd	nd	nd	nd	nd
179209	bdl	bdl	nd	0.05	0.05	0.02	0.03	0.03	0.03	0.03	0.03	0.03

DSS  
1035

No mdl is available for summed combinations of analytes. In summed columns (eg., BTEX), the reported values should be considered ESTIMATED if any of the individual compounds were reported as bdl.

GORE SORBER SCREENING SURVEY ANALYTICAL RESULTS  
 SANDIA NATIONAL LABS, ALBUQUERQUE, NM  
 GORE STANDARD TARGET VOCs/SVOCs (A1)  
 NON-ER DRAIN AND SEPTIC, KIRTLAND AFB, NM  
 SITES CCT AND CCX - PRODUCTION ORDER #10960025

SAMPLE NAME	TCE, ug	OCT, ug	PCE, ug	14DCB, ug	CHCl3, ug	CCl4, ug	CIBENZ, ug
MDL=	0.02	0.02	0.01	0.01	0.03	0.03	0.01
179172	nd	nd	nd	nd	nd	nd	nd
179173	nd	0.14	0.02	nd	nd	nd	nd
179174	nd	nd	nd	nd	nd	nd	nd
179175	nd	nd	0.04	nd	nd	nd	nd
179176	nd	nd	0.03	nd	nd	nd	nd
179177	nd	0.09	0.02	nd	nd	nd	nd
179178	nd	nd	0.01	nd	nd	nd	nd
179179	0.13	nd	0.07	nd	0.05	nd	nd
179180	0.08	nd	0.02	nd	nd	nd	nd
179181	0.11	nd	0.03	nd	nd	nd	nd
179182	0.15	nd	0.04	nd	nd	nd	nd
179183	0.59	nd	0.08	nd	nd	nd	nd
179184	nd	nd	nd	nd	nd	nd	nd
179185	0.06	nd	nd	nd	nd	nd	nd
179186	nd	nd	nd	nd	nd	nd	nd
179187	0.13	nd	0.08	nd	nd	nd	nd
179188	nd	nd	0.11	nd	nd	nd	nd
179189	0.06	nd	0.02	nd	nd	nd	nd
179190	nd	nd	bdl	nd	nd	bdl	nd
179191	nd	nd	0.03	nd	nd	0.03	nd
179192	nd	nd	0.03	nd	nd	nd	nd
179193	nd	nd	0.08	nd	nd	nd	nd
179194	nd	nd	0.04	nd	nd	nd	nd
179195	nd	nd	nd	nd	nd	nd	nd
179196	nd	nd	nd	nd	nd	0.03	nd
179197	nd	nd	nd	nd	nd	bdl	nd
179198	nd	0.09	nd	nd	nd	nd	nd
179199	nd	nd	nd	nd	nd	bdl	nd
179200	nd	nd	0.09	nd	nd	nd	nd
179201	nd	nd	0.12	nd	nd	nd	nd
179202	nd	nd	0.12	nd	nd	nd	nd
179203	nd	nd	0.09	nd	nd	nd	nd
179204	1.49	nd	3.01	nd	nd	nd	nd
179205	4.14	nd	6.74	nd	nd	nd	nd
179206	4.72	nd	2.69	nd	nd	nd	nd
179207	2.89	nd	2.57	nd	nd	nd	nd
179208	nd	nd	nd	nd	0.05	nd	nd
179209	nd	nd	nd	nd	nd	nd	nd

1035

No mdl is available for summed combinations of analytes. In summed columns (eg., BTEX), the reported values should be considered ESTIMATED if any of the individual compounds were reported as bdl.



**ANNEX C**  
**DSS Site 1035**  
**Soil Sample Data Validation Results**

CONTRACT LABORATORY ANALYSIS REQUEST AND CHAIN OF CUSTODY

Internal Lab

Batch No. <b>N/A</b>	Project/Task No. <b>7223.02.03.02</b>	AR/COC <b>605672</b>										
Dept. No./Mail Stop: <b>6135/1089</b>	Date Samples Shipped: <b>9-16-07</b>	Waste Characterization: <input type="checkbox"/> Send preliminary/copy report to:										
Project/Task Manager: <b>Mike Sanders</b>	SMO Authorization: <b>DP</b>	Released by COC No.: <input type="checkbox"/> Validation Required: <input checked="" type="checkbox"/>										
Project Name: <b>DSS soil sampling</b>	Carrier/Waybill No. <b>13479</b>	Contract # PO 21871										
Record Center Code: <b>ER/1295/DSS/DAT</b>	Lab Contact: <b>GEL</b>	BIR To: <b>Sandia National Labs (Accounts Payable)</b>										
Logbook Ref. No.: <b>ER 090</b>	Lab Destination: <b>580 Attention 807W</b>	P.O. Box 5800 MS 0154										
Service Order No. <b>CF032-073</b>	SMO Contact/Phone: <b>Pam Putsant/505-844-3185</b>	Albuquerque, NM 87185-0154										
Location: <b>Tech Area</b>	Send Report to SMO: <b>Wendy Palencia/505-844-3132</b>											
Building <b>6536-6715</b>												
Room												
<b>Reference LOV (available at SMO)</b>												
Sample No. - Fraction	ER Sample ID or Sample Location Detail	Pump Depth (ft)	ER Site No.	Date/Time Collected	Sample Matrix	Container Type	Volume	Preservative	Collection Method	Sample Type	Parameter & Method Requested	Lab Sample ID
059828-001	6536 HP/1110-DF1-BH1-15-S	15'	1110	9-10-07/1115	S	AS	4oz	4c	G	SA	VOC(8260B)	
059829-001	6536 HP/1110-DF1-BH1-20-S	20'		1145	S	AS	4oz	4c	G	SA	VOC(8260B)	
059828-002	6538 HP/1110-DF1-BH1-15-S	15'		1120	S	AG	500ml	4c	G	SA	see below for parameter	
059829-002	6538 HP/1110-DF1-BH1-20-S	20'		1150	S	AG	500ml	4c	G	SA	see below for parameter	
059836-001	6536 HP/1110-DF1-BH2-10-S	10'		9-12-07/0855	S	AS	4oz	4c	G	SA	VOC(8260B)	
059837-001	6538 HP/1110-DF1-BH2-15-S	15'		0910	S	AS	4oz	4c	G	SA	VOC(8260B)	
059838-002	6536 HP/1110-DF1-BH2-10-S	10'		0900	S	AG	500ml	4c	G	SA	see below for parameter	
059837-002	6538 HP/1110-DF1-BH2-15-S	15'		0915	S	AG	500ml	4c	G	SA	see below for parameter	
059838-001	6715/1035-SP1-BH1-11-S	11'	1035	1410	S	AS	4oz	4c	G	SA	VOC(8260B)	
059839-001	6715/1035-SP1-BH1-16-S	16'	1035	1430	S	AS	4oz	4c	G	SA	VOC(8260B)	
RMMA												
Sample Disposal	<input type="checkbox"/> Yes <input checked="" type="checkbox"/> No	Ref. No.										
Turnaround Time	<input type="checkbox"/> Return to Client <input checked="" type="checkbox"/> Normal	Disposition by lab										
Return Samples By:	Level of Rush:	Signature	Name	Int	Company/Organization/Phone/Cellular	Sample Tracking	Date Entered (mm/dd/yyyy)	QC Inits.	Special Instructions/QC Requirements	Abnormal Conditions on Receipt		
		J. Lee	J. Lee		Weston/6135/505-284-3309	09/18/07			SVOC(8270C_)			
		W. Gibson	W. Gibson		MDM/6135/505-845-3267				PCB(8082)HE(8330)			
		G. Quintana	G. Quintana		Shaw/6135/505-284-3306				Total Cyanide(9010)			
									Cr6+(7197)			
									RCRA metals(8020, 7000,7471)Gross alpha-beta(900)			
1. Relinquished by	Org.	Date	Time	4. Relinquished by	Org.	Date	Time					
1. Received by	Org.	Date	Time	4. Received by	Org.	Date	Time					
2. Relinquished by	Org.	Date	Time	5. Relinquished by	Org.	Date	Time					
2. Received by	Org.	Date	Time	5. Received by	Org.	Date	Time					
3. Relinquished by	Org.	Date	Time	6. Relinquished by	Org.	Date	Time					
3. Received by	Org.	Date	Time	6. Received by	Org.	Date	Time					





Sample Findings Summary

Site: DSS soil sampling

ARCC: 606671, 72, 73

Date: Organic, Inorganic and Radiochemistry

Sample ID	VOC(s)	Sample ID	SVOC(s)	117-B-17 (bis(2-ethylhexyl)phthalate)	129-00-0 (pyrene)	All PCBs (002)	HE(1330)	1940-61-0 (4-amino-2,6-dimercaptoethane)	479-65-8 (stry)	Metals	7440-50-3 (barium)	7440-47-3 (chromium)	7782-49-2 (selenium)	7440-38-2 (arsenic)	General Chemistry	5955-70-0 (total cyanide)	18540-29-8 (hexavalent chromium)	Radiochemistry
059827-001 87151035-SP1-TB	U	059826-003 6639HP1110-EB			P2													
059829-001 6639HP1110-EB	U	059828-009 6639HP1110-EB																
059840-001 6639HP1110-TB	U	059828-007 6639HP1110-EB																
059846-001 87211090-DF1-TB	U																	
059820-001 MO 228-2301082-DF1-BH1-6-S	U	059820-002 MO 228-2301082-DF1-BH1-6-S	362U,B															
059821-001 MO 228-2301082-DF1-BH1-11-S	U	059821-002 MO 228-2301082-DF1-BH1-11-S	333U,B															
059822-001 MO 228-2301082-DF1-BH2-6-S	U	059822-002 MO 228-2301082-DF1-BH2-6-S	333U,B															
059823-001 MO 228-2301082-DF1-BH2-11-S	U	059823-002 MO 228-2301082-DF1-BH2-11-S	333U,B															
059824-001 MO 228-2301082-DF1-BH3-6-S	U	059824-002 MO 228-2301082-DF1-BH3-6-S	333U,B															
059825-001 MO 228-2301082-DF1-BH3-11-S	U	059825-002 MO 228-2301082-DF1-BH3-11-S	333U,B															
059826-001 6639 HP1110-DF1-BH1-15-S	U	059826-002 6639 HP1110-DF1-BH1-15-S	333U,B															
059829-001 6639 HP1110-DF1-BH1-20-S	U	059829-002 6639 HP1110-DF1-BH1-20-S	333U,B															
059835-001 6639 HP1110-DF1-BH2-10-S	U	059835-002 6639 HP1110-DF1-BH2-10-S	333U,B															
059837-001 6639 HP1110-DF1-BH2-15-S	U	059837-002 6639 HP1110-DF1-BH2-15-S	333U,B															
059839-001 87151035-SP1-BH1-11-S	U	059839-002 87151035-SP1-BH1-11-S	333U,B															
059839-001 87151035-SP1-BH1-16-S	U	059839-002 87151035-SP1-BH1-16-S	333U,B															
059841-001 87211090-DF1-BH1-4-S	U	059841-002 87211090-DF1-BH1-4-S	333U,B															
059842-001 87211090-DF1-BH1-6-S	U	059842-002 87211090-DF1-BH1-6-S	333U,B															
059843-001 87211090-DF1-BH2-4-S	U	059843-002 87211090-DF1-BH2-4-S	333U,B															
059844-001 87211090-DF1-BH2-6-S	U	059844-002 87211090-DF1-BH2-6-S	333U,B															
059845-001 87211090-DF1-BH2-4-DU	U	059845-002 87211090-DF1-BH2-4-DU	333U,B															
059847-001 87211090-DF1-BH3-4-S	U	059847-002 87211090-DF1-BH3-4-S	333U,B															
059848-001 87211090-DF1-BH3-6-S	U	059848-002 87211090-DF1-BH3-6-S	333U,B															

Verified By: *A. Neal*

Date: 11/18/02

All OC acceptance criteria were met. No data will be qualified.



Analytical Quality Associates, Inc.



616 Maxine NE  
Albuquerque, NM 87123  
Phone: 505-299-5201  
Fax: 505-299-6744  
Email: [minteer@aol.com](mailto:minteer@aol.com)

**MEMORANDUM**

DATE: 11/19/02  
TO: File  
FROM: Linda Thal  
SUBJECT: Inorganic Data Review and Validation - SNL  
Site: DSS soil sampling  
ARCO # 605671, -72, -73  
GEL SDG # 67158 and 67169  
Project/Task No. 7223.02.03.02

See the attached Data Validation Worksheets for supporting documentation on the data review and validation. Data are evaluated using SNL/NM ER Project AOP 00-03.

**Summary**

The samples were prepared and analyzed with approved procedures using methods SW-846 6010 (ICP-AES metals), SW-846 7471/7470 (Hg), SW-846 9012A (total CN) and SW-846 7196A (hexavalent chromium).

Problems were identified with the data package that resulted in the qualification of data.

**ICP-AES – Metals Batch # 202762 (Samples 67158-020 through -038)**

Selenium was detected in the MB and CCB at a value > DL but < RL. All associated sample results that are detect, < 5X the blank value will be qualified "J". The descriptor flags "B" (MB) and "B3" (CCB) will be added.

Selenium was detected in the CCB at a negative value with an absolute value > DL but < RL. All associated sample results that are non-detect will be qualified "UJ, B3". All associated sample results that are detect, but < 5X the MDL will be qualified "J, B3".

The replicate RPD (44%) failed QC acceptance criteria (<35%) for arsenic. All associated sample results were > 5X RL and will be qualified "J".

**ICP-AES-Metals Batch # 204455 (Sample 67169-010)**

Barium was detected in the CCB, and chromium in the MB at values > DL but < RL. The sample results were <5X the blank value and will be qualified "J, B" for chromium and "J, B3" for barium.

**Total Cyanide - Batch #202749 (Samples 67158-020 through -038)**

The MB had a value > DL but < RL. All associated sample results that were > DL but < 5X MB value will be qualified "J, B".

**Hexavalent Chromium – Batch # 201822**

Sample 67169-009 was received by the laboratory and analyzed after 2X the holding time had expired. The sample result was non-detect and will be qualified "R, HT".

Data are acceptable except as mentioned above and QC measures appear to be adequate. The following sections discuss the data review and validation.

**Holding Times/Preservation**

**All Analyses:** The samples were analyzed within the prescribed holding time and properly preserved except as mentioned above in the summary section.

**Calibration**

**All Analyses:** The initial and continuing calibration data met QC acceptance criteria.

**Blanks**

**All Analyses:** All blank criteria were met except as mentioned above in the summary section and as follows:

**ICP-AES – Metals Batch # 202762 (Samples 67158-020 through -038)**

Selenium was detected in the MB and CCB at a value > DL but < RL. All associated sample results that are non-detect will not be qualified.

Selenium was detected in the CCB at a negative value with an absolute value > DL but < RL. All associated sample results that are detect with values > 5X the MDL, will not be qualified.

Barium and chromium were detected in the EB, and arsenic in the CCB, at values > DL but < RL. All associated sample results were > 5X the blank values and will not be qualified.

**ICP-AES-Metals Batch # 204455 (Sample 67169-010)**

Cadmium and arsenic were detected in the CCB at values > DL but < RL. The sample results were non-detect and no data will be qualified.

**Total Cyanide - Batch #202749 (Samples 67158-020 through -038)**

The MB had a value > DL but < RL. Sample 67158-021, -026, -027 -029 and -033 were all non-detect and will not be qualified. Sample 67158-035 had a value at the RL and >5X MB value and will not be qualified.

### **Laboratory Control Sample/Laboratory Control Sample Duplicate (LCS/LCSD) Analyses**

**All Analyses:** The LCS met QC acceptance criteria. No LCSD was analyzed. No data will be qualified as a result.

### **Matrix Spike (MS) Analysis**

**All Analyses:** The MS met QC acceptance criteria except as follows:

**ICP-AES-Metals Batch # 204455 (Sample 67169-010)**

The sample used for the MS was of similar matrix from another SNL SDG. No data will be qualified as a result.

**CVAH-Hg Batch # 204420 (Sample 67169-010)**

The sample used for the MS was of similar matrix from another SNL SDG. No data will be qualified as a result.

**Total Cyanide - Batch #202747 (Samples 67169-008)**

The sample used for the MS was of similar matrix from another SNL SDG. No data will be qualified as a result.

### **Replicate Analysis**

**All Analyses:** The replicate analysis met QC acceptance criteria except as mentioned above in the summary section and as follows:

**ICP-AES-Metals Batch # 204455 (Sample 67169-010)**

The sample used for the replicate was of similar matrix from another SNL SDG. No data will be qualified as a result.

**CVAH-Hg Batch # 204420 (Sample 67169-010)**

The sample used for the replicate was of similar matrix from another SNL SDG. No data will be qualified as a result.

**Total Cyanide - Batch #202747 (Samples 67169-008)**

The sample used for the replicate was of similar matrix from another SNL SDG. No data will be qualified as a result.

### **ICP Interference Check Sample (ICS)**

**ICP-AES (All batches):** The ICS-AB met QC acceptance criteria.

**All Other Analyses:** No ICS required.

### **ICP Serial Dilution**

**ICP-AES (All batches):** The serial dilution met QC acceptance criteria.

**ICP-AES-Metals Batch # 204455 (Sample 67169-010)**

The sample used for the serial dilution was of similar matrix from another SNL SDG.  
No data will be qualified as a result.

All Other Analyses: No serial dilutions required.

**Detection Limits/Dilutions**

All Analyses: All detection limits were properly reported.

ICP-AES: All soil samples were diluted 2X.

All Other Analyses: No dilutions were performed.

**Other QC**

All Analyses: An equipment blank and a field duplicate was submitted on the ARCOC. There are no "required" validation procedures for assessing a field duplicate.  
No field blank was submitted on the ARCOC.

It should be noted that the COC requested that metals be analyzed by method SW-846 6020.

No raw data was submitted with the package.

No other specific issues were identified which affect data quality.

---

Analytical Quality Associates, Inc.



616 Maxine NE  
Albuquerque, NM 87123  
Phone: 505-299-5201  
Fax: 505-299-6744  
Email: minteer@aol.com

**MEMORANDUM**

DATE: 11/19/02  
TO: File  
FROM: Linda Thal  
SUBJECT: Organic Data Review and Validation - SNL  
Site: DSS soil sampling  
ARCOC # 605671, -72, -73 GEL SDG # 67158 and 67169  
Project/Task No. 7223.02.03.02

See the attached Data Validation Worksheets for supporting documentation on the data review and validation. Data are evaluated using SNL/NM ER Project AOP 00-03.

**Summary**

The samples were prepared and analyzed with approved procedures using methods SW-846 8260A/B (VOC), 8270C (SVOC), 8082 (PCBs) and 8330 (HEs). Problems were identified with the data package that resulted in the qualification of data.

**VOC Batch # 202140 and 203595**

Trichloroethene had a RF (0.21/0.23) < than the specified minimum (0.30) but > 0.01. All associated sample results were non-detect and will be qualified "UJ".

**SVOC - Batch 201961 (Sample 67158-020 through 038)**

Pyrene had a correlation coefficient < 0.99. All associated sample results were non-detect and will not be qualified, with the exception of samples 67158-021, and 034 through 037. These sample results will be qualified "J".

Bis(2-ethylhexyl)phthalate was detected in the method blank (MB) and the equipment blank (EB) at a value > DL but < RL. Sample 67158-021 through 038 had bis(2-ethylhexyl)phthalate values > DL, < RL and <10X the MB value and will be qualified "U, B" at the RL. Sample 67158-020 had a bis(2-ethylhexyl)phthalate value > RL but <10X MB value and will be qualified "U, B" at the reported value.

**PCB Batch # 202231**

No MS/MSD, LCS/LCSD or replicate was performed for sample 67169-008(EB). As there is no measure of precision for the sample, all results will be qualified "P2".

**HE - Batch # 202056 (Sample 67158-020 through -038)**

The MS %R (58%) and RPD (44%) failed QC acceptance criteria (71-120%/<20%) for 4-amino-2,6-dinitrotoluene. All associated sample results were non-detect and will be qualified "UJ, A2, P1".

The MS/MSD %R (32/18%) and RPD (58%) failed QC acceptance criteria (65-135%/<30%) for tetryl. All associated sample results were non-detect and will be qualified "UJ, A2, P1".

Data are acceptable and QC measures appear to be adequate. The following sections discuss the data review and validation.

### **Holding Times/Preservation**

**All Analysis:** The samples were properly preserved and analyzed within the method prescribed holding time.

### **Calibration**

**All Analysis:** All initial and continuing calibration acceptance criteria were met except as mentioned above in the summary section and as follows:

#### **VOC Batch # 203595**

Chloroethane had %D > 20% but < 40% (23%). All associated sample results were non-detect and no data will be qualified.

#### **SVOC – Batch 201961 and 201951**

The CCVs preceding the samples had a %D > 20% but < 40% for several compounds (see DV worksheet). All associated sample results were non-detect and no data will be qualified.

### **Blanks**

**All Analysis:** All method blank, equipment blank and trip blank acceptance criteria were met except as mentioned above in the summary section and as follows:

#### **VOC Batch # 202140**

Sample 67169-004 (trip blank) had a toluene value > DL but < RL. All associated samples (67158-013 through -019) were non-detect for toluene and no data will be qualified.

#### **PCB Batch # 201940**

Aroclor 1260 was detected in the EB at a value > DL but < RL. All associated sample results were either non-detect or > 5X EB value; no data will be qualified.

### **Surrogates**

**All Analysis:** All surrogate acceptance criteria were met.

### **Internal Standards (ISs)**

**All Analysis:** All internal standard acceptance criteria were met.

### **Matrix Spike/Matrix Spike Duplicate (MS/MSD) Analysis**

**All Analysis:** All MS/MSD acceptance criteria were met except as mentioned above in the summary section and as follows:

#### **VOC Batch # 203595**

The PS/PSD was run on a sample of similar matrix from another SNL SDG. No data will be qualified as a result.

---

**SVOC – Batch 201961 and 201951**

Several compounds (see DV worksheet) had %R < QC acceptance criteria (75 – 125%). Using professional judgment, no data will be qualified.

**SVOC – Batch 201951**

It should be noted that only 500ml (DF=2x) of sample was used for the MS/MSD. It is not known what affect this would have on the extraction procedure and no data will be qualified.

**HE - Batch 202049**

No MS/MSD was extracted with this batch. An LCS/LCSD was extracted and met all QC acceptance criteria for accuracy and precision. No data will be qualified.

**Laboratory Control Samples (LCS/LCSD) Analysis**

**All Analysis:** The LCS/LCSD acceptance criteria were met.

**VOC Batch # 202140 and 203595**

It should be noted that no compound was associated with internal standard 1,4-dichlorobenzene-d4. No data will be qualified as a result.

**SVOC – Batch 201961 and 201951**

It should be noted that no compound was associated with internal standard perylene-d12. No data will be qualified as a result.

**Detection Limits/Dilutions**

**All Analysis:** All detection limits were properly reported. Samples were not diluted.

**Confirmation Analyses**

**VOC and SVOC:** No confirmation analyses required.

**PCB:** All confirmation acceptance criteria were met.

**HE:** The sample results were non-detect and therefore no confirmation analysis was required.

**Other QC**

**VOC:** A trip blank, equipment blank and a field dup were submitted on the ARCOG. There are no "required" criteria for assessing a field dup. It should be noted that vinyl acetate is on the TAL for soils but not for waters.

**SVOC, PCB and HE:** An equipment blank and a field dup were submitted on the ARCOG. There are no "required" criteria for assessing a field dup. No field blank was submitted on the ARCOG.

No raw data was submitted with the package.

No other specific issues were identified which affect data quality.

Analytical Quality Associates, Inc.



616 Maxine NE  
Albuquerque, NM 87123  
Phone: 505-299-5201  
Fax: 505-299-6744  
Email: minteer@aol.com

**MEMORANDUM**

DATE: November 19, 2002  
TO: File  
FROM: Linda Thal  
SUBJECT: Radiochemical Data Review and Validation - SNL  
Site: DSS soil sampling  
ARCOC 605671, -72, -73  
GEL SDG # 67158 and 67169 Project/Task No. 7223.02.03.02

See the attached Data Validation Worksheets for supporting documentation on the data review and validation. This validation was performed according to SNL/NM ER Project AOP 00-03.

**Summary**

All samples were prepared and analyzed with approved procedures using method EPA 900.0 (Gross Alpha/Beta). No problems were identified with the data package that resulted in the qualification of data.

Data are acceptable and QC measures appear to be adequate. The following sections discuss the data review and validation.

**Holding Times/Preservation**

All Analyses: All samples were analyzed within the prescribed holding times and properly preserved.

**Calibration**

All Analyses: The case narrative stated the instruments used were properly calibrated.

**Blanks**

No target analytes were detected in the method blank or equipment blank at concentrations > the associated MDAs.

**Matrix Spike (MS) Analysis**

The MS analyses met all QC acceptance criteria.



**Laboratory Control Sample (LCS) Analysis**

The LCS analyses met all QC acceptance criteria.

**Replicates**

The replicate analyses met all QC acceptance criteria.

**Tracer/Carrier Recoveries**

No tracer/carrier required.

**Negative Bias**

All sample results met negative bias QC acceptance criteria.

**Detection Limits/Dilutions**

All detection limits were properly reported. No samples were diluted.

**Other QC**

An equipment blank and a field duplicate were submitted on the ARCOC. There are however, no "required" data validation procedures for assessing a field duplicate. No field blank was submitted on the ARCOC.

No raw data was submitted with the package.

No other specific issues were identified which affect data quality.

---

Contract Verification Review (CVR)

Project Leader Collins      Project Name DSS Soil Sampling      Case No. 7223\_02.03.02  
 AR/COC No. 605671, 605672, 605673      Analytical Lab GEL      SDG No. 67158A, B, C

In the tables below, mark any information that is missing or incorrect and give an explanation.

Line No.	Item	Complete?		If no, explain	Resolved?	
		Yes	No		Yes	No
1.0 Analysis Request and Chain of Custody Record and Log-In Information						
1.1	All items on COC complete - data entry clerk initiated and dated	X				
1.2	Container type(s) correct for analyses requested	X				
1.3	Sample volume adequate for # and types of analyses requested	X				
1.4	Preservative correct for analyses requested	X				
1.5	Custody records continuous and complete	X				
1.6	Lab sample number(s) provided and SNL sample number(s) cross referenced and correct	X				
1.7	Date samples received	X				
1.8	Condition upon receipt information provided	X				

2.0 Analytical Laboratory Report						
Line No.	Item	Complete?		If no, explain	Resolved?	
		Yes	No		Yes	No
2.1	Data reviewed, signature	X				
2.2	Method reference number(s) complete and correct	X				
2.3	QC analysis and acceptance limits provided (MB, LCS, Replicate)	X				
2.4	Matrix spike/matrix spike duplicate data provided (if requested)	X				
2.5	Detection limits provided; PQL and MDL (or IDL), MDA and L <sub>s</sub>	X				
2.6	QC batch numbers provided	X				
2.7	Dilution factors provided and all dilution levels reported	X				
2.8	Data reported in appropriate units and using correct significant figures	X				
2.9	Radiochemistry analysis uncertainty (2 sigma error) and tracer recovery (if applicable) reported	X				
2.10	Narrative provided	X				
2.11	TAT met					
2.12	Hold times met	X				
2.13	Contractual qualifiers provided	X				
2.14	All requested result and TIC (if requested) data provided	X				

Contract Verification Review (Continued)

3.0 Data Quality Evaluation


Item	Yes	No	If no, Sample ID No., Fraction(s) and Analysis
3.1 Are reporting units appropriate for the matrix and meet contract specified or project-specific requirements? Inorganics and metals reported as ppm (mg/liter or mg/Kg)? Tritium reported in picocuries per liter with percent moisture for soil samples? Units consistent between QC samples and sample data	X		
3.2 Quantitation limit met for all samples	X		
3.3 Accuracy	X		
a) Laboratory control samples accuracy reported and met for all samples	X		
b) Surrogate data reported and met for all organic samples analyzed by a gas chromatography technique	X		
c) Matrix spike recovery data reported and met		X	Several HPLC MS recoveries not within acceptance limits
3.4 Precision		X	Arsenic not within acceptable limits
a) Replicate sample precision reported and met for all inorganic and radiochemistry samples		X	HPLC RPD not within acceptance limits; HPLC MS/MSD not performed due to limited sample.
b) Matrix spike duplicate RPD data reported and met for all organic samples		X	bis(2-Ethylhexyl)phthalate detected in SVOC method blank; selenium and chromium detected in inorganic method blank; cyanide detected in method blank
3.5 Blank data		X	Toluene detected in trip blank; bis(2-Ethylhexyl)phthalate detected in SVOC method blank; Aroclor 1280 detected in PCB equipment blank; barium and chromium detected in RCRA equipment blank
a) Method or reagent blank data reported and met for all samples		X	
b) Sampling blank (e.g., field, trip, and equipment) data reported and met		X	
3.6 Contractual qualifiers provided: "J"-estimated quantity; "B"-analyte found in method blank above the MDL for organic or above the PQL for inorganic; "U"-analyte undetected (results are below the MDL, IDL, or MDA (radiochemicals)); "H"-analysis done beyond the holding time	X		
3.7 Narrative addresses planchet flaring for gross alpha/beta	X		
3.8 Narrative included, correct, and complete	X		
3.9 Second column confirmation data provided for methods 8330 (high explosives) and 8082 (pesticides/PCBs)	X		

Contract Verification Review (Continued)

4.0 Calibration and Validation Documentation

Item	Yes	No	Comments
4.1 GC/MS (8260, 8270, etc.)			
a) 12-hour tune check provided	X		
b) Initial calibration provided	X		
c) Continuing calibration provided	X		
d) Internal standard performance data provided	X		
e) Instrument run logs provided	X		
4.2 GC/HPLC (8330 and 8010 and 8082)			
a) Initial calibration provided	X		
b) Continuing calibration provided	X		
c) Instrument run logs provided	X		
4.3 Inorganics (metals)			
a) Initial calibration provided	X		
b) Continuing calibration provided	X		
c) ICP interference check sample data provided	X		
d) ICP serial dilution provided	X		
e) Instrument run logs provided	X		
4.4 Radiochemistry			
a) Instrument run logs provided	X		



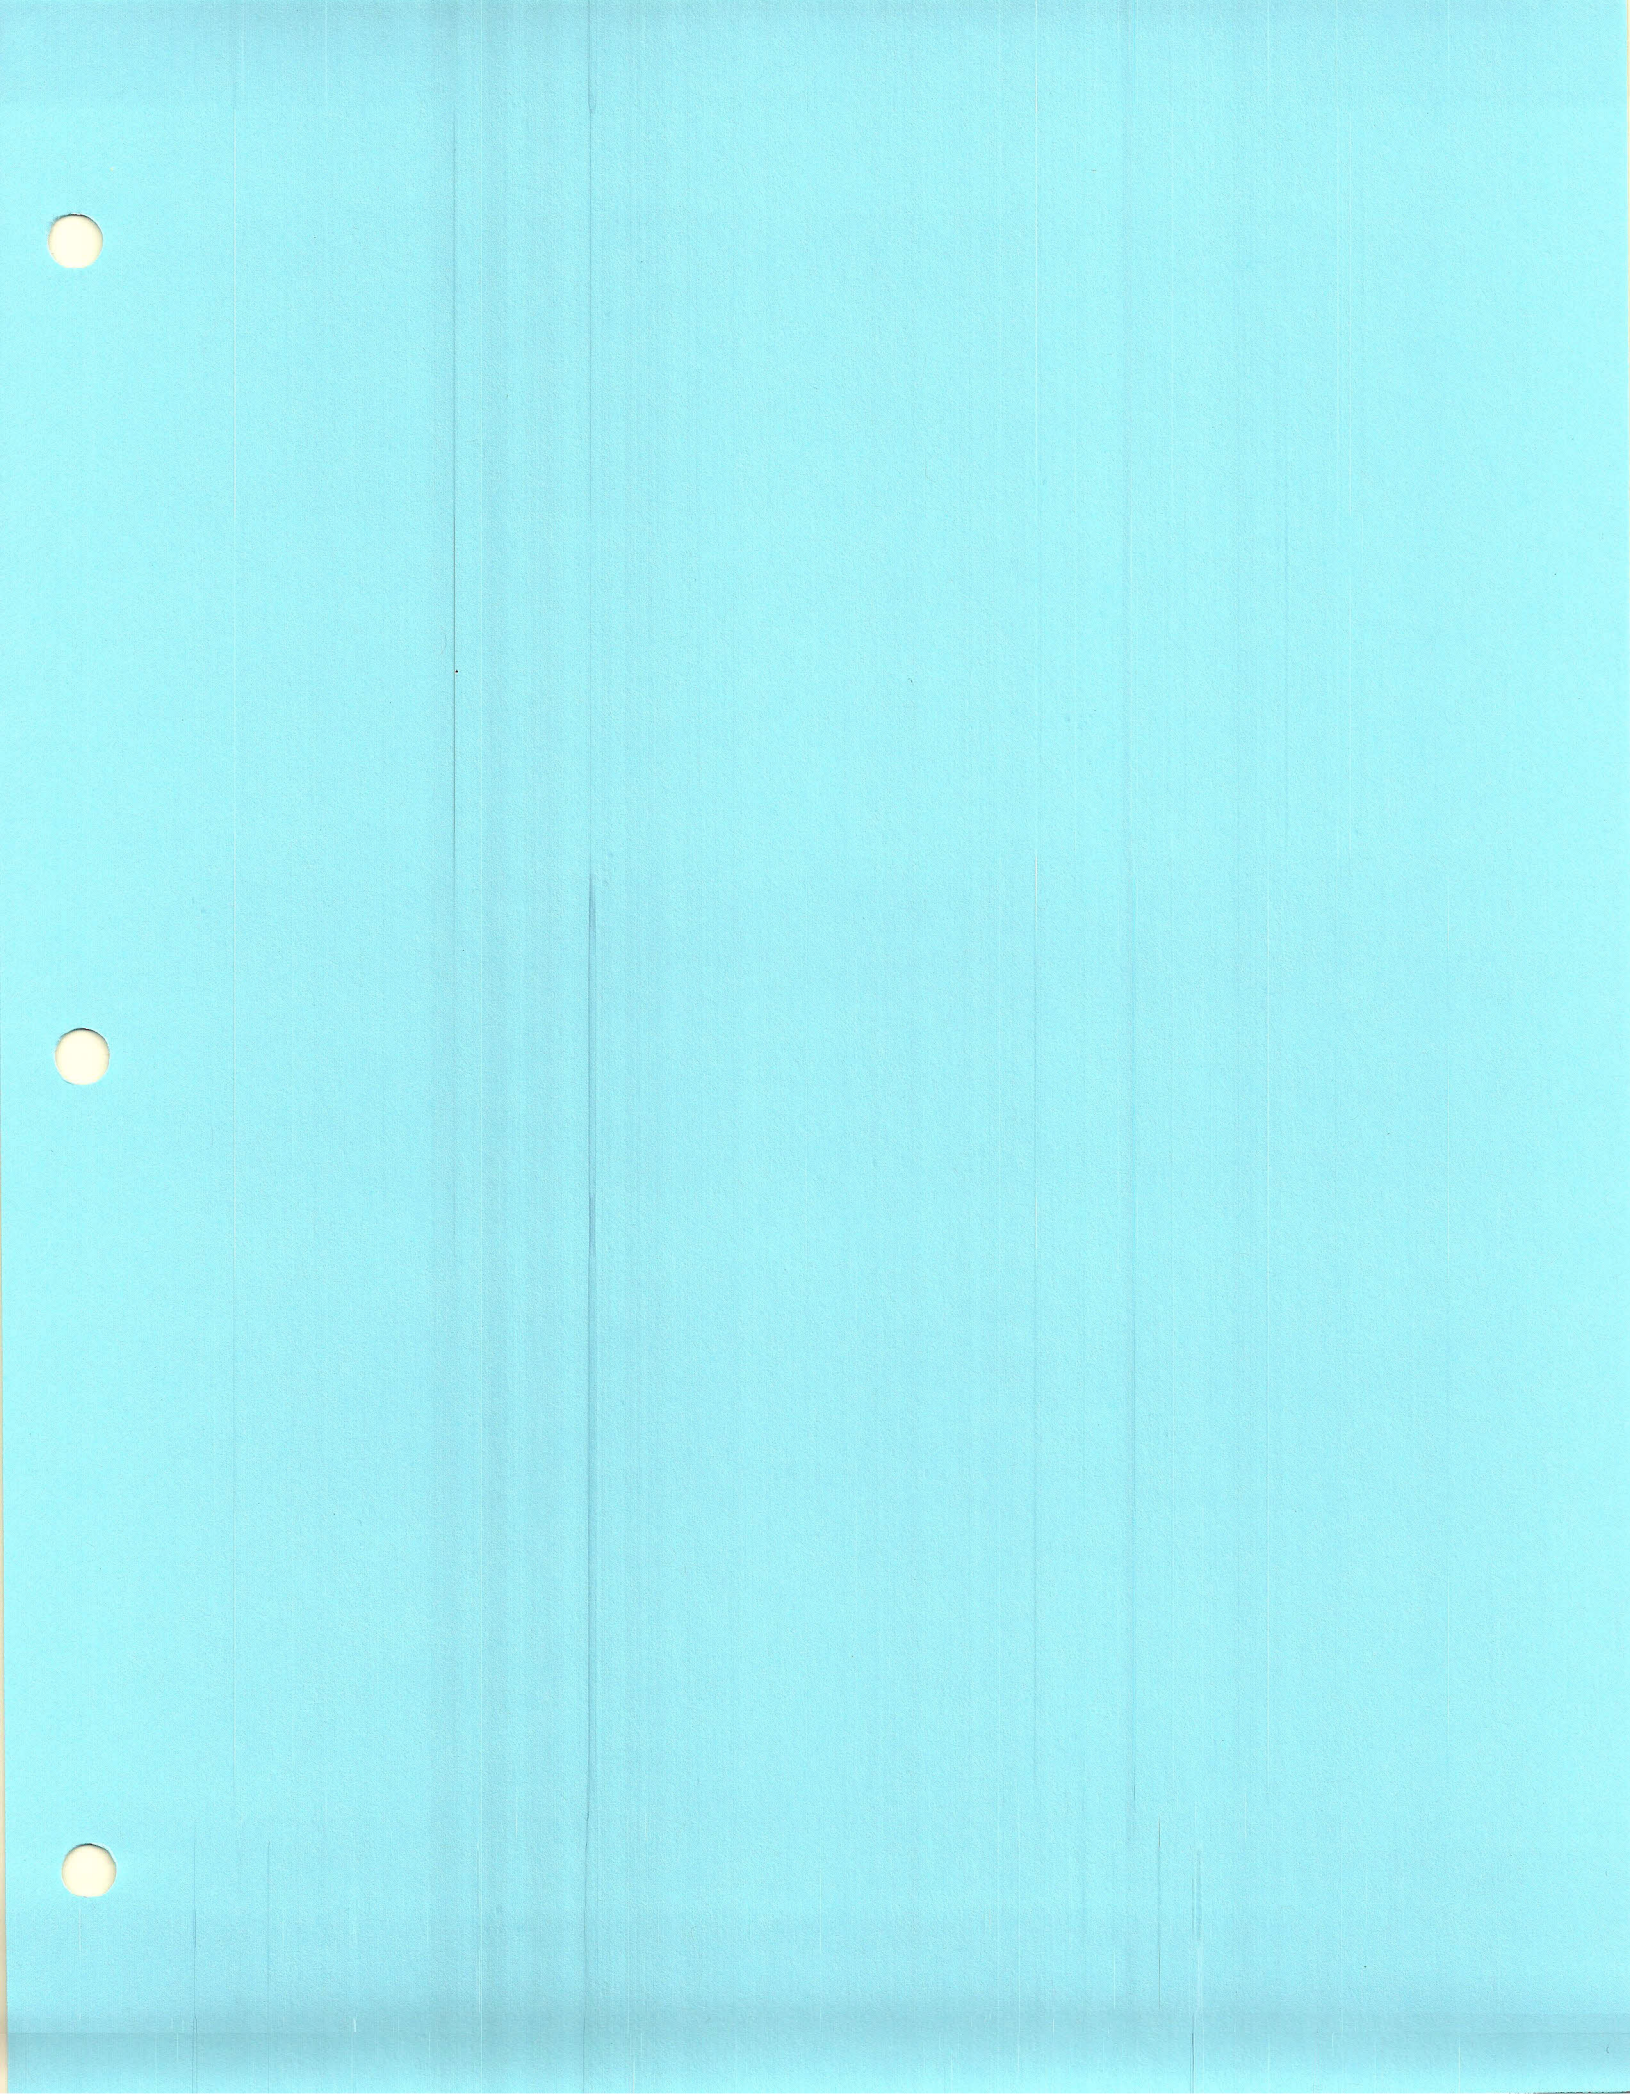

**ANNEX D  
DSS Site 1035  
Risk Assessment**

## TABLE OF CONTENTS

I.	Site Description and History .....	D-1
II.	Data Quality Objectives.....	D-1
III.	Determination of Nature, Rate, and Extent of Contamination .....	D-5
III.1	Introduction .....	D-5
III.2	Nature of Contamination .....	D-5
III.3	Rate of Contaminant Migration .....	D-5
III.4	Extent of Contamination.....	D-6
IV.	Comparison of COCs to Background Levels .....	D-6
V.	Fate and Transport.....	D-6
VI.	Human Health Risk Assessment.....	D-10
VI.1	Introduction .....	D-10
VI.2	Step 1. Site Data.....	D-10
VI.3	Step 2. Pathway Identification.....	D-10
VI.4	Step 3. Background Screening Procedure.....	D-11
VI.4.1	Methodology .....	D-11
VI.4.2	Results .....	D-11
VI.5	Step 4. Identification of Toxicological Parameters .....	D-15
VI.6	Step 5. Exposure Assessment and Risk Characterization.....	D-15
VI.6.1	Exposure Assessment .....	D-15
VI.6.2	Risk Characterization .....	D-17
VI.7	Step 6. Comparison of Risk Values to Numerical Guidelines .....	D-19
VI.8	Step 7. Uncertainty Discussion .....	D-20
VI.9	Summary.....	D-21
VII.	Ecological Risk Assessment .....	D-22
VII.1	Introduction .....	D-22
VII.2	Scoping Assessment .....	D-22
VII.2.1	Data Assessment.....	D-23
VII.2.2	Bioaccumulation .....	D-23
VII.2.3	Fate and Transport Potential .....	D-23
VII.2.4	Scoping Risk-Management Decision .....	D-23
VIII.	References.....	D-23
	Appendix 1 .....	D-29



**This page intentionally left blank.**

**LIST OF TABLES**

<b>Table</b>	<b>Page</b>
1	Summary of Sampling Performed to Meet DQOs ..... D-2
2	Number of Confirmatory Soil and QA/QC Samples Collected from DSS Site 1035 ..... D-3
3	Summary of Data Quality Requirements for DSS Site 1035 ..... D-4
4	Nonradiological COCs for Human Health Risk Assessment at DSS Site 1035 with Comparison to the Associated SNL/NM Background Screening Value, BCF, and Log $K_{ow}$ ..... D-7
5	Radiological COCs for Human Health Risk Assessment at DSS Site 1035 with Comparison to the Associated SNL/NM Background Screening Value and BCF ..... D-8
6	Summary of Fate and Transport at DSS Site 1035 ..... D-9
7	Toxicological Parameter Values for DSS Site 1035 Nonradiological COCs.... D-16
8	Radiological Toxicological Parameter Values for DSS Site 1035 COCs Obtained from RESRAD Risk Coefficients ..... D-17
9	Risk Assessment Values for DSS Site 1035 Nonradiological COCs..... D-18
10	Risk Assessment Values for DSS Site 1035 Nonradiological Background Constituents ..... D-18
11	Summation of Incremental Radiological and Nonradiological Risks from DSS Site 1035, Building 6715 Septic System Carcinogens ..... D-22

**LIST OF FIGURES**

<b>Figure</b>	<b>Page</b>
1	Conceptual Site Model Flow Diagram for DSS Site 1035, Building 6715 Septic System ..... D-13

**This page intentionally left blank.**

## **DSS SITE 1035: RISK ASSESSMENT REPORT**

### **I. Site Description and History**

Drain and Septic Systems (DSS) Site 1035, the Building 6715 Septic System, at Sandia National Laboratories/New Mexico (SNL/NM), is located in Technical Area (TA)-III on federally owned land controlled by Kirtland Air Force Base (KAFB) and permitted to the U.S. Department of Energy (DOE). The abandoned septic system consisted of a 750-gallon septic tank connected to a single seepage pit. Available information indicates that Building 6715 was constructed in 1962 (SNL/NM March 2003), and it is assumed that the septic system was also constructed at that time. In the early 1990s, the septic system discharges were routed to the City of Albuquerque sanitary sewer system (Jones June 1991). The old septic system line was disconnected and capped, and the system was abandoned in place concurrent with this change (Romero September 2003).

Environmental concern about DSS Site 1035 is based upon the potential for the release of constituents of concern (COCs) in effluent discharged to the environment via the septic system at this site. Because operational records were not available, the investigation was planned to be consistent with other DSS site investigations and to sample for possible COCs that may have been released during facility operations.

The ground surface in the vicinity of the site is flat or slopes slightly to the west. The closest major drainage is the Arroyo del Coyote, located approximately 1.1 miles northeast of the site. No springs or perennial surface-water bodies are located within 2 miles of the site. Average annual rainfall in the SNL/NM and KAFB area, as measured at Albuquerque International Sunport, is 8.1 inches (NOAA 1990). Surface-water runoff in the vicinity of the site is minor because the surface is flat or slopes gently to the west. Infiltration of precipitation is almost nonexistent as virtually all of the moisture subsequently undergoes evapotranspiration. The estimates of evapotranspiration for the KAFB area range from 95 to 99 percent of the annual rainfall (SNL/NM March 1996). Most of the area immediately surrounding DSS Site 1035 is unpaved with some native vegetation, and no storm sewers are used to direct surface water away from the site.

DSS Site 1035 lies at an average elevation of approximately 5,390 feet above mean sea level (SNL/NM April 2003). The groundwater beneath the site occurs in unconfined conditions in essentially unconsolidated silts, sands, and gravels. The depth to groundwater is approximately 470 feet below ground surface (bgs). Groundwater flow is thought to be to the west in this area (SNL/NM March 2002). The nearest groundwater monitoring well is TAV-MW5 located approximately 1,000 feet northeast of the site. The nearest production wells are northwest and northeast of the site and include KAFB-4 and KAFB-11, which are approximately 2.7 and 3.2 miles away, respectively.

### **II. Data Quality Objectives**

The Data Quality Objectives (DQOs) presented in the "Sampling and Analysis Plan [SAP] for Characterizing and Assessing Potential Releases to the Environment From Septic and Other Miscellaneous Drain Systems at Sandia National Laboratories/New Mexico" (SNL/NM October 1999) and "Field Implementation Plan [FIP], Characterization of Non-Environmental Restoration

Drain and Septic Systems" (SNL/NM November 2001), identified the site-specific sample locations, sample depths, sampling procedures, and analytical requirements for this and many other DSS sites. The DQOs outlined the quality assurance (QA)/quality control (QC) requirements necessary for producing defensible analytical data suitable for risk assessment purposes. The sampling conducted at this site was designed to:

- Determine whether hazardous waste or hazardous constituents were released at the site.
- Characterize the nature and extent of any releases.
- Provide analytical data of sufficient quality to support risk assessments.

Table 1 summarizes the rationale for determining the sampling locations at this site. The source of potential COCs at DSS Site 1035 was effluent discharged to the environment from the septic system seepage pit at the site.

**Table 1**  
**Summary of Sampling Performed to Meet DQOs**

<b>DSS Site 1035 Sampling Area</b>	<b>Potential COC Source</b>	<b>Number of Sampling Locations</b>	<b>Sample Density (samples/acre)</b>	<b>Sampling Location Rationale</b>
Soil beneath the septic system seepage pit	Effluent discharged to the environment from the septic system seepage pit	1	NA	Evaluate potential COC releases to the environment from effluent discharged from the septic system seepage pit

COC = Constituent of concern.  
DQO = Data Quality Objective.  
DSS = Drain and Septic Systems.  
NA = Not applicable.

The soil samples were collected at one location at DSS Site 1035 with a Geoprobe™ from two 3- or 4-foot-long sampling intervals in the single boring. The sampling intervals started at 11 and 16 feet bgs in the seepage pit borehole. The soil samples were collected in accordance with the procedures described in the SAP (SNL/NM October 1999) and FIP (SNL/NM November 2001). Table 2 summarizes the types of confirmatory and QA/QC samples collected at the site and the laboratories that performed the analyses.

The soil samples were analyzed for volatile organic compounds (VOCs), semivolatile organic compounds (SVOCs), high explosive (HE) compounds, polychlorinated biphenyls (PCBs), Resource Conservation and Recovery Act (RCRA) metals, hexavalent chromium, cyanide, radionuclides, and gross alpha/beta activity. The samples were analyzed by an off-site laboratory (General Engineering Laboratories, Inc.) and the on-site SNL/NM Radiation

Table 2  
Number of Confirmatory Soil and QA/QC Samples Collected from DSS Site 1035

Sample Type	VOCs	SVOCs	PCBs	HE	RCRA Metals	Hexavalent Chromium	Cyanide	Gamma Spectroscopy Radionuclides	Gross Alpha/Beta Activity
Confirmatory	2	2	2	2	2	2	2	2	2
Duplicates	0	0	0	0	0	0	0	0	0
EBs and TBs <sup>a</sup>	1	0	0	0	0	0	0	0	0
Total Samples	3	2	2	2	2	2	2	2	2
Analytical Laboratory	GEL	GEL	GEL	GEL	GEL	GEL	GEL	RPSD	GEL

<sup>a</sup>TBs for VOCs only.

DSS = Drain and Septic Systems.

EB = Equipment blank.

GEL = General Engineering Laboratories, Inc.

HE = High explosive(s).

PCB = Polychlorinated biphenyl.

QA/QC = Quality assurance/quality control.

RCRA = Resource Conservation and Recovery Act.

RPSD = Radiation Protection Sample Diagnostics Laboratory.

SVOC = Semivolatle organic compound.

TB = Trip blank.

VOC = Volatile organic compound.

Protection Sample Diagnostics (RPSD) Laboratory. Table 3 summarizes the analytical methods and the data quality requirements from the SAP (SNL/NM October 1999) and FIP (SNL/NM November 2001).

**Table 3**  
**Summary of Data Quality Requirements for DSS Site 1035**

Analytical Method <sup>a</sup>	Data Quality Level	GEL	RPSD
VOCs EPA Method 8260	Defensible	2	None
SVOCs EPA Method 8270	Defensible	2	None
PCBs EPA Method 8082	Defensible	2	None
HE Compounds EPA Method 8330	Defensible	2	None
RCRA Metals EPA Method 6000/7000	Defensible	2	None
Hexavalent Chromium EPA Method 7196A	Defensible	2	None
Total Cyanide EPA Method 9012A	Defensible	2	None
Gamma Spectroscopy Radionuclides EPA Method 901.1	Defensible	None	2
Gross Alpha/Beta Activity EPA Method 900.0	Defensible	2	None

Note: The number of samples does not include QA/QC samples such as duplicates, trip blanks, and equipment blanks.

<sup>a</sup>EPA November 1986.

DSS = Drain and Septic Systems.

EPA = U.S. Environmental Protection Agency.

GEL = General Engineering Laboratories, Inc.

HE = High explosive(s).

PCB = Polychlorinated biphenyl.

QA/QC = Quality assurance/quality control.

RCRA = Resource Conservation and Recovery Act.

RPSD = Radiation Protection Sample Diagnostics Laboratory.

SVOC = Semivolatile organic compound.

VOC = Volatile organic compound.

The QA/QC samples were collected during the sampling effort according to the Environmental Restoration (ER) Project Quality Assurance Project Plan. The QA/QC samples consisted of one trip blank (for VOCs only). No significant QA/QC problems were identified in the QA/QC samples.

All of the soil sample results were verified/validated by SNL/NM according to "Verification and Validation of Chemical and Radiochemical Data," Technical Operating Procedure (TOP) 94-03, Rev. 0 (SNL/NM July 1994) or SNL/NM ER Project "Data Validation Procedure for Chemical and Radiochemical Data," Administrative Operating Procedure (AOP) 00-03 (SNL/NM

December 1999). The data validation reports are presented in the associated DSS Site 1035 request for a determination of Corrective Action Complete (CAC) without controls. The gamma spectroscopy data from the RPSD Laboratory were reviewed according to "Laboratory Data Review Guidelines," Procedure No. RPSD-02-11, Issue No. 2 (SNL/NM July 1996). The gamma spectroscopy results are presented in the CAC proposal. The reviews confirmed that the analytical data are defensible and therefore acceptable for use in the request for a determination of CAC without controls. Therefore, the DQOs have been fulfilled.

### **III. Determination of Nature, Rate, and Extent of Contamination**

#### **III.1 Introduction**

The determination of the nature, migration rate, and extent of contamination at DSS Site 1035 is based upon an initial conceptual model validated with confirmatory sampling at the site. The initial conceptual model was developed from archival site research, site inspections, soil sampling, and passive soil-vapor sampling. The DQOs contained in the SAP (SNL/NM October 1999) and FIP (SNL/NM November 2001) identified the sample locations, sample density, sample depth, and analytical requirements. The sample data were subsequently used to develop the final conceptual site model for DSS Site 1035, which is presented in Section 4.0 of the associated request for a determination of CAC without controls. The quality of the data specifically used to determine the nature, migration rate, and extent of contamination is described in the following sections.

#### **III.2 Nature of Contamination**

Both the nature of contamination and the potential for the degradation of COCs at DSS Site 1035 were evaluated using laboratory analyses of the soil samples. The analytical requirements included analyses for VOCs, SVOCs, HE compounds, PCBs, RCRA metals, hexavalent chromium, cyanide, radionuclides by gamma spectroscopy, and gross alpha/beta activity. The analytes and methods listed in Tables 2 and 3 are appropriate to characterize the COCs and potential degradation products at DSS Site 1035.

#### **III.3 Rate of Contaminant Migration**

The septic system at DSS Site 1035 was deactivated in the early 1990s when Building 6715 was connected to an extension of the City of Albuquerque sanitary sewer system. The migration rate of COCs that may have been introduced into the subsurface via the septic system at this site was therefore dependent upon the volume of aqueous effluent discharged to the environment from this system when it was operational. Any migration of COCs from this site after use of the septic system was discontinued has been predominantly dependent upon precipitation. However, it is highly unlikely that sufficient precipitation has fallen on the site to reach the depth at which COCs may have been discharged to the subsurface from this system. Analytical data generated from the soil sampling conducted at the site are adequate to characterize the rate of COC migration at DSS Site 1035.



#### III.4 Extent of Contamination

Subsurface soil samples were collected from one borehole drilled beneath the seepage pit at the site to assess whether releases of effluent from the septic system caused any environmental contamination.

The soil samples were collected at sampling depths starting at 11 and 16 feet bgs beneath the seepage pit. Sampling intervals started at the depths at which effluent discharged from the seepage pit would have entered the subsurface environment at the site. This sampling procedure was required by New Mexico Environment Department (NMED) regulators and has been used at numerous DSS-type sites at SNL/NM. The soil samples are considered to be representative of the soil potentially contaminated with the COCs at this site and are sufficient to determine the vertical extent, if any, of COCs.

#### IV. Comparison of COCs to Background Levels

Site history and characterization activities are used to identify potential COCs. The DSS Site 1035 request for a determination of CAC without controls describes the identification of COCs and the sampling that was conducted in order to determine the concentration levels of those COCs across the site. Generally, COCs evaluated in this risk assessment include all detected organic and all inorganic and radiological COCs for which samples were analyzed. When the detection limit of an organic compound is too high (i.e., could possibly cause an adverse effect to human health or the environment), the compound is retained. Nondetected organic compounds not included in this assessment were determined to have detection limits low enough to ensure protection of human health and the environment. In order to provide conservatism in this risk assessment, the calculation uses only the maximum concentration value of each COC found for the entire site. The SNL/NM maximum background concentration (Dinwiddie September 1997) was selected to provide the background screen listed in Tables 4 and 5.

Nonradiological inorganic constituents that are essential nutrients, such as iron, magnesium, calcium, potassium, and sodium, are not included in this risk assessment (EPA 1989). Both radiological and nonradiological COCs are evaluated. The nonradiological COCs included in this risk assessment consist of both inorganic and organic compounds.

Table 4 lists the nonradiological COCs and Table 5 lists the radiological COCs for the human health risk assessment at DSS Site 1035. All samples were collected from depths greater than 5 feet bgs; therefore, evaluation of ecological risk was not performed. Both tables show the associated SNL/NM maximum background concentration values (Dinwiddie September 1997). Section VI.4 discusses the results presented in Tables 4 and 5.

#### V. Fate and Transport

The primary releases of COCs at DSS Site 1035 were to the subsurface soil resulting from the discharge of effluents from the Building 6715 septic system. Wind, water, and biota are natural mechanisms of COC transport from the primary release point; however, because the

**Table 4**  
**Nonradiological COCs for Human Health Risk Assessment at DSS Site 1035 with**  
**Comparison to the Associated SNL/NM Background Screening Value, BCF, and Log K<sub>ow</sub>**

COC	Maximum Concentration (All Samples) (mg/kg)	SNL/NM Background Concentration (mg/kg) <sup>a</sup>	Is Maximum COC Concentration Less Than or Equal to the Applicable SNL/NM Background Screening Value?	BCF (maximum aquatic)	Log K <sub>ow</sub> (for organic COCs)	Bioaccumulator? <sup>b</sup> (BCF>40, Log K <sub>ow</sub> >4)
<b>Inorganic</b>						
Arsenic	3.91 J	4.4	Yes	44 <sup>c</sup>	–	<b>Yes</b>
Barium	232	214	<b>No</b>	170 <sup>d</sup>	–	<b>Yes</b>
Cadmium	0.213 J	0.9	Yes	64 <sup>c</sup>	–	<b>Yes</b>
Chromium, total	11.2	15.9	Yes	16 <sup>c</sup>	–	No
Chromium VI	0.0261 <sup>e</sup>	1	Yes	16 <sup>c</sup>	–	No
Cyanide	0.0462 J	NC	<b>Unknown</b>	NC	–	<b>Unknown</b>
Lead	6.26	11.8	Yes	49 <sup>c</sup>	–	<b>Yes</b>
Mercury	0.0061 J	<0.1	Yes	5,500 <sup>c</sup>	–	<b>Yes</b>
Selenium	0.351 J	<1	Yes	800 <sup>f</sup>	–	<b>Yes</b>
Silver	0.0451 <sup>e</sup>	<1	Yes	0.5 <sup>c</sup>	–	No
<b>Organic</b>						
Acetone	0.00417 J	NA	<b>NA</b>	0.69 <sup>g</sup>	-0.24 <sup>g</sup>	No
2-Butanone	0.00674	NA	<b>NA</b>	1 <sup>g</sup>	0.29 <sup>g</sup>	No
bis(2-Ethylhexyl) phthalate	0.142 J	NA	<b>NA</b>	851 <sup>h</sup>	7.6 <sup>i</sup>	<b>Yes</b>

Note: **Bold** indicates the COCs that exceed the background screening values and/or are bioaccumulators.

<sup>a</sup>Dinwiddie September 1997, Southwest Area Supergroup.

<sup>b</sup>NMED March 1998.

<sup>c</sup>Yanicak March 1997.

<sup>d</sup>Neumann 1976.

<sup>e</sup>Parameter was not detected. Concentration listed is one-half the maximum detection limit.

<sup>f</sup>Callahan et al. 1979.

<sup>g</sup>Howard 1990.

<sup>h</sup>Howard 1989.

<sup>i</sup>Micromedex, Inc. 1998.

BCF = Bioconcentration factor.

COC = Constituent of concern.

DSS = Drain and Septic Systems.

J = Estimated concentration.

K<sub>ow</sub> = Octanol-water partition coefficient.

Log = Logarithm (base 10).

mg/kg = Milligram(s) per kilogram.

NA = Not applicable.

NC = Not calculated.

NMED = New Mexico Environment Department.

SNL/NM = Sandia National Laboratories/New Mexico.

– = Information not available.

**Table 5**  
**Radiological COCs for Human Health Risk Assessment at DSS Site 1035 with**  
**Comparison to the Associated SNL/NM Background Screening Value and BCF**

COC	Maximum Activity (All Samples) (pCi/g) <sup>a</sup>	SNL/NM Background Activity (pCi/g) <sup>b</sup>	Is Maximum COC Activity Less Than or Equal to the Applicable SNL/NM Background Screening Value?	BCF (maximum aquatic)	Is COC a Bioaccumulator? <sup>c</sup> (BCF >40)
Cs-137	ND (0.0344)	0.079	Yes	3,000 <sup>d</sup>	Yes
Th-232	0.794	1.01	Yes	3,000 <sup>e</sup>	Yes
U-235	<b>ND (0.199)</b>	0.16	<b>No</b>	900 <sup>e</sup>	Yes
U-238	ND (0.516)	1.4	Yes	900 <sup>e</sup>	Yes

Note: **Bold** indicates COCs that exceed the background screening values and/or are bioaccumulators.

<sup>a</sup>Value is the greater of either the maximum detection or the highest MDA.

<sup>b</sup>Dinwiddie September 1997, Southwest Area Supergroup.

<sup>c</sup>NMED March 1998.

<sup>d</sup>Whicker and Schultz 1982.

<sup>e</sup>Baker and Soldat 1992.

BCF = Bioconcentration factor.

COC = Constituent of concern.

DSS = Drain and Septic Systems.

MDA = Minimum detectable activity.

ND ( ) = Not detected above the MDA, shown in parentheses.

**ND ( )** = Not detected, but the MDA (shown in parentheses) exceeds background activity.

NMED = New Mexico Environment Department.

pCi/g = Picocurie(s) per gram.

SNL/NM = Sandia National Laboratories/New Mexico.

discharge was to subsurface soil, none of these are considered to be of potential significance as transport mechanisms at this site. Because the septic system is no longer active, additional infiltration of water is not expected. Infiltration of precipitation is essentially nonexistent at DSS Site 1035, as virtually all of the moisture either drains away from the site or evaporates. Because groundwater at this site is approximately 470 feet bgs, the potential for COCs to reach groundwater through the unsaturated zone above the water table is extremely low.

The COCs at DSS Site 1035 include both inorganic and organic constituents. The inorganic COCs include both radiological and nonradiological analytes. With the exception of cyanide, the inorganic COCs are elemental in form and are not considered to be degradable. Transformations of these inorganic constituents could include changes in valence (oxidation/reduction reactions) or incorporation into organic forms (e.g., the conversion of selenite or selenate from soil to seleno-amino acids in plants). Cyanide can be metabolized by soil biota. Radiological COCs will undergo decay to stable isotopes or radioactive daughter elements. However, because of the long half-life of the radiological COC (U-235), the aridity of the environment at this site, and the lack of potential contact with biota, none of these mechanisms are expected to result in significant losses or transformations of the inorganic COCs.

The organic COCs at DSS Site 1035 are limited to acetone, 2-butanone, and bis(2-ethylhexyl) phthalate. Organic COCs may be degraded through photolysis, hydrolysis, and biotransformation. Photolysis requires light and therefore takes place in the air, at the ground surface, or in surface water. Hydrolysis includes chemical transformations in water and may occur in the soil solution. Biotransformation (i.e., transformation caused by plants, animals, and microorganisms) may occur; however, biological activity may be limited by the arid environment at this site. Because of the depth of the COCs in the soil, the loss of acetone and 2-butanone through volatilization is expected to be minimal.

Table 6 summarizes the fate and transport processes that can occur at DSS Site 1035. The COCs at this site include both radiological and nonradiological inorganic analytes as well as organic analytes. Wind, surface water, and biota are considered to be of low significance as potential transport mechanisms at this site. Significant leaching into the subsurface soil is unlikely, and leaching into the groundwater at this site is highly unlikely. The potential for transformation of COCs is low, and loss through decay of the radiological COC is insignificant because of its long half-life.

**Table 6**  
**Summary of Fate and Transport at DSS Site 1035**

Transport and Fate Mechanism	Existence at Site	Significance
Wind	Yes	Low
Surface runoff	Yes	Low
Migration to groundwater	No	None
Food chain uptake	Yes	Low
Transformation/degradation	Yes	Low to moderate

DSS = Drain and Septic Systems.

## VI. Human Health Risk Assessment

### VI.1 Introduction

The human health risk assessment of this site includes a number of steps that culminate in a quantitative evaluation of the potential adverse human health effects caused by constituents located at the site. The steps to be discussed include the following:

Step 1.	Site data are described that provide information on the potential COCs, as well as the relevant physical characteristics and properties of the site.
Step 2.	Potential pathways are identified by which a representative population might be exposed to the COCs.
Step 3.	The potential intake of these COCs by the representative population is calculated using a tiered approach. The first component of the tiered approach is a screening procedure that compares the maximum concentration of the COC to an SNL/NM maximum background screening value. COCs that are not eliminated during the first screening procedure are carried forward in the risk assessment process.
Step 4.	Toxicological parameters are identified and referenced for COCs that were not eliminated during the screening procedure.
Step 5.	Potential toxicity effects (specified as a hazard index [HI]) and estimated excess cancer risks are calculated for nonradiological COCs and background. For radiological COCs, the incremental total effective dose equivalent (TEDE) and incremental estimated cancer risk are calculated by subtracting applicable background concentrations directly from maximum on-site contaminant values. This background subtraction applies only when a radiological COC occurs as contamination and exists as a natural background radionuclide.
Step 6.	These values are compared with guidelines established by the U.S. Environmental Protection Agency (EPA), NMED, and the DOE to determine whether further evaluation and potential site cleanup are required. Nonradiological COC risk values also are compared to background risk so that an incremental risk can be calculated.
Step 7.	Uncertainties of the above steps are addressed.

### VI.2 Step 1. Site Data

Section I of this risk assessment provides the site description and history for DSS Site 1035. Section II presents a comparison of results to DQOs. Section III discusses the nature, rate, and extent of contamination.

### VI.3 Step 2. Pathway Identification

DSS Site 1035 has been designated with a future land-use scenario of industrial (DOE et al. September 1995) (see Appendix 1 for default exposure pathways and parameters). However, the residential land-use scenario is also considered in the pathway analysis. Because of the location and characteristics of the potential contaminants, the primary pathway for human exposure is considered to be soil ingestion for the nonradiological COCs and direct gamma exposure for the radiological COCs. The inhalation pathway for both nonradiological and radiological COCs is included because the potential exists to inhale dust and volatiles. Soil ingestion is included for the radiological COCs as well. The dermal pathway is included for the nonradiological COCs because of the potential for the receptor to be exposed to contaminated soil. No water pathways to the groundwater are considered. Depth to groundwater at DSS

Site 1035 is approximately 470 feet bgs. No intake routes through plant, meat, or milk ingestion are considered appropriate for either the industrial or residential land-use scenarios. Figure 1 shows the conceptual site model flow diagram for DSS Site 1035.

### Pathway Identification

Nonradiological Constituents	Radiological Constituents
Soil ingestion	Soil ingestion
Inhalation (dust and volatiles)	Inhalation (dust)
Dermal contact	Direct gamma

#### VI.4 Step 3. Background Screening Procedure

This section discusses Step 3, the background screening procedure, which compares the maximum COC concentration to the background screening level. The methodology and results are described in the following sections.

##### VI.4.1 Methodology


Maximum concentrations of nonradiological COCs are compared to the approved SNL/NM maximum screening levels for this area. The SNL/NM maximum background concentration was selected to provide the background screen in Table 4 and used to calculate risk attributable to background in Section VI.6.2. Only the COCs that were detected above the corresponding SNL/NM maximum background screening levels or that do not have either a quantifiable or calculated background screening level are considered in further risk assessment analyses.

For radiological COCs that exceed the SNL/NM background screening levels, background values are subtracted from the individual maximum radionuclide concentrations. Those that do not exceed these background levels are not carried any further in the risk assessment. This approach is consistent with DOE Order 5400.5, "Radiation Protection of the Public and the Environment" (DOE 1993). Radiological COCs that do not have a background value and are detected above the analytical minimum detectable activity (MDA) are carried through the risk assessment at the maximum levels. The resultant radiological COCs remaining after this step are referred to as background-adjusted radiological COCs.

##### VI.4.2 Results

Tables 4 and 5 show the DSS Site 1035 maximum COC concentrations that were compared to the SNL/NM maximum background values (Dinwiddie September 1997) for the human health risk assessment. For the nonradiological COCs, one constituent was measured at a concentration greater than the background screening value. One constituent does not have a quantified background screening concentration; therefore it is unknown whether this COC exceeds the background level. Three constituents are organic compounds that do not have corresponding background screening values.

**This page intentionally left blank.**

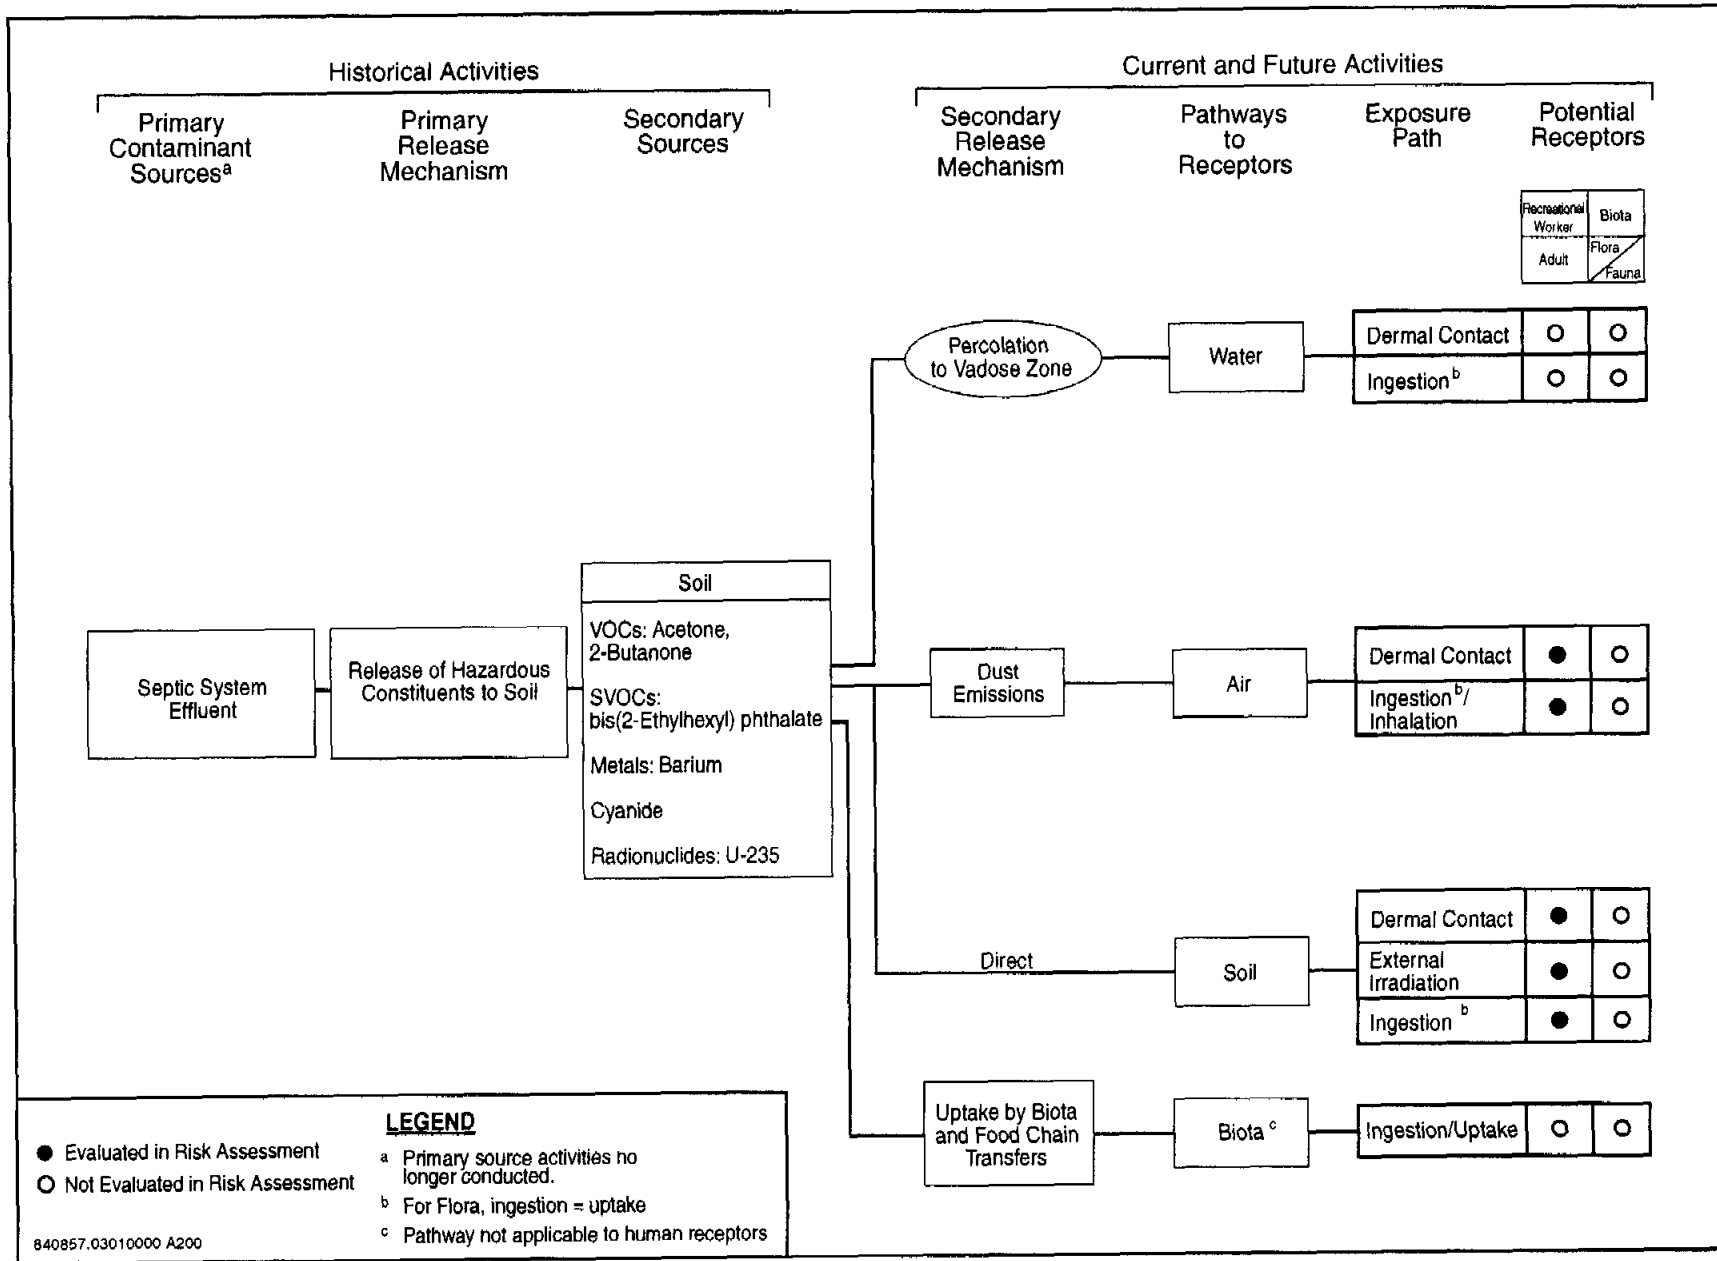

**Figure 1**  
**Conceptual Site Model Flow Diagram for DSS Site 1035, Building 6715 Septic System**



For the radiological COCs, one constituent (U-235) exhibited an MDA greater than its background screening level.

#### VI.5 Step 4. Identification of Toxicological Parameters

Tables 7 (nonradiological) and 8 (radiological) list the COCs retained in the risk assessment and provide the values for the available toxicological information. The toxicological values for the nonradiological COCs presented in Table 7 were obtained from the Integrated Risk Information System (IRIS) (EPA 2003), the Health Effects Assessment Summary Tables (HEAST) (EPA 1997a), the Technical Background Document for Development of Soil Screening Levels (NMED December 2000), the EPA Region 6 electronic database (EPA 2002a), and the Risk Assessment Information System (ORNL 2003) electronic database. Dose conversion factors (DCFs) used in determining the excess TEDE values for radiological COCs for the individual pathways were the default values provided in the RESRAD computer code (Yu et al. 1993a) as developed in the following documents:

- DCFs for ingestion and inhalation were taken from "Federal Guidance Report No. 11, Limiting Values of Radionuclide Intake and Air Concentration and Dose Conversion Factors for Inhalation, Submersion, and Ingestion" (EPA 1988).
- DCFs for surface contamination (contamination on the surface of the site) were taken from DOE/EH-0070, "External Dose-Rate Conversion Factors for Calculation of Dose to the Public" (DOE 1988).
- DCFs for volume contamination (exposure to contamination deeper than the immediate surface of the site) were calculated using the methods discussed in "Dose-Rate Conversion Factors for External Exposure to Photon Emitters in Soil" (Kocher 1983) and in ANL/EAIS-8, "Data Collection Handbook to Support Modeling the Impacts of Radioactive Material in Soil" (Yu et al. 1993b).

#### VI.6 Step 5. Exposure Assessment and Risk Characterization

Section VI.6.1 describes the exposure assessment for this risk assessment. Section VI.6.2 provides the risk characterization, including the HI and excess cancer risk for both the potential nonradiological COCs and associated background for the industrial and residential land-use scenarios. The incremental TEDE and incremental estimated cancer risk are provided for the background-adjusted radiological COC for both the industrial and residential land-use scenarios.

##### VI.6.1 Exposure Assessment

Appendix 1 provides the equations and parameter input values used in calculating intake values and subsequent HI and excess cancer risk values for the individual exposure pathways.

**Table 7**  
**Toxicological Parameter Values for DSS Site 1035 Nonradiological COCs**

COC	RfD <sub>o</sub> (mg/kg-d)	Confidence <sup>a</sup>	RfD <sub>inh</sub> (mg/kg-d)	Confidence <sup>a</sup>	SF <sub>o</sub> (mg/kg-d) <sup>-1</sup>	SF <sub>inh</sub> (mg/kg-d) <sup>-1</sup>	Cancer Class <sup>b</sup>	ABS
<b>Inorganic</b>								
Barium	7E-2 <sup>c</sup>	M	1.4E-4 <sup>d</sup>	-	-	-	D	0.01 <sup>e</sup>
Cyanide	2E-2 <sup>c</sup>	M	-	-	-	-	D	0.1 <sup>e</sup>
<b>Organic</b>								
Acetone	1E-1 <sup>c</sup>	L	1E-1 <sup>f</sup>	-	-	-	D	0.01 <sup>g</sup>
2-Butanone	6E-1 <sup>c</sup>	L	2.9E-1 <sup>c</sup>	L	-	-	D	0.1 <sup>e</sup>
bis(2-Ethylhexyl) phthalate	2E-2 <sup>f</sup>	-	2E-2 <sup>f</sup>	-	1.4E-2 <sup>f</sup>	1.4E-2 <sup>f</sup>	-	0.01 <sup>g</sup>

<sup>a</sup>Confidence associated with IRIS (EPA 2003) database values. Confidence: L = low, M = medium.

<sup>b</sup>EPA weight-of-evidence classification system for carcinogenicity (EPA 1989) taken from IRIS (EPA 2003):

D = Not classifiable as to human carcinogenicity.

<sup>c</sup>Toxicological parameter values from IRIS electronic database (EPA 2003).

<sup>d</sup>Toxicological parameter values from HEAST (EPA 1997a).

<sup>e</sup>Toxicological parameter values from NMED (December 2000).

<sup>f</sup>Toxicological parameter values from EPA Region 6 (EPA 2002a).

<sup>g</sup>Toxicological parameter values from Risk Assessment Information System (ORNL 2003).

ABS = Gastrointestinal absorption coefficient.

COC = Constituent of concern.

DSS = Drain and Septic Systems.

EPA = U.S. Environmental Protection Agency.

HEAST = Health Effects Assessment Summary Tables.

IRIS = Integrated Risk Information System.

mg/kg-d = Milligram(s) per kilogram-day.

(mg/kg-d)<sup>-1</sup> = Per milligram per kilogram-day.

NMED = New Mexico Environment Department.

RfD<sub>inh</sub> = Inhalation chronic reference dose.

RfD<sub>o</sub> = Oral chronic reference dose.

SF<sub>inh</sub> = Inhalation slope factor.

SF<sub>o</sub> = Oral slope factor.

- = Information not available.

**Table 8**  
**Radiological Toxicological Parameter Values for DSS Site 1035 COCs**  
**Obtained from RESRAD Risk Coefficients<sup>a</sup>**

COC	SF <sub>o</sub> (1/pCi)	SF <sub>inh</sub> (1/pCi)	SF <sub>ev</sub> (g/pCi-yr)	Cancer Class <sup>b</sup>
U-235	4.70E-11	1.30E-08	2.70E-07	A

<sup>a</sup>Yu et al. 1993a.

<sup>b</sup>EPA weight-of-evidence classification system for carcinogenicity (EPA 1989): A = Human carcinogen for high dose and high dose rate (i.e., greater than 50 rem per year). For low-level environmental exposures, the carcinogenic effect has not been observed and documented.

1/pCi = One per picocurie.

COC = Constituent of concern.

DSS = Drain and Septic Systems.

EPA = U.S. Environmental Protection Agency.

g/pCi-yr = Gram(s) per picocurie-year.

SF<sub>ev</sub> = External volume exposure slope factor.

SF<sub>inh</sub> = Inhalation slope factor.

SF<sub>o</sub> = Oral (ingestion) slope factor.

The appendix shows parameters for both industrial and residential land-use scenarios. The equations for nonradiological COCs are based upon the Risk Assessment Guidance for Superfund (RAGS) (EPA 1989). Parameters are based upon information from the RAGS (EPA 1989), the Technical Background Document for Development of Soil Screening Levels (NMED December 2000), as well as other EPA and NMED guidance documents, and reflect the reasonable maximum exposure (RME) approach advocated by the RAGS (EPA 1989). For the radiological COC, the coded equation provided in RESRAD computer code is used to estimate the incremental TEDE and cancer risk for individual exposure pathways. Further discussion of this process is provided in the "Manual for Implementing Residual Radioactive Material Guidelines Using RESRAD" (Yu et al. 1993a).

Although the designated land-use scenario for this site is industrial, risk and TEDE values for a residential land-use scenario are also presented.

## VI.6.2 Risk Characterization

Table 9 shows an HI of 0.00 for the DSS Site 1035 nonradiological COCs and an estimated excess cancer risk of 7E-10 for the designated industrial land-use scenario. The numbers presented include exposure from soil ingestion, dermal contact, and dust and volatile inhalation for nonradiological COCs. Table 10 shows an HI of 0.00 and no quantified estimated excess cancer risk for the DSS Site 1035 associated background constituents under the designated industrial land-use scenario.

For the radiological COC, contribution from the direct gamma exposure pathway is included. For the industrial land-use scenario, a TEDE was calculated that results in an incremental TEDE of 4.3E-3 millirem (mrem)/year (yr). In accordance with EPA guidance found in Office of Solid Waste and Emergency Response (OSWER) Directive No. 9200.4-18 (EPA 1997b), an incremental TEDE of 15 mrem/yr is used for the probable land-use scenario (industrial in this

**Table 9**  
**Risk Assessment Values for DSS Site 1035 Nonradiological COCs**

COC	Maximum Concentration (mg/kg)	Industrial Land-Use Scenario <sup>a</sup>		Residential Land-Use Scenario <sup>a</sup>	
		Hazard Index	Cancer Risk	Hazard Index	Cancer Risk
<b>Inorganic</b>					
Barium	232	0.00	–	0.04	–
Cyanide	0.0462 J	0.00	–	0.00	–
<b>Organic</b>					
Acetone	0.00417 J	0.00	–	0.00	–
2-Butanone	0.00674	0.00	–	0.00	–
bis(2-Ethylhexyl) phthalate	0.142 J	0.00	7E-10	0.00	3E-9
<b>Total</b>		0.00	7E-10	0.04	3E-9

<sup>a</sup>EPA 1989.

COC = Constituent of concern.

DSS = Drain and Septic Systems.

EPA = U.S. Environmental Protection Agency.

J = Estimated concentration.

mg/kg = Milligram(s) per kilogram.

– = Information not available.

**Table 10**  
**Risk Assessment Values for DSS Site 1035 Nonradiological Background Constituents**

COC	Background Concentration <sup>a</sup> (mg/kg)	Industrial Land-Use Scenario <sup>b</sup>		Residential Land-Use Scenario <sup>b</sup>	
		Hazard Index	Cancer Risk	Hazard Index	Cancer Risk
Barium	214	0.00	–	0.04	–
Cyanide	NC	–	–	–	–
<b>Total</b>		0.00	–	0.04	–

<sup>a</sup>Dinwiddie September 1997, Southwest Area Supergroup.

<sup>b</sup>EPA 1989.

COC = Constituent of concern.

DSS = Drain and Septic Systems.

EPA = U.S. Environmental Protection Agency.

mg/kg = Milligram(s) per kilogram.

NC = Not calculated.

– = Information not available.

case); the calculated dose value for DSS Site 1035 for the industrial land-use scenario is well below this guideline. The estimated excess cancer risk is  $5.0E-8$ .

For the nonradiological COCs under the residential land-use scenario, the HI is 0.04 with an estimated excess cancer risk of  $3E-9$  (Table 9). The numbers in the table include exposure from soil ingestion, dermal contact, and dust and volatile inhalation. Although the EPA (1991) guidelines generally recommend that inhalation not be included in a residential land-use scenario, this pathway is included because of the potential for soil in Albuquerque, New Mexico, to be eroded and for dust to be present in predominantly residential areas. Because of the nature of the local soil, other exposure pathways are not considered (see Appendix 1). Table 10 shows an HI of 0.04 and no quantified estimated excess cancer risk for the DSS Site 1035 associated background constituents under the residential land-use scenario.

For the radiological COCs, the incremental TEDE for the residential land-use scenario is  $1.1E-2$  mrem/yr. The guideline being used is an excess TEDE of 75 mrem/yr (SNL/NM February 1998) for a complete loss of institutional controls (residential land use in this case); the calculated dose value for DSS Site 1035 for the residential land-use scenario is well below this guideline. Consequently, DSS Site 1035 is eligible for unrestricted radiological release as the residential land-use scenario results in an incremental TEDE of less than 75 mrem/yr to the on-site receptor. The estimated excess cancer risk is  $1.5E-7$ . The excess cancer risk from the nonradiological and radiological COCs should be summed to provide risk estimates for persons exposed to both types of carcinogenic contaminants, as noted in OSWER Directive No. 9200.4-18 "Establishment of Cleanup Levels for CERCLA [Comprehensive Environmental Response, Compensation, and Liability Act] Sites with Radioactive Contamination," (EPA 1997b). This summation is tabulated in Section VI.9, Summary.

#### VI.7 Step 6. Comparison of Risk Values to Numerical Guidelines

The human health risk assessment analysis evaluates the potential for adverse health effects for both the industrial (the designated land-use scenario for this site) and residential land-use scenarios.

For the nonradiological COCs under the industrial land-use scenario, the HI is 0.00 (less than the numerical guideline of 1 suggested in the RAGS [EPA 1989]). The estimated excess cancer risk is  $7E-10$ . NMED guidance states that cumulative excess lifetime cancer risk must be less than  $1E-5$  (Bearzi January 2001); thus the excess cancer risk for this site is below the suggested acceptable risk value. This assessment also determines risks considering background concentrations of the potential nonradiological COCs for both the industrial and residential land-use scenarios. Assuming the industrial land-use scenario, there is an HI of 0.0 and no quantifiable excess cancer risk for nonradiological COCs. The incremental risk is determined by subtracting risk associated with background from potential COC risk. These numbers are not rounded before the difference is determined and therefore may appear to be inconsistent with numbers presented in tables and within the text. For conservatism, the background constituents that do not have quantified background screening concentrations are assumed to have a hazard quotient of 0.00. The incremental HI is 0.00 and the incremental estimated excess cancer risk is  $7.41E-10$  for the industrial land-use scenario. These incremental risk calculations indicate insignificant risk to human health from nonradiological COCs under an industrial land-use scenario.

For the radiological COC under the industrial land-use scenario, the incremental TEDE is  $4.3E-3$  mrem/yr, which is significantly lower than EPA's numerical guideline of 15 mrem/yr. The incremental estimated excess cancer risk is  $5.0E-8$ .

The calculated HI for the nonradiological COCs under the residential land-use scenario is 0.04, which is below numerical guidance. The estimated excess cancer risk is  $3E-9$ . NMED guidance states that cumulative excess lifetime cancer risk must be less than  $1E-5$  (Bearzi January 2001); thus the excess cancer risk for this site is below the suggested acceptable risk value. The incremental HI is 0.00 and the estimated incremental cancer risk is  $3.21E-9$  for the residential land-use scenario. These incremental risk calculations indicate insignificant risk to human health from nonradiological COCs under the residential land-use scenario.

The incremental TEDE for a residential land-use scenario from the radiological component is  $1.1E-2$  mrem/yr, which is significantly lower than the numerical guideline of 75 mrem/yr suggested in the SNL/NM "RESRAD Input Parameter Assumptions and Justification" (SNL/NM February 1998). The estimated incremental excess cancer risk is  $1.5E-7$ .

#### VI.8 Step 7. Uncertainty Discussion

The determination of the nature, rate, and extent of contamination at DSS Site 1035 is based upon an initial conceptual model that was validated with sampling conducted at the site. The sampling was implemented in accordance with the SAP (SNL/NM October 1999) and FIP (SNL/NM November 2001). The DQOs contained in these two documents are appropriate for use in risk assessments. The data from soil samples collected at effluent release points are representative of potential COC releases to the site. The analytical requirements and results satisfy the DQOs, and data quality was verified/validated in accordance with SNL/NM procedures. Therefore, there is no uncertainty associated with the data quality used to perform the risk assessment at DSS Site 1035.

Because of the location, history of the site, and future land use (DOE et al. September 1995), there is low uncertainty in the land-use scenario and the potentially affected populations that were considered in performing the risk assessment analysis. Based upon the COCs found in the near-surface soil and the location and physical characteristics of the site, there is little uncertainty in the exposure pathways relevant to the analysis.

An RME approach is used to calculate the risk assessment values. Specifically, the parameter values in the calculations are conservative and calculated intakes are probably overestimated. Maximum measured values of COC concentrations are used to provide conservative results.

Table 7 shows the uncertainties (confidence levels) in nonradiological toxicological parameter values. There is a combination of estimated values and values from the IRIS (EPA 2003), HEAST (EPA 1997a), EPA Region 6 (EPA 2002a), Technical Background Document for Development of Soil Screening Levels (NMED December 2000), and Risk Assessment Information System (ORNL 2003). Where values are not provided, information is not available from the HEAST (EPA 1997a), IRIS (EPA 2003), Technical Background Document for Development of Soil Screening Levels (NMED December 2000), Risk Assessment Information System (ORNL 2003), or EPA regions (EPA 2002a, EPA 2002b, EPA 2002c). Because of the conservative nature of the RME approach, uncertainties in toxicological values are not expected to change the conclusion from the risk assessment analysis.

Risk assessment values for nonradiological COCs are within the acceptable range for human health under the industrial and residential land-use scenarios compared to established numerical guidance.

For the radiological COC, the conclusion of the risk assessment is that potential effects on human health for both the industrial and residential land-use scenarios are below background and represent only a small fraction of the estimated 360 mrem/yr received by the average U.S. population (NCRP 1987).

The overall uncertainty in all of the steps in the risk assessment process is not considered to be significant with respect to the conclusion reached.

## VI.9 Summary

DSS Site 1035 contains identified COCs consisting of some inorganic, organic, and radiological compounds. Because of the location of the site, the designated industrial land-use scenario, and the nature of contamination, potential exposure pathways identified for this site include soil ingestion, dermal contact, and dust and volatile inhalation for chemical COCs, and soil ingestion, dust inhalation, and direct gamma exposure for radionuclides. The same exposure pathways are applied to the residential land-use scenario.

Using conservative assumptions and an RME approach to risk assessment, calculations for the nonradiological COCs show that for the industrial land-use scenario the HI (0.00) is significantly lower than the accepted numerical guidance from the EPA. The estimated excess cancer risk is  $7E-10$ ; thus, excess cancer risk is also below the acceptable risk value provided by the NMED for an industrial land-use scenario (Bearzi January 2001). The incremental HI is 0.00 and the incremental estimated excess cancer risk is  $7.41E-10$  for the industrial land-use scenario. The incremental risk calculations indicate insignificant risk to human health for the industrial land-use scenario.

Using conservative assumptions and an RME approach to risk assessment, calculations for the nonradiological COCs show that for the residential land-use scenario the HI (0.04) is below the accepted numerical guidance from the EPA. The estimated excess cancer risk is  $3E-9$ . Thus, excess cancer risk is below the acceptable risk value provided by the NMED for a residential land-use scenario (Bearzi January 2001). The incremental HI is 0.00 and the estimated incremental excess cancer risk is  $3.21E-9$  for the residential land-use scenario. The incremental risk calculations indicate insignificant risk to human health for the residential land-use scenario.

The incremental TEDE and corresponding estimated cancer risk from the radiological COC are much lower than EPA guidance values. The estimated TEDE is  $4.3E-3$  mrem/yr for the industrial land-use scenario, which is much lower than the EPA's numerical guidance of 15 mrem/yr (EPA 1997b). The corresponding incremental estimated cancer risk value is  $5.0E-8$  for the industrial land-use scenario. Furthermore, the incremental TEDE for the residential land-use scenario that results from a complete loss of institutional control is  $1.1E-2$  mrem/yr with an associated risk of  $1.5E-7$ . The guideline for this scenario is 75 mrem/yr (SNL/NM February 1998). Therefore, DSS Site 1035 is eligible for unrestricted radiological release.

The excess cancer risk from the nonradiological and radiological COCs should be summed to provide risk estimates for persons exposed to both types of carcinogenic contaminants, as

noted in OSWER Directive No. 9200.4-18 (EPA 1997b). The summation of the incremental nonradiological and radiological carcinogenic risks is tabulated in Table 11.

**Table 11**  
**Summation of Incremental Radiological and Nonradiological Risks from**  
**DSS Site 1035, Building 6715 Septic System Carcinogens**

Scenario	Nonradiological Risk	Radiological Risk	Total Risk
Industrial	7.41E-10	5.0E-8	5.0E-8
Residential	3.21E-9	1.5E-7	1.5E-7

DSS = Drain and Septic Systems.

Uncertainties associated with the calculations are considered small relative to the conservatism of the risk assessment analysis. Therefore, it is concluded that this site poses insignificant risk to human health under both the industrial and residential land-use scenarios.

## VII. Ecological Risk Assessment

### VII.1 Introduction

This section addresses the ecological risks associated with exposure to constituents of potential ecological concern (COPECs) in the soil at DSS Site 1035. A component of the NMED Risk-Based Decision Tree (NMED March 1998) is to conduct an ecological risk assessment that corresponds with that presented in EPA's Ecological RAGS (EPA 1997c). The current methodology is tiered and contains an initial scoping assessment followed by a more detailed risk assessment if warranted by the results of the scoping assessment. Initial components of NMED's decision tree (a discussion of DQOs, data assessment, and evaluations of bioaccumulation as well as fate and transport potential) are addressed in previous sections of this report. At the end of the scoping assessment, a determination is made as to whether a more detailed examination of potential ecological risk is necessary.

### VII.2 Scoping Assessment

The scoping assessment focuses primarily on the likelihood of exposure of biota at, or adjacent to, the site to constituents associated with site activities. Included in this section are an evaluation of existing data with respect to the existence of complete ecological exposure pathways, an evaluation of bioaccumulation potential, and a summary of fate and transport potential. A scoping risk management decision (Section VII.2.4) summarizes the scoping results and assesses the need for further examination of potential ecological impacts.



### VII.2.1 Data Assessment

As indicated in Section IV, all COCs at DSS Site 1035 are at depths of 5 feet bgs or greater. Therefore, no complete ecological exposure pathways exist at this site, and no COCs are considered to be COPECs.

### VII.2.2 Bioaccumulation

Because no COPECs are associated with this site, bioaccumulation potential was not evaluated.

### VII.2.3 Fate and Transport Potential

The potential for the COCs to migrate from the source of contamination to other media or biota is discussed in Section V. As noted in Table 6 (Section V), wind, surface water, and biota (food chain uptake) are expected to be of low significance as transport mechanisms for COCs at this site. Degradation, transformation, and decay of the radiological COC also are expected to be of low significance.

### VII.2.4 Scoping Risk-Management Decision

Based upon information gathered through the scoping assessment, it is concluded that complete ecological pathways are not associated with COCs at this site. Therefore, no COPECs exist at the site, and a more detailed risk assessment was not deemed necessary to predict the potential level of ecological risk associated with the site.

## VIII. References

Baker, D.A., and J.K. Soldat, 1992. "Methods for Estimating Doses to Organisms from Radioactive Materials Released into the Aquatic Environment," PNL-8150, Pacific Northwest Laboratory, Richland, Washington.

Bearzi, J.P. (New Mexico Environment Department), January 2001. Memorandum to RCRA-Regulated Facilities, "Risk-Based Screening Levels for RCRA Corrective Action Sites in New Mexico," Hazardous Waste Bureau, New Mexico Environment Department, Santa Fe, New Mexico. January 23, 2001.

Callahan, M.A., M.W. Slimak, N.W. Gabel, I.P. May, C.F. Fowler, J.R. Freed, P. Jennings, R.L. Durfee, F.C. Whitmore, B. Maestri, W.R. Mabey, B.R. Holt, and C. Gould, 1979. "Water-Related Environmental Fate of 129 Priority Pollutants," EPA-440/4-79-029, Office of Water and Waste Management, Office of Water Planning and Standards, U.S. Environmental Protection Agency, Washington, D.C.

Dinwiddie, R.S. (New Mexico Environment Department), September 1997. Letter to M.J. Zamorski (U.S. Department of Energy), "Request for Supplemental Information: Background Concentrations Report, SNL/KAFB." September 24, 1997.

DOE, see U.S. Department of Energy.

EPA, see U.S. Environmental Protection Agency.

Howard, P.H., 1989. Volume I: "Large Production and Priority Pollutants," *Handbook of Environmental Fate and Exposure Data for Organic Chemicals*, Lewis Publishers, Inc., Chelsea, Michigan.

Howard, P.H., 1990. Volume II: "Solvents," *Handbook of Environmental Fate and Exposure Data for Organic Chemicals*, Lewis Publishers, Inc. Chelsea, Michigan.

Jones, J. (Sandia National Laboratories/New Mexico), June 1991. Internal memorandum to D. Dionne listing the septic tanks that were removed from service with the construction of the Area III sanitary sewer system. June 21, 1991.

Kocher, D.C. 1983. "Dose-Rate Conversion Factors for External Exposure to Photon Emitters in Soil," *Health Physics*, Vol. 28, pp. 193–205.

Micromedex, Inc., 1998, Hazardous Substances Databank.

National Council on Radiation Protection and Measurements (NCRP), 1987. "Exposure of the Population in the United States and Canada from Natural Background Radiation," *NCRP Report No. 94*, National Council on Radiation Protection and Measurements, Bethesda, Maryland.

National Oceanic and Atmospheric Administration (NOAA), 1990. "Local Climatological Data, Annual Summary with Comparative Data," Albuquerque, New Mexico.

NCRP, see National Council on Radiation Protection and Measurements.

Neumann, G., 1976. "Concentration Factors for Stable Metals and Radionuclides in Fish, Mussels and Crustaceans—A Literature Survey," Report 85-04-24, National Swedish Environmental Protection Board.

New Mexico Environment Department (NMED), March 1998. "Risk-Based Decision Tree Description," in New Mexico Environment Department, "RPMP Document Requirement Guide," RCRA Permits Management Program, Hazardous and Radioactive Materials Bureau, New Mexico Environment Department, Santa Fe, New Mexico.

New Mexico Environment Department (NMED), December 2000. "Technical Background Document for Development of Soil Screening Levels," Hazardous Waste Bureau and Ground Water Quality Bureau Voluntary Remediation Program, New Mexico Environment Department, Santa Fe, New Mexico.

NMED, see New Mexico Environment Department.

NOAA, see National Oceanographic and Atmospheric Administration.

Oak Ridge National Laboratory, 2003. "Risk Assessment Information System," electronic database maintained by Oak Ridge National Laboratory, Oak Ridge, Tennessee.

ORNL, Oak Ridge National Laboratory.

Romero, T. (Sandia National Laboratories/New Mexico), September 2003. Internal communication to M. Sanders stating that during the connection of septic systems to the new City of Albuquerque sewer system, the old systems were disconnected and the lines capped. September 16, 2003.

Sandia National Laboratories/New Mexico (SNL/NM), July 1994. "Verification and Validation of Chemical and Radiochemical Data," Technical Operating Procedure (TOP) 94-03, Rev. 0, Sandia National Laboratories, Albuquerque, New Mexico.

Sandia National Laboratories/New Mexico (SNL/NM), March 1996. "Site-Wide Hydrogeologic Characterization Project, Calendar Year 1995 Annual Report," Environmental Restoration Project, Sandia National Laboratories, Albuquerque, New Mexico.

Sandia National Laboratories/New Mexico (SNL/NM), July 1996. "Laboratory Data Review Guidelines," Radiation Protection Diagnostics Procedure No. RPSD-02-11, Issue No. 2, Sandia National Laboratories, Albuquerque, New Mexico.

Sandia National Laboratories/New Mexico (SNL/NM), February 1998. "RESRAD Input Parameter Assumptions and Justification," Environmental Restoration Project, Sandia National Laboratories, Albuquerque, New Mexico.

Sandia National Laboratories/New Mexico (SNL/NM), October 1999. "Sampling and Analysis Plan for Characterizing and Assessing Potential Releases to the Environment From Septic and Other Miscellaneous Drain Systems at Sandia National Laboratories/New Mexico," Sandia National Laboratories, Albuquerque, New Mexico. October 19, 1999.

Sandia National Laboratories/New Mexico (SNL/NM), December 1999. "Data Validation Procedure for Chemical and Radiochemical Data," Administrative Operating Procedure (AOP) 00-03, Environmental Restoration Project, Sandia National Laboratories, Albuquerque, New Mexico.

Sandia National Laboratories/New Mexico (SNL/NM), November 2001. "Field Implementation Plan, Characterization of Non-Environmental Restoration Drain and Septic Systems," Sandia National Laboratories, Albuquerque, New Mexico.

Sandia National Laboratories/New Mexico (SNL/NM), March 2002. "Annual Groundwater Monitoring Report, Fiscal Year 2000," Sandia National Laboratories, Albuquerque, New Mexico.

Sandia National Laboratories/New Mexico (SNL/NM), March 2003. Database printout provided by SNL/NM Facilities Engineering showing the year that numerous SNL/NM buildings were constructed, Sandia National Laboratories, Albuquerque, New Mexico.

Sandia National Laboratories/New Mexico (SNL/NM), April 2003. "DSS Sites Mean Elevation Report," GIS Group, Environmental Restoration Department, Sandia National Laboratories, Albuquerque, New Mexico.

SNL/NM, See Sandia National Laboratories, New Mexico.

U.S. Department of Energy (DOE), 1988. "External Dose-Rate Conversion Factors for Calculation of Dose to the Public," DOE/EH-0070, Assistant Secretary for Environment, Safety and Health, U.S. Department of Energy, Washington, D.C.

U.S. Department of Energy (DOE), 1993. "Radiation Protection of the Public and the Environment," DOE Order 5400.5, U.S. Department of Energy, Washington, D.C.

U.S. Department of Energy (DOE), U.S. Air Force, and U.S. Forest Service, September 1995. "Workbook: Future Use Management Area 2," prepared by the Future Use Logistics and Support Working Group in cooperation with U.S. Department of Energy Affiliates, the U.S. Air Force, and the U.S. Forest Service.

U.S. Environmental Protection Agency (EPA), November 1986. "Test Methods for Evaluating Solid Waste," 3rd ed., Update 3, SW-846, Office of Solid Waste and Emergency Response, U.S. Environmental Protection Agency, Washington, D.C.

U.S. Environmental Protection Agency (EPA), 1988. "Federal Guidance Report No. 11, Limiting Values of Radionuclide Intake and Air Concentration and Dose Conversion Factors for Inhalation, Submersion, and Ingestion," Office of Radiation Programs, U.S. Environmental Protection Agency, Washington, D.C.

U.S. Environmental Protection Agency (EPA), 1989. "Risk Assessment Guidance for Superfund, Vol. I: Human Health Evaluation Manual," EPA/540-1089/002, Office of Emergency and Remedial Response, U.S. Environmental Protection Agency, Washington, D.C.

U.S. Environmental Protection Agency (EPA), 1991. "Risk Assessment Guidance for Superfund, Volume I: Human Health Evaluation Manual (Part B)," Office of Emergency and Remedial Response, U.S. Environmental Protection Agency, Washington, D.C.

U.S. Environmental Protection Agency (EPA), 1997a. "Health Effects Assessment Summary Tables (HEAST), FY 1997 Update," EPA-540-R-97-036, Office of Research and Development and Office of Solid Waste and Emergency Response, U.S. Environmental Protection Agency, Washington, D.C.

U.S. Environmental Protection Agency (EPA), 1997b. "Establishment of Cleanup Levels for CERCLA Sites with Radioactive Contamination," OSWER Directive No. 9200.4-18, Office of Solid Waste and Emergency Response, U.S. Environmental Protection Agency, Washington, D.C.

U.S. Environmental Protection Agency (EPA), 1997c. "Ecological Risk Assessment Guidance for Superfund: Process for Designing and Conducting Ecological Risks," Interim Final, U.S. Environmental Protection Agency, Washington, D.C.

U.S. Environmental Protection Agency (EPA), 2002a. "Region 6 Preliminary Remediation Goals (PRGs) 2002," electronic database maintained by Region 6, U.S. Environmental Protection Agency, Dallas, Texas.

U.S. Environmental Protection Agency (EPA), 2002b. "Region 9 Preliminary Remediation Goals (PRGs) 2002," electronic database maintained by Region 9, U.S. Environmental Protection Agency, San Francisco, California.

U.S. Environmental Protection Agency (EPA), 2002c. "Risk-Based Concentration Table," electronic database maintained by Region 3, U.S. Environmental Protection Agency, Philadelphia, Pennsylvania.

U.S. Environmental Protection Agency (EPA), 2003. Integrated Risk Information System (IRIS) electronic database, maintained by the U.S. Environmental Protection Agency, Washington, D.C.

Whicker, F.W., and V. Schultz, 1982. *Radioecology: Nuclear Energy and the Environment*, Volume II, CRC Press, Boca Raton, Florida.

Yanicak, S. (Oversight Bureau, Department of Energy, New Mexico Environment Department), March 1997. Letter to M. Johansen (DOE/AIP/POC Los Alamos National Laboratory), "(Tentative) list of constituents of potential ecological concern (COPECs) which are considered to be bioconcentrators and/or biomagnifiers." March 3, 1997.

Yu, C., A.J. Zielen, J.-J. Cheng, Y.C. Yuan, L.G. Jones, D.J. LePoire, Y.Y. Wang, C.O. Loureiro, E. Gnanapragasam, E. Faillace, A. Wallo III, W.A. Williams, and H. Peterson, 1993a. "Manual for Implementing Residual Radioactive Material Guidelines Using RESRAD," Version 5.0. Environmental Assessment Division, Argonne National Laboratory, Argonne, Illinois.

Yu, C., C. Loureiro, J.-J. Cheng, L.G. Jones, Y.Y. Wang, Y.P. Chia, and E. Faillace, 1993b. "Data Collection Handbook to Support Modeling the Impacts of Radioactive Material in Soil," ANL/EAIS-8, Argonne National Laboratory, Argonne, Illinois.

**This page intentionally left blank.**

## APPENDIX 1 EXPOSURE PATHWAY DISCUSSION FOR CHEMICAL AND RADIONUCLIDE CONTAMINATION

### Introduction

Sandia National Laboratories/New Mexico (SNL/NM) uses a default set of exposure routes and associated default parameter values developed for each future land-use designation being considered for SNL/NM Environmental Restoration (ER) Project sites. This default set of exposure scenarios and parameter values are invoked for risk assessments unless site-specific information suggests other parameter values. Because many SNL/NM solid waste management units (SWMUs) have similar types of contamination and physical settings, SNL/NM believes that the risk assessment analyses at these sites can be similar. A default set of exposure scenarios and parameter values facilitates the risk assessments and subsequent review.

The default exposure routes and parameter values used are those that SNL/NM views as resulting in a Reasonable Maximum Exposure (RME) value. Subject to comments and recommendations by the U.S. Environmental Protection Agency (EPA) Region VI and New Mexico Environment Department (NMED), SNL/NM will use these default exposure routes and parameter values in future risk assessments.

At SNL/NM, all SWMUs exist within the boundaries of the Kirtland Air Force Base. Approximately 240 potential waste and release sites have been identified where hazardous, radiological, or mixed materials may have been released to the environment. Evaluation and characterization activities have occurred at all of these sites to varying degrees. Among other documents, the SNL/NM ER draft Environmental Assessment (DOE 1996) presents a summary of the hydrogeology of the sites and the biological resources present. When evaluating potential human health risk the current or reasonably foreseeable land use negotiated and approved for the specific SWMU/AOC, aggregate, or watershed will be used. The following references generally document these land uses: Workbook: Future Use Management Area 2 (DOE et al. September 1995); Workbook: Future Use Management Area 1 (DOE et al. October 1995); Workbook: Future Use Management Areas 3, 4, 5, and 6 (DOE and USAF January 1996); Workbook: Future Use Management Area 7 (DOE and USAF March 1996). At this time, all SNL/NM SWMUs have been tentatively designated for either industrial or recreational future land use. The NMED has also requested that risk calculations be performed based upon a residential land-use scenario. Therefore, all three land-use scenarios will be addressed in this document.

The SNL/NM ER Project has screened the potential exposure routes and identified default parameter values to be used for calculating potential intake and subsequent hazard index (HI), excess cancer risk and dose values. The EPA (EPA 1989) provides a summary of exposure routes that could potentially be of significance at a specific waste site. These potential exposure routes consist of:

- Ingestion of contaminated drinking water
- Ingestion of contaminated soil

- Ingestion of contaminated fish and shellfish
- Ingestion of contaminated fruits and vegetables
- Ingestion of contaminated meat, eggs, and dairy products
- Ingestion of contaminated surface water while swimming
- Dermal contact with chemicals in water
- Dermal contact with chemicals in soil
- Inhalation of airborne compounds (vapor phase or particulate)
- External exposure to penetrating radiation (immersion in contaminated air; immersion in contaminated water; and exposure from ground surfaces with photon-emitting radionuclides)

Based upon the location of the SNL/NM SWMUs and the characteristics of the surface and subsurface at the sites, we have evaluated these potential exposure routes for different land-use scenarios to determine which should be considered in risk assessment analyses (the last exposure route is pertinent to radionuclides only). At SNL/NM SWMUs, there is currently no consumption of fish, shellfish, fruits, vegetables, meat, eggs, or dairy products that originate on site. Additionally, no potential for swimming in surface water is present due to the high-desert environmental conditions. As documented in the RESRAD computer code manual (ANL 1993), risks resulting from immersion in contaminated air or water are not significant compared to risks from other radiation exposure routes.

For the industrial and recreational land-use scenarios, SNL/NM ER has, therefore, excluded the following five potential exposure routes from further risk assessment evaluations at any SNL/NM SWMU:

- Ingestion of contaminated fish and shellfish
- Ingestion of contaminated fruits and vegetables
- Ingestion of contaminated meat, eggs, and dairy products
- Ingestion of contaminated surface water while swimming
- Dermal contact with chemicals in water

That part of the exposure pathway for radionuclides related to immersion in contaminated air or water is also eliminated.

Based upon this evaluation, for future risk assessments the exposure routes that will be considered are shown in Table 1.



**Table 1**  
**Exposure Pathways Considered for Various Land-Use Scenarios**

<b>Industrial</b>	<b>Recreational</b>	<b>Residential</b>
Ingestion of contaminated drinking water	Ingestion of contaminated drinking water	Ingestion of contaminated drinking water
Ingestion of contaminated soil	Ingestion of contaminated soil	Ingestion of contaminated soil
Inhalation of airborne compounds (vapor phase or particulate)	Inhalation of airborne compounds (vapor phase or particulate)	Inhalation of airborne compounds (vapor phase or particulate)
Dermal contact (nonradiological constituents only) soil only	Dermal contact (nonradiological constituents only) soil only	Dermal contact (nonradiological constituents only) soil only
External exposure to penetrating radiation from ground surfaces	External exposure to penetrating radiation from ground surfaces	External exposure to penetrating radiation from ground surfaces

#### Equations and Default Parameter Values for Identified Exposure Routes

In general, SNL/NM expects that ingestion of compounds in drinking water and soil will be the more significant exposure routes for chemicals; external exposure to radiation may also be significant for radionuclides. All of the above routes will, however, be considered for their appropriate land-use scenarios. The general equation for calculating potential intakes via these routes is shown below. The equations are taken from "Assessing Human Health Risks Posed by Chemicals: Screening-Level Risk Assessment" (NMED March 2000) and "Technical Background Document for Development of Soil Screening Levels" (NMED December 2000). Equations from both documents are based upon the "Risk Assessment Guidance for Superfund" (RAGS): Volume 1 (EPA 1989, 1991). These general equations also apply to calculating potential intakes for radionuclides. A more in-depth discussion of the equations used in performing radiological pathway analyses with the RESRAD code may be found in the RESRAD Manual (ANL 1993). RESRAD is the only code designated by the U.S. Department of Energy (DOE) in DOE Order 5400.5 for the evaluation of radioactively contaminated sites (DOE 1993). The Nuclear Regulatory Commission (NRC) has approved the use of RESRAD for dose evaluation by licensees involved in decommissioning, NRC staff evaluation of waste disposal requests, and dose evaluation of sites being reviewed by NRC staff. EPA Science Advisory Board reviewed the RESRAD model. EPA used RESRAD in their rulemaking on radiation site cleanup regulations. RESRAD code has been verified, undergone several benchmarking analyses, and been included in the International Atomic Energy Agency's VAMP and BIOMOV5 II projects to compare environmental transport models.

Also shown are the default values SNL/NM ER will use in RME risk assessment calculations for industrial, recreational, and residential land-use scenarios, based upon EPA and other governmental agency guidance. The pathways and values for chemical contaminants are discussed first, followed by those for radionuclide contaminants. RESRAD input parameters that are left as the default values provided with the code are not discussed. Further information relating to these parameters may be found in the RESRAD Manual (ANL 1993) or by directly accessing the RESRAD websites at: <http://web.ead.anl.gov/resrad/home2/> or <http://web.ead.anl.gov/resrad/documents/>.

### Generic Equation for Calculation of Risk Parameter Values

The equation used to calculate the risk parameter values (i.e., hazard quotients/HI, excess cancer risk, or radiation total effective dose equivalent [TEDE] [dose]) is similar for all exposure pathways and is given by:

$$\begin{aligned} \text{Risk (or Dose)} &= \text{Intake} \times \text{Toxicity Effect (either carcinogenic, noncarcinogenic, or radiological)} \\ &= C \times (\text{CR} \times \text{EFD}/\text{BW}/\text{AT}) \times \text{Toxicity Effect} \end{aligned} \quad (1)$$

where;

- C = contaminant concentration (site specific)
- CR = contact rate for the exposure pathway
- EFD = exposure frequency and duration
- BW = body weight of average exposure individual
- AT = time over which exposure is averaged.

For nonradiological constituents of concern (COCs), the total risk/dose (either cancer risk or HI) is the sum of the risks/doses for all of the site-specific exposure pathways and contaminants. For radionuclides, the calculated radiation exposure, expressed as TEDE is compared directly to the exposure guidelines of 15 millirem per year (mrem/year) for industrial and recreational future use and 75 mrem/year for the unlikely event that institutional control of the site is lost and the site is used for residential purposes (EPA 1997).

The evaluation of the carcinogenic health hazard produces a quantitative estimate for excess cancer risk resulting from the COCs present at the site. This estimate is evaluated for determination of further action by comparison of the quantitative estimate with the potentially acceptable risk of 1E-5 for nonradiological carcinogens. The evaluation of the noncarcinogenic health hazard produces a quantitative estimate (i.e., the HI) for the toxicity resulting from the COCs present at the site. This estimate is evaluated for determination of further action by comparison of this quantitative estimate with the EPA standard HI of unity (1). The evaluation of the health hazard from radioactive compounds produces a quantitative estimate of doses resulting from the COCs present at the site. This estimated dose is used to calculate an assumed risk. However, this calculated risk is presented for illustration purposes only, not to determine compliance with regulations.

The specific equations used for the individual exposure pathways can be found in RAGS (EPA 1989) and are outlined below. The RESRAD Manual (ANL 1993) describes similar equations for the calculation of radiological exposures.

### Soil Ingestion

A receptor can ingest soil or dust directly by working in the contaminated soil. Indirect ingestion can occur from sources such as unwashed hands introducing contaminated soil to food that is then eaten. An estimate of intake from ingesting soil will be calculated as follows:

$$I_s = \frac{C_s * IR * CF * EF * ED}{BW * AT}$$

where:

- $I_s$  = Intake of contaminant from soil ingestion (milligrams [mg]/kilogram [kg]-day)
- $C_s$  = Chemical concentration in soil (mg/kg)
- IR = Ingestion rate (mg soil/day)
- CF = Conversion factor (1E-6 kg/mg)
- EF = Exposure frequency (days/year)
- ED = Exposure duration (years)
- BW = Body weight (kg)
- AT = Averaging time (period over which exposure is averaged) (days)

It should be noted that it is conservatively assumed that the receptor only ingests soil from the contaminated source.

### Soil Inhalation

A receptor can inhale soil or dust directly by working in the contaminated soil. An estimate of intake from inhaling soil will be calculated as follows (EPA August 1997):

$$I_s = \frac{C_s * IR * EF * ED * \left( \frac{1}{VF} \text{ or } \frac{1}{PEF} \right)}{BW * AT}$$

where:

- $I_s$  = Intake of contaminant from soil inhalation (mg/kg-day)
- $C_s$  = Chemical concentration in soil (mg/kg)
- IR = Inhalation rate (cubic meters [m<sup>3</sup>]/day)
- EF = Exposure frequency (days/year)
- ED = Exposure duration (years)
- VF = soil-to-air volatilization factor (m<sup>3</sup>/kg)
- PEF = particulate emission factor (m<sup>3</sup>/kg)
- BW = Body weight (kg)
- AT = Averaging time (period over which exposure is averaged) (days)

### Soil Dermal Contact

$$D_e = \frac{C_s * CF * SA * AF * ABS * EF * ED}{BW * AT}$$

where:

- $D_a$  = Absorbed dose (mg/kg-day)
- $C_s$  = Chemical concentration in soil (mg/kg)
- CF = Conversion factor (1E-6 kg/mg)
- SA = Skin surface area available for contact (cm<sup>2</sup>/event)
- AF = Soil to skin adherence factor (mg/cm<sup>2</sup>)
- ABS = Absorption factor (unitless)
- EF = Exposure frequency (events/year)

ED = Exposure duration (years)  
 BW = Body weight (kg)  
 AT = Averaging time (period over which exposure is averaged) (days)

### Groundwater Ingestion

A receptor can ingest water by drinking it or through using household water for cooking. An estimate of intake from ingesting water will be calculated as follows (EPA August 1997):

$$I_w = \frac{C_w * IR * EF * ED}{BW * AT}$$

where:

$I_w$  = Intake of contaminant from water ingestion (mg/kg/day)  
 $C_w$  = Chemical concentration in water (mg/liter [L])  
 IR = Ingestion rate (L/day)  
 EF = Exposure frequency (days/year)  
 ED = Exposure duration (years)  
 BW = Body weight (kg)  
 AT = Averaging time (period over which exposure is averaged) (days)

### Groundwater Inhalation

The amount of a constituent taken into the body via exposure to volatilization from showering or other household water uses will be evaluated using the concentration of the constituent in the water source (EPA 1991 and 1992). An estimate of intake from volatile inhalation from groundwater will be calculated as follows (EPA 1991):

$$I_w = \frac{C_w * K * IR_i * EF * ED}{BW * AT}$$

where:

$I_w$  = Intake of volatile in water from inhalation (mg/kg/day)  
 $C_w$  = Chemical concentration in water (mg/L)  
 K = volatilization factor (0.5 L/m<sup>3</sup>)  
 $IR_i$  = Inhalation rate (m<sup>3</sup>/day)  
 EF = Exposure frequency (days/year)  
 ED = Exposure duration (years)  
 BW = Body weight (kg)  
 AT = Averaging time (period over which exposure is averaged—days)

For volatile compounds, volatilization from groundwater can be an important exposure pathway from showering and other household uses of groundwater. This exposure pathway will only be evaluated for organic chemicals with a Henry's Law constant greater than  $1 \times 10^{-5}$  and with a molecular weight of 200 grams/mole or less (EPA 1991).

Tables 2 and 3 show the default parameter values suggested for use by SNL/NM at SWMUs, based upon the selected land-use scenarios for nonradiological and radiological COCs,

respectively. References are given at the end of the table indicating the source for the chosen parameter values. SNL/NM uses default values that are consistent with both regulatory guidance and the RME approach. Therefore, the values chosen will, in general, provide a conservative estimate of the actual risk parameter. These parameter values are suggested for use for the various exposure pathways, based upon the assumption that a particular site has no unusual characteristics that contradict the default assumptions. For sites for which the assumptions are not valid, the parameter values will be modified and documented.

### Summary

SNL/NM will use the described default exposure routes and parameter values in risk assessments at sites that have an industrial, recreational, or residential future land-use scenario. There are no current residential land-use designations at SNL/NM ER sites, but NMED has requested this scenario to be considered to provide perspective of the risk under the more restrictive land-use scenario. For sites designated as industrial or recreational land use, SNL/NM will provide risk parameter values based upon a residential land-use scenario to indicate the effects of data uncertainty on risk value calculations or in order to potentially mitigate the need for institutional controls or restrictions on SNL/NM ER sites. The parameter values are based upon EPA guidance and supplemented by information from other government sources. If these exposure routes and parameters are acceptable, SNL/NM will use them in risk assessments for all sites where the assumptions are consistent with site-specific conditions. All deviations will be documented.

**Table 2**  
**Default Nonradiological Exposure Parameter Values for Various Land-Use Scenarios**

Parameter	Industrial	Recreational	Residential
<b>General Exposure Parameters</b>			
Exposure Frequency (day/yr)	250 <sup>a,b</sup>	8.7 (4 hr/wk for 52 wk/yr) <sup>a,b</sup>	350 <sup>a,b</sup>
Exposure Duration (yr)	25 <sup>a,b,c</sup>	30 <sup>a,b,c</sup>	30 <sup>a,b,c</sup>
Body Weight (kg)	70 <sup>a,b,c</sup>	70 Adult <sup>a,b,c</sup> 15 Child <sup>a,b,c</sup>	70 Adult <sup>a,b,c</sup> 15 Child <sup>a,b,c</sup>
Averaging Time (days) for Carcinogenic Compounds (= 70 yr x 365 day/yr)	25,550 <sup>a,b</sup>	25,550 <sup>a,b</sup>	25,550 <sup>a,b</sup>
for Noncarcinogenic Compounds (= ED x 365 day/yr)	9,125 <sup>a,b</sup>	10,950 <sup>a,b</sup>	10,950 <sup>a,b</sup>
<b>Soil Ingestion Pathway</b>			
Ingestion Rate (mg/day)	100 <sup>a,b</sup>	200 Child <sup>a,b</sup> 100 Adult <sup>a,b</sup>	200 Child <sup>a,b</sup> 100 Adult <sup>a,b</sup>
<b>Inhalation Pathway</b>			
Inhalation Rate (m <sup>3</sup> /day)	20 <sup>a,b</sup>	15 Child <sup>a</sup> 30 Adult <sup>a</sup>	10 Child <sup>a</sup> 20 Adult <sup>a</sup>
Volatilization Factor (m <sup>3</sup> /kg)	Chemical Specific	Chemical Specific	Chemical Specific
Particulate Emission Factor (m <sup>3</sup> /kg)	1.36E9 <sup>a</sup>	1.36E9 <sup>a</sup>	1.36E9 <sup>a</sup>
<b>Water Ingestion Pathway</b>			
Ingestion Rate (liter/day)	2.4 <sup>a</sup>	2.4 <sup>a</sup>	2.4 <sup>a</sup>
<b>Dermal Pathway</b>			
Skin Adherence Factor (mg/cm <sup>2</sup> )	0.2 <sup>a</sup>	0.2 Child <sup>a</sup> 0.07 Adult <sup>a</sup>	0.2 Child <sup>a</sup> 0.07 Adult <sup>a</sup>
Exposed Surface Area for Soil/Dust (cm <sup>2</sup> /day)	3,300 <sup>a</sup>	2,800 Child <sup>a</sup> 5,700 Adult <sup>a</sup>	2,800 Child <sup>a</sup> 5,700 Adult <sup>a</sup>
Skin Adsorption Factor	Chemical Specific	Chemical Specific	Chemical Specific

<sup>a</sup>Technical Background Document for Development of Soil Screening Levels (NMED December 2000).

<sup>b</sup>Risk Assessment Guidance for Superfund, Vol. 1, Part B (EPA 1991).

<sup>c</sup>Exposure Factors Handbook (EPA August 1997).

ED = Exposure duration.

EPA = U.S. Environmental Protection Agency.

hr = Hour(s).

kg = Kilogram(s).

m = Meter(s).

mg = Milligram(s).

NA = Not available.

wk = Week(s).

yr = Year(s).

**Table 3**  
**Default Radiological Exposure Parameter Values for Various Land-Use Scenarios**

Parameter	Industrial	Recreational	Residential
<b>General Exposure Parameters</b>			
Exposure Frequency	8 hr/day for 250 day/yr	4 hr/wk for 52 wk/yr	365 day/yr
Exposure Duration (yr)	25 <sup>a,b</sup>	30 <sup>a,b</sup>	30 <sup>a,b</sup>
Body Weight (kg)	70 Adult <sup>a,b</sup>	70 Adult <sup>a,b</sup>	70 Adult <sup>a,b</sup>
<b>Soil Ingestion Pathway</b>			
Ingestion Rate	100 mg/day <sup>c</sup>	100 mg/day <sup>c</sup>	100 mg/day <sup>c</sup>
Averaging Time (days) (= 30 yr x 365 day/yr)	10,950 <sup>d</sup>	10,950 <sup>d</sup>	10,950 <sup>d</sup>
<b>Inhalation Pathway</b>			
Inhalation Rate (m <sup>3</sup> /yr)	7,300 <sup>d,e</sup>	10,950 <sup>e</sup>	7,300 <sup>d,e</sup>
Mass Loading for Inhalation g/m <sup>3</sup>	1.36 E-5 <sup>d</sup>	1.36 E-5 <sup>d</sup>	1.36 E-5 <sup>d</sup>
<b>Food Ingestion Pathway</b>			
Ingestion Rate, Leafy Vegetables (kg/yr)	NA	NA	16.5 <sup>c</sup>
Ingestion Rate, Fruits, Non-Leafy Vegetables & Grain (kg/yr)	NA	NA	101.8 <sup>b</sup>
Fraction Ingested	NA	NA	0.25 <sup>b,d</sup>

<sup>a</sup>Risk Assessment Guidance for Superfund, Vol. 1, Part B (EPA 1991).

<sup>b</sup>Exposure Factors Handbook (EPA August 1997).

<sup>c</sup>EPA Region VI guidance (EPA 1996).

<sup>d</sup>For radionuclides, RESRAD (ANL 1993).

<sup>e</sup>SNL/NM (February 1998).

EPA = U.S. Environmental Protection Agency.

g = Gram(s)

hr = Hour(s).

kg = Kilogram(s).

m = Meter(s).

mg = Milligram(s).

NA = Not applicable.

wk = Week(s).

yr = Year(s).

References

ANL, see Argonne National Laboratory.

Argonne National Laboratory (ANL), 1993. *Manual for Implementing Residual Radioactive Material Guidelines Using RESRAD*, Version 5.0, ANL/EAD/LD-2, Argonne National Laboratory, Argonne, IL.

DOE, see U.S. Department of Energy.

DOE and USAF, see U.S. Department of Energy and U.S. Air Force.

EPA, see U.S. Environmental Protection Agency.

New Mexico Environment Department (NMED), March 2000. "Assessing Human Health Risks Posed by Chemical: Screening-level Risk Assessment," Hazardous and Radioactive Materials Bureau, NMED, March 6, 2000.

New Mexico Environment Department (NMED), December 2000. "Technical Background Document for Development of Soil Screening Levels," Hazardous Waste Bureau and Ground Water Quality Bureau Voluntary Remediation Program, December 18, 2000.

Sandia National Laboratories/New Mexico (SNL/NM), February 1998. "RESRAD Input Parameter Assumptions and Justification," Sandia National Laboratories/New Mexico Environmental Restoration Project, Albuquerque, New Mexico.

U.S. Department of Energy (DOE), 1993. DOE Order 5400.5, "Radiation Protection of the Public and the Environment," U.S. Department of Energy, Washington, D.C.

U.S. Department of Energy (DOE), 1996. "Environmental Assessment of the Environmental Restoration Project at Sandia National Laboratories/New Mexico," U.S. Department of Energy, Kirtland Area Office.

U.S. Department of Energy, U.S. Air Force, and U.S. Forest Service, September 1995. "Workbook: Future Use Management Area 2," prepared by the Future Use Logistics and Support Working Group in cooperation with U.S. Department of Energy Affiliates, the U.S. Air Force, and the U.S. Forest Service.

U.S. Department of Energy, U.S. Air Force, and U.S. Forest Service, October 1995. "Workbook: Future Use Management Area 1," prepared by the Future Use Logistics and Support Working Group in cooperation with U.S. Department of Energy Affiliates, the U.S. Air Force, and the U.S. Forest Service.

U.S. Department of Energy and U.S. Air Force (DOE and USAF), January 1996. "Workbook: Future Use Management Areas 3,4,5,and 6," prepared by the Future Use Logistics and Support Working Group in cooperation with U.S. Department of Energy Affiliates, and the U.S. Air Force.

U.S. Department of Energy and U.S. Air Force (DOE and USAF), March 1996. "Workbook: Future Use Management Area 7," prepared by the Future Use Logistics and Support Working Group in cooperation with U.S. Department of Energy Affiliates and the U.S. Air Force.



U.S. Environmental Protection Agency (EPA), 1989. "Risk Assessment Guidance for Superfund, Volume I: Human Health Evaluation Manual," EPA/540-1089/002, U.S. Environmental Protection Agency, Office of Emergency and Remedial Response, Washington, D.C.

U.S. Environmental Protection Agency (EPA), 1991. "Risk Assessment Guidance for Superfund, Volume I: Human Health Evaluation Manual (Part B)," EPA/540/R-92/003, U.S. Environmental Protection Agency, Office of Emergency and Remedial Response, Washington, D.C.

U.S. Environmental Protection Agency (EPA), 1992. "Dermal Exposure Assessment: Principles and Applications," EPA/600/8-91/011B, Office of Research and Development, Washington, D.C.

U.S. Environmental Protection Agency (EPA), 1996. "Soil Screening Guidance: Technical Background Document," EPA/540/1295/128, Office of Solid Waste and Emergency Response, Washington, D.C.

U.S. Environmental Protection Agency (EPA), August 1997. *Exposure Factors Handbook*, EPA/600/8-89/043, U.S. Environmental Protection Agency, Office of Health and Environmental Assessment, Washington, D.C.

U.S. Environmental Protection Agency (EPA), 1997. (OSWER No. 9200.4-18) *Establishment of Cleanup Levels for CERCLA Sites with Radioactive Contamination*, U.S. EPA Office of Radiation and Indoor Air, Washington D.C, August 1997.

RSI



APR 7 2005

CERTIFIED MAIL – RETURN RECEIPT REQUESTED

Mr James Bearzi, Chief  
Hazardous Waste Bureau  
New Mexico Environment Department  
2905 Rodeo Park Road East, Building 1  
Santa Fe, NM 87505

Dear Mr. Bearzi,

On behalf of the Department of Energy (DOE) and Sandia Corporation, DOE is submitting the enclosed Quality Control (QC) Report, and copies of gamma spectroscopy analytical results for the entire Drain and Septic Systems (DSS) project, in response to the New Mexico Environment Department Request for Supplemental Information: Environmental Restoration Project SWMU Assessment Reports and Proposals for Corrective Action Complete: Drain and Septic Systems Sites 1034, 1035, 1036, 1078, 1079, 1084, 1098, 1104, and 1120, (DSS Round 6); September 2004, Environmental Restoration Project at Sandia National Laboratories, New Mexico, EPA ID No. NM589011518, dated January 14, 2005.

One hardcopy (consisting of seven volumes) will be delivered to Will Moats (NMED), and an electronic CD will be sent by certified mail to you and Laurie King (EPA).

If you have any questions, please contact John Gould at (505) 845-6089.

Sincerely,

Patty Wagner  
Manager

Enclosure

Mr. J. Bearzi

(2)

APR 7 2005

cc w/ enclosure:

W. Moats, NMED-HWB (via Certified Mail)

L. King, EPA, Region 6 (Via Certified Mail)

M. Gardipe, NNSA/SC/ERD

J. Volkerding, DOE-NMED-OB

cc w/o enclosure:

D. Pepe, NMED-OB

J. Estrada, NNSA/SSO, MS 0184

F. Nimick, SNL, MS 1089

R. E. Fate, SNL, MS 1089

M. J. Davis, SNL, MS 1089


D. Stockham, SNL, MS 1087

~~B. Langkopf~~, SNL, MS 1087

P. Puissant, SNL, MS 1087

M. Sanders, SNL, MS 1087

A. Blumberg, SNL, MS 0141



Sandia National Laboratories

---

Drain and Septic Systems Project  
Quality Control (QC) Report

April 2005

Volume 1 of 7  
Master Index  
and

Field Duplicate Relative Percent Difference Tables

Environmental  
Restoration  
Project



United States Department of Energy  
Sandia Site Office

---

**Sandia National Laboratories/New Mexico**  
**Drain and Septic Systems Project Quality Control Report**  
**April 2005**

In response to the New Mexico Environmental Department (NMED) request for supplemental information dated January 14, 2005, the Sandia National Laboratories/New Mexico (SNL/NM) Environmental Restoration (ER) project is providing a complete set of laboratory analytical quality control (QC) documentation for approximately 1,200 soil and associated field blank and duplicate samples collected at the SNL/NM Drain and Septic System (DSS) sites from 1998 to 2002.

The documentation set is comprised of seven report binders. The first binder contains a master index sorted by DSS Site number, and then by analytical parameter. The master index also includes the site names, binder number in which the pertinent QC information can be found for any individual sample, Analytical Request/Chain of Custody (AR/COC) numbers, ER sample IDs, ER sample numbers, sample collection dates, sample matrix, analytical laboratory, and the laboratory analytical batch number for these DSS samples. The first binder also contains tables of calculated relative percent differences (RPDs) for primary and field duplicate sample pairs collected at the DSS sites from 1998 to 2002.

Binders 2 through 5 include the detailed QC information for General Engineering Laboratories (GEL). Binder 6 includes the same type of information for the ER Chemistry Laboratory (ERCL). Binders 2 through 6 include general narratives which address condition on receipt at the laboratory, and sample integrity issues (proper preservation, shipping, AR/COC, etc.). Technical narratives are also provided for each analytical method used. These narratives address holding time and any other specific QC method conformance issues. QC summaries are included for each QC batch. These include the result data and applicable calculations (percent recovery, RPD) for analytical blanks, spikes, and replicates. Finally, Binder 7 includes both complete gamma spectroscopy data documentation, and the associated batch QC from the SNL Radiation Protection Sample Diagnostic (RPSD) Laboratory. For each data set indicated by the AR/COC number, an individual cross reference summary sheet is provided.

**DRAIN AND SEPTIC SYSTEMS PROJECT QC MASTER INDEX**

Site #	Site Name	Binder #	CO#	ER Sample ID	Sample #	SAMPLE DATE	MATRIX	LAB TEST	Lab	BATCH #
1033	Bldg. 6631 SS	Volume 7	600398	ER-1295-6631-DF1-BH1-6-S	041255-005	24-JUN-98	SOIL	GAMMA SPEC	RPSD	801284
1033	Bldg. 6631 SS	Volume 7	600398	ER-1295-6631-DF1-BH2-11-S	041258-005	24-JUN-98	SOIL	GAMMA SPEC	RPSD	801284
1033	Bldg. 6631 SS	Volume 7	600398	ER-1295-6631-DF1-BH2-6-S	041257-005	24-JUN-98	SOIL	GAMMA SPEC	RPSD	801284
1033	Bldg. 6631 SS	Volume 2	600396	ER-1295-6631-BH1-6-11-SD	041255-003	24-JUN-98	SOIL	RCRA METALS	GEL	125097, 125220
1033	Bldg. 6631 SS	Volume 6	600397	ER-1295-6631-DF1-BH1-11-S	041256-004	24-JUN-98	SOIL	MEKC_HE	ERCL	HE-025
1033	Bldg. 6631 SS	Volume 6	600397	ER-1295-6631-DF1-BH1-6-S	041255-004	24-JUN-98	SOIL	MEKC_HE	ERCL	HE-025
1033	Bldg. 6631 SS	Volume 6	600397	ER-1295-6631-DF1-BH2-11-S	041258-004	24-JUN-98	SOIL	MEKC_HE	ERCL	HE-025
1033	Bldg. 6631 SS	Volume 6	600397	ER-1295-6631-DF1-BH2-6-S	041257-004	24-JUN-98	SOIL	MEKC_HE	ERCL	HE-025
1033	Bldg. 6631 SS	Volume 6	600397	ER-1295-6631-EB	041284-008	24-JUN-98	WATER	MEKC_HE	ERCL	HE-025
1033	Bldg. 6631 SS	Volume 6	600397	ER-1295-6631-DF1-BH1-11-S	041256-004	24-JUN-98	SOIL	EPA6020	ERCL	SI98-18
1033	Bldg. 6631 SS	Volume 6	600397	ER-1295-6631-DF1-BH1-6-S	041255-004	24-JUN-98	SOIL	EPA6020	ERCL	SI98-18
1033	Bldg. 6631 SS	Volume 6	600397	ER-1295-6631-DF1-BH2-11-S	041258-004	24-JUN-98	SOIL	EPA6020	ERCL	SI98-18
1033	Bldg. 6631 SS	Volume 6	600397	ER-1295-6631-DF1-BH2-6-S	041257-004	24-JUN-98	SOIL	EPA6020	ERCL	SI98-18
1033	Bldg. 6631 SS	Volume 6	600397	ER-1295-6631-DF1-BH1-11-S	041256-001	24-JUN-98	SOIL	EPA8260	ERCL	SVOC-039
1033	Bldg. 6631 SS	Volume 6	600397	ER-1295-6631-DF1-BH1-6-S	041255-001	24-JUN-98	SOIL	EPA8260	ERCL	SVOC-039
1033	Bldg. 6631 SS	Volume 6	600397	ER-1295-6631-DF1-BH2-11-S	041258-001	24-JUN-98	SOIL	EPA8260	ERCL	SVOC-039
1033	Bldg. 6631 SS	Volume 6	600397	ER-1295-6631-TB	041282-001	24-JUN-98	WATER	EPA8260	ERCL	SVOC-040
1033	Bldg. 6631 SS	Volume 6	600397	ER-1295-6631-DF1-BH2-6-S	041257-001	24-JUN-98	SOIL	EPA8260	ERCL	SVOC-040
1033	Bldg. 6631 SS	Volume 6	600397	ER-1295-6631-EB	041283-001	24-JUN-98	WATER	EPA8260	ERCL	SVOC-040
1033	Bldg. 6631 SS	Volume 6	600397	ER-1295-6631-EB	041284-007	24-JUN-98	WATER	EPA6020	ERCL	WI98-11
1034	Bldg. 6710 SS	Volume 7	605731	6710/1034-SP1-BH1-14-S	059903-003	19-SEP-02	SOIL	GAMMA SPEC	RPSD	201342
1034	Bldg. 6710 SS	Volume 7	605731	6710/1034-SP1-BH1-19-S	059904-003	19-SEP-02	SOIL	GAMMA SPEC	RPSD	201342
1034	Bldg. 6710 SS	Volume 5	605728	6710/1034-SP1-BH1-14-S	059903-002	19-SEP-02	SOIL	PCB-8082	GEL	204381
1034	Bldg. 6710 SS	Volume 5	605728	6710/1034-SP1-BH1-19-S	059904-002	19-SEP-02	SOIL	PCB-8082	GEL	204381
1034	Bldg. 6710 SS	Volume 5	605728	6710/1034-SP1-BH1-14-S	059903-002	19-SEP-02	SOIL	BNA-8270	GEL	204423
1034	Bldg. 6710 SS	Volume 5	605728	6710/1034-SP1-BH1-19-S	059904-002	19-SEP-02	SOIL	BNA-8270	GEL	204423
1034	Bldg. 6710 SS	Volume 5	605728	6710/1034-SP1-BH1-14-S	059903-001	19-SEP-02	SOIL	VOA-8260	GEL	204483
1034	Bldg. 6710 SS	Volume 5	605728	6710/1034-SP1-BH1-19-S	059904-001	19-SEP-02	SOIL	VOA-8260	GEL	204483
1034	Bldg. 6710 SS	Volume 5	605728	6710/1034-SP1-BH1-14-S	059903-002	19-SEP-02	SOIL	HE-8330	GEL	204696
1034	Bldg. 6710 SS	Volume 5	605728	6710/1034-SP1-BH1-19-S	059904-002	19-SEP-02	SOIL	HE-8330	GEL	204696
1034	Bldg. 6710 SS	Volume 5	605728	6710/1034-SP1-BH1-14-S	059903-002	19-SEP-02	SOIL	GROSS-A/B	GEL	205013
1034	Bldg. 6710 SS	Volume 5	605728	6710/1034-SP1-BH1-19-S	059904-002	19-SEP-02	SOIL	GROSS-A/B	GEL	205013
1034	Bldg. 6710 SS	Volume 5	605728	6710/1034-SP1-BH1-14-S	059903-002	19-SEP-02	SOIL	TOTAL-CN	GEL	205123
1034	Bldg. 6710 SS	Volume 5	605728	6710/1034-SP1-BH1-19-S	059904-002	19-SEP-02	SOIL	TOTAL-CN	GEL	205123
1034	Bldg. 6710 SS	Volume 5	605728	6710/1034-SP1-BH1-14-S	059903-002	19-SEP-02	SOIL	Cr+6	GEL	205618
1034	Bldg. 6710 SS	Volume 5	605728	6710/1034-SP1-BH1-19-S	059904-002	19-SEP-02	SOIL	Cr+6	GEL	205620
1034	Bldg. 6710 SS	Volume 5	605728	6710/1034-SP1-BH1-14-S	059903-002	19-SEP-02	SOIL	RCRA METALS	GEL	204452, 204440
1034	Bldg. 6710 SS	Volume 5	605728	6710/1034-SP1-BH1-19-S	059904-002	19-SEP-02	SOIL	RCRA METALS	GEL	204452, 204440
1034	Bldg. 6710 SS	Volume 5	605728	6710/1034-SP1-BH1-14-S	059903-002	19-SEP-02	SOIL	GAMMA SPEC	RPSD	201315
1035	Bldg. 6715 SS	Volume 7	605732	6715/1035-SP1-BH1-11-S	059838-003	12-SEP-02	SOIL	GAMMA SPEC	RPSD	201315
1035	Bldg. 6715 SS	Volume 7	605732	6715/1035-SP1-BH1-16-S	059839-003	12-SEP-02	SOIL	GAMMA SPEC	RPSD	201940
1035	Bldg. 6715 SS	Volume 4	605672	6715/1035-SP1-BH1-11-S	059838-002	12-SEP-02	SOIL	PCB-8082	GEL	201940
1035	Bldg. 6715 SS	Volume 4	605672	6715/1035-SP1-BH1-16-S	059839-002	12-SEP-02	SOIL	PCB-8082	GEL	201940

NOTE: Multiple batch numbers are listed for reanalysis and RCRA metals for the ICP run and the mercury CVAA run.


**DRAIN AND SEPTIC SYSTEMS PROJECT QC MASTER INDEX**

Site #	Site Name	Binder #	COC#	ER Sample ID	Sample #	SAMPLE DATE	MATRIX	LAB TEST	Lab	BATCH #
1035	Bldg. 6715 SS	Volume 4	605672	6715/1035-SP1-BH1-11-S	059838-002	12-SEP-02	SOIL	BNA-8270	GEL	201961
1035	Bldg. 6715 SS	Volume 4	605672	6715/1035-SP1-BH1-16-S	059839-002	12-SEP-02	SOIL	BNA-8270	GEL	201961
1035	Bldg. 6715 SS	Volume 4	605672	6715/1035-SP1-BH1-11-S	059838-002	12-SEP-02	SOIL	HE-8330	GEL	202056
1035	Bldg. 6715 SS	Volume 4	605672	6715/1035-SP1-BH1-16-S	059839-002	12-SEP-02	SOIL	HE-8330	GEL	202056
1035	Bldg. 6715 SS	Volume 4	605672	6715/1035-SP1-BH1-11-S	059838-001	12-SEP-02	SOIL	VOA-8260	GEL	202140
1035	Bldg. 6715 SS	Volume 4	605672	6715/1035-SP1-BH1-16-S	059839-001	12-SEP-02	SOIL	VOA-8260	GEL	202140
1035	Bldg. 6715 SS	Volume 4	605672	6715/1035-SP1-BH1-11-S	059838-002	12-SEP-02	SOIL	TOTAL-CN	GEL	202749
1035	Bldg. 6715 SS	Volume 4	605672	6715/1035-SP1-BH1-16-S	059839-002	12-SEP-02	SOIL	TOTAL-CN	GEL	202749
1035	Bldg. 6715 SS	Volume 4	605672	6715/1035-SP1-BH1-11-S	059838-002	12-SEP-02	SOIL	GROSS-A/B	GEL	203325
1035	Bldg. 6715 SS	Volume 4	605672	6715/1035-SP1-BH1-16-S	059839-002	12-SEP-02	SOIL	GROSS-A/B	GEL	203325
1035	Bldg. 6715 SS	Volume 4	605672	6715/1035-SP1-TB	059827-001	12-SEP-02	AQUEOUS	VOA-8260	GEL	203595
1035	Bldg. 6715 SS	Volume 4	605672	6715/1035-SP1-BH1-11-S	059838-002	12-SEP-02	SOIL	Cr+6	GEL	203661
1035	Bldg. 6715 SS	Volume 4	605672	6715/1035-SP1-BH1-16-S	059839-002	12-SEP-02	SOIL	Cr+6	GEL	203661
1035	Bldg. 6715 SS	Volume 4	605672	6715/1035-SP1-BH1-11-S	059838-002	12-SEP-02	SOIL	RCRA METALS	GEL	202762, 202730
1035	Bldg. 6715 SS	Volume 4	605672	6715/1035-SP1-BH1-16-S	059839-002	12-SEP-02	SOIL	RCRA METALS	GEL	202762, 202730
1036	Bldg. 6922 SS	Volume 2	600351	ER-1295-6922-DF1-BH1-10-S	041273-002	16-JUN-98	SOIL	BNA-8270	GEL	124739
1036	Bldg. 6922 SS	Volume 2	600351	ER-1295-6922-DF1-BH1-5-S	041272-002	16-JUN-98	SOIL	BNA-8270	GEL	124739
1036	Bldg. 6922 SS	Volume 2	600351	ER-1295-6922-DF1-BH2-10-S	041271-003	17-JUN-98	SOIL	BNA-8270	GEL	124739
1036	Bldg. 6922 SS	Volume 2	600351	ER-1295-6922-DF1-BH2-5-S	041275-002	17-JUN-98	SOIL	BNA-8270	GEL	124739
1036	Bldg. 6922 SS	Volume 2	600351	ER-1295-6922-DF1-TB	041274-002	17-JUN-98	SOIL	BNA-8270	GEL	124739
1036	Bldg. 6922 SS	Volume 2	600351	ER-1295-6922-DF1-BH2-10-S	041278-001	16-JUN-98	AQUEOUS	VOA-8260	GEL	124866
1036	Bldg. 6922 SS	Volume 2	600351	ER-1295-6922-DF1-BH2-10-S	041271-003	17-JUN-98	SOIL	HE-8330	GEL	124879
1036	Bldg. 6922 SS	Volume 2	600351	ER-1295-6922-DF1-BH1-10-S	041273-002	16-JUN-98	SOIL	GROSS-A/B	GEL	124917
1036	Bldg. 6922 SS	Volume 2	600351	ER-1295-6922-DF1-BH1-5-S	041272-002	16-JUN-98	SOIL	GROSS-A/B	GEL	124917
1036	Bldg. 6922 SS	Volume 2	600351	ER-1295-6922-DF1-BH2-10-S	041275-002	17-JUN-98	SOIL	GROSS-A/B	GEL	124917
1036	Bldg. 6922 SS	Volume 2	600351	ER-1295-6922-DF1-BH2-5-S	041274-002	17-JUN-98	SOIL	GROSS-A/B	GEL	124917
1036	Bldg. 6922 SS	Volume 2	600351	ER-1295-6922-DF1-BH2-10-SD	041271-001	17-JUN-98	SOIL	VOA-8260	GEL	124946
1036	Bldg. 6922 SS	Volume 2	600351	ER-1295-6922-DF1-BH2-10-S	041271-003	17-JUN-98	SOIL	GAMMA SPEC	GEL	124985
1036	Bldg. 6922 SS	Volume 2	602761	B6922-DF1-BH1-10-S	048279-002	16-AUG-99	SOIL	PCB-8082	GEL	156726
1036	Bldg. 6922 SS	Volume 2	602761	B6922-DF1-BH1-5-S	048278-002	16-AUG-99	SOIL	PCB-8082	GEL	156726
1036	Bldg. 6922 SS	Volume 2	602761	B6922-DF1-BH2-10-S	048281-002	16-AUG-99	SOIL	PCB-8082	GEL	156726
1036	Bldg. 6922 SS	Volume 2	602761	B6922-DF1-BH2-5-S	048280-002	16-AUG-99	SOIL	PCB-8082	GEL	156726
1036	Bldg. 6922 SS	Volume 2	602761	B6922-DF1-BH1-10-S	048279-002	16-AUG-99	SOIL	TOTAL-CN	GEL	156845
1036	Bldg. 6922 SS	Volume 2	602761	B6922-DF1-BH1-5-S	048278-002	16-AUG-99	SOIL	TOTAL-CN	GEL	156845
1036	Bldg. 6922 SS	Volume 2	602761	B6922-DF1-BH2-10-S	048281-002	16-AUG-99	SOIL	TOTAL-CN	GEL	156845
1036	Bldg. 6922 SS	Volume 2	602761	B6922-DF1-BH2-5-S	048280-002	16-AUG-99	SOIL	TOTAL-CN	GEL	156845
1036	Bldg. 6922 SS	Volume 2	602761	B6922-DF1-BH1-10-S	048279-002	16-AUG-99	SOIL	Cr+6	GEL	157829
1036	Bldg. 6922 SS	Volume 2	602761	B6922-DF1-BH1-5-S	048278-002	16-AUG-99	SOIL	Cr+6	GEL	157829
1036	Bldg. 6922 SS	Volume 2	602761	B6922-DF1-BH2-10-S	048281-002	16-AUG-99	SOIL	Cr+6	GEL	157829
1036	Bldg. 6922 SS	Volume 2	602761	B6922-DF1-BH2-5-S	048280-002	16-AUG-99	SOIL	Cr+6	GEL	157829
1036	Bldg. 6922 SS	Volume 7	600353	ER-1295-6922-DF1-BH1-10-S	041273-005	16-JUN-98	SOIL	GAMMA SPEC	RPSD	801228
1036	Bldg. 6922 SS	Volume 7	600353	ER-1295-6922-DF1-BH1-5-S	041272-005	16-JUN-98	SOIL	GAMMA SPEC	RPSD	801228

NOTE: Multiple batch numbers are listed for reanalysis and RCRA metals for the ICP run and the mercury CVAA run.







Sandia National Laboratories

---

Drain and Septic Systems Project  
Quality Control (QC) Report

April 2005

Volume 4 of 7

General Engineering Laboratories, Inc. (GEL) QC Data

Environmental  
Restoration  
Project



United States Department of Energy  
Sandia Site Office

---

GEL QC CROSS REFERENCE


COC 605672


Site #	Site Name	SAMPLE#	F#	DISP_ER_SAMP_LOC	SAMPLE DATE	MATRIX	LAB TEST	BATCH #
1110	Bldg. 6536 Drain	059836	002	6536 HP/1110-DF1-BH2-10-S	12-SEP-02	SOIL	HE-8330	202056
1110	Bldg. 6536 Drain	059836	002	6536 HP/1110-DF1-BH2-10-S	12-SEP-02	SOIL	PCB-8082	201940
1110	Bldg. 6536 Drain	059836	002	6536 HP/1110-DF1-BH2-10-S	12-SEP-02	SOIL	RCRA METALS	202762, 202730
1110	Bldg. 6536 Drain	059836	002	6536 HP/1110-DF1-BH2-10-S	12-SEP-02	SOIL	TOTAL-CN	202749
1110	Bldg. 6536 Drain	059837	001	6536 HP/1110-DF1-BH2-15-S	12-SEP-02	SOIL	VOA-8260	202140
1110	Bldg. 6536 Drain	059837	002	6536 HP/1110-DF1-BH2-15-S	12-SEP-02	SOIL	BNA-8270	201961
1110	Bldg. 6536 Drain	059837	002	6536 HP/1110-DF1-BH2-15-S	12-SEP-02	SOIL	Cr+6	203661
1110	Bldg. 6536 Drain	059837	002	6536 HP/1110-DF1-BH2-15-S	12-SEP-02	SOIL	GROSS-A/B	203325
1110	Bldg. 6536 Drain	059837	002	6536 HP/1110-DF1-BH2-15-S	12-SEP-02	SOIL	HE-8330	202056
1110	Bldg. 6536 Drain	059837	002	6536 HP/1110-DF1-BH2-15-S	12-SEP-02	SOIL	PCB-8082	201940
1110	Bldg. 6536 Drain	059837	002	6536 HP/1110-DF1-BH2-15-S	12-SEP-02	SOIL	RCRA METALS	202762, 202730
1110	Bldg. 6536 Drain	059837	002	6536 HP/1110-DF1-BH2-15-S	12-SEP-02	SOIL	TOTAL-CN	202749
1035	Bldg. 6715 SS	059838	001	6715/1035-SP1-BH1-11-S	12-SEP-02	SOIL	VOA-8260	202140
1035	Bldg. 6715 SS	059838	002	6715/1035-SP1-BH1-11-S	12-SEP-02	SOIL	BNA-8270	201961
1035	Bldg. 6715 SS	059838	002	6715/1035-SP1-BH1-11-S	12-SEP-02	SOIL	Cr+6	203661
1035	Bldg. 6715 SS	059838	002	6715/1035-SP1-BH1-11-S	12-SEP-02	SOIL	GROSS-A/B	203325
1035	Bldg. 6715 SS	059838	002	6715/1035-SP1-BH1-11-S	12-SEP-02	SOIL	HE-8330	202056
1035	Bldg. 6715 SS	059838	002	6715/1035-SP1-BH1-11-S	12-SEP-02	SOIL	PCB-8082	201940
1035	Bldg. 6715 SS	059838	002	6715/1035-SP1-BH1-11-S	12-SEP-02	SOIL	RCRA METALS	202762, 202730
1035	Bldg. 6715 SS	059838	002	6715/1035-SP1-BH1-11-S	12-SEP-02	SOIL	TOTAL-CN	202749
1035	Bldg. 6715 SS	059839	001	6715/1035-SP1-BH1-16-S	12-SEP-02	SOIL	VOA-8260	202140
1035	Bldg. 6715 SS	059839	002	6715/1035-SP1-BH1-16-S	12-SEP-02	SOIL	BNA-8270	201961
1035	Bldg. 6715 SS	059839	002	6715/1035-SP1-BH1-16-S	12-SEP-02	SOIL	Cr+6	203661
1035	Bldg. 6715 SS	059839	002	6715/1035-SP1-BH1-16-S	12-SEP-02	SOIL	GROSS-A/B	203325
1035	Bldg. 6715 SS	059839	002	6715/1035-SP1-BH1-16-S	12-SEP-02	SOIL	HE-8330	202056
1035	Bldg. 6715 SS	059839	002	6715/1035-SP1-BH1-16-S	12-SEP-02	SOIL	PCB-8082	201940
1035	Bldg. 6715 SS	059839	002	6715/1035-SP1-BH1-16-S	12-SEP-02	SOIL	RCRA METALS	202762, 202730
1035	Bldg. 6715 SS	059839	002	6715/1035-SP1-BH1-16-S	12-SEP-02	SOIL	TOTAL-CN	202749
1110	Bldg. 6536 Drain	059840	001	6536/HP1110-TB	12-SEP-02	AQUEOUS	VOA-8260	202140

GEL QC CROSS REFERENCE

COC 605672

Site #	Site Name	SAMPLE#	F#	DISP_ER_SAMP_LOC	SAMPLE DATE	MATRIX	LAB TEST	BATCH #
1110	Bldg. 6536 Drain	059836	002	6536 HP/1110-DF1-BH2-10-S	12-SEP-02	SOIL	HE-8330	202056
1110	Bldg. 6536 Drain	059836	002	6536 HP/1110-DF1-BH2-10-S	12-SEP-02	SOIL	PCB-8082	201940
1110	Bldg. 6536 Drain	059836	002	6536 HP/1110-DF1-BH2-10-S	12-SEP-02	SOIL	RCRA METALS	202762, 202730
1110	Bldg. 6536 Drain	059836	002	6536 HP/1110-DF1-BH2-10-S	12-SEP-02	SOIL	TOTAL-CN	202749
1110	Bldg. 6536 Drain	059836	002	6536 HP/1110-DF1-BH2-10-S	12-SEP-02	SOIL	VOA-8260	202140
1110	Bldg. 6536 Drain	059837	001	6536 HP/1110-DF1-BH2-15-S	12-SEP-02	SOIL	BNA-8270	201961
1110	Bldg. 6536 Drain	059837	002	6536 HP/1110-DF1-BH2-15-S	12-SEP-02	SOIL	Cr+6	203661
1110	Bldg. 6536 Drain	059837	002	6536 HP/1110-DF1-BH2-15-S	12-SEP-02	SOIL	GROSS-A/B	203325
1110	Bldg. 6536 Drain	059837	002	6536 HP/1110-DF1-BH2-15-S	12-SEP-02	SOIL	HE-8330	202056
1110	Bldg. 6536 Drain	059837	002	6536 HP/1110-DF1-BH2-15-S	12-SEP-02	SOIL	PCB-8082	201940
1110	Bldg. 6536 Drain	059837	002	6536 HP/1110-DF1-BH2-15-S	12-SEP-02	SOIL	RCRA METALS	202762, 202730
1110	Bldg. 6536 Drain	059837	002	6536 HP/1110-DF1-BH2-15-S	12-SEP-02	SOIL	TOTAL-CN	202749
1110	Bldg. 6536 Drain	059837	002	6536 HP/1110-DF1-BH2-15-S	12-SEP-02	SOIL	VOA-8260	202140
1035	Bldg. 6715 SS	059838	001	6715/1035-SP1-BH1-11-S	12-SEP-02	SOIL	BNA-8270	201961
1035	Bldg. 6715 SS	059838	002	6715/1035-SP1-BH1-11-S	12-SEP-02	SOIL	Cr+6	203661
1035	Bldg. 6715 SS	059838	002	6715/1035-SP1-BH1-11-S	12-SEP-02	SOIL	GROSS-A/B	203325
1035	Bldg. 6715 SS	059838	002	6715/1035-SP1-BH1-11-S	12-SEP-02	SOIL	HE-8330	202056
1035	Bldg. 6715 SS	059838	002	6715/1035-SP1-BH1-11-S	12-SEP-02	SOIL	PCB-8082	201940
1035	Bldg. 6715 SS	059838	002	6715/1035-SP1-BH1-11-S	12-SEP-02	SOIL	RCRA METALS	202762, 202730
1035	Bldg. 6715 SS	059838	002	6715/1035-SP1-BH1-11-S	12-SEP-02	SOIL	TOTAL-CN	202749
1035	Bldg. 6715 SS	059838	002	6715/1035-SP1-BH1-11-S	12-SEP-02	SOIL	VOA-8260	202140
1035	Bldg. 6715 SS	059839	001	6715/1035-SP1-BH1-16-S	12-SEP-02	SOIL	BNA-8270	201961
1035	Bldg. 6715 SS	059839	002	6715/1035-SP1-BH1-16-S	12-SEP-02	SOIL	Cr+6	203661
1035	Bldg. 6715 SS	059839	002	6715/1035-SP1-BH1-16-S	12-SEP-02	SOIL	GROSS-A/B	203325
1035	Bldg. 6715 SS	059839	002	6715/1035-SP1-BH1-16-S	12-SEP-02	SOIL	HE-8330	202056
1035	Bldg. 6715 SS	059839	002	6715/1035-SP1-BH1-16-S	12-SEP-02	SOIL	PCB-8082	201940
1035	Bldg. 6715 SS	059839	002	6715/1035-SP1-BH1-16-S	12-SEP-02	SOIL	RCRA METALS	202762, 202730
1035	Bldg. 6715 SS	059839	002	6715/1035-SP1-BH1-16-S	12-SEP-02	SOIL	TOTAL-CN	202749
1035	Bldg. 6715 SS	059839	002	6715/1035-SP1-BH1-16-S	12-SEP-02	SOIL	VOA-8260	202140
1110	Bldg. 6536 Drain	059840	001	6536/HP1110-TB	12-SEP-02	AQUEOUS	VOA-8260	202140





Sandia National Laboratories

---

Drain and Septic Systems Project  
Quality Control (QC) Report

April 2005

Volume 7 of 7  
Radiation Protection & Sample Diagnostics (RPSD)  
Laboratory Data

Environmental  
Restoration  
Project



United States Department of Energy  
Sandia Site Office

---

RPSD QC CROSS REFERENCE

COC 605732  
 BATCH NO. 201315

Site #	Site Name	SAMPLE#	F#	ER SAMPLE ID	SAMPLE DATE	MATRIX	LAB TEST
1110	Bldg. 6536 Drain	059828	003	6536HP/1110-DF1-BH1-15-S	10-SEP-02	SOIL	GAMMA SPEC
1110	Bldg. 6536 Drain	059829	003	6536HP/1110-DF1-BH1-20-S	10-SEP-02	SOIL	GAMMA SPEC
1110	Bldg. 6536 Drain	059836	003	6536HP/1110-DF1-BH2-10-S	13-SEP-02	SOIL	GAMMA SPEC
1110	Bldg. 6536 Drain	059837	003	6536HP/1110-DF1-BH2-15-S	13-SEP-02	SOIL	GAMMA SPEC
1035	Bldg. 6715 SS	059838	003	6715/1035-SP1-BH1-11-S	12-SEP-02	SOIL	GAMMA SPEC
1035	Bldg. 6715 SS	059839	003	6715/1035-SP1-BH1-16-S	12-SEP-02	SOIL	GAMMA SPEC
1090	Bldg. 6721 SS	059841	003	6721/1090-DF1-BH1-4-S	13-SEP-02	SOIL	GAMMA SPEC
1090	Bldg. 6721 SS	059842	003	6721/1090-DF1-BH1-9-S	13-SEP-02	SOIL	GAMMA SPEC
1090	Bldg. 6721 SS	059843	003	6721/1090-DF1-BH2-4-S	13-SEP-02	SOIL	GAMMA SPEC
1090	Bldg. 6721 SS	059844	003	6721/1090-DF1-BH2-9-S	13-SEP-02	SOIL	GAMMA SPEC
1090	Bldg. 6721 SS	059847	003	6721/1090-DF1-BH3-4-S	13-SEP-02	SOIL	GAMMA SPEC
1090	Bldg. 6721 SS	059848	003	6721/1090-DF1-BH3-9-S	13-SEP-02	SOIL	GAMMA SPEC
1111	Bldg. 6720 SP	059850	003	6720/1111-SP1-BH1-10-S	13-SEP-02	SOIL	GAMMA SPEC
1111	Bldg. 6720 SP	059851	003	6720/1111-SP1-BH1-15-S	13-SEP-02	SOIL	GAMMA SPEC
1087	Bldg. 6743 SP	059852	003	6743/1087-SP1-BH1-8-S	17-SEP-02	SOIL	GAMMA SPEC
1087	Bldg. 6743 SP	059853	003	6743/1087-SP1-BH1-13-S	17-SEP-02	SOIL	GAMMA SPEC
1089	Bldg. 6734 SP	059854	003	6734/1089-SP1-BH1-9-S	17-SEP-02	SOIL	GAMMA SPEC
1089	Bldg. 6734 SP	059855	003	6734/1089-SP1-BH1-14-S	17-SEP-02	SOIL	GAMMA SPEC
1090	Bldg. 6721 SS	059859	001	6721/1090-DF1-BH2-4-DU	13-SEP-02	SOIL	GAMMA SPEC

J  
COC# 605672



**CASE NARRATIVE**  
**for**  
**Sandia National Laboratories**  
**ARCOC-605671**  
**SDG#67158A**  
**ARCOC-605672**  
**SDG#67158B**  
**ARCOC-605673**  
**SDG#67158C**  
**Case No. 7223.02.03.02**

**October 14, 2002**

**Laboratory Identification:**

General Engineering Laboratories, Inc.

**Mailing Address:**

P.O. Box 30712  
Charleston, South Carolina 29417

**Express Mail Delivery and Shipping Address:**

2040 Savage Road  
Charleston, South Carolina 29407

**Telephone Number:**

(843) 556-8171

**Summary:**

**Sample receipt**

Sandia collected thirty-eight soil samples and eleven aqueous samples on September 9, 10, 12, and 13, 2002. The samples arrived at General Engineering Laboratories, Inc., (GEL) Charleston, South Carolina on September 17, 2002, for environmental analyses. Cooler clearance (screening, temperature check, etc.) was done upon login. The coolers arrived without any visible signs of tampering and with custody seals intact. The samples were delivered with chain of custody documentation and signatures. The temperature of the samples was 3.0, 4.0, and 5.0°C, as measured from the temperature control bottles.

Sample ID 059826-006 was received out of holding. This was the equipment blank for Cr6. Client was contacted regarding the issue. An NCR was generated.

GENERAL ENGINEERING LABORATORIES  
P O Box 30712 • Charleston, SC 29417 • 2040 Savage Road • 29407  
(843) 556-8171 • Fax (843) 766-1178

The samples were screened according to GEL Standard Operating Procedures (SOP) EPI SOP S-007 rev. 2 "The Receiving of Radioactive Samples." The samples were stored properly according to SW-846 procedures and GEL SOP.

The samples were received and collected as listed in the table below:

ARCOC	SDG#	#of samples	Collection Date	Date Rec'd by Lab
605671	67158A	12	09/09/02	09/17/02
605672	67158B	22	09/10/02,09/12/02	09/17/02
605673	67158C	15	09/13/02	09/17/02

The laboratory received the following samples:

**Laboratory ID**  
**ARCOC-605671:**

**Description**

67158001	059820-001
67158002	059821-001
67158003	059822-001
67158004	059823-001
67158005	059824-001
67158006	059825-001
67158020	059820-002
67158021	059821-002
67158022	059822-002
67158023	059823-002
67158024	059824-002
67158025	059825-002

**ARCOC-605672:**

67158007	059828-001
67158008	059829-001
67158009	059836-001
67158010	059837-001
67158011	059838-001
67158012	059839-001
67158026	059828-002
67158027	059829-002
67158028	059836-002
67158029	059837-002
67158030	059838-002
67158031	059839-002
67169001	059827-001
67169002	059826-001
67169003	059840-001
67169005	059826-002
67169006	059826-003

GENERAL ENGINEERING LABORATORIES

P O Box 30712 • Charleston, SC 29417 • 2040 Savage Road • 29407

(843) 556-8171 • Fax (843) 766-1178

Handwritten mark resembling a stylized 'H' or 'A'.

67169007  
67169008  
67169009  
67169010  
67169011

059826-004  
059826-005  
059826-006  
059826-007  
059826-008

**ARCOC-605673:**

67158013  
67158014  
67158015  
67158016  
67158017  
67158018  
67158019  
67158032  
67158033  
67158034  
67158035  
67158036  
67158037  
67158038  
67169004

059841-001  
059842-001  
059843-001  
059844-001  
059845-001  
059847-001  
059848-001  
059841-002  
059842-002  
059843-002  
059844-002  
059846-001  
059847-002  
059848-002  
059849-001

**Case Narrative**

Sample analyses were conducted using methodology as outlined in General Engineering Laboratories (GEL) Standard Operating Procedures. Any technical or administrative problems during analysis, data review, and reduction are contained in the analytical case narratives in the enclosed data package.

**Internal Chain of Custody:**

Custody was maintained for the samples.


6

**Data Package:**

The enclosed data package contains the following sections: Case Narrative, Chain of Custody, Cooler Receipt Checklist, Qualifier Flag and Data Package Definitions, Laboratory Certifications, Volatiles Data, Volatiles QC Summary, Semivolatiles Data, Semivolatiles QC Summary, PCB Data, PCB QC Summary, Explosives Data, Explosives QC Summary, Metals Data, Metals QC Summary, General Chemistry Data, General Chemistry QC Summary, Radiochemistry Data, Radiochemistry QC Summary, and Level C Data Package.

This data package, to the best of my knowledge, is in compliance with technical and administrative requirements.

Edith M. Kent



Project Manager

GENERAL ENGINEERING LABORATORIES

P O Box 30712 • Charleston, SC 29417 • 2040 Savage Road • 29407

(843) 556-8171 • Fax (843) 766-1178

7

**REVISED**

GC/MS Volatile Organics  
Sandia National Labs (SNLS)  
SDG# 67158-1

**Method/Analysis Information**

Procedure: Volatile Organic Compounds (VOC) by Gas Chromatograph/Mass Spectrometer  
Analytical Method: SW846 8260B  
Prep Method: SW846 5030B  
Analytical Batch Number: 203595

**Sample Analysis**

The following client and quality control samples were analyzed to complete this sample delivery group/work order using the methods referenced in the Analysis Information section:

Sample ID	Client ID
67169001	059827-001
67169002	059826-001
67169003	059840-001
67169004	059849-001
1200305537	VBLK01 (Blank)
1200305538	VBLK01LCS (Laboratory Control Sample)

**Preparation/Analytical Method Verification**

**SOP Reference**

Procedure(s) for preparation, analysis and reporting of analytical data are controlled by General Engineering Laboratories, Inc. as Standard Operating Procedure(s) (SOP). The data discussed in this narrative has been analyzed in accordance with GL-OA-E-038 REV.6.

**Calibration Information**

Due to software limitations, all the data files comprising the initial calibration curve may not be listed on the initial calibration summary form. All calibration files are listed in the calibration history report in the "Standard Data" section.

SDG# 67158-1 -VOA

**REVISED**

**Initial Calibration**

All the initial calibration requirements were met.

**CCV Requirements**

All the calibration verification standard (CCV) requirements were met.

**Quality Control (QC) Information**

**Surrogate Recoveries**

Surrogate recoveries, in all samples and quality control samples, were within the acceptance limits.

**Blank Acceptance**

Target analytes were not detected above the reporting limit in the blank.

**LCS Recovery Statement**

All the required analyte recoveries in the laboratory control sample were within the acceptance limits.

**QC Sample Designation**

Matrix spike analyses were analyzed on a sample of similar matrix in SNLS sample delivery group order, # 67354.

**MS Recovery Statement**

All the required matrix spike recoveries were within the acceptance limits.

**MSD Recovery Statement**

All the required matrix spike duplicate recoveries were within the acceptance limits.

**MS/MSD RPD Statement**

The relative percent differences (RPD) between the matrix spike and matrix spike duplicate recoveries were within the acceptance limits.

**Technical Information**

**Holding Time Specifications**

All the samples were prepared and/or analyzed within the required holding time period.

**Sample Preservation and Integrity**

All samples met the sample preservation and integrity requirements.

**Preparation/Analytical Method Verification**

All procedures were performed as stated in the SOP.

**Sample Dilutions**

The samples in this sample delivery group/work order did not require dilutions.

**Sample Re-prep/Re-analysis**

Re-analyses were not required for samples in this sample group/work order.

**Miscellaneous Information**

**Nonconformance (NCR) Documentation**

A nonconformance report was not required for this sample delivery group/work order.

SDG# 67158-1 -VOA



**Manual Integrations**

Data files associated with the initial calibration, continuing calibration check, and samples did not require manual integrations

**Additional Comments**

The following package was generated using an electronic data processing program referred to as "virtual packaging". In an effort to increase quality and efficiency, the laboratory is developing systems to eventually generate all data packages electronically. The following change from "traditional" packages should be noted:

Analyst/peer reviewer initials and dates are not present on the electronic data files. Presently, all initials and dates are on the original raw data. These hard copies are temporary stored in the laboratory. An electronic signature page inserted after the case narrative of each electronic package will indicate the analyst, reviewer, and report specialist names associated with the generation of the data package. The data validator will always sign and date the case narrative. Data that are not generated electronically, and such as hand written pages, will be scanned and inserted into the electronic package.

**TIC Comment**

Tentatively identified compounds (TIC) were not required for this sample delivery group/work order.

**System Configuration**

The laboratory utilizes the following GC/MS configurations:

**Chromatographic Columns**

Chromatographic separation of volatile components is accomplished through analysis on one of the following columns:

Column ID	Column Description
J&W1	DB-624, 60m x 0.25mm, 1.4um
J&W2	DB-624, 75m x 0.53mm, 3.0um

**Instrument Configuration**

Instrument systems are reference in the raw data and individual form headers by the Instrument ID designations below:

Instrument ID	System Configuration	Chromatographic Column	P & T Trap
VOA1	HP6890/HP5973	J&W1	Trap C
VOA2	HP6890/HP5973	J&W1	Trap C
VOA4	HP5890/HP5972	J&W1	Trap K
VOA5	HP5890/HP5972	J&W1	Trap C
VOA7	HP5890/HP5972	J&W2	Trap K

SDG# 67158-1 -VOA

VOA8	HP6890/HP5973	J&W1	Trap K
VOA9	HP6890/HP5973	J&W1	Trap C

**Certification Statement**

Where the analytical method has been performed under NELAP certification, the analysis has met all of the requirements of the NELAC standard unless otherwise noted in the analytical case narrative.

**Review Validation**

GEL requires all analytical data to be verified by a qualified data validator. In addition, all data designated for CLP or CLP-like packaging will receive a third level validation upon completion of the data package.

The following data validator verified the information presented in this case narrative:

Reviewer: *Nick Mulley* Date: 10/15/02



## QC Summary

Client : Sandia National Laboratories  
 MS-0756  
 P.O. Box 5800  
 Albuquerque, New Mexico  
 Contact: Pamela M. Puissant  
 Workorder: 67169

Report Date: September 30, 2002  
 Page 1 of 4

Parameter	NOM	Sample Qual	QC	Units	RPD%	REC%	Range	Anlst	Date Time
<b>Volatile-GC/MS Federal</b>									
Batch	203595								
QC1200305538	LCS								
1,1-Dichloroethylene	50.0		45.0	ug/L		90	(78%-140%)	MAP	09/24/02 06:58
Benzene	50.0		45.8	ug/L		92	(78%-119%)		
Chlorobenzene	50.0		49.4	ug/L		99	(82%-120%)		
Toluene	50.0		50.3	ug/L		101	(68%-133%)		
Trichloroethylene	50.0		47.1	ug/L		94	(80%-123%)		
**Bromofluorobenzene	50.0		64.8	ug/L		130	(67%-136%)		
**Dibromofluoromethane	50.0		60.5	ug/L		121	(62%-148%)		
**Toluene-d8	50.0		58.7	ug/L		117	(58%-139%)		
QC1200306542	LCS								
1,1-Dichloroethylene	50.0		49.6	ug/L		99	(78%-140%)		09/25/02 10:00
Benzene	50.0		46.9	ug/L		94	(78%-119%)		
Chlorobenzene	50.0		50.9	ug/L		102	(82%-120%)		
Toluene	50.0		52.0	ug/L		104	(68%-133%)		
Trichloroethylene	50.0		50.7	ug/L		101	(80%-123%)		
**Bromofluorobenzene	50.0		64.2	ug/L		128	(67%-136%)		
**Dibromofluoromethane	50.0		61.4	ug/L		123	(62%-148%)		
**Toluene-d8	50.0		57.7	ug/L		115	(58%-139%)		
QC1200307213	LCS								
1,1-Dichloroethylene	50.0		44.0	ug/L		88	(78%-140%)		09/24/02 18:08
Benzene	50.0		45.4	ug/L		91	(78%-119%)		
Chlorobenzene	50.0		47.2	ug/L		94	(82%-120%)		
Toluene	50.0		46.7	ug/L		93	(68%-133%)		
Trichloroethylene	50.0		46.9	ug/L		94	(80%-123%)		
**Bromofluorobenzene	50.0		62.7	ug/L		125	(67%-136%)		
**Dibromofluoromethane	50.0		63.4	ug/L		127	(62%-148%)		
**Toluene-d8	50.0		56.8	ug/L		114	(58%-139%)		
QC1200305537	MB								
1,1,1-Trichloroethane		U	ND	ug/L					09/24/02 08:17
1,1,2,2-Tetrachloroethane		U	ND	ug/L					
1,1,2-Trichloroethane		U	ND	ug/L					
1,1-Dichloroethane		U	ND	ug/L					
1,1-Dichloroethylene		U	ND	ug/L					
1,2-Dichloroethane		U	ND	ug/L					
1,2-Dichloropropane		U	ND	ug/L					
2-Butanone		U	ND	ug/L					
2-Hexanone		U	ND	ug/L					
4-Methyl-2-pentanone		U	ND	ug/L					
Acetone		U	ND	ug/L					
Benzene		U	ND	ug/L					
Bromodichloromethane		U	ND	ug/L					
Bromoform		U	ND	ug/L					
Bromomethane		U	ND	ug/L					

## QC Summary

Workorder: 67169

Parname	NOM	Sample	Qual	QC	Units	RPD%	REC%	Range	Anlst	Date	Time
Volatile-GC/MS Federal											
Batch	203595										
Carbon disulfide			U	ND	ug/L						
Carbon tetrachloride			U	ND	ug/L						
Chlorobenzene			U	ND	ug/L						
Chloroethane			U	ND	ug/L						
Chloroform			U	ND	ug/L						
Chloromethane			U	ND	ug/L						
Dibromochloromethane			U	ND	ug/L						
Ethylbenzene			U	ND	ug/L						
Methylene chloride			U	ND	ug/L						
Styrene			U	ND	ug/L						
Tetrachloroethylene			U	ND	ug/L						
Toluene			U	ND	ug/L						
Trichloroethylene			U	ND	ug/L						
Vinyl chloride			U	ND	ug/L						
Xylenes (total)			U	ND	ug/L						
cis-1,2-Dichloroethylene			U	ND	ug/L						
cis-1,3-Dichloropropylene			U	ND	ug/L						
trans-1,2-Dichloroethylene			U	ND	ug/L						
trans-1,3-Dichloropropylene			U	ND	ug/L						
**Bromofluorobenzene	50.0			63.9	ug/L		128	(67%-136%)			
**Dibromofluoromethane	50.0			63.1	ug/L		126	(62%-148%)			
Toluene-d8	50.0			56.8	ug/L		114	(58%-139%)			
QC1200306541 MB											09/25/02 11:19
1,1,1-Trichloroethane			U	ND	ug/L						
1,1,2,2-Tetrachloroethane			U	ND	ug/L						
1,1,2-Trichloroethane			U	ND	ug/L						
1,1-Dichloroethane			U	ND	ug/L						
1,1-Dichloroethylene			U	ND	ug/L						
1,2-Dichloroethane			U	ND	ug/L						
1,2-Dichloropropane			U	ND	ug/L						
2-Butanone			U	ND	ug/L						
2-Hexanone			U	ND	ug/L						
4-Methyl-2-pentanone			U	ND	ug/L						
Acetone			U	ND	ug/L						
Benzene			U	ND	ug/L						
Bromodichloromethane			U	ND	ug/L						
Bromoform			U	ND	ug/L						
Bromomethane			U	ND	ug/L						
Carbon disulfide			U	ND	ug/L						
Carbon tetrachloride			U	ND	ug/L						
Chlorobenzene			U	ND	ug/L						
Chloroethane			U	ND	ug/L						
Chloroform			U	ND	ug/L						
Chloromethane			U	ND	ug/L						
Dibromochloromethane			U	ND	ug/L						
Ethylbenzene			U	ND	ug/L						
Methylene chloride			U	ND	ug/L						
Styrene			U	ND	ug/L						

## QC Summary

Workorder: 67169

Page 3 of 4

Parname	NOM	Sample	Qual	QC	Units	RPD%	REC%	Range	Anlist	Date	Time
Volatile-GC/MS Federal											
Batch	203595										
Tetrachloroethylene			U	ND	ug/L						
Toluene			U	ND	ug/L						
Trichloroethylene			U	ND	ug/L						
Vinyl chloride			U	ND	ug/L						
Xylenes (total)			U	ND	ug/L						
cis-1,2-Dichloroethylene			U	ND	ug/L						
cis-1,3-Dichloropropylene			U	ND	ug/L						
trans-1,2-Dichloroethylene			U	ND	ug/L						
trans-1,3-Dichloropropylene			U	ND	ug/L						
**Bromofluorobenzene	50.0			61.9	ug/L		124	(67%-136%)			
**Dibromofluoromethane	50.0			60.7	ug/L		121	(62%-148%)			
**Toluene-d8	50.0			56.3	ug/L		113	(58%-139%)			
QC1200307212 MB											
1,1,1-Trichloroethane			U	ND	ug/L					09/24/02	19:27
1,1,2,2-Tetrachloroethane			U	ND	ug/L						
1,1,2-Trichloroethane			U	ND	ug/L						
1,1-Dichloroethane			U	ND	ug/L						
1,1-Dichloroethylene			U	ND	ug/L						
1,2-Dichloroethane			U	ND	ug/L						
1,2-Dichloropropane			U	ND	ug/L						
2-Butanone			U	ND	ug/L						
2-Hexanone			U	ND	ug/L						
4-Methyl-2-pentanone			U	ND	ug/L						
Acetone			U	ND	ug/L						
Benzene			U	ND	ug/L						
Bromodichloromethane			U	ND	ug/L						
Bromoform			U	ND	ug/L						
Bromomethane			U	ND	ug/L						
Carbon disulfide			U	ND	ug/L						
Carbon tetrachloride			U	ND	ug/L						
Chlorobenzene			U	ND	ug/L						
Chloroethane			U	ND	ug/L						
Chloroform			U	ND	ug/L						
Chloromethane			U	ND	ug/L						
Dibromochloromethane			U	ND	ug/L						
Ethylbenzene			U	ND	ug/L						
Methylene chloride			U	ND	ug/L						
Styrene			U	ND	ug/L						
Tetrachloroethylene			U	ND	ug/L						
Toluene			U	ND	ug/L						
Trichloroethylene			U	ND	ug/L						
Vinyl chloride			U	ND	ug/L						
Xylenes (total)			U	ND	ug/L						
cis-1,2-Dichloroethylene			U	ND	ug/L						
cis-1,3-Dichloropropylene			U	ND	ug/L						
trans-1,2-Dichloroethylene			U	ND	ug/L						
trans-1,3-Dichloropropylene			U	ND	ug/L						
**Bromofluorobenzene	50.0			60.6	ug/L		121	(67%-136%)			

## QC Summary

Workorder: 67169

Page 4 of 4

Parmaame	NOM	Sample	Qual	QC	Units	RPD%	REC%	Range	Anist	Date	Time
Volatile-GC/MS Federal											
Batch 203595											
**Dibromofluoromethane	50.0			62.2	ug/L		124	(62%-148%)			
**Toluene-d8	50.0			56.8	ug/L		114	(58%-139%)			
QC1200305539 67354001 PS											
1,1-Dichloroethylene	50.0	U	ND	43.1	ug/L		86	(67%-129%)		09/25/02	15:07
Benzene	50.0	U	ND	44.0	ug/L		88	(74%-112%)			
Chlorobenzene	50.0	U	ND	45.8	ug/L		92	(77%-113%)			
Toluene	50.0	U	ND	46.1	ug/L		92	(74%-109%)			
Trichloroethylene	50.0	U	ND	44.8	ug/L		90	(71%-118%)			
**Bromofluorobenzene	50.0		61.5	64.1	ug/L		128	(67%-136%)			
**Dibromofluoromethane	50.0		61.2	64.1	ug/L		128	(62%-148%)			
**Toluene-d8	50.0		56.6	59.1	ug/L		118	(58%-139%)			
QC1200305540 67354001 PSD											
1,1-Dichloroethylene	50.0	U	ND	40.5	ug/L	6	81	(0%-11%)		09/25/02	15:33
Benzene	50.0	U	ND	42.0	ug/L	5	84	(0%-8%)			
Chlorobenzene	50.0	U	ND	44.4	ug/L	3	89	(0%-11%)			
Toluene	50.0	U	ND	44.1	ug/L	5	88	(0%-12%)			
Trichloroethylene	50.0	U	ND	42.9	ug/L	4	86	(0%-9%)			
**Bromofluorobenzene	50.0		61.5	65.5	ug/L		131	(67%-136%)			
**Dibromofluoromethane	50.0		61.2	63.3	ug/L		127	(62%-148%)			
**Toluene-d8	50.0		56.6	59.2	ug/L		118	(58%-139%)			

**Notes:**

RER is calculated at the 95% confidence level (2-sigma).

The Qualifiers in this report are defined as follows:

- \* Recovery or %RPD not within acceptance limits and/or spike amount not compatible with the sample or the duplicate RPD's are not applicable where t
- \*\* Indicates analyte is a surrogate compound.
- B The analyte was found in the blank above the effective MDL.
- H Holding time was exceeded
- J Estimated value, the analyte concentration fell above the effective MDL and below the effective PQL
- P The response between the confirmation column and the primary column is >40%D
- U The analyte was analyzed for but not detected below this concentration. For Organic and Inorganic analytes the result is less than the effective MDL. J
- X Presumptive evidence that the analyte is not present. Please see narrative for further information.
- X Presumptive evidence that the analyte is not present. Please see narrative for further information.
- X Uncertain identification for gamma spectroscopy.

N/A indicates that spike recovery limits do not apply when sample concentration exceeds spike conc. by a factor of 4 or more.

^ The Relative Percent Difference (RPD) obtained from the sample duplicate (DUP) is evaluated against the acceptance criteria when the sample is greater than five times (5X) the contract required detection limit (RL). In cases where either the sample or duplicate value is less than 5X the RL, a control limit of +/- the RL is used to evaluate the DUP result.

For PS, PSD, and SDILT results, the values listed are the measured amounts, not final concentrations.

Where the analytical method has been performed under NELAP certification, the analysis has met all of the requirements of the NELAC standard unless qualified on the QC Summary.

**REVISED**

GC/MS Volatile Organics  
Sandia National Labs (SNLS)  
SDG# 67158

Method/Analysis Information

Procedure: Volatile Organic Compounds (VOC) by Gas Chromatograph/Mass Spectrometer  
Analytical Method: SW846 8260A  
Prep Method: SW846 5030  
Analytical Batch Number: 202140  
Prep Batch Number: 202138

Sample Analysis

The following client and quality control samples were analyzed to complete this sample delivery group/work order using the methods referenced in the Analysis Information section:

Sample ID	Client ID
67158001	059820-001
67158002	059821-001
67158003	059822-001
67158004	059823-001
67158005	059824-001
67158006	059825-001
67158007	059828-001
67158008	059829-001
67158009	059836-001
67158010	059837-001
67158011	059838-001
67158012	059839-001
67158013	059841-001

SDG# 67158 -VOA

**REVISED**

67158014	059842-001
67158015	059843-001
67158016	059844-001
67158017	059845-001
67158018	059847-001
67158019	059848-001
1200301914	VBLK01 (Blank)
1200301915	VBLK01LCS (Laboratory Control Sample)
1200301916	059820-001MS (Matrix Spike)
1200301917	059820-001MSD (Matrix Spike Duplicate)

**Preparation/Analytical Method Verification**

**SOP Reference**

Procedure for preparation, analysis and reporting of analytical data are controlled by General Engineering Laboratories, Inc. as Standard Operating Procedure (SOP). The data discussed in this narrative has been analyzed in accordance with GL-OA E 026 REV.8.

**Calibration Information**

Due to software limitations, all the data files comprising the initial calibration curve may not be listed on the initial calibration summary form. All calibration files are listed in the calibration history report in the "Standard Data" section.

**Initial Calibration**

All the initial calibration requirements were met.

**CCV Requirements**

All the calibration verification standard (CCV) requirements were met.

**Quality Control (QC) Information**

**Surrogate Recoveries**

Surrogate recoveries, in all samples and quality control samples, were within the acceptance limits.

**Blank Acceptance**

Target analytes were not detected above the reporting limit in the blank.

**LCS Recovery Statement**

All the required analyte recoveries in the laboratory control sample were within the acceptance limits.

**QC Sample Designation**

The following sample was designated for matrix spike analysis:

SDG# 67158 -VOA

Page 2 of 4

**REVISED**

67158001 059820 001

**MS Recovery Statement**

All the required matrix spike recoveries were within the acceptance limits.

**MSD Recovery Statement**

All the required matrix spike duplicate recoveries were within the acceptance limits.

**MS/MSD RPD Statement**

The relative percent differences (RPD) between the matrix spike and matrix spike duplicate recoveries were within the acceptance limits.

**Internal Standard (ISTD) Acceptance**

The internal standard responses, in all samples and quality control samples, met the required acceptance criteria.

**Technical Information**

**Holding Time Specifications**

All the samples were prepared and/or analyzed within the required holding time period.

**Sample Preservation and Integrity**

All samples met the sample preservation and integrity requirements.

**Preparation/Analytical Method Verification**

All procedures were performed as stated in the SOP.

**Sample Dilutions**

The samples in this sample delivery group/work order did not require dilutions.

**Sample Re-prep/Re-analysis**

Re-analyses were not required for samples in this sample group/work order.

**Miscellaneous Information**

**Nonconformance (NCR) Documentation**

A nonconformance report was not required for this sample delivery group/work order.

**Manual Integrations**

Data files associated with the initial calibration, continuing calibration check, and samples did not require manual integrations.

**Additional Comments**

The following package was generated using an electronic data processing program referred to as "virtual packaging". In an effort to increase quality and efficiency, the laboratory is developing systems to eventually generate all data packages electronically. The following change from "traditional" packages should be noted: Analyst/peer reviewer initials and dates are not present on the electronic data files. Presently, all initials and dates are on the original raw data. These hard copies are temporarily stored in the laboratory. An electronic signature page inserted after the case narrative of each electronic package will indicate the analyst, reviewer, and report specialist names associated with the generation of the data package. The data validator will always sign and date the case narrative. Data that are not generated electronically, and such as hand written pages, will be scanned and inserted into the electronic package.

SDG# 67158 -VOA

Page 3 of 4

**REVISED**

**TIC Comment**

Tentatively identified compounds (TIC) were not required for this sample delivery group/work order.

**System Configuration**

The laboratory utilizes the following GC/MS configurations:

**Chromatographic Columns**

Chromatographic separation of volatile components is accomplished through analysis on one of the following columns:

Column ID	Column Description
J&W1	DB-624, 60m x 0.25mm, 1.4um
J&W2	DB-624, 75m x 0.53mm, 3.0um

**Instrument Configuration**

Instrument systems are reference in the raw data and individual form headers by the Instrument ID designations below:

Instrument ID	System Configuration	Chromatographic Column	P & T Trap
VOA1	HP6890/HP5973	J&W1	Trap C
VOA2	HP6890/HP5973	J&W1	Trap C
VOA4	HP5890/HP5972	J&W1	Trap K
VOA5	HP5890/HP5972	J&W1	Trap C
VOA7	HP5890/HP5972	J&W2	Trap K
VOA8	HP6890/HP5973	J&W1	Trap K
VOA9	HP6890/HP5973	J&W1	Trap C

**Certification Statement**

Where the analytical method has been performed under NELAP certification, the analysis has met all of the requirements of the NELAC standard unless otherwise noted in the analytical case narrative.

**Review Validation**

GEL requires all analytical data to be verified by a qualified data validator. In addition, all data designated for CLP or CLP-like packaging will receive a third level validation upon completion of the data package.

The following data validator verified the information presented in this case narrative:

Reviewer: *Neil Mulligan* Date: 10/15/02

SDG# 67158 -VOA



## QC Summary

Report Date: October 10, 2002

Page 1 of 3

Client : Sandia National Laboratories  
 MS-0756  
 P.O. Box 5800  
 Albuquerque, New Mexico

Contact: Pamela M. Puissant

Workorder: 67158

Parname	NOM	Sample Qual	QC	Units	RPD%	REC%	Range	Anlst	Date Time
Volatile-GC/MS Federal									
Batch 202140									
QC1200301915 LCS									
1,1-Dichloroethylene	50.0		45.8	ug/kg		92	(75%-134%)	TLW	09/20/02 21:06
Benzene	50.0		47.3	ug/kg		95	(80%-120%)		
Chlorobenzene	50.0		49.0	ug/kg		98	(82%-118%)		
Toluene	50.0		47.5	ug/kg		95	(74%-115%)		
Trichloroethylene	50.0		46.1	ug/kg		92	(80%-119%)		
**Bromofluorobenzene	50.0		56.1	ug/kg		112	(69%-138%)		
**Dibromofluoromethane	50.0		62.7	ug/kg		125	(67%-137%)		
**Toluene-d8	50.0		61.0	ug/kg		122	(67%-139%)		
QC1200301914 MB									
1,1,1-Trichloroethane		U	ND	ug/kg					09/20/02 22:02
1,1,2,2-Tetrachloroethane		U	ND	ug/kg					
1,1,2-Trichloroethane		U	ND	ug/kg					
1,1-Dichloroethane		U	ND	ug/kg					
1,1-Dichloroethylene		U	ND	ug/kg					
1,2-Dichloroethane		U	ND	ug/kg					
1,2-Dichloropropane		U	ND	ug/kg					
2-Butanone		U	ND	ug/kg					
2-Hexanone		U	ND	ug/kg					
4-Methyl-2-pentanone		U	ND	ug/kg					
Acetone		U	ND	ug/kg					
Benzene		U	ND	ug/kg					
Bromodichloromethane		U	ND	ug/kg					
Bromoform		U	ND	ug/kg					
Bromomethane		U	ND	ug/kg					
Carbon disulfide		U	ND	ug/kg					
Carbon tetrachloride		U	ND	ug/kg					
Chlorobenzene		U	ND	ug/kg					
Chloroethane		U	ND	ug/kg					
Chloroform		U	ND	ug/kg					
Chloromethane		U	ND	ug/kg					
Dibromochloromethane		U	ND	ug/kg					
Ethylbenzene		U	ND	ug/kg					
Methylene chloride		U	ND	ug/kg					
Styrene		U	ND	ug/kg					
Tetrachloroethylene		U	ND	ug/kg					
Toluene		U	ND	ug/kg					
Trichloroethylene		U	ND	ug/kg					
Vinyl acetate		U	ND	ug/kg					
Vinyl chloride		U	ND	ug/kg					
Xylenes (total)		U	ND	ug/kg					
cis-1,2-Dichloroethylene		U	ND	ug/kg					
cis-1,3-Dichloropropylene		U	ND	ug/kg					

## QC Summary

Workorder: 67158

Page 2 of 3

Parname	NOM	Sample	Qual	QC	Units	RPD%	REC%	Range	Anlst	Date Time
Volatile-GC/MS Federal										
Batch 202140										
trans-1,2-Dichloroethylene			U	ND	ug/kg					
trans-1,3-Dichloropropylene			U	ND	ug/kg					
**Bromofluorobenzene	50.0			59.0	ug/kg		118	(69%-138%)		
**Dibromofluoromethane	50.0			62.8	ug/kg		126	(67%-137%)		
**Toluene-d8	50.0			64.4	ug/kg		129	(67%-139%)		
QC1200301916 67158001 PS										
1,1-Dichloroethylene	50.0	U	ND	43.7	ug/L		87	(55%-128%)		09/21/02 07:12
Benzene	50.0	U	ND	41.5	ug/L		83	(53%-118%)		
Chlorobenzene	50.0	U	ND	39.2	ug/L		78	(53%-116%)		
Toluene	50.0	U	ND	39.8	ug/L		80	(56%-113%)		
Trichloroethylene	50.0	U	ND	44.7	ug/L		89	(54%-119%)		
**Bromofluorobenzene	50.0		60.0	58.0	ug/L		116	(69%-138%)		
**Dibromofluoromethane	50.0		63.5	67.3	ug/L		135	(67%-137%)		
**Toluene-d8	50.0		62.0	61.0	ug/L		122	(67%-139%)		
QC1200301917 67158001 PSD										
1,1-Dichloroethylene	50.0	U	ND	41.6	ug/L	5	83	(0%-21%)		09/21/02 07:40
Benzene	50.0	U	ND	42.0	ug/L	1	84	(0%-17%)		
Chlorobenzene	50.0	U	ND	39.7	ug/L	1	80	(0%-21%)		
Toluene	50.0	U	ND	39.9	ug/L	0	80	(0%-25%)		
Trichloroethylene	50.0	U	ND	43.3	ug/L	3	87	(0%-25%)		
**Bromofluorobenzene	50.0		60.0	59.7	ug/L		119	(69%-138%)		
**Dibromofluoromethane	50.0		63.5	64.0	ug/L		128	(67%-137%)		
*Toluene-d8	50.0		62.0	62.1	ug/L		124	(67%-139%)		

**Notes:**

RER is calculated at the 95% confidence level (2-sigma).

The Qualifiers in this report are defined as follows:

- \* Recovery or %RPD not within acceptance limits and/or spike amount not compatible with the sample or the duplicate; RPD's are not applicable where
- \*\* Indicates analyte is a surrogate compound.
- B The analyte was found in the blank above the effective MDL.
- H Holding time was exceeded
- J Estimated value, the analyte concentration fell above the effective MDL and below the effective PQL
- P The response between the confirmation column and the primary column is >40%D
- U The analyte was analyzed for but not detected below this concentration. For Organic and Inorganic analytes the result is less than the effective MDL. I
- X Presumptive evidence that the analyte is not present. Please see narrative for further information.
- X Presumptive evidence that the analyte is not present. Please see narrative for further information.
- X Uncertain identification for gamma spectroscopy.

## QC Summary

Workorder: 67158

Page 3 of 3

Parmname	NOM	Sample	Qual	QC	Units	RPD%	REC%	Range	Anlst	Date	Time
----------	-----	--------	------	----	-------	------	------	-------	-------	------	------

N/A indicates that spike recovery limits do not apply when sample concentration exceeds spike conc. by a factor of 4 or more.

^ The Relative Percent Difference (RPD) obtained from the sample duplicate (DUP) is evaluated against the acceptance criteria when the sample is greater than five times (5X) the contract required detection limit (RL). In cases where either the sample or duplicate value is less than 5X the RL, a control limit of +/- the RL is used to evaluate the DUP result.

For PS, PSD, and SDILT results, the values listed are the measured amounts, not final concentrations.

Where the analytical method has been performed under NELAP certification, the analysis has met all of the requirements of the NELAC standard unless qualified on the QC Summary.

**Semi-Volatile Case Narrative  
Sandia National Labs (SNLS)  
SDG 67158-1**

**Method/Analysis Information**

**Procedure:** Semivolatile Analysis by Gas Chromatograph/Mass Spectrometer  
**Analytical Method:** SW846 8270C  
**Prep Method:** SW846 3510C  
**Analytical Batch Number:** 201951  
**Prep Batch Number:** 201948

**Sample Analysis**

The following samples were analyzed using the analytical protocol as established in SW846 8270C:

<b>Sample ID</b>	<b>Client ID</b>
67169005	059826-002
1200301424	SBLK01 (Blank)
1200301425	SBLK01LCS (Laboratory Control Sample)
1200301426	059826-002MS (Matrix Spike)
1200301427	059826-002MSD (Matrix Spike Duplicate)

**Preparation/Analytical Method Verification**

Procedures for preparation, analysis, and reporting of analytical data are documented by General Engineering Laboratories, Inc. (GEL) as Standard Operating Procedures (SOP).

**Calibration Information**

Due to the limited capacity of software we do not display all of the current initial calibration files here. If necessary, a calibration history will be inserted in the package prior to the appropriate Form 6.

Diphenylamine has now superseded N-Nitroso-diphenylamine as a CCC on Quantitation Reports, Initial Calibration Reports, Calibration Check Standard Reports, etc. Previous versions of EPA Method 8270 (prior to 8270C) listed N-Nitroso-diphenylamine as a CCC. However, as stated in EPA Method 8270C, Revision 3, December, 1996, Section 1.4.5, "N-Nitroso-diphenylamine decomposes in the gas chromatographic inlet and cannot be separated from Diphenylamine." Studies of these two compounds at GEL, both independent of each other and together, show that they not only coelute, but also have similar mass spectra. N-Nitroso-diphenylamine and Diphenylamine will be reported as Diphenylamine on all reports and forms.

When calibrations are performed for Appendix IX compounds some of the compounds may not be calibrated exactly according to the criteria in Method 8270C. If the %RSD is greater than 15% or the correlation coefficient is less than 0.99 then the analyte is quantitated using the response factor. If the analyte is detected then the sample is reanalyzed for that analyte on an instrument that is compliant with the criteria in the method.

**Initial Calibration**

All initial calibration requirements have been met for this SDG.

**CCV Requirements**

All calibration verification standard (CVS, ICV or CCV) requirements have been met for this SDG.

**Quality Control (QC) Information**

**Surrogate Recoveries**

All the surrogate recoveries were within the established acceptance criteria for this SDG.

**Blank Acceptance**

Target analytes were detected in the blank below the reporting limit.

**LCS Recovery Statement**

The laboratory control sample (LCS) spike recoveries for this SDG were within the established acceptance limits.

**QC Sample Designation**

The following sample analyzed with this SDG was chosen for matrix spike analysis.  
67169005 (059826-002)

**MS Recovery Statement**

The matrix spike recoveries for this SDG were within the established acceptance limits.

**MSD Recovery Statement**

The matrix spike duplicate (MSD) recoveries for this SDG were within the established acceptance limits.

**MS/MSD RPD Statement**

The relative percent differences (RPD) between each MS and MSD were within the required acceptance limits.

**Internal Standard (ISTD) Acceptance**

The internal standard responses were within the required acceptance criteria for all samples and QC.

**Technical Information:****Holding Time Specifications**

All samples in this SDG met the specified holding time requirements. GEL assigns holding times based on the associated methodology that assigns the date and time from sample collection or sample receipt. Those holding times expressed in hours are calculated in the AlphaLIMS system. Those holding times expressed as days expire at midnight on the day of expiration. GEL assigns holding times based on the associated methodology that assigns the date and time from sample collection or sample receipt. Those holding times expressed in hours are calculated in the AlphaLIMS system. Those holding times expressed as days expire at midnight on the day of expiration.

**Preparation/Analytical Method Verification**

All procedures were performed as stated in the SOP.

**Sample Dilutions**

None of the samples analyzed in this SDG required dilution.

**Miscellaneous Information:****Nonconformance (NCR) Documentation**

No nonconformance report (NCR) was generated for this SDG.

**Manual Integrations**

No manual integrations were required for any data file in this SDG.

**Additional Comments**

No additional comments are needed for this SDG.

**System Configuration**

The laboratory utilizes a HP 6890 Series gas chromatograph and a HP 5973 Mass Selective Detector. The configuration is equipped with the electronic pressure control. All MS interfaces are capillary direct.

## Chromatographic Columns

Chromatographic separation of semivolatile components is accomplished through analysis on one or more of the following columns (all with dimensions of 30 meters x 0.25 millimeters ID and 0.25 micron film except J&W DB-5MS2 which is 25 meters x 0.20 mm ID and 0.33 micron film):

Column ID	Column Description
J&W	DB-5.625(5% Phenyl)-methylpolysiloxane (identified by a DB-5.625 designation on quantitation reports and reconstructed ion chromatograms)
J&W DB-5MS	Similar to the J&W DB-5.625 with low bleed characteristics (identified by a DB-5MS designation)
Alltech	EC-5 (SE-54) 5% Phenyl, 95% Methylpolysiloxane (identified by a HP-5MS designation)
HP	HP-5MS 5% Phenylmethylsiloxane (identified by a HP-5MS designation)
Phenomenex	ZB-5 5% Phenyl Polysiloxane (identified by a ZB-5 designation)
J&W DB-5MS2	Similar to the J&W DB-5.625 with low bleed characteristics (identified by a DB-5MS2 designation)

## Instrument Configuration

The samples reported in this SDG were analyzed on one or more of the following instrument systems. Instrument systems are referenced in the raw data and individual form headers by the Instrument ID designations listed below:

Instrument ID	System Configuration	Chromatographic Column
MSD2	HP6890/HP5973	DB-5MS2
MSD4	HP6890/HP5973	DB-5MS2
MSD5	HP6890/HP5973	DB-5MS2
MSD7	HP6890/HP5973	DB-5MS2
MSD8	HP6890/HP5973	DB-5MS2

**Certification Statement**

\* Where the analytical method has been performed under NELAP certification, the analysis has met all of the requirements of the NELAC standard unless otherwise noted in the analytical case narrative.

**Review Validation:**

GEL requires all analytical data to be verified by a qualified data validator. In addition, all data designated for CLP or CLP-like packaging will receive a third level validation upon completion of the data package.

Reviewer: Grim Hubert Date: 10/9/02



## QC Summary

Report Date: October 9, 2002  
Page 1 of 4

Client : Sandia National Laboratories  
MS-0756  
P.O. Box 5800  
Albuquerque, New Mexico  
Contact: Pamela M. Puissant  
Workorder: 67169

Paramname	NOM	Sample	Qual	QC	Units	RPD%	REC%	Range	Analst	Date	Time
Semi-Volatiles-GC/MS											
Batch 201951											
QC1200301425 LCS											
1,2,4-Trichlorobenzene	50.0			38.5	ug/L		77	(53%-104%)	JWF	09/18/02	15:21
1,4-Dichlorobenzene	50.0			39.1	ug/L		78	(47%-102%)			
2,4,5-Trichlorophenol	100			89.1	ug/L		89	(67%-106%)			
2,4,6-Trichlorophenol	100			86.0	ug/L		86	(45%-111%)			
2,4-Dinitrotoluene	50.0			45.3	ug/L		91	(55%-121%)			
2-Chlorophenol	100			71.9	ug/L		72	(47%-87%)			
4-Chloro-3-methylphenol	100			81.1	ug/L		81	(51%-100%)			
4-Nitrophenol	100			32.1	ug/L		32	(10%-55%)			
Acenaphthene	50.0			44.0	ug/L		88	(63%-111%)			
Hexachlorobenzene	50.0			42.0	ug/L		84	(67%-114%)			
Hexachlorobutadiene	50.0			38.5	ug/L		77	(44%-106%)			
Hexachloroethane	50.0			37.3	ug/L		75	(47%-97%)			
N-Nitrosodipropylamine	50.0			42.5	ug/L		85	(52%-118%)			
Nitrobenzene	50.0			41.7	ug/L		83	(49%-110%)			
Pentachlorophenol	100			75.6	ug/L		76	(31%-110%)			
Phenol	100			31.9	ug/L		32	(16%-44%)			
Pyrene	50.0			38.3	ug/L		77	(68%-117%)			
m,p-Cresols	100			62.1	ug/L		61	(43%-100%)			
o-Cresol	100			68.3	ug/L		68	(47%-87%)			
*2,4,6-Tribromophenol	100			93.1	ug/L		93	(27%-126%)			
*2-Fluorobiphenyl	50.0			39.9	ug/L		80	(32%-109%)			
*2-Fluorophenol	100			45.4	ug/L		45	(13%-73%)			
*Nitrobenzene-d5	50.0			36.8	ug/L		74	(33%-107%)			
*Phenol-d5	100			30.2	ug/L		30	(14%-66%)			
*p-Terphenyl-d14	50.0			40.8	ug/L		82	(36%-130%)			
QC1200301424 MB											
1,2,4-Trichlorobenzene			U	ND	ug/L					09/18/02	14:59
1,2-Dichlorobenzene			U	ND	ug/L						
1,3-Dichlorobenzene			U	ND	ug/L						
1,4-Dichlorobenzene			U	ND	ug/L						
2,4,5-Trichlorophenol			U	ND	ug/L						
2,4,6-Trichlorophenol			U	ND	ug/L						
2,4-Dichlorophenol			U	ND	ug/L						
2,4-Dimethylphenol			U	ND	ug/L						
2,4-Dinitrophenol			U	ND	ug/L						
2,4-Dinitrotoluene			U	ND	ug/L						
2,6-Dinitrotoluene			U	ND	ug/L						
2-Chloronaphthalene			U	ND	ug/L						
2-Chlorophenol			U	ND	ug/L						
2-Methyl-4,6-dinitrophenol			U	ND	ug/L						
2-Methylnaphthalene			U	ND	ug/L						
2-Nitrophenol			U	ND	ug/L						

## QC Summary

Workorder: 67169

Page 2 of 4

Parname	NOM	Sample	Qual	QC	Units	RPD%	REC%	Range	Anlst	Date	Time
Semi-Volatiles-GC/MS											
Batch: 201951											
3,3'-Dichlorobenzidine			U	ND	ug/L						
4-Bromophenylphenylether			U	ND	ug/L						
4-Chloro-3-methylphenol			U	ND	ug/L						
4-Chloroaniline			U	ND	ug/L						
4-Chlorophenylphenylether			U	ND	ug/L						
4-Nitrophenol			U	ND	ug/L						
Acenaphthene			U	ND	ug/L						
Acenaphthylene			U	ND	ug/L						
Anthracene			U	ND	ug/L						
Benzo(a)anthracene			U	ND	ug/L						
Benzo(a)pyrene			U	ND	ug/L						
Benzo(b)fluoranthene			U	ND	ug/L						
Benzo(ghi)perylene			U	ND	ug/L						
Benzo(k)fluoranthene			U	ND	ug/L						
Butylbenzylphthalate			U	ND	ug/L						
Carbazole			U	ND	ug/L						
Chrysene			U	ND	ug/L						
Di-n-butylphthalate			U	ND	ug/L						
Di-n-octylphthalate			U	ND	ug/L						
Dibenzo(a,h)anthracene			U	ND	ug/L						
Dibenzofuran			U	ND	ug/L						
Diethylphthalate			U	ND	ug/L						
Dimethylphthalate			U	ND	ug/L						
Diphenylamine			U	ND	ug/L						
Fluoranthene			U	ND	ug/L						
Fluorene			U	ND	ug/L						
Hexachlorobenzene			U	ND	ug/L						
Hexachlorobutadiene			U	ND	ug/L						
Hexachlorocyclopentadiene			U	ND	ug/L						
Hexachloroethane			U	ND	ug/L						
Indeno(1,2,3-cd)pyrene			U	ND	ug/L						
Isophorone			U	ND	ug/L						
N-Nitrosodipropylamine			U	ND	ug/L						
Naphthalene			U	ND	ug/L						
Nitrobenzene			U	ND	ug/L						
Pentachlorophenol			U	ND	ug/L						
Phenanthrene			U	ND	ug/L						
Phenol			U	ND	ug/L						
Pyrene			U	ND	ug/L						
bis(2-Chloroethoxy)methane			U	ND	ug/L						
bis(2-Chloroethyl) ether			U	ND	ug/L						
bis(2-Chloroisopropyl)ether			U	ND	ug/L						
bis(2-Ethylhexyl)phthalate			U	ND	ug/L						
m,p-Cresols			U	ND	ug/L						
m-Nitroaniline			U	ND	ug/L						
o-Cresol			U	ND	ug/L						
o-Nitroaniline			U	ND	ug/L						
p-Nitroaniline			U	ND	ug/L						

## QC Summary

Workorder: 67169

Page 3 of 4

Parmaame	NOM	Sample Qual	QC	Units	RPD%	REC%	Range	Anlst	Date Time
Semi-Volatiles-GC/MS									
Batch 201951									
*2,4,6-Tribromophenol	100		75.0	ug/L		75	(27%-126%)		
*2-Fluorobiphenyl	50.0		42.5	ug/L		85	(32%-109%)		
*2-Fluorophenol	100		46.7	ug/L		47	(13%-73%)		
*Nitrobenzene-d5	50.0		42.1	ug/L		84	(33%-107%)		
*Phenol-d5	100		31.3	ug/L		31	(14%-66%)		
*p-Terphenyl-d14	50.0		49.8	ug/L		100	(36%-130%)		
QC1200301426 67169005 MS									
1,2,4-Trichlorobenzene	100		82.9	ug/L		83	(44%-102%)		09/18/02 18:49
1,4-Dichlorobenzene	100		80.3	ug/L		80	(48%-95%)		
2,4,5-Trichlorophenol	200		185	ug/L		93			
2,4,6-Trichlorophenol	200		183	ug/L		91			
2,4-Dinitrotoluene	100		96.4	ug/L		96	(48%-120%)		
2-Chlorophenol	200		150	ug/L		75	(32%-98%)		
4-Chloro-3-methylphenol	200		177	ug/L		88	(40%-107%)		
4-Nitrophenol	200		110	ug/L		55	(16%-78%)		
Acenaphthene	100		94.3	ug/L		94	(32%-127%)		
Hexachlorobenzene	100		86.2	ug/L		86			
Hexachlorobutadiene	100		84.4	ug/L		84			
Hexachloroethane	100		78.6	ug/L		79			
N-Nitrosodipropylamine	100		85.5	ug/L		86	(44%-119%)		
Nitrobenzene	100		82.9	ug/L		83			
Pentachlorophenol	200		180	ug/L		90	(44%-104%)		
Phenol	200		89.2	ug/L		45	(15%-70%)		
Pyrene	100		75.0	ug/L		75	(29%-142%)		
m,p-Cresols	200		145	ug/L		72			
o-Cresol	200		153	ug/L		76			
*2,4,6-Tribromophenol	200		200	ug/L		100	(27%-126%)		
*2-Fluorobiphenyl	100		80.5	ug/L		81	(32%-109%)		
*2-Fluorophenol	200		113	ug/L		57	(13%-73%)		
*Nitrobenzene-d5	100		74.9	ug/L		75	(33%-107%)		
*Phenol-d5	200		86.7	ug/L		43	(14%-66%)		
*p-Terphenyl-d14	100		80.4	ug/L		80	(36%-130%)		
QC1200301427 67169005 MSD									
1,2,4-Trichlorobenzene	100		77.5	ug/L	7	78	(0%-20%)		09/18/02 19:12
1,4-Dichlorobenzene	100		75.6	ug/L	6	76	(0%-20%)		
2,4,5-Trichlorophenol	200		184	ug/L	1	92			
2,4,6-Trichlorophenol	200		179	ug/L	2	90			
2,4-Dinitrotoluene	100		91.0	ug/L	6	91	(0%-16%)		
2-Chlorophenol	200		144	ug/L	4	72	(0%-25%)		
4-Chloro-3-methylphenol	200		165	ug/L	7	83	(0%-25%)		
4-Nitrophenol	200		100	ug/L	9	50	(0%-25%)		
Acenaphthene	100		90.9	ug/L	4	91	(0%-24%)		
Hexachlorobenzene	100		85.4	ug/L	1	85			
Hexachlorobutadiene	100		79.3	ug/L	6	80			
Hexachloroethane	100		73.0	ug/L	7	73			
N-Nitrosodipropylamine	100		83.4	ug/L	3	83	(0%-20%)		
Nitrobenzene	100		78.9	ug/L	5	79			
Pentachlorophenol	200		165	ug/L	8	83	(0%-17%)		

## QC Summary

Workorder: 67169

Page 4 of 4

Parname	NOM	Sample	Qual	QC	Units	RPD%	REC%	Range	Analst	Date	Time
<i>Semi-Volatiles-GC/MS</i>											
Batch	201951										
Phenol	200			86.3	ug/L	3	43	(0%-29%)			
Pyrene	100			82.3	ug/L	9	82	(0%-30%)			
m,p-Cresols	200			143	ug/L	2	71				
o-Cresol	200			149	ug/L	3	75				
*2,4,6-Tribromophenol	200			186	ug/L		93	(27%-126%)			
*2-Fluorobiphenyl	100			78.2	ug/L		78	(32%-109%)			
*2-Fluorophenol	200			109	ug/L		54	(13%-73%)			
*Nitrobenzene-d5	100			72.0	ug/L		72	(33%-107%)			
*Phenol-d5	200			84.8	ug/L		42	(14%-66%)			
*p-Terphenyl-d14	100			87.4	ug/L		87	(36%-130%)			

**Notes:**

RER is calculated at the 95% confidence level (2-sigma).

The Qualifiers in this report are defined as follows:

- \* Recovery or %RPD not within acceptance limits and/or spike amount not compatible with the sample or the duplicate RPD's are not applicable where the
- \*\* Indicates analyte is a surrogate compound.
- B The analyte was found in the blank above the effective MDL.
- H Holding time was exceeded
- J Estimated value, the analyte concentration fell above the effective MDL and below the effective PQL
- P The response between the confirmation column and the primary column is >40%D
- U The analyte was analyzed for but not detected below this concentration. For Organic and Inorganic analytes the result is less than the effective MDL. F
- X Presumptive evidence that the analyte is not present. Please see narrative for further information.
- X Presumptive evidence that the analyte is not present. Please see narrative for further information.
- X Uncertain identification for gamma spectroscopy.

N/A indicates that spike recovery limits do not apply when sample concentration exceeds spike conc. by a factor of 4 or more.

^ The Relative Percent Difference (RPD) obtained from the sample duplicate (DUP) is evaluated against the acceptance criteria when the sample is greater than five times (5X) the contract required detection limit (RL). In cases where either the sample or duplicate value is less than 5X the RL, a control limit of +/- the RL is used to evaluate the DUP result.

For PS, PSD, and SDILT results, the values listed are the measured amounts, not final concentrations.

Where the analytical method has been performed under NELAP certification, the analysis has met all of the requirements of the NELAC standard unless qualified on the QC Summary.

**Semi-Volatile Case Narrative  
Sandia National Labs (SNLS)  
SDG 67158**

**Method/Analysis Information**

**Procedure:** Semivolatile Analysis by Gas Chromatograph/Mass Spectrometer  
**Analytical Method:** SW846 8270C  
**Prep Method:** SW846 3550B  
**Analytical Batch Number:** 201961  
**Prep Batch Number:** 201960

**Sample Analysis**

The following samples were analyzed using the analytical protocol as established in SW846 8270C:

<b>Sample ID</b>	<b>Client ID</b>
67158020	059820-002
67158021	059821-002
67158022	059822-002
67158023	059823-002
67158024	059824-002
67158025	059825-002
67158026	059828-002
67158027	059829-002
67158028	059836-002
67158029	059837-002
67158030	059838-002
67158031	059839-002

67158032	059841-002
67158033	059842-002
67158034	059843-002
67158035	059844-002
67158036	059846-001
67158037	059847-002
67158038	059848-002
1200301450	MBSBLK01 (Blank)
1200301451	SBLK01LCS (Laboratory Control Sample)
1200301452	059820-002MS (Matrix Spike)
1200301453	059820-002MSD (Matrix Spike Duplicate)

#### **Preparation/Analytical Method Verification**

Procedures for preparation, analysis, and reporting of analytical data are documented by General Engineering Laboratories, Inc. (GEL) as Standard Operating Procedures (SOP).

#### **Calibration Information**

Due to the limited capacity of software we do not display all of the current initial calibration files here. If necessary, a calibration history will be inserted in the package prior to the appropriate Form 6.

Diphenylamine has now superseded N-Nitroso-diphenylamine as a CCC on Quantitation Reports, Initial Calibration Reports, Calibration Check Standard Reports, etc. Previous versions of EPA Method 8270 (prior to 8270C) listed N-Nitroso-diphenylamine as a CCC. However, as stated in EPA Method 8270C, Revision 3, December, 1996, Section 1.4.5, "N-Nitroso-diphenylamine decomposes in the gas chromatographic inlet and cannot be separated from Diphenylamine." Studies of these two compounds at GEL, both independent of each other and together, show that they not only coelute, but also have similar mass spectra. N-Nitroso-diphenylamine and Diphenylamine will be reported as Diphenylamine on all reports and forms.

When calibrations are performed for Appendix IX compounds some of the compounds may not be calibrated exactly according to the criteria in Method 8270C. If the %RSD is greater than 15% or the correlation coefficient is less than 0.99 then the analyte is quantitated using the response factor. If the analyte is detected then the sample is reanalyzed for that analyte on an

instrument that is compliant with the criteria in the method.

**Initial Calibration**

All initial calibration requirements have been met for this SDG.

**CCV Requirements**

All calibration verification standard (CVS, ICV or CCV) requirements have been met for this SDG.

**Quality Control (QC) Information**

**Surrogate Recoveries**

All the surrogate recoveries were within the established acceptance criteria for this SDG.

**Blank Acceptance**

Target analytes were detected in the method blank; however, the hits were below the reporting limit.

**LCS Recovery Statement**

The laboratory control sample (LCS) spike recoveries for this SDG were within the established acceptance limits.

**QC Sample Designation**

The following sample analyzed with this SDG was chosen for matrix spike analysis.  
67158020 (059820-002)

**MS Recovery Statement**

The matrix spike recoveries for this SDG were within the established acceptance limits.

**MSD Recovery Statement**

The matrix spike duplicate (MSD) recoveries for this SDG were within the established acceptance limits.

**MS/MSD RPD Statement**

The relative percent differences (RPD) between each MS and MSD were within the required acceptance limits.

**Internal Standard (ISTD) Acceptance**

The internal standard responses were within the required acceptance criteria for all samples and QC.

**Technical Information:**

**Holding Time Specifications**

All samples in this SDG met the specified holding time requirements. GEL assigns holding times

based on the associated methodology that assigns the date and time from sample collection or sample receipt. Those holding times expressed in hours are calculated in the AlphaLIMS system. Those holding times expressed as days expire at midnight on the day of expiration. GEL assigns holding times based on the associated methodology that assigns the date and time from sample collection or sample receipt. Those holding times expressed in hours are calculated in the AlphaLIMS system. Those holding times expressed as days expire at midnight on the day of expiration.

#### **Preparation/Analytical Method Verification**

All procedures were performed as stated in the SOP.

#### **Sample Dilutions**

None of the samples analyzed in this SDG required dilution.

#### **Miscellaneous Information:**

##### **Nonconformance (NCR) Documentation**

No nonconformance report (NCR) was generated for this SDG.

##### **Manual Integrations**

No manual integrations were required for any data file in this SDG.

##### **Additional Comments**

No additional comments are needed for this SDG.

#### **System Configuration**

The laboratory utilizes a HP 6890 Series gas chromatograph and a HP 5973 Mass Selective Detector. The configuration is equipped with the electronic pressure control. All MS interfaces are capillary direct.

#### **Chromatographic Columns**

Chromatographic separation of semivolatile components is accomplished through analysis on one or more of the following columns (all with dimensions of 30 meters x 0.25 millimeters ID and 0.25 micron film except J&W DB-5MS2 which is 25 meters x 0.20 mm ID and 0.33 micron film):

<b>Column ID</b>	<b>Column Description</b>
J&W	DB-5.625(5% Phenyl)-methylpolysiloxane (identified by a DB-5.625 designation on quantitation reports and reconstructed ion chromatograms)



J&W DB-5MS	Similar to the J&W DB-5.625 with low bleed characteristics (identified by a DB-5MS designation)
Alltech	EC-5 (SE-54) 5% Phenyl, 95% Methylpolysiloxane (identified by a HP-5MS designation)
HP	HP-5MS 5% Phenylmethylsiloxane (identified by a HP-5MS designation)
Phenomenex	ZB-5 5% Phenyl Polysiloxane (identified by a ZB-5 designation)
J&W DB-5MS2	Similar to the J&W DB-5.625 with low bleed characteristics (identified by a DB-5MS2 designation)

### **Instrument Configuration**

The samples reported in this SDG were analyzed on one or more of the following instrument systems. Instrument systems are referenced in the raw data and individual form headers by the Instrument ID designations listed below:

<b>Instrument ID</b>	<b>System Configuration</b>	<b>Chromatographic Column</b>
MSD2	HP6890/HP5973	DB-5MS2
MSD4	HP6890/HP5973	DB-5MS2
MSD5	HP6890/HP5973	DB-5MS2
MSD7	HP6890/HP5973	DB-5MS2
MSD8	HP6890/HP5973	DB-5MS2

### **Certification Statement**

\* Where the analytical method has been performed under NELAP certification, the analysis has met all of the requirements of the NELAC standard unless otherwise noted in the analytical case narrative.

### **Review Validation:**

GEL requires all analytical data to be verified by a qualified data validator. In addition, all data designated for CLP or CLP-like packaging will receive a third level validation upon completion of the data package.

Reviewer: Erin Hawtal Date: 10/9/02

## QC Summary

Client : Sandia National Laboratories  
 MS-0756  
 P.O. Box 5800  
 Albuquerque, New Mexico  
 Contact: Pamela M. Puissant  
 Workorder: 67158

Report Date: October 9, 2002  
 Page 1 of 4

Parname	NOM	Sample	Qual	QC	Units	RPD%	REC%	Range	Anist	Date	Time
Semi-Volatiles-GC/MS Federal											
Batch 201961											
QC1200301451 LCS											
Pyridine	1670			730	ug/kg		44		GBI	09/18/02	16:48
1,2,4-Trichlorobenzene	1670			1170	ug/kg		70	(27%-91%)			
1,4-Dichlorobenzene	1670			1060	ug/kg		64	(25%-85%)			
2,4,5-Trichlorophenol	3330			2750	ug/kg		83	(42%-96%)			
2,4,6-Trichlorophenol	3330			2520	ug/kg		76	(32%-91%)			
2,4-Dinitrotoluene	1670			1320	ug/kg		79	(50%-109%)			
2-Chlorophenol	3330			2310	ug/kg		69	(31%-85%)			
4-Chloro-3-methylphenol	3330			2760	ug/kg		83	(34%-97%)			
4-Nitrophenol	3330			2410	ug/kg		72	(22%-128%)			
Acenaphthene	1670			1250	ug/kg		75	(39%-98%)			
Hexachlorobenzene	1670			1310	ug/kg		79	(41%-105%)			
Hexachlorobutadiene	1670			1080	ug/kg		65	(21%-94%)			
Hexachloroethane	1670			1060	ug/kg		64	(25%-86%)			
N-Nitrosodipropylamine	1670			1160	ug/kg		69	(34%-90%)			
Nitrobenzene	1670			1130	ug/kg		68	(30%-84%)			
Pentachlorophenol	3330			1910	ug/kg		57	(27%-109%)			
Phenol	3330			2430	ug/kg		73	(31%-83%)			
Pyrene	1670			1230	ug/kg		74	(37%-110%)			
m,p-Cresols	3330			2420	ug/kg		73	(40%-83%)			
o-Cresol	3330			2350	ug/kg		70	(34%-86%)			
*2,4,6-Tribromophenol	3330			2490	ug/kg		75	(23%-111%)			
*2-Fluorobiphenyl	1670			1200	ug/kg		72	(21%-104%)			
*2-Fluorophenol	3330			2390	ug/kg		72	(22%-93%)			
*Nitrobenzene-d5	1670			1110	ug/kg		67	(24%-97%)			
*Phenol-d5	3330			2480	ug/kg		74	(22%-99%)			
*p-Terphenyl-d14	1670			1470	ug/kg		88	(30%-133%)			
QC1200301450 MB											
1,2,4-Trichlorobenzene			U	ND	ug/kg					09/18/02	16:27
1,2-Dichlorobenzene			U	ND	ug/kg						
1,3-Dichlorobenzene			U	ND	ug/kg						
1,4-Dichlorobenzene			U	ND	ug/kg						
2,4,5-Trichlorophenol			U	ND	ug/kg						
2,4,6-Trichlorophenol			U	ND	ug/kg						
2,4-Dichlorophenol			U	ND	ug/kg						
2,4-Dimethylphenol			U	ND	ug/kg						
2,4-Dinitrophenol			U	ND	ug/kg						
2,4-Dinitrotoluene			U	ND	ug/kg						
2,6-Dinitrotoluene			U	ND	ug/kg						
2-Chloronaphthalene			U	ND	ug/kg						
2-Chlorophenol			U	ND	ug/kg						
2-Methyl-4,6-dinitrophenol			U	ND	ug/kg						
2-Methylnaphthalene			U	ND	ug/kg						

## QC Summary

Workorder: 67158

Page 2 of 4

Parameter	NOM	Sample	Qual	QC	Units	RPD%	REC%	Range	Anlst	Date	Time
Semi-Volatiles-GC/MS Federal											
Batch 201961											
2-Nitrophenol			U	ND	ug/kg						
3,3'-Dichlorobenzidine			U	ND	ug/kg						
4-Bromophenylphenylether			U	ND	ug/kg						
4-Chloro-3-methylphenol			U	ND	ug/kg						
4-Chloroaniline			J	ND	ug/kg						
4-Chlorophenylphenylether			U	ND	ug/kg						
4-Nitrophenol			U	ND	ug/kg						
Acenaphthene			U	ND	ug/kg						
Acenaphthylene			U	ND	ug/kg						
Anthracene			U	ND	ug/kg						
Benzo(a)anthracene			U	ND	ug/kg						
Benzo(a)pyrene			U	ND	ug/kg						
Benzo(b)fluoranthene			U	ND	ug/kg						
Benzo(ghi)perylene			U	ND	ug/kg						
Benzo(k)fluoranthene			U	ND	ug/kg						
Butylbenzylphthalate			U	ND	ug/kg						
Carbazole			U	ND	ug/kg						
Chrysene			U	ND	ug/kg						
Di-n-butylphthalate			U	ND	ug/kg						
Di-n-octylphthalate			U	ND	ug/kg						
Dibenzo(a,h)anthracene			U	ND	ug/kg						
Dibenzofuran			U	ND	ug/kg						
Diethylphthalate			U	ND	ug/kg						
Dimethylphthalate			U	ND	ug/kg						
Diphenylamine			U	ND	ug/kg						
Fluoranthene			U	ND	ug/kg						
Fluorene			U	ND	ug/kg						
Hexachlorobenzene			U	ND	ug/kg						
Hexachlorobutadiene			U	ND	ug/kg						
Hexachlorocyclopentadiene			U	ND	ug/kg						
Hexachloroethane			U	ND	ug/kg						
Indeno(1,2,3-cd)pyrene			U	ND	ug/kg						
Isophorone			U	ND	ug/kg						
N-Nitrosodipropylamine			U	ND	ug/kg						
Naphthalene			U	ND	ug/kg						
Nitrobenzene			U	ND	ug/kg						
Pentachlorophenol			U	ND	ug/kg						
Phenanthrene			U	ND	ug/kg						
Pterol			U	ND	ug/kg						
Pyrene			U	ND	ug/kg						
bis(2-Chloroethoxy)methane			U	ND	ug/kg						
bis(2-Chloroethyl) ether			U	ND	ug/kg						
bis(2-Chloroisopropyl)ether			U	ND	ug/kg						
bis(2-Ethylhexyl)phthalate			J	105	ug/kg						
m,p-Cresols			U	ND	ug/kg						
m-Nitroaniline			U	ND	ug/kg						
o-Cresol			U	ND	ug/kg						
o-Nitroaniline			U	ND	ug/kg						

## QC Summary

Workorder: 67158

Page 3 of 4

Parname	NOM	Sample	Qual	QC	Units	RPD%	REC%	Range	Anlst	Date	Time
Semi-Volatiles-GC/MS Federal											
Batch 201961											
p-Nitroaniline			U	ND	ug/kg						
*2,4,6-Tribromophenol	3330			2100	ug/kg		63	(23%-111%)			
*2-Fluorobiphenyl	1670			1110	ug/kg		67	(21%-104%)			
*2-Fluorophenol	3330			2330	ug/kg		70	(22%-93%)			
*Nitrobenzene-d5	1670			1180	ug/kg		71	(24%-97%)			
*Phenol-d5	3330			2300	ug/kg		69	(22%-99%)			
*p-Terphenyl-d14	1670			1350	ug/kg		81	(30%-133%)			
QC1200301452 67158020 MS											
Pyridine	1670			0.00	ug/kg					09/18/02	17:30
1,2,4-Trichlorobenzene	1670	U	ND	1010	ug/kg		61	(15%-112%)			
1,4-Dichlorobenzene	1670	U	ND	923	ug/kg		55	(19%-69%)			
2,4,5-Trichlorophenol	3330	U	ND	2300	ug/kg		69				
2,4,6-Trichlorophenol	3330	U	ND	2020	ug/kg		61				
2,4-Dinitrotoluene	1670	U	ND	1230	ug/kg		74	(32%-117%)			
2-Chlorophenol	3330	U	ND	1940	ug/kg		58	(13%-101%)			
4-Chloro-3-methylphenol	3330	U	ND	2460	ug/kg		74	(23%-114%)			
4-Nitrophenol	3330	U	ND	2300	ug/kg		69	(20%-126%)			
Acenaphthene	1670	U	ND	1010	ug/kg		61	(15%-114%)			
Hexachlorobenzene	1670	U	ND	1220	ug/kg		73				
Hexachlorobutadiene	1670	U	ND	928	ug/kg		56				
Hexachloroethane	1670	U	ND	940	ug/kg		56				
N-Nitrosodipropylamine	1670	U	ND	986	ug/kg		59	(18%-106%)			
Nitrobenzene	1670	U	ND	1010	ug/kg		61				
Pentachlorophenol	3330	U	ND	1640	ug/kg		49	(34%-110%)			
Phenol	3330	U	ND	2010	ug/kg		60	(17%-104%)			
Pyrene	1670	U	ND	1180	ug/kg		71	(26%-130%)			
m,p-Cresols	3330	U	ND	2060	ug/kg		62				
o-Cresol	3330	U	ND	1990	ug/kg		60				
*2,4,6-Tribromophenol	3330	2030		2310	ug/kg		69	(23%-111%)			
*2-Fluorobiphenyl	1670	983		947	ug/kg		57	(21%-104%)			
*2-Fluorophenol	3330	2140		1980	ug/kg		59	(22%-93%)			
*Nitrobenzene-d5	1670	1090		992	ug/kg		60	(24%-97%)			
*Phenol-d5	3330	2050		2020	ug/kg		61	(22%-99%)			
*p-Terphenyl-d14	1670	1360		1390	ug/kg		84	(30%-133%)			
QC1200301453 67158020 MSD											
Pyridine	1670			0.00	ug/kg					09/18/02	17:51
1,2,4-Trichlorobenzene	1670	U	ND	1080	ug/kg	6	65	(0%-31%)			
1,4-Dichlorobenzene	1670	U	ND	1030	ug/kg	11	62	(0%-36%)			
2,4,5-Trichlorophenol	3330	U	ND	2680	ug/kg	15	80				
2,4,6-Trichlorophenol	3330	U	ND	2220	ug/kg	10	67				
2,4-Dinitrotoluene	1670	U	ND	1380	ug/kg	12	83	(0%-37%)			
2-Chlorophenol	3330	U	ND	2180	ug/kg	12	65	(0%-34%)			
4-Chloro-3-methylphenol	3330	U	ND	2710	ug/kg	10	81	(0%-34%)			
4-Nitrophenol	3330	U	ND	2550	ug/kg	10	77	(0%-35%)			
Acenaphthene	1670	U	ND	1140	ug/kg	12	69	(0%-33%)			
Hexachlorobenzene	1670	U	ND	1420	ug/kg	15	85				
Hexachlorobutadiene	1670	U	ND	996	ug/kg	7	60				
Hexachloroethane	1670	U	ND	1010	ug/kg	7	61				

## QC Summary

Workorder: 67158

Page 4 of 4

Parname	NOM	Sample	Qual	QC	Units	RPD%	REC%	Range	Anlst	Date	Time
Semi-Volatiles-GC/MS Federal											
Batch 201961											
N-Nitrosodipropylamine	1670	U	ND	1090	ug/kg	10	66	(0%-29%)			
Nitrobenzene	1670	U	ND	1080	ug/kg	6	65				
Pentachlorophenol	3330	U	ND	1800	ug/kg	9	54	(0%-40%)			
Phenol	3330	U	ND	2260	ug/kg	12	68	(0%-37%)			
Pyrene	1670	U	ND	1230	ug/kg	5	74	(0%-39%)			
m,p-Cresols	3330	U	ND	2400	ug/kg	15	72				
o-Cresol	3330	U	ND	2270	ug/kg	13	68				
*2,4,6-Tribromophenol	3330		2030	2610	ug/kg		78	(23%-111%)			
*2-Fluorobiphenyl	1670		983	1000	ug/kg		60	(21%-104%)			
*2-Fluorophenol	3330		2140	2120	ug/kg		64	(22%-93%)			
*Nitrobenzene-d5	1670		1090	983	ug/kg		59	(24%-57%)			
*Phenol-d5	3330		2050	2220	ug/kg		67	(22%-99%)			
*p-Terphenyl-d14	1670		1360	1370	ug/kg		83	(30%-133%)			

**Notes.**

RER is calculated at the 95% confidence level (2-sigma).

The Qualifiers in this report are defined as follows:

- \* Recovery or %RPD not within acceptance limits and/or spike amount not compatible with the sample or the duplicate RPD's are not applicable where th
- \*\* Indicates analyte is a surrogate compound.
- B The analyte was found in the blank above the effective MDL.
- H Holding time was exceeded
- J Estimated value, the analyte concentration fell above the effective MDL and below the effective PQL.
- P The response between the confirmation column and the primary column is >40%D
- U The analyte was analyzed for but not detected below this concentration. For Organic and Inorganic analytes the result is less than the effective MDL. F
- X Presumptive evidence that the analyte is not present. Please see narrative for further information.
- X Presumptive evidence that the analyte is not present. Please see narrative for further information.
- X Uncertain identification for gamma spectroscopy.

N/A indicates that spike recovery limits do not apply when sample concentration exceeds spike conc. by a factor of 4 or more.

^ The Relative Percent Difference (RPD) obtained from the sample duplicate (DUP) is evaluated against the acceptance criteria when the sample is greater than five times (5X) the contract required detection limit (RL). In cases where either the sample or duplicate value is less than 5X the RL, a control limit of +/- the RL is used to evaluate the DUP result.

For PS, PSD, and SDILT results, the values listed are the measured amounts, not final concentrations.

Where the analytical method has been performed under NELAP certification, the analysis has met all of the requirements of the NELAC standard unless qualified on the QC Summary.

PCB Case Narrative  
Sandia National Labs (SNLS)  
SDG# 67158

Method/Analysis Information

Procedure: Polychlorinated Biphenyls by Method 8082  
Analytical Method: SW846 8082  
Prep Method: SW846 3550B  
Analytical Batch Number: 201940  
Prep Batch Number: 201939

Sample Analysis

The following samples were analyzed using the analytical protocol as established in SW846 8082:

Sample ID	Client ID
67158020	059820-002
67158021	059821-002
67158022	059822-002
67158023	059823-002
67158024	059824-002
67158025	059825-002
67158026	059828-002
67158027	059829-002
67158028	059836-002
67158029	059837-002
67158030	059838-002
67158031	059839-002
67158032	059841-002
67158033	059842-002
67158034	059843-002

SNLS SDG#67158 - PCB

67158035	059844-002
67158036	059846-001
67158037	059847-002
67158038	059848-002
1200301403	PBLK01(Method Blank)
1200301404	PBLK01LCS(Laboratory Control Sample)
1200301405	059820-002MS(Matrix Spike)
1200301406	059820-002MSD(Matrix Spike Duplicate)

### System Configuration

#### Chromatographic Columns

Column ID	Column Description
J&W1	DB-5(5%-Phenyl)-methylsiloxane 30m x 0.53mm x 1.5um DB-608 Durabond stationary phase* 30m x 0.53mm x 0.5um
J&W2	DB-5(5%-Phenyl)-methylsiloxane 30m x 0.32mm x 1.0um DB-1701 Durabond stationary phase* 30m x 0.32mm x 0.5um
J&W3	DB-5(5%-Phenyl)-methylsiloxane 30m x 0.53mm x 1.5um DB-1701(14% Cyanopropylphenyl)-methylsiloxane 30m x 0.53mm x 0.5um
J&W4	DB-608 Durabond stationary phase* 30m x 0.53mm x .83um DB-XLB* 30m x 0.53mm x 1.5um
J&W5	DB-XLB* 30m x 0.25mm x 0.25um DB-17MS(50%-Phenyl)-methylsiloxane 30m x 0.25mm x 0.25um
J&W6	DB-5(5%-Phenyl)-methylsiloxane 30m x 0.25mm x 0.25um DB-17MS(50%-Phenyl)-methylsiloxane 30m x 0.25mm x 0.25um
RESTEK	Rtx-CLPesticides 30m x 0.25mm x 0.25um Rtx-CLPesticides II 30m x 0.25mm x 0.20um

\* Durabond and DB-XLB are trademarks of J & W.

## **Instrument Configuration**

The samples reported in this SDG were analyzed on one or more of the following instrument systems. Instrument systems are referenced in the raw data and individual form headers by the Instrument ID designations listed below.

<b>Instrument ID</b>	<b>System Configuration</b>	<b>Chromatographic Column</b>
ECD1	HP 6890 Series GC ECD/ECD	RESTEK
ECD2	HP 6890 Series GC ECD/ECD	RESTEK
ECD3	HP 6890 Series GC ECD/ECD	RESTEK
ECD4	HP 5890 Series II Plus GC ECD/ECD	J&W5
ECD5	HP 6890 Series GC ECD/ECD	J&W5
ECD7	HP 6890 Series GC ECD/ECD	J&W5
ECD8	HP 6890 Series GC ECD/ECD	RESTEK

## **Preparation/Analytical Method Verification**

Procedures for preparation, analysis, and reporting of analytical data are documented by General Engineering Laboratories, Inc. (GEL) as Standard Operating Procedures (SOP).

## **Calibration Information**

### **Initial Calibration**

All initial calibration requirements have been met for this SDG.

### **CCV Requirements**

All calibration verification standard(s) (CVS, ICV or CCV) requirements have been met for this SDG.

## **Quality Control (QC) Information**

### **Surrogate Recoveries**

All the surrogate recoveries were within the established acceptance criteria for this SDG.

### **Blank Acceptance**

The blank(s) analyzed with this SDG met the established acceptance criteria.

### **LCS Recovery Statement**

The laboratory Control Sample (LCS) spike recoveries for this SDG were within the established acceptance limits.



## QC Sample Designation

The following sample was selected for the PCB method QC:

<u>Client Sample ID#</u>	<u>Laboratory Sample ID#</u>
059820-002	67158020

The method QC included a Matrix Spike (MS) and Matrix Spike Duplicate (MSD).

## MS Recovery Statement

The matrix spike recoveries for this SDG were within the established acceptance limits.

## MSD Recovery Statement

The matrix spike duplicate recoveries for this SDG were within the established acceptance limits.

## MS/MSD RPD Statement

The relative percent differences (RPD) between each MS and MSD were within the required acceptance limits.

## Technical Information

### Holding Time Specifications

GEL assigns holding times based on the associated methodology which assigns the date and time from sample collection or sample receipt. Those holding times expressed in hours are calculated in the AlphaLIMS system. Those holding times expressed as days expire at midnight on the day of expiration. All samples in this SDG met the specified holding time requirements.

### Preparation/Analytical Method Verification

All procedures were performed as stated in the SOP. All samples underwent sulfur and alumina cleanup procedure.

### Sample Dilutions

None of the samples in this SDG were required dilutions.

### Sample Re-prep/Re-analysis

None of the samples in this sample group were repped or reanalyzed.

## Miscellaneous Information

### Nonconformance (NCR) Documentation

No nonconformance reports (NCRs) have been generated for this SDG.

### Manual Integrations

Due to software limitations, some manual integrations were performed on standards or samples in order for the integration of some analytes to match their integration in the calibration used. Certain standards and QC samples may have required manual integrations to correctly position the baseline as set in the calibration standard injections. If manual integrations were performed, copies of all manual integration peak profiles are included in the raw data section of this PCB fraction.

### Additional Comments

The additional comments field is used to address special issues associated with each analysis, clarify method/contractual issues pertaining to the analysis and to list any report documents generated as a result of sample analysis or review. The following additional comments were required for this sample set:

Aroclors quantitated on the raw data report by the Target data system do not necessarily represent positive aroclor identification. In order for positive identification to be made, the aroclor must match in pattern and retention time; as well as quantitate relatively close between the primary and confirmation columns, as specified in SW846 method 8000. When these conditions are not met, the aroclor is reported as a non-detect on the data report. These situations will be noted on the raw data as DMP, representing "does not match pattern", or DNC "does not confirm".

### Certification Statement

\* Where the analytical method has been performed under NELAP certification, the analysis has met all of the requirements of the NELAC standard unless otherwise noted in the analytical case narrative.

### Review Validation:

GEL requires all analytical data to be verified by a qualified data validator. In addition, all data designated for CLP or CLP-like packaging will receive a third level validation upon completion of the data package.

The following data validator verified the information presented in this case narrative:

Reviewer: Jimi Cao Date: 10/11/02

## QC Summary

Workorder: 67158

Page 2 of 2

Parmname	NOM	Sample	Qual	QC	Units	RPD%	REC%	Range	Anist	Date	Time
----------	-----	--------	------	----	-------	------	------	-------	-------	------	------

N/A indicates that spike recovery limits do not apply when sample concentration exceeds spike conc. by a factor of 4 or more.

^ The Relative Percent Difference (RPD) obtained from the sample duplicate (DUP) is evaluated against the acceptance criteria when the sample is greater than five times (5X) the contract required detection limit (RL). In cases where either the sample or duplicate value is less than 5X the RL, a control limit of +/- the RL is used to evaluate the DUP result.

For PS, PSD, and SDILT results, the values listed are the measured amounts, not final concentrations.

Where the analytical method has been performed under NELAP certification, the analysis has met all of the requirements of the NELAC standard unless qualified on the QC Summary.

## QC Summary

Client : Sandia National Laboratories  
 MS-0756  
 P.O. Box 5800  
 Albuquerque, New Mexico  
 Contact: Pamela M. Puissant  
 Workorder: 67158

Report Date: October 10, 2002  
 Page 1 of 2

Parname	NOM	Sample	Qual	QC	Units	RPD%	REC%	Range	Anlst	Date	Time
<b>Semi-Volatiles-PCB Federal</b>											
Batch 201940											
QC1200301404	LCS										
Aroclor-1260	33.3			29.0	ug/kg		87	(48%-116%)	GH1	09/25/02	17:05
**4cmx	6.67			171	ug/kg		86	(31%-120%)			
**Decachlorobiphenyl	6.67			187	ug/kg		93	(34%-115%)			
QC1200301403	MB										
Aroclor-1016			U	ND	ug/kg					09/25/02	16:53
Aroclor-1221			U	ND	ug/kg						
Aroclor-1232			U	ND	ug/kg						
Aroclor-1242			U	ND	ug/kg						
Aroclor-1248			U	ND	ug/kg						
Aroclor-1254			U	ND	ug/kg						
Aroclor-1260			U	ND	ug/kg						
**4cmx	6.67			170	ug/kg		85	(31%-120%)			
**Decachlorobiphenyl	6.67			183	ug/kg		91	(34%-115%)			
QC1200301405	67158020	MS									
Aroclor-1260	33.3	10.9		37.2	ug/kg		79	(36%-134%)		09/25/02	17:29
**4cmx	6.67	5.06		151	ug/kg		75	(31%-120%)			
**Decachlorobiphenyl	6.67	5.24		147	ug/kg		74	(34%-115%)			
QC1200301406	67158020	MSD									
Aroclor-1260	33.3	10.9		37.8	ug/kg	2	81	(0%-30%)		09/25/02	17:42
**4cmx	6.67	5.06		140	ug/kg		70	(31%-120%)			
**Decachlorobiphenyl	6.67	5.24		151	ug/kg		75	(34%-115%)			

**Notes:**

RER is calculated at the 95% confidence level (2-sigma).  
 The Qualifiers in this report are defined as follows:

- \* Recovery or %RPD not within acceptance limits and/or spike amount not compatible with the sample or the duplicate RPD's are not applicable where t
- \*\* Indicates analyte is a surrogate compound.
- B The analyte was found in the blank above the effective MDL.
- H Holding time was exceeded
- J Estimated value, the analytic concentration fell above the effective MDL and below the effective PQL
- P The response between the confirmation column and the primary column is >40%D
- U The analyte was analyzed for but not detected below this concentration. For Organic and Inorganic analytes the result is less than the effective MDL. J
- X Presumptive evidence that the analyte is not present. Please see narrative for further information.
- X Presumptive evidence that the analyte is not present. Please see narrative for further information.
- X Uncertain identification for gamma spectroscopy.

PCB Case Narrative  
Sandia National Labs (SNLS)  
SDG# 67158-1

Method/Analysis Information

Procedure: Polychlorinated Biphenyls by Method 8082  
Analytical Method: SW846 8082  
Prep Method: SW846 3510C  
Analytical Batch Number: 202231  
Prep Batch Number: 202230

Sample Analysis

The following samples were analyzed using the analytical protocol as established in SW846 8082:

Sample ID	Client ID
67169006	059826-003
1200302125	PBLK01(Method Blank)
1200302128	PBLK01LCS(Laboratory Control Sample)

System Configuration

Chromatographic Columns

Column ID	Column Description
J&W1	DB-5(5%-Phenyl)-methylsiloxane 30m x 0.53mm x 1.5um DB-608 Durabond stationary phase* 30m x 0.53mm x 0.5um
J&W2	DB-5(5%-Phenyl)-methylsiloxane 30m x 0.32mm x 1.0um DB-1701 Durabond stationary phase* 30m x 0.32mm x 0.5um
J&W3	DB-5(5%-Phenyl)-methylsiloxane 30m x 0.53mm x 1.5um DB-1701(14% Cyanopropylphenyl)-methylsiloxane 30m x 0.53mm x 0.5um
J&W4	DB-608 Durabond stationary phase* 30m x 0.53mm x .83um DB-XLB* 30m x 0.53mm x 1.5um
J&W5	DB-XLB* 30m x 0.25mm x 0.25um DB-17MS(50%-Phenyl)-methylsiloxane 30m x 0.25mm x 0.25um

J&W6 DB-5(5%-Phenyl)-methylsiloxane 30m x 0.25mm x 0.25um  
DB-17MS(50%-Phenyl)-methylsiloxane 30m x 0.25mm x 0.25um

RESTEK Rtx-CLPesticides 30m x 0.25mm x 0.25um  
Rtx-CLPesticides II 30m x 0.25mm x 0.20um

\* Durabond and DB-XLB are trademarks of J & W.

### **Instrument Configuration**

The samples reported in this SDG were analyzed on one or more of the following instrument systems. Instrument systems are referenced in the raw data and individual form headers by the Instrument ID designations listed below.

<b>Instrument ID</b>	<b>System Configuration</b>	<b>Chromatographic Column</b>
ECD1	HP 6890 Series GC ECD/ECD	RESTEK
ECD2	HP 6890 Series GC ECD/ECD	RESTEK
ECD3	HP 6890 Series GC ECD/ECD	RESTEK
ECD4	HP 5890 Series II Plus GC ECD/ECD	J&W5
ECD5	HP 6890 Series GC ECD/ECD	J&W5
ECD7	HP 6890 Series GC ECD/ECD	J&W5
ECD8	HP 6890 Series GC ECD/ECD	RESTEK

### **Preparation/Analytical Method Verification**

Procedures for preparation, analysis, and reporting of analytical data are documented by General Engineering Laboratories, Inc. (GEL) as Standard Operating Procedures (SOP).

### **Calibration Information**

#### **Initial Calibration**

All initial calibration requirements have been met for this SDG.

#### **CCV Requirements**

All calibration verification standard(s) (CVS, ICV or CCV) requirements have been met for this SDG.

### **Quality Control (QC) Information**

#### **Surrogate Recoveries**

All the surrogate recoveries were within the established acceptance criteria for this SDG.

**Blank Acceptance**

The blank(s) analyzed with this SDG met the established acceptance criteria.

**LCS Recovery Statement**

The laboratory Control Sample (LCS) spike recoveries for this SDG were within the established acceptance limits.

**QC Sample Designation**

The MS and MSD were analyzed on a sample contained in a non-client's SDG.

**MS Recovery Statement**

The matrix spike recoveries for this SDG were within the established acceptance limits.

**MSD Recovery Statement**

The matrix spike duplicate recoveries for this SDG were within the established acceptance limits.

**MS/MSD RPD Statement**

The relative percent differences (RPD) between each MS and MSD were within the required acceptance limits.

**Technical Information****Holding Time Specifications**

GEL assigns holding times based on the associated methodology which assigns the date and time from sample collection or sample receipt. Those holding times expressed in hours are calculated in the AlphaLIMS system. Those holding times expressed as days expire at midnight on the day of expiration. All samples in this SDG met the specified holding time requirements.

**Preparation/Analytical Method Verification**

All procedures were performed as stated in the SOP. All samples underwent sulfur and alumina cleanup procedure.

**Sample Dilutions**

None of the samples in this SDG were required dilutions.

**Sample Re-prep/Re-analysis**

None of the samples in this sample group were re-prepped or reanalyzed.

**Miscellaneous Information**

**Nonconformance (NCR) Documentation**

No nonconformance reports (NCRs) have been generated for this SDG.

**Manual Integrations**

Due to software limitations, some manual integrations were performed on standards or samples in order for the integration of some analytes to match their integration in the calibration used. Certain standards and QC samples may have required manual integrations to correctly position the baseline as set in the calibration standard injections. If manual integrations were performed, copies of all manual integration peak profiles are included in the raw data section of this PCB fraction.

**Additional Comments**

The additional comments field is used to address special issues associated with each analysis, clarify method/contractual issues pertaining to the analysis and to list any report documents generated as a result of sample analysis or review. The following additional comments were required for this sample set:

Aroclors quantitated on the raw data report by the Target data system do not necessarily represent positive aroclor identification. In order for positive identification to be made, the aroclor must match in pattern and retention time; as well as quantitate relatively close between the primary and confirmation columns, as specified in SW846 method 8000. When these conditions are not met, the aroclor is reported as a non-detect on the data report. These situations will be noted on the raw data as DMP, representing "does not match pattern", or DNC "does not confirm".

**Certification Statement**

\* Where the analytical method has been performed under NELAP certification, the analysis has met all of the requirements of the NELAC standard unless otherwise noted in the analytical case narrative.

**Review Validation:**

GEL requires all analytical data to be verified by a qualified data validator. In addition, all data designated for CLP or CLP-like packaging will receive a third level validation upon completion of the data package.

The following data validator verified the information presented in this case narrative:

Reviewer:         Jimmie Cao         Date:         10/11/02



## QC Summary

Report Date: October 11, 2002  
Page 1 of 1

Client: Sandia National Laboratories  
MS-0756  
P.O. Box 5800  
Albuquerque, New Mexico  
Contact: Pamela M. Puissant  
Workorder: 67169

Parname	NOM	Sample	Qual	QC	Units	RPD%	REC%	Range	Anlst	Date	Time
Semi-Volatiles-PCB Federal											
Batch 202231											
QC1200302128	LCS										
Aroclor-1260	1.00			0.840	ug/L	84	(47%-131%)	GH1	09/23/02	11:39	
**4cmx	0.200			154	ug/L	77	(34%-116%)				
**Decachlorobiphenyl	0.200			123	ug/L	62	(21%-122%)				
QC1200302125 MB											
Aroclor-1016			U	ND	ug/L					09/23/02	11:27
Aroclor-1221			U	ND	ug/L						
Aroclor-1232			U	ND	ug/L						
Aroclor-1242			U	ND	ug/L						
Aroclor-1248			U	ND	ug/L						
Aroclor-1254			U	ND	ug/L						
Aroclor-1260			U	ND	ug/L						
**4cmx	0.200			162	ug/L	81	(34%-116%)				
**Decachlorobiphenyl	0.200			136	ug/L	68	(21%-122%)				

**Notes:**

RER is calculated at the 95% confidence level (2-sigma).

The Qualifiers in this report are defined as follows:

- \* Recovery or %RPD not within acceptance limits and/or spike amount not compatible with the sample or the duplicate RPD's are not applicable where E
- \*\* Indicates analyte is a surrogate compound.
- B The analyte was found in the blank above the effective MDL.
- H Holding time was exceeded
- I Estimated value, the analyte concentration fell above the effective MDL and below the effective PQL
- P The response between the confirmation column and the primary column is >40% D
- U The analyte was analyzed for but not detected below this concentration. For Organic and Inorganic analytes the result is less than the effective MDL. )
- X Presumptive evidence that the analyte is not present. Please see narrative for further information.
- X Presumptive evidence that the analyte is not present. Please see narrative for further information.
- X Uncertain identification for gamma spectroscopy.

N/A indicates that spike recovery limits do not apply when sample concentration exceeds spike conc. by a factor of 4 or more

^ The Relative Percent Difference (RPD) obtained from the sample duplicate (DUP) is evaluated against the acceptance criteria when the sample is greater than five times (5X) the contract required detection limit (RL). In cases where either the sample or duplicate value is less than 5X the RL, a control limit of +/- the RL is used to evaluate the DUP result.

For PS, PSD, and SDILT results, the values listed are the measured amounts, not final concentrations.

Where the analytical method has been performed under NELAP certification, the analysis has met all of the requirements of the NELAC standard unless qualified on the QC Summary.

**CASE NARRATIVE**  
**for**  
**Sandia National Laboratories**  
**ARCOC-605671**  
**SDG#67158A**  
**ARCOC-605672**  
**SDG#67158B**  
**ARCOC-605673**  
**SDG#67158C**  
**Case No. 7223.02.03.02**

**October 14, 2002**

**Laboratory Identification:**

General Engineering Laboratories, Inc.

**Mailing Address:**

P.O. Box 30712  
Charleston, South Carolina 29417

**Express Mail Delivery and Shipping Address:**

2040 Savage Road  
Charleston, South Carolina 29407

**Telephone Number:**

(843) 556-8171

**Summary:**

**Sample receipt**

Sandia collected thirty-eight soil samples and eleven aqueous samples on September 9, 10, 12, and 13, 2002. The samples arrived at General Engineering Laboratories, Inc., (GEL) Charleston, South Carolina on September 17, 2002, for environmental analyses. Cooler clearance (screening, temperature check, etc.) was done upon login. The coolers arrived without any visible signs of tampering and with custody seals intact. The samples were delivered with chain of custody documentation and signatures. The temperature of the samples was 3.0, 4.0, and 5.0°C, as measured from the temperature control bottles.

Sample ID 059826-006 was received out of holding. This was the equipment blank for Cr6. Client was contacted regarding the issue. An NCR was generated.

GENERAL ENGINEERING LABORATORIES  
P O Box 30712 • Charleston, SC 29417 • 2040 Savage Road • 29407  
(843) 556-8171 • Fax (843) 766-1178

*[Handwritten signature]*

The samples were screened according to GEL Standard Operating Procedures (SOP) EPI SOP S-007 rev. 2 "The Receiving of Radioactive Samples." The samples were stored properly according to SW-846 procedures and GEL SOP.

The samples were received and collected as listed in the table below:

ARCOC	SDG#	#of samples	Collection Date	Date Rec'd by Lab
605671	67158A	12	09/09/02	09/17/02
605672	67158B	22	09/10/02,09/12/02	09/17/02
605673	67158C	15	09/13/02	09/17/02

The laboratory received the following samples:

**Laboratory ID**  
**ARCOC-605671:**

**Description**

67158001	059820-001
67158002	059821-001
67158003	059822-001
67158004	059823-001
67158005	059824-001
67158006	059825-001
67158020	059820-002
67158021	059821-002
67158022	059822-002
67158023	059823-002
67158024	059824-002
67158025	059825-002

**ARCOC-605672:**

67158007	059828-001
67158008	059829-001
67158009	059836-001
67158010	059837-001
67158011	059838-001
67158012	059839-001
67158026	059828-002
67158027	059829-002
67158028	059836-002
67158029	059837-002
67158030	059838-002
67158031	059839-002
67169001	059827-001
67169002	059826-001
67169003	059840-001
67169005	059826-002
67169006	059826-003

GENERAL ENGINEERING LABORATORIES

P O Box 30712 • Charleston, SC 29417 • 2040 Savage Road • 29407

(843) 556-8171 • Fax (843) 766-1178

5

67169007  
67169008  
67169009  
67169010  
67169011

059826-004  
059826-005  
059826-006  
059826-007  
059826-008

**ARCOC-605673:**

67158013  
67158014  
67158015  
67158016  
67158017  
67158018  
67158019  
67158032  
67158033  
67158034  
67158035  
67158036  
67158037  
67158038  
67169004

059841-001  
059842-001  
059843-001  
059844-001  
059845-001  
059847-001  
059848-001  
059841-002  
059842-002  
059843-002  
059844-002  
059846-001  
059847-002  
059848-002  
059849-001

**Case Narrative**

Sample analyses were conducted using methodology as outlined in General Engineering Laboratories (GEL) Standard Operating Procedures. Any technical or administrative problems during analysis, data review, and reduction are contained in the analytical case narratives in the enclosed data package.

**Internal Chain of Custody:**

Custody was maintained for the samples.


6

**Data Package:**

The enclosed data package contains the following sections: Case Narrative, Chain of Custody, Cooler Receipt Checklist, Qualifier Flag and Data Package Definitions, Laboratory Certifications, Volatiles Data, Volatiles QC Summary, Semivolatiles Data, Semivolatiles QC Summary, PCB Data, PCB QC Summary, Explosives Data, Explosives QC Summary, Metals Data, Metals QC Summary, General Chemistry Data, General Chemistry QC Summary, Radiochemistry Data, Radiochemistry QC Summary, and Level C Data Package.

This data package, to the best of my knowledge, is in compliance with technical and administrative requirements.

Edith M. Kent



Project Manager

**REVISED**

GC/MS Volatile Organics  
Sandia National Labs (SNLS)  
SDG# 67158-1

Method/Analysis Information

Procedure: Volatile Organic Compounds (VOC) by Gas Chromatograph/Mass Spectrometer  
Analytical Method: SW846 8260B  
Prep Method: SW846 5030B  
Analytical Batch Number: 203595

Sample Analysis

The following client and quality control samples were analyzed to complete this sample delivery group's work order using the methods referenced in the Analysis Information section:

Sample ID	Client ID
67169001	059827-001
67169002	059826-001
67169003	059840-001
67169004	059849-001
1200305537	VBLK01 (Blank)
1200305538	VBLK01LCS (Laboratory Control Sample)

Preparation/Analytical Method Verification

**SOP Reference**

Procedure(s) for preparation, analysis and reporting of analytical data are controlled by General Engineering Laboratories, Inc. as Standard Operating Procedure(s) (SOP). The data discussed in this narrative has been analyzed in accordance with GL-OA-E-038 REV.6.

Calibration Information

Due to software limitations, all the data files comprising the initial calibration curve may not be listed on the initial calibration summary form. All calibration files are listed in the calibration history report in the "Standard Data" section.

SDG# 67158-1 -VOA

**REVISED**

**Initial Calibration**

All the initial calibration requirements were met.

**CCV Requirements**

All the calibration verification standard (CCV) requirements were met.

**Quality Control (QC) Information**

**Surrogate Recoveries**

Surrogate recoveries, in all samples and quality control samples, were within the acceptance limits.

**Blank Acceptance**

Target analytes were not detected above the reporting limit in the blank.

**LCS Recovery Statement**

All the required analyte recoveries in the laboratory control sample were within the acceptance limits.

**QC Sample Designation**

Matrix spike analyses were analyzed on a sample of similar matrix in SNLS sample delivery group order, # 67354.

**MS Recovery Statement**

All the required matrix spike recoveries were within the acceptance limits.

**MSD Recovery Statement**

All the required matrix spike duplicate recoveries were within the acceptance limits.

**MS/MSD RPD Statement**

The relative percent differences (RPD) between the matrix spike and matrix spike duplicate recoveries were within the acceptance limits.

**Technical Information**

**Holding Time Specifications**

All the samples were prepared and/or analyzed within the required holding time period.

**Sample Preservation and Integrity**

All samples met the sample preservation and integrity requirements.

**Preparation/Analytical Method Verification**

All procedures were performed as stated in the SOP.

**Sample Dilutions**

The samples in this sample delivery group/work order did not require dilutions.

**Sample Re-prep/Re-analysis**

Re-analyses were not required for samples in this sample group/work order.

**Miscellaneous Information**

**Nonconformance (NCR) Documentation**

A nonconformance report was not required for this sample delivery group/work order.

SDG# 67156-1 -VOA



**Manual Integrations**

Data files associated with the initial calibration, continuing calibration check, and samples did not require manual integrations

**Additional Comments**

The following package was generated using an electronic data processing program referred to as "virtual packaging". In an effort to increase quality and efficiency, the laboratory is developing systems to eventually generate all data packages electronically. The following change from "traditional" packages should be noted:

Analyst/peer reviewer initials and dates are not present on the electronic data files. Presently, all initials and dates are on the original raw data. These hard copies are temporary stored in the laboratory. An electronic signature page inserted after the case narrative of each electronic package will indicate the analyst, reviewer, and report specialist names associated with the generation of the data package. The data validator will always sign and date the case narrative. Data that are not generated electronically, and such as hand written pages, will be scanned and inserted into the electronic package.

**TIC Comment**

Tentatively identified compounds (TIC) were not required for this sample delivery group/work order.

**System Configuration**

The laboratory utilizes the following GC/MS configurations:

**Chromatographic Columns**

Chromatographic separation of volatile components is accomplished through analysis on one of the following columns:

Column ID	Column Description
J&W1	DB-624, 60m x 0.25mm, 1.4um
J&W2	DB-624, 75m x 0.53mm, 3.0um

**Instrument Configuration**

Instrument systems are reference in the raw data and individual form headers by the Instrument ID designations below:

Instrument ID	System Configuration	Chromatographic Column	P & T Trap
VOA1	HP6890/HP5973	J&W1	Trap C
VOA2	HP6890/HP5973	J&W1	Trap C
VOA4	HP5890/HP5972	J&W1	Trap K
VOA5	HP5890/HP5972	J&W1	Trap C
VOA7	HP5890/HP5972	J&W2	Trap K

SDG# 67158-1 -VOA



VOA8	HP6890/HP5973	J&W1	Trap K
VOA9	HP6890/HP5973	J&W1	Trap C

**Certification Statement**

Where the analytical method has been performed under NELAP certification, the analysis has met all of the requirements of the NELAC standard unless otherwise noted in the analytical case narrative.

**Review Validation**

GEL requires all analytical data to be verified by a qualified data validator. In addition, all data designated for CLP or CLP-like packaging will receive a third level validation upon completion of the data package.

The following data validator verified the information presented in this case narrative:

Reviewer: *Nick Malley* Date: 10/15/02

## QC Summary

Report Date: September 30, 2002  
Page 1 of 4

Client: Sandia National Laboratories  
MS-0756  
P.O. Box 5800  
Albuquerque, New Mexico  
Contact: Pamela M. Puissant  
Workorder: 67169

Paramname	NOM	Sample Qual	QC	Units	RPD%	REC%	Range	Anlst	Date Time
Volatile-GC/MS Federal									
Batch 203595									
QC1200305538 LCS									
1,1-Dichloroethylene	50.0		45.0	ug/L		90	(78%-140%)	MAP	09/24/02 06:58
Benzene	50.0		45.8	ug/L		92	(78%-119%)		
Chlorobenzene	50.0		49.4	ug/L		99	(82%-120%)		
Toluene	50.0		50.3	ug/L		101	(68%-133%)		
Trichloroethylene	50.0		47.1	ug/L		94	(50%-123%)		
**Bromofluorobenzene	50.0		64.8	ug/L		130	(67%-136%)		
**Dibromofluoromethane	50.0		60.5	ug/L		121	(62%-148%)		
**Toluene-d8	50.0		58.7	ug/L		117	(58%-139%)		
QC1200306542 LCS									
1,1-Dichloroethylene	50.0		49.6	ug/L		99	(78%-140%)		09/25/02 10:00
Benzene	50.0		46.9	ug/L		94	(78%-119%)		
Chlorobenzene	50.0		50.9	ug/L		102	(82%-120%)		
Toluene	50.0		52.0	ug/L		104	(68%-133%)		
Trichloroethylene	50.0		50.7	ug/L		101	(80%-123%)		
**Bromofluorobenzene	50.0		64.2	ug/L		128	(67%-136%)		
**Dibromofluoromethane	50.0		61.4	ug/L		123	(62%-148%)		
**Toluene-d8	50.0		57.7	ug/L		115	(58%-139%)		
QC1200307213 LCS									
1,1-Dichloroethylene	50.0		44.0	ug/L		88	(78%-140%)		09/24/02 18:08
Benzene	50.0		45.4	ug/L		91	(78%-119%)		
Chlorobenzene	50.0		47.2	ug/L		94	(82%-120%)		
Toluene	50.0		46.7	ug/L		93	(68%-133%)		
Trichloroethylene	50.0		46.9	ug/L		94	(80%-123%)		
**Bromofluorobenzene	50.0		62.7	ug/L		125	(67%-136%)		
**Dibromofluoromethane	50.0		63.4	ug/L		127	(62%-148%)		
**Toluene-d8	50.0		56.8	ug/L		114	(58%-139%)		
QC1200305537 MB									
1,1,1-Trichloroethane		U	ND	ug/L					09/24/02 08:17
1,1,2,2-Tetrachloroethane		U	ND	ug/L					
1,1,2-Trichloroethane		U	ND	ug/L					
1,1-Dichloroethane		U	ND	ug/L					
1,1-Dichloroethylene		U	ND	ug/L					
1,2-Dichloroethane		U	ND	ug/L					
1,2-Dichloropropane		U	ND	ug/L					
2-Butanone		U	ND	ug/L					
2-Hexanone		U	ND	ug/L					
4-Methyl-2-pentanone		U	ND	ug/L					
Acetone		U	ND	ug/L					
Benzene		U	ND	ug/L					
Bromodichloromethane		U	ND	ug/L					
Bromoform		U	ND	ug/L					
Bromomethane		U	ND	ug/L					

## QC Summary

Workorder: 67169

Parname	NOM	Sample	Qual	QC	Units	RPD%	REC%	Range	Anlst	Date	Time
Volatile-GC/MS Federal											
Batch 203595											
Carbon disulfide			U	ND	ug/L						
Carbon tetrachloride			U	ND	ug/L						
Chlorobenzene			U	ND	ug/L						
Chloroethane			U	ND	ug/L						
Chloroform			U	ND	ug/L						
Chloromethane			U	ND	ug/L						
Dibromochloromethane			U	ND	ug/L						
Ethylbenzene			U	ND	ug/L						
Methylene chloride			U	ND	ug/L						
Styrene			U	ND	ug/L						
Tetrachloroethylene			U	ND	ug/L						
Toluene			U	ND	ug/L						
Trichloroethylene			U	ND	ug/L						
Vinyl chloride			U	ND	ug/L						
Xylenes (total)			U	ND	ug/L						
cis-1,2-Dichloroethylene			U	ND	ug/L						
cis-1,3-Dichloropropylene			U	ND	ug/L						
trans-1,2-Dichloroethylene			U	ND	ug/L						
trans-1,3-Dichloropropylene			U	ND	ug/L						
**Bromofluorobenzene	50.0			63.9	ug/L		128	(67%-136%)			
**Dibromofluoromethane	50.0			63.1	ug/L		126	(62%-148%)			
Toluene-d8	50.0			56.8	ug/L		114	(58%-139%)			
QC1200306541 MB											
1,1,1-Trichloroethane			U	ND	ug/L						
1,1,2,2-Tetrachloroethane			U	ND	ug/L						
1,1,2-Trichloroethane			U	ND	ug/L						
1,1-Dichloroethane			U	ND	ug/L						
1,1-Dichloroethylene			U	ND	ug/L						
1,2-Dichloroethane			U	ND	ug/L						
1,2-Dichloropropane			U	ND	ug/L						
2-Butanone			U	ND	ug/L						
2-Hexanone			U	ND	ug/L						
4-Methyl-2-pentanone			U	ND	ug/L						
Acetone			U	ND	ug/L						
Benzene			U	ND	ug/L						
Bromodichloromethane			U	ND	ug/L						
Bromoform			U	ND	ug/L						
Bromomethane			U	ND	ug/L						
Carbon disulfide			U	ND	ug/L						
Carbon tetrachloride			U	ND	ug/L						
Chlorobenzene			U	ND	ug/L						
Chloroethane			U	ND	ug/L						
Chloroform			U	ND	ug/L						
Chloromethane			U	ND	ug/L						
Dibromochloromethane			U	ND	ug/L						
Ethylbenzene			U	ND	ug/L						
Methylene chloride			U	ND	ug/L						
Styrene			U	ND	ug/L						

09/25/02 11:19

## QC Summary

Workorder: 67169

Page 3 of 4

Parname	NOM	Sample	Qual	QC	Units	RPD%	REC%	Range	Anist	Date	Time
Volatile-GC/MS Federal											
Batch	203595										
Tetrachloroethylene			U	ND	ug/L						
Toluene			U	ND	ug/L						
Trichloroethylene			U	ND	ug/L						
Vinyl chloride			U	ND	ug/L						
Xylenes (total)			U	ND	ug/L						
cis-1,2-Dichloroethylene			U	ND	ug/L						
cis-1,3-Dichloropropylene			U	ND	ug/L						
trans-1,2-Dichloroethylene			U	ND	ug/L						
trans-1,3-Dichloropropylene			U	ND	ug/L						
**Bromofluorobenzene	50.0			61.9	ug/L		124	(67%-136%)			
**Dibromofluoromethane	50.0			60.7	ug/L		121	(62%-148%)			
**Toluene-d8	50.0			56.3	ug/L		113	(58%-139%)			
QC1200307212 MB											
1,1,1-Trichloroethane			U	ND	ug/L					09/24/02	19:27
1,1,2,2-Tetrachloroethane			U	ND	ug/L						
1,1,2-Trichloroethane			U	ND	ug/L						
1,1-Dichloroethane			U	ND	ug/L						
1,1-Dichloroethylene			U	ND	ug/L						
1,2-Dichloroethane			U	ND	ug/L						
1,2-Dichloropropane			U	ND	ug/L						
2-Butanone			U	ND	ug/L						
2-Hexanone			U	ND	ug/L						
4-Methyl-2-pentanone			U	ND	ug/L						
Acetone			U	ND	ug/L						
Benzene			U	ND	ug/L						
Bromodichloromethane			U	ND	ug/L						
Bromoform			U	ND	ug/L						
Bromomethane			U	ND	ug/L						
Carbon disulfide			U	ND	ug/L						
Carbon tetrachloride			U	ND	ug/L						
Chlorobenzene			U	ND	ug/L						
Chloroethane			U	ND	ug/L						
Chloroform			U	ND	ug/L						
Chloromethane			U	ND	ug/L						
Dibromochloromethane			U	ND	ug/L						
Ethylbenzene			U	ND	ug/L						
Methylene chloride			U	ND	ug/L						
Styrene			U	ND	ug/L						
Tetrachloroethylene			U	ND	ug/L						
Toluene			U	ND	ug/L						
Trichloroethylene			U	ND	ug/L						
Vinyl chloride			U	ND	ug/L						
Xylenes (total)			U	ND	ug/L						
cis-1,2-Dichloroethylene			U	ND	ug/L						
cis-1,3-Dichloropropylene			U	ND	ug/L						
trans-1,2-Dichloroethylene			U	ND	ug/L						
trans-1,3-Dichloropropylene			U	ND	ug/L						
**Bromofluorobenzene	50.0			60.6	ug/L		121	(67%-136%)			

## QC Summary

Workorder: 67169

Page 4 of 4

Partname	NOM	Sample	Qual	QC	Units	RPD%	REC%	Range	Anist	Date	Time
Volatile-GC/MS Federal											
Bach	203595										
**Dibromofluoromethane	50.0			62.2	ug/L		124	(62%-148%)			
**Toluene-d8	50.0			56.8	ug/L		114	(58%-139%)			
QC1200305539 67354001 PS											
1,1-Dichloroethylene	50.0	U	ND	43.1	ug/L		86	(67%-129%)		09/25/02	15:07
Benzene	50.0	U	ND	44.0	ug/L		88	(74%-112%)			
Chlorobenzene	50.0	U	ND	45.8	ug/L		92	(77%-113%)			
Toluene	50.0	U	ND	46.1	ug/L		92	(74%-109%)			
Trichloroethylene	50.0	U	ND	44.8	ug/L		90	(71%-118%)			
**Bromofluorobenzene	50.0		61.5	64.1	ug/L		128	(67%-136%)			
**Dibromofluoromethane	50.0		61.2	64.1	ug/L		128	(62%-148%)			
**Toluene-d8	50.0		56.6	59.1	ug/L		118	(58%-139%)			
QC1200305540 67354001 PSD											
1,1-Dichloroethylene	50.0	U	ND	40.5	ug/L	6	81	(0%-11%)		09/25/02	15:33
Benzene	50.0	U	ND	42.0	ug/L	5	84	(0%-8%)			
Chlorobenzene	50.0	U	ND	44.4	ug/L	3	89	(0%-11%)			
Toluene	50.0	U	ND	44.1	ug/L	5	88	(0%-12%)			
Trichloroethylene	50.0	U	ND	42.9	ug/L	4	86	(0%-9%)			
**Bromofluorobenzene	50.0		61.5	65.5	ug/L		131	(67%-136%)			
**Dibromofluoromethane	50.0		61.2	63.3	ug/L		127	(62%-148%)			
**Toluene-d8	50.0		56.6	59.2	ug/L		118	(58%-139%)			

**Notes:**

RER is calculated at the 95% confidence level (2-sigma).

The Qualifiers in this report are defined as follows:

- \* Recovery or %RPD not within acceptance limits and/or spike amount not compatible with the sample or the duplicate RPD's are not applicable where it
- \*\* Indicates analyte is a surrogate compound.
- B The analyte was found in the blank above the effective MDL.
- H Holding time was exceeded
- J Estimated value, the analyte concentration fell above the effective MDL and below the effective PQL
- P The response between the confirmation column and the primary column is >40%D
- U The analyte was analyzed for but not detected below this concentration. For Organic and Inorganic analytes the result is less than the effective MDL. ]
- X Presumptive evidence that the analyte is not present. Please see narrative for further information.
- X Presumptive evidence that the analyte is not present. Please see narrative for further information.
- X Uncertain identification for gamma spectroscopy.

N/A indicates that spike recovery limits do not apply when sample concentration exceeds spike conc. by a factor of 4 or more.

^ The Relative Percent Difference (RPD) obtained from the sample duplicate (DUP) is evaluated against the acceptance criteria when the sample is greater than five times (5X) the contract required detection limit (RL). In cases where either the sample or duplicate value is less than 5X the RL, a control limit of +/- the RL is used to evaluate the DUP result.

For PS, PSD, and SDILT results, the values listed are the measured amounts, not final concentrations.

Where the analytical method has been performed under NELAP certification, the analysis has met all of the requirements of the NELAC standard unless qualified on the QC Summary.

**REVISED**

GC/MS Volatile Organics  
Sandia National Labs (SNLS)  
SDG# 67158

Method/Analysis Information

Procedure: Volatile Organic Compounds (VOC) by Gas Chromatograph/Mass Spectrometer  
Analytical Method: SW846 8260A  
Prep Method: SW846 5030  
Analytical Batch Number: 202140  
Prep Batch Number: 202138

Sample Analysis

The following client and quality control samples were analyzed to complete this sample delivery group/work order using the methods referenced in the Analysis Information section:

Sample ID	Client ID
67158001	059820-001
67158002	059821-001
67158003	059822-001
67158004	059823-001
67158005	059824-001
67158006	059825-001
67158007	059828-001
67158008	059829-001
67158009	059836-001
67158010	059837-001
67158011	059838-001
67158012	059839-001
67158013	059841-001

SDG# 67158 -VOA

**REVISED**

67158014	059842-001
67158015	059843-001
67158016	059844-001
67158017	059845-001
67158018	059847-001
67158019	059848-001
1200301914	VBLK01 (Blank)
1200301915	VBLK01LCS (Laboratory Control Sample)
1200301916	059820-001MS (Matrix Spike)
1200301917	059820-001MSD (Matrix Spike Duplicate)

**Preparation/Analytical Method Verification**

**SOP Reference**

Procedure for preparation, analysis and reporting of analytical data are controlled by General Engineering Laboratories, Inc. as Standard Operating Procedure (SOP). The data discussed in this narrative has been analyzed in accordance with GL-OA E 026 REV.8.

**Calibration Information**

Due to software limitations, all the data files comprising the initial calibration curve may not be listed on the initial calibration summary form. All calibration files are listed in the calibration history report in the "Standard Data" section.

**Initial Calibration**

All the initial calibration requirements were met.

**CCV Requirements**

All the calibration verification standard (CCV) requirements were met.

**Quality Control (QC) Information**

**Surrogate Recoveries**

Surrogate recoveries, in all samples and quality control samples, were within the acceptance limits.

**Blank Acceptance**

Target analytes were not detected above the reporting limit in the blank.

**LCS Recovery Statement**

All the required analyte recoveries in the laboratory control sample were within the acceptance limits.

**QC Sample Designation**

The following sample was designated for matrix spike analysis:

SDG# 67158 -VOA

67158001 059820 001

**MS Recovery Statement**

All the required matrix spike recoveries were within the acceptance limits.

**MSD Recovery Statement**

All the required matrix spike duplicate recoveries were within the acceptance limits.

**MS/MSD RPD Statement**

The relative percent differences (RPD) between the matrix spike and matrix spike duplicate recoveries were within the acceptance limits.

**Internal Standard (ISTD) Acceptance**

The internal standard responses, in all samples and quality control samples, met the required acceptance criteria.

**Technical Information****Holding Time Specifications**

All the samples were prepared and/or analyzed within the required holding time period.

**Sample Preservation and Integrity**

All samples met the sample preservation and integrity requirements.

**Preparation/Analytical Method Verification**

All procedures were performed as stated in the SOP.

**Sample Dilutions**

The samples in this sample delivery group/work order did not require dilutions.

**Sample Re-prep/Re-analysis**

Re-analyses were not required for samples in this sample group/work order.

**Miscellaneous Information****Nonconformance (NCR) Documentation**

A nonconformance report was not required for this sample delivery group/work order.

**Manual Integrations**

Data files associated with the initial calibration, continuing calibration check, and samples did not require manual integrations.

**Additional Comments**

The following package was generated using an electronic data processing program referred to as "virtual packaging". In an effort to increase quality and efficiency, the laboratory is developing systems to eventually generate all data packages electronically. The following change from "traditional" packages should be noted: Analyst/peer reviewer initials and dates are not present on the electronic data files. Presently, all initials and dates are on the original raw data. These hard copies are temporarily stored in the laboratory. An electronic signature page inserted after the case narrative of each electronic package will indicate the analyst, reviewer, and report specialist names associated with the generation of the data package. The data validator will always sign and date the case narrative. Data that are not generated electronically, and such as hand written pages, will be scanned and inserted into the electronic package.

SDG# 67158 -VOA

Page 3 of 4



**REVISED**

**TIC Comment**

Tentatively identified compounds (TIC) were not required for this sample delivery group/work order.

**System Configuration**

The laboratory utilizes the following GC/MS configurations:

**Chromatographic Columns**

Chromatographic separation of volatile components is accomplished through analysis on one of the following columns:

Column ID	Column Description
J&W1	DB-624, 60m x 0.25mm, 1.4um
J&W2	DB-624, 75m x 0.53mm, 3.0um

**Instrument Configuration**

Instrument systems are reference in the raw data and individual form headers by the Instrument ID designations below:

Instrument ID	System Configuration	Chromatographic Column	P & T Trap
VOA1	HP6890/HP5973	J&W1	Trap C
VOA2	HP6890/HP5973	J&W1	Trap C
VOA4	HP5890/HP5972	J&W1	Trap K
VOA5	HP5890/HP5972	J&W1	Trap C
VOA7	HP5890/HP5972	J&W2	Trap K
VOA8	HP6890/HP5973	J&W1	Trap K
VOA9	HP6890/HP5973	J&W1	Trap C

**Certification Statement**

Where the analytical method has been performed under NELAP certification, the analysis has met all of the requirements of the NELAC standard unless otherwise noted in the analytical case narrative.

**Review Validation**

GEL requires all analytical data to be verified by a qualified data validator. In addition, all data designated for CLP or CLP-like packaging will receive a third level validation upon completion of the data package.

The following data validator verified the information presented in this case narrative:

Reviewer: Steph McLean Date: 10/15/02

SDG# 67158 -VOA

## QC Summary

Report Date: October 10, 2002  
Page 1 of 3

Client : Sandia National Laboratories  
MS-0756  
P.O. Box 5800  
Albuquerque, New Mexico  
Contact: Pamela M. Puissant  
Workorder: 67158

Parname	NOM	Sample	Qual	QC	Units	RPD%	REC%	Range	Anlst	Date	Time
Volatile-GC/MS Federal											
Batch	202140										
QC1200301915	LCS										
1,1-Dichloroethylene	50.0			45.8	ug/kg		92	(75%-134%)	TLW	09/20/02	21:06
Benzene	50.0			47.3	ug/kg		95	(80%-120%)			
Chlorobenzene	50.0			49.0	ug/kg		98	(82%-118%)			
Toluene	50.0			47.5	ug/kg		95	(74%-115%)			
Trichloroethylene	50.0			46.1	ug/kg		92	(80%-119%)			
**Bromofluorobenzene	50.0			56.1	ug/kg		112	(69%-138%)			
**Dibromofluoromethane	50.0			62.7	ug/kg		125	(67%-137%)			
**Toluene-d8	50.0			61.0	ug/kg		122	(67%-139%)			
QC1200301914	MB										
1,1,1-Trichloroethane			U	ND	ug/kg					09/20/02	22:02
1,1,2,2-Tetrachloroethane			U	ND	ug/kg						
1,1,2-Trichloroethane			U	ND	ug/kg						
1,1-Dichloroethane			U	ND	ug/kg						
1,1-Dichloroethylene			U	ND	ug/kg						
1,2-Dichloroethane			U	ND	ug/kg						
1,2-Dichloropropane			U	ND	ug/kg						
2-Butanone			U	ND	ug/kg						
2-Hexanone			U	ND	ug/kg						
4-Methyl-2-pentanone			U	ND	ug/kg						
Acetone			U	ND	ug/kg						
Benzene			U	ND	ug/kg						
Bromodichloromethane			U	ND	ug/kg						
Bromoform			U	ND	ug/kg						
Bromomethane			U	ND	ug/kg						
Carbon disulfide			U	ND	ug/kg						
Carbon tetrachloride			U	ND	ug/kg						
Chlorobenzene			U	ND	ug/kg						
Chloroethane			U	ND	ug/kg						
Chloroform			U	ND	ug/kg						
Chloromethane			U	ND	ug/kg						
Dibromochloromethane			U	ND	ug/kg						
Ethylbenzene			U	ND	ug/kg						
Methylene chloride			U	ND	ug/kg						
Styrene			U	ND	ug/kg						
Tetrachloroethylene			U	ND	ug/kg						
Toluene			U	ND	ug/kg						
Trichloroethylene			U	ND	ug/kg						
Vinyl acetate			U	ND	ug/kg						
Vinyl chloride			U	ND	ug/kg						
Xylenes (total)			U	ND	ug/kg						
cis-1,2-Dichloroethylene			U	ND	ug/kg						
cis-1,3-Dichloropropylene			U	ND	ug/kg						

## QC Summary

Workorder: 67158

Page 2 of 3

Parname	NOM	Sample	Qual	QC	Units	RPD%	REC%	Range	Anlst	Date	Time
Volatile-GC/MS Federal											
Batch 202140											
trans-1,2-Dichloroethylene			U	ND	ug/kg						
trans-1,3-Dichloropropylene			U	ND	ug/kg						
**Bromofluorobenzene	50.0			59.0	ug/kg		118	(69%-138%)			
**Dibromofluoromethane	50.0			62.8	ug/kg		126	(67%-137%)			
**Toluene-d8	50.0			64.4	ug/kg		129	(67%-139%)			
QC1200301916 67158001 PS											
1,1-Dichloroethylene	50.0	U	ND	43.7	ug/L		87	(55%-128%)		09/21/02	07:12
Benzene	50.0	U	ND	41.5	ug/L		83	(53%-118%)			
Chlorobenzene	50.0	U	ND	39.2	ug/L		78	(53%-116%)			
Toluene	50.0	U	ND	39.8	ug/L		80	(56%-113%)			
Trichloroethylene	50.0	U	ND	44.7	ug/L		89	(54%-119%)			
**Bromofluorobenzene	50.0		60.0	58.0	ug/L		116	(69%-138%)			
**Dibromofluoromethane	50.0		63.5	67.3	ug/L		135	(67%-137%)			
**Toluene-d8	50.0		62.0	61.0	ug/L		122	(67%-139%)			
QC1200301917 67158001 PSD											
1,1-Dichloroethylene	50.0	U	ND	41.6	ug/L	5	83	(0%-21%)		09/21/02	07:40
Benzene	50.0	U	ND	42.0	ug/L	1	84	(0%-17%)			
Chlorobenzene	50.0	U	ND	39.7	ug/L	1	80	(0%-21%)			
Toluene	50.0	U	ND	39.9	ug/L	0	80	(0%-25%)			
Trichloroethylene	50.0	U	ND	43.3	ug/L	3	87	(0%-25%)			
**Bromofluorobenzene	50.0		60.0	59.7	ug/L		119	(69%-138%)			
**Dibromofluoromethane	50.0		63.5	64.0	ug/L		128	(67%-137%)			
**Toluene-d8	50.0		62.0	62.1	ug/L		124	(67%-139%)			

**Notes:**

RER is calculated at the 95% confidence level (2-sigma).

The Qualifiers in this report are defined as follows:

- \* Recovery or %RPD not within acceptance limits and/or spike amount not compatible with the sample or the duplicate; RPD's are not applicable where t
- \*\* Indicates analyte is a surrogate compound.
- B The analyte was found in the blank above the effective MDL.
- H Holding time was exceeded
- J Estimated value, the analyte concentration fell above the effective MDL and below the effective PQL
- P The response between the confirmation column and the primary column is >40%D
- U The analyte was analyzed for but not detected below this concentration. For Organic and Inorganic analytes the result is less than the effective MDL. I
- X Presumptive evidence that the analyte is not present. Please see narrative for further information.
- X Presumptive evidence that the analyte is not present. Please see narrative for further information.
- X Uncertain identification for gamma spectroscopy.

## QC Summary

Workorder: 67158

Page 3 of 3

Parmname	NOM	Sample	Qual	QC	Units	RPD%	REC%	Range	Anlst	Date	Time
----------	-----	--------	------	----	-------	------	------	-------	-------	------	------

N/A indicates that spike recovery limits do not apply when sample concentration exceeds spike conc. by a factor of 4 or more.

^ The Relative Percent Difference (RPD) obtained from the sample duplicate (DUP) is evaluated against the acceptance criteria when the sample is greater than five times (5X) the contract required detection limit (RL). In cases where either the sample or duplicate value is less than 5X the RL, a control limit of +/- the RL is used to evaluate the DUP result.

For PS, PSD, and SDILT results, the values listed are the measured amounts, not final concentrations.

Where the analytical method has been performed under NELAP certification, the analysis has met all of the requirements of the NELAC standard unless qualified on the QC Summary.

Semi-Volatile Case Narrative  
Sandia National Labs (SNLS)  
SDG 67158-1

Method/Analysis Information

Procedure: Semivolatile Analysis by Gas Chromatograph/Mass Spectrometer  
Analytical Method: SW846 8270C  
Prep Method: SW846 3510C  
Analytical Batch Number: 201951  
Prep Batch Number: 201948

Sample Analysis

The following samples were analyzed using the analytical protocol as established in SW846 8270C:

Sample ID	Client ID
67169005	059826-002
1200301424	SBLK01 (Blank)
1200301425	SBLK01LCS (Laboratory Control Sample)
1200301426	059826-002MS (Matrix Spike)
1200301427	059826-002MSD (Matrix Spike Duplicate)

Preparation/Analytical Method Verification

Procedures for preparation, analysis, and reporting of analytical data are documented by General Engineering Laboratories, Inc. (GEL) as Standard Operating Procedures (SOP).

Calibration Information

Due to the limited capacity of software we do not display all of the current initial calibration files here. If necessary, a calibration history will be inserted in the package prior to the appropriate Form 6.

Diphenylamine has now superseded N-Nitroso-diphenylamine as a CCC on Quantitation Reports, Initial Calibration Reports, Calibration Check Standard Reports, etc. Previous versions of EPA Method 8270 (prior to 8270C) listed N-Nitroso-diphenylamine as a CCC. However, as stated in EPA Method 8270C, Revision 3, December, 1996, Section 1.4.5, "N-Nitroso-diphenylamine decomposes in the gas chromatographic inlet and cannot be separated from Diphenylamine." Studies of these two compounds at GEL, both independent of each other and together, show that they not only coelute, but also have similar mass spectra. N-Nitroso-diphenylamine and Diphenylamine will be reported as Diphenylamine on all reports and forms.

When calibrations are performed for Appendix IX compounds some of the compounds may not be calibrated exactly according to the criteria in Method 8270C. If the %RSD is greater than 15% or the correlation coefficient is less than 0.99 then the analyte is quantitated using the response factor. If the analyte is detected then the sample is reanalyzed for that analyte on an instrument that is compliant with the criteria in the method.

**Initial Calibration**

All initial calibration requirements have been met for this SDG.

**CCV Requirements**

All calibration verification standard (CVS, ICV or CCV) requirements have been met for this SDG.

**Quality Control (QC) Information**

**Surrogate Recoveries**

All the surrogate recoveries were within the established acceptance criteria for this SDG.

**Blank Acceptance**

Target analytes were detected in the blank below the reporting limit.

**LCS Recovery Statement**

The laboratory control sample (LCS) spike recoveries for this SDG were within the established acceptance limits.

**QC Sample Designation**

The following sample analyzed with this SDG was chosen for matrix spike analysis.  
67169005 (059826-002)

**MS Recovery Statement**

The matrix spike recoveries for this SDG were within the established acceptance limits.

**MSD Recovery Statement**

The matrix spike duplicate (MSD) recoveries for this SDG were within the established acceptance limits.

**MS/MSD RPD Statement**

The relative percent differences (RPD) between each MS and MSD were within the required acceptance limits.

**Internal Standard (ISTD) Acceptance**

The internal standard responses were within the required acceptance criteria for all samples and QC.

**Technical Information:****Holding Time Specifications**

All samples in this SDG met the specified holding time requirements. GEL assigns holding times based on the associated methodology that assigns the date and time from sample collection or sample receipt. Those holding times expressed in hours are calculated in the AlphaLIMS system. Those holding times expressed as days expire at midnight on the day of expiration. GEL assigns holding times based on the associated methodology that assigns the date and time from sample collection or sample receipt. Those holding times expressed in hours are calculated in the AlphaLIMS system. Those holding times expressed as days expire at midnight on the day of expiration.

**Preparation/Analytical Method Verification**

All procedures were performed as stated in the SOP.

**Sample Dilutions**

None of the samples analyzed in this SDG required dilution.

**Miscellaneous Information:****Nonconformance (NCR) Documentation**

No nonconformance report (NCR) was generated for this SDG.

**Manual Integrations**

No manual integrations were required for any data file in this SDG.

**Additional Comments**

No additional comments are needed for this SDG.

**System Configuration**

The laboratory utilizes a HP 6890 Series gas chromatograph and a HP 5973 Mass Selective Detector. The configuration is equipped with the electronic pressure control. All MS interfaces are capillary direct.

## Chromatographic Columns

Chromatographic separation of semivolatile components is accomplished through analysis on one or more of the following columns (all with dimensions of 30 meters x 0.25 millimeters ID and 0.25 micron film except J&W DB-5MS2 which is 25 meters x 0.20 mm ID and 0.33 micron film):

Column ID	Column Description
J&W	DB-5.625(5% Phenyl)-methylpolysiloxane (identified by a DB-5.625 designation on quantitation reports and reconstructed ion chromatograms)
J&W DB-5MS	Similar to the J&W DB-5.625 with low bleed characteristics (identified by a DB-5MS designation)
Alltech	EC-5 (SE-54) 5% Phenyl, 95% Methylpolysiloxane (identified by a HP-5MS designation)
HP	HP-5MS 5% Phenylmethylsiloxane (identified by a HP-5MS designation)
Phenomenex	ZB-5 5% Phenyl Polysiloxane (identified by a ZB-5 designation)
J&W DB-5MS2	Similar to the J&W DB-5.625 with low bleed characteristics (identified by a DB-5MS2 designation)

## Instrument Configuration

The samples reported in this SDG were analyzed on one or more of the following instrument systems. Instrument systems are referenced in the raw data and individual form headers by the Instrument ID designations listed below:

Instrument ID	System Configuration	Chromatographic Column
MSD2	HP6890/HP5973	DB-5MS2
MSD4	HP6890/HP5973	DB-5MS2
MSD5	HP6890/HP5973	DB-5MS2
MSD7	HP6890/HP5973	DB-5MS2
MSD8	HP6890/HP5973	DB-5MS2



**Certification Statement**

\* Where the analytical method has been performed under NELAP certification, the analysis has met all of the requirements of the NELAC standard unless otherwise noted in the analytical case narrative.

**Review Validation:**

GFL requires all analytical data to be verified by a qualified data validator. In addition, all data designated for CLP or CLP-like packaging will receive a third level validation upon completion of the data package.

Reviewer: Erin Haubert Date: 12/9/02

## QC Summary

Report Date: October 9, 2002

Page 1 of 4

Client : Sandia National Laboratories  
 MS-0756  
 P.O. Box 5800  
 Albuquerque, New Mexico

Contact: Pamela M. Puissant

Workorder: 67169

Parname	NOM	Sample Qual	QC	Units	RPD%	REC%	Range	Anlst	Date Time
Semi-Volatiles-GC/MS									
Batch: 201951									
QC1200301425 LCS									
1,2,4-Trichlorobenzene	50.0		38.5	ug/L		77	(53%-104%)	JWF	09/18/02 15:21
1,4-Dichlorobenzene	50.0		39.1	ug/L		78	(47%-102%)		
2,4,5-Trichlorophenol	100		89.1	ug/L		89	(67%-106%)		
2,4,6-Trichlorophenol	100		86.0	ug/L		86	(45%-111%)		
2,4-Dinitrotoluene	50.0		45.3	ug/L		91	(55%-121%)		
2-Chlorophenol	100		71.9	ug/L		72	(47%-87%)		
4-Chloro-3-methylphenol	100		81.1	ug/L		81	(51%-100%)		
4-Nitrophenol	100		32.1	ug/L		32	(10%-55%)		
Acenaphthene	50.0		44.0	ug/L		38	(63%-111%)		
Hexachlorobenzene	50.0		42.0	ug/L		84	(67%-114%)		
Hexachlorobutadiene	50.0		38.5	ug/L		77	(44%-106%)		
Hexachlorocyclohexane	50.0		37.3	ug/L		75	(47%-97%)		
N-Nitrosodipropylamine	50.0		42.5	ug/L		85	(52%-118%)		
Nitrobenzene	50.0		41.7	ug/L		83	(49%-110%)		
Pentachlorophenol	100		75.6	ug/L		76	(31%-110%)		
Phenol	100		31.9	ug/L		32	(16%-44%)		
Pyrene	50.0		38.3	ug/L		77	(68%-117%)		
m,p-Cresols	100		61.1	ug/L		61	(43%-100%)		
o-Cresol	100		68.3	ug/L		68	(47%-87%)		
*2,4,6-Tribromophenol	100		93.1	ug/L		93	(27%-126%)		
*2-Fluorobiphenyl	50.0		39.9	ug/L		80	(32%-109%)		
*2-Fluorophenol	100		45.4	ug/L		45	(13%-73%)		
*Nitrobenzene-d5	50.0		36.8	ug/L		74	(33%-107%)		
*Phenol-d5	100		30.2	ug/L		30	(14%-66%)		
*p-Terphenyl-d14	50.0		40.8	ug/L		82	(36%-130%)		
QC1200301424 MB									
1,2,4-Trichlorobenzene		U	ND	ug/L					09/18/02 14:59
1,2-Dichlorobenzene		U	ND	ug/L					
1,3-Dichlorobenzene		U	ND	ug/L					
1,4-Dichlorobenzene		U	ND	ug/L					
2,4,5-Trichlorophenol		U	ND	ug/L					
2,4,6-Trichlorophenol		U	ND	ug/L					
2,4-Dichlorophenol		U	ND	ug/L					
2,4-Dimethylphenol		U	ND	ug/L					
2,4-Dinitrophenol		U	ND	ug/L					
2,4-Dinitrotoluene		U	ND	ug/L					
2,6-Dinitrotoluene		U	ND	ug/L					
2-Chloronaphthalene		U	ND	ug/L					
2-Chlorophenol		U	ND	ug/L					
2-Methyl-4,6-dinitrophenol		U	ND	ug/L					
2-Methylnaphthalene		U	ND	ug/L					
2-Nitrophenol		U	ND	ug/L					

## QC Summary

Workorder: 67169

Parname	NOM	Sample	Qual	QC	Units	RPD%	REC%	Range	Anist	Date	Time
Semi-Volatiles-GC/MS											
Batch: 201951											
3,3'-Dichlorobenzidine			U	ND	ug/L						
4-Bromophenylphenylether			U	ND	ug/L						
4-Chloro-3-methylphenol			U	ND	ug/L						
4-Chloroaniline			U	ND	ug/L						
4-Chlorophenylphenylether			U	ND	ug/L						
4-Nitrophenol			U	ND	ug/L						
Acenaphthene			U	ND	ug/L						
Acenaphthylene			U	ND	ug/L						
Anthracene			U	ND	ug/L						
Benzo(a)anthracene			U	ND	ug/L						
Benzo(a)pyrene			U	ND	ug/L						
Benzo(b)fluoranthene			U	ND	ug/L						
Benzo(ghi)perylene			U	ND	ug/L						
Benzo(k)fluoranthene			U	ND	ug/L						
Butylbenzylphthalate			U	ND	ug/L						
Carbazole			U	ND	ug/L						
Chrysene			U	ND	ug/L						
Di-n-butylphthalate			U	ND	ug/L						
Di-n-octylphthalate			U	ND	ug/L						
Dibenzo(a,h)anthracene			U	ND	ug/L						
Dibenzofuran			U	ND	ug/L						
Diethylphthalate			U	ND	ug/L						
Dimethylphthalate			U	ND	ug/L						
Diphenylamine			U	ND	ug/L						
Fluoranthene			U	ND	ug/L						
Fluorene			U	ND	ug/L						
Hexachlorobenzene			U	ND	ug/L						
Hexachlorobutadiene			U	ND	ug/L						
Hexachlorocyclopentadiene			U	ND	ug/L						
Hexachloroethane			U	ND	ug/L						
Indeno(1,2,3-cd)pyrene			U	ND	ug/L						
Isophorone			U	ND	ug/L						
N-Nitrosodipropylamine			U	ND	ug/L						
Naphthalene			U	ND	ug/L						
Nitrobenzene			U	ND	ug/L						
Pentachlorophenol			U	ND	ug/L						
Phenanthrene			U	ND	ug/L						
Phenol			U	ND	ug/L						
Pyrene			U	ND	ug/L						
bis(2-Chloroethoxy)methane			U	ND	ug/L						
bis(2-Chloroethyl) ether			U	ND	ug/L						
bis(2-Chloroisopropyl)ether			U	ND	ug/L						
bis(2-Ethylhexyl)phthalate			U	ND	ug/L						
m,p-Cresols			U	ND	ug/L						
m-Nitroaniline			U	ND	ug/L						
o-Cresol			U	ND	ug/L						
o-Nitroaniline			U	ND	ug/L						
p-Nitroaniline			U	ND	ug/L						

## QC Summary

Workorder: 67169

Page 3 of 4

Parname	NOM	Sample Qual	QC	Units	RPD%	REC%	Range	Anlst	Date Time
<i>Semi-Volatiles-GC/MS</i>									
Batch	201951								
*2,4,6-Tribromophenol	100		75.0	ug/L		75	(27%-126%)		
*2-Fluorobiphenyl	50.0		42.5	ug/L		85	(32%-109%)		
*2-Fluorophenol	100		46.7	ug/L		47	(13%-73%)		
*Nitrobenzene-d5	50.0		42.1	ug/L		84	(33%-107%)		
*Phenol-d5	100		31.3	ug/L		31	(14%-66%)		
*p-Terphenyl-d14	50.0		49.8	ug/L		100	(36%-130%)		
QC1200301426 67169005 MS									
1,2,4-Trichlorobenzene	100		82.9	ug/L		83	(44%-102%)		09/18/02 18:49
1,4-Dichlorobenzene	100		80.3	ug/L		80	(48%-95%)		
2,4,5-Trichlorophenol	200		185	ug/L		93			
2,4,6-Trichlorophenol	200		183	ug/L		91			
2,4-Dinitrotoluene	100		96.4	ug/L		96	(48%-120%)		
2-Chlorophenol	200		159	ug/L		75	(32%-98%)		
4-Chloro-3-methylphenol	200		177	ug/L		88	(40%-107%)		
4-Nitrophenol	200		110	ug/L		55	(16%-78%)		
Acenaphthene	100		94.3	ug/L		94	(32%-127%)		
Hexachlorobenzene	100		86.2	ug/L		86			
Hexachlorobutadiene	100		84.4	ug/L		84			
Hexachloroethane	100		78.6	ug/L		79			
N-Nitrosodipropylamine	100		85.5	ug/L		86	(44%-119%)		
Nitrobenzene	100		82.9	ug/L		83			
Pentachlorophenol	200		180	ug/L		90	(44%-104%)		
Phenol	200		89.2	ug/L		45	(15%-70%)		
Pyrene	100		75.0	ug/L		75	(29%-142%)		
m,p-Cresols	200		145	ug/L		72			
o-Cresol	200		153	ug/L		76			
*2,4,6-Tribromophenol	200		200	ug/L		100	(27%-126%)		
*2-Fluorobiphenyl	100		80.5	ug/L		81	(32%-109%)		
*2-Fluorophenol	200		113	ug/L		57	(13%-73%)		
*Nitrobenzene-d5	100		74.9	ug/L		75	(33%-107%)		
*Phenol-d5	200		86.7	ug/L		43	(14%-66%)		
*p-Terphenyl-d14	100		80.4	ug/L		80	(36%-130%)		
QC1200301427 67169005 MSD									
1,2,4-Trichlorobenzene	100		77.5	ug/L	7	78	(0%-20%)		09/18/02 19:12
1,4-Dichlorobenzene	100		75.6	ug/L	6	76	(0%-20%)		
2,4,5-Trichlorophenol	200		184	ug/L	1	92			
2,4,6-Trichlorophenol	200		179	ug/L	2	90			
2,4-Dinitrotoluene	100		91.0	ug/L	6	91	(0%-16%)		
2-Chlorophenol	200		144	ug/L	4	72	(0%-25%)		
4-Chloro-3-methylphenol	200		165	ug/L	7	85	(0%-25%)		
4-Nitrophenol	200		100	ug/L	9	50	(0%-25%)		
Acenaphthene	100		90.9	ug/L	4	91	(0%-24%)		
Hexachlorobenzene	100		85.4	ug/L	1	85			
Hexachlorobutadiene	100		79.8	ug/L	6	80			
Hexachloroethane	100		73.0	ug/L	7	73			
N-Nitrosodipropylamine	100		82.4	ug/L	3	83	(0%-20%)		
Nitrobenzene	100		78.9	ug/L	5	79			
Pentachlorophenol	200		165	ug/L	8	83	(0%-17%)		

## QC Summary

Workorder: 67169

Page 4 of 4

Parma name	NOM	Sample	Qual	QC	Units	RPD%	REC%	Range	Analst	Date	Time
Semi-Volatiles-GC/MS											
Batch	201951										
Phenol	200			86.3	ug/L	3	43	(0%-29%)			
Pyrene	100			82.3	ug/L	9	82	(0%-30%)			
m,p-Cresols	200			143	ug/L	2	71				
o-Cresol	200			149	ug/L	3	75				
*2,4,6-Tribromophenol	200			186	ug/L		93	(27%-126%)			
*2-Fluorobiphenyl	100			78.2	ug/L		78	(32%-109%)			
*2-Fluorophenol	200			109	ug/L		54	(13%-73%)			
*Nitrobenzene-d5	100			72.0	ug/L		72	(33%-107%)			
*Phenol-d5	200			84.8	ug/L		42	(14%-66%)			
*p-Terphenyl-d14	100			87.4	ug/L		87	(36%-130%)			

**Notes:**

RER is calculated at the 95% confidence level (2-sigma).

The Qualifiers in this report are defined as follows:

- \* Recovery or %RPD not within acceptance limits and/or spike amount not compatible with the sample or the duplicate RPD's are not applicable where th
- \*\* Indicates analyte is a surrogate compound.
- B The analyte was found in the blank above the effective MDL.
- H Holding time was exceeded
- J Estimated value, the analyte concentration fell above the effective MDL and below the effective PQL
- P The response between the confirmation column and the primary column is >40%D
- U The analyte was analyzed for but not detected below this concentration. For Organic and Inorganic analytes the result is less than the effective MDL. F
- X Presumptive evidence that the analyte is not present. Please see narrative for further information.
- X Presumptive evidence that the analyte is not present. Please see narrative for further information.
- X Uncertain identification for gamma spectroscopy.

N/A indicates that spike recovery limits do not apply when sample concentration exceeds spike conc. by a factor of 4 or more.

The Relative Percent Difference (RPD) obtained from the sample duplicate (DUP) is evaluated against the acceptance criteria when the sample is greater than five times (5X) the contract required detection limit (RL). In cases where either the sample or duplicate value is less than 5X the RL, a control limit of +/- the RL is used to evaluate the DUP result.

For PS, PSD, and SDILT results, the values listed are the measured amounts, not final concentrations.

Where the analytical method has been performed under NELAP certification, the analysis has met all of the requirements of the NELAC standard unless qualified on the QC Summary.

Semi-Volatile Case Narrative  
Sandia National Labs (SNLS)  
SDG 67158

Method/Analysis Information

Procedure: Semivolatile Analysis by Gas Chromatograph/Mass Spectrometer  
Analytical Method: SW846 8270C  
Prep Method: SW846 3550B  
Analytical Batch Number: 201961  
Prep Batch Number: 201960

Sample Analysis

The following samples were analyzed using the analytical protocol as established in SW846 8270C:

<b>Sample ID</b>	<b>Client ID</b>
67158020	059820-002
67158021	059821-002
67158022	059822-002
67158023	059823-002
67158024	059824-002
67158025	059825-002
67158026	059828-002
67158027	059829-002
67158028	059836-002
67158029	059837-002
67158030	059838-002
67158031	059839-002

67158032	059841-002
67158033	059842-002
67158034	059843-002
67158035	059844-002
67158036	059846-001
67158037	059847-002
67158038	059848-002
1200301450	MBSBLK01 (Blank)
1200301451	SBLK01LCS (Laboratory Control Sample)
1200301452	059820-002MS (Matrix Spike)
1200301453	059820-002MSD (Matrix Spike Duplicate)

**Preparation/Analytical Method Verification**

Procedures for preparation, analysis, and reporting of analytical data are documented by General Engineering Laboratories, Inc. (GEL) as Standard Operating Procedures (SOP).

**Calibration Information**

Due to the limited capacity of software we do not display all of the current initial calibration files here. If necessary, a calibration history will be inserted in the package prior to the appropriate Form 6.

Diphenylamine has now superseded N-Nitroso-diphenylamine as a CCC on Quantitation Reports, Initial Calibration Reports, Calibration Check Standard Reports, etc. Previous versions of EPA Method 8270 (prior to 8270C) listed N-Nitroso-diphenylamine as a CCC. However, as stated in EPA Method 8270C, Revision 3, December, 1996, Section 1.4.5, "N-Nitroso-diphenylamine decomposes in the gas chromatographic inlet and cannot be separated from Diphenylamine." Studies of these two compounds at GEL, both independent of each other and together, show that they not only coelute, but also have similar mass spectra. N-Nitroso-diphenylamine and Diphenylamine will be reported as Diphenylamine on all reports and forms.

When calibrations are performed for Appendix IX compounds some of the compounds may not be calibrated exactly according to the criteria in Method 8270C. If the %RSD is greater than 15% or the correlation coefficient is less than 0.99 then the analyte is quantitated using the response factor. If the analyte is detected then the sample is reanalyzed for that analyte on an

instrument that is compliant with the criteria in the method.

**Initial Calibration**

All initial calibration requirements have been met for this SDG.

**CCV Requirements**

All calibration verification standard (CVS, ICV or CCV) requirements have been met for this SDG.

**Quality Control (QC) Information**

**Surrogate Recoveries**

All the surrogate recoveries were within the established acceptance criteria for this SDG.

**Blank Acceptance**

Target analytes were detected in the method blank; however, the hits were below the reporting limit.

**LCS Recovery Statement**

The laboratory control sample (LCS) spike recoveries for this SDG were within the established acceptance limits.

**QC Sample Designation**

The following sample analyzed with this SDG was chosen for matrix spike analysis.  
67158020 (059820-002)

**MS Recovery Statement**

The matrix spike recoveries for this SDG were within the established acceptance limits.

**MSD Recovery Statement**

The matrix spike duplicate (MSD) recoveries for this SDG were within the established acceptance limits.

**MS/MSD RPD Statement**

The relative percent differences (RPD) between each MS and MSD were within the required acceptance limits.

**Internal Standard (ISTD) Acceptance**

The internal standard responses were within the required acceptance criteria for all samples and QC.

**Technical Information:**

**Holding Time Specifications**

All samples in this SDG met the specified holding time requirements. GEL assigns holding times



based on the associated methodology that assigns the date and time from sample collection or sample receipt. Those holding times expressed in hours are calculated in the AlphaLIMS system. Those holding times expressed as days expire at midnight on the day of expiration. GEL assigns holding times based on the associated methodology that assigns the date and time from sample collection or sample receipt. Those holding times expressed in hours are calculated in the AlphaLIMS system. Those holding times expressed as days expire at midnight on the day of expiration.

**Preparation/Analytical Method Verification**

All procedures were performed as stated in the SOP.

**Sample Dilutions**

None of the samples analyzed in this SDG required dilution.

**Miscellaneous Information:**

**Nonconformance (NCR) Documentation**

No nonconformance report (NCR) was generated for this SDG.

**Manual Integrations**

No manual integrations were required for any data file in this SDG.

**Additional Comments**

No additional comments are needed for this SDG.

**System Configuration**

The laboratory utilizes a HP 6890 Series gas chromatograph and a HP 5973 Mass Selective Detector. The configuration is equipped with the electronic pressure control. All MS interfaces are capillary direct.

**Chromatographic Columns**

Chromatographic separation of semivolatile components is accomplished through analysis on one or more of the following columns (all with dimensions of 30 meters x 0.25 millimeters ID and 0.25 micron film except J&W DB-5MS2 which is 25 meters x 0.20 mm ID and 0.33 micron film):

Column ID	Column Description
J&W	DB-5.625(5% Phenyl)-methylpolysiloxane (identified by a DB-5.625 designation on quantitation reports and reconstructed ion chromatograms)

J&W DB-5MS	Similar to the J&W DB-5.625 with low bleed characteristics (identified by a DB-5MS designation)
Alltech	EC-5 (SE-54) 5% Phenyl, 95% Methylpolysiloxane (identified by a HP-5MS designation)
HP	HP-5MS 5% Phenylmethylsiloxane (identified by a HP-5MS designation)
Phenomenex	ZB-5 5% Phenyl Polysiloxane (identified by a ZB-5 designation)
J&W DB-5MS2	Similar to the J&W DB-5.625 with low bleed characteristics (identified by a DB-5MS2 designation)

### **Instrument Configuration**

The samples reported in this SDG were analyzed on one or more of the following instrument systems. Instrument systems are referenced in the raw data and individual form headers by the Instrument ID designations listed below:

<b>Instrument ID</b>	<b>System Configuration</b>	<b>Chromatographic Column</b>
MSD2	HP6890/HP5973	DB-5MS2
MSD4	HP6890/HP5973	DB-5MS2
MSD5	HP6890/HP5973	DB-5MS2
MSD7	HP6890/HP5973	DB-5MS2
MSD8	HP6890/HP5973	DB-5MS2

### **Certification Statement**

\* Where the analytical method has been performed under NELAP certification, the analysis has met all of the requirements of the NELAC standard unless otherwise noted in the analytical case narrative.

### **Review Validation:**

GEL requires all analytical data to be verified by a qualified data validator. In addition, all data designated for CLP or CLP-like packaging will receive a third level validation upon completion of the data package.

Reviewer: Erin Haupt Date: 10/9/02

## QC Summary

Report Date: October 9, 2002  
Page 1 of 4

Client : Sandia National Laboratories  
MS-0756  
P.O. Box 5800  
Albuquerque, New Mexico  
Contact: Pamela M. Puissant  
Workorder: 67158

Parname	NOM	Sample	Quai	QC	Units	RPD%	REC%	Range	Anlst	Date	Time
Semi-Volatiles-GC/MS Federal											
Batch 201961											
QC1200301451 LCS											
Pyridine	1670			730	ug/kg		44		GB1	09/18/02	16:48
1,2,4-Trichlorobenzene	1670			1170	ug/kg		70	(27%-91%)			
1,4-Dichlorobenzene	1670			1060	ug/kg		64	(25%-85%)			
2,4,5-Trichlorophenol	3330			2750	ug/kg		83	(42%-96%)			
2,4,6-Trichlorophenol	3330			2520	ug/kg		76	(32%-91%)			
2,4-Dinitrotoluene	1670			1320	ug/kg		79	(50%-109%)			
2-Chlorophenol	3330			2310	ug/kg		69	(31%-85%)			
4-Chloro-3-methylphenol	3330			2760	ug/kg		83	(34%-97%)			
4-Nitrophenol	3330			2410	ug/kg		72	(22%-128%)			
Acenaphthene	1670			1250	ug/kg		75	(39%-98%)			
Hexachlorobenzene	1670			1310	ug/kg		79	(41%-105%)			
Hexachlorobutadiene	1670			1080	ug/kg		65	(21%-94%)			
Hexachloroethane	1670			1060	ug/kg		64	(25%-86%)			
N-Nitrosodipropylamine	1670			1160	ug/kg		69	(34%-90%)			
Nitrobenzene	1670			1130	ug/kg		68	(30%-84%)			
Pentachlorophenol	3330			1910	ug/kg		57	(27%-109%)			
Phenol	3330			2430	ug/kg		73	(31%-83%)			
Pyrene	1670			1230	ug/kg		74	(37%-110%)			
m,p-Cresols	3330			2420	ug/kg		73	(40%-83%)			
o-Cresol	3330			2350	ug/kg		70	(34%-86%)			
*2,4,6-Tribromophenol	3330			2490	ug/kg		75	(23%-111%)			
*2-Fluorobiphenyl	1670			1200	ug/kg		72	(21%-104%)			
*2-Fluorophenol	3330			2390	ug/kg		72	(22%-93%)			
*Nitrobenzene-d5	1670			1110	ug/kg		67	(24%-97%)			
*Phenol-d5	3330			2480	ug/kg		74	(22%-99%)			
*p-Torphenyl-d14	1670			1470	ug/kg		88	(30%-133%)			
QC1200301450 MB											
1,2,4-Trichlorobenzene			U	ND	ug/kg					09/18/02	16:27
1,2-Dichlorobenzene			U	ND	ug/kg						
1,3-Dichlorobenzene			U	ND	ug/kg						
1,4-Dichlorobenzene			U	ND	ug/kg						
2,4,5-Trichlorophenol			U	ND	ug/kg						
2,4,6-Trichlorophenol			U	ND	ug/kg						
2,4-Dichlorophenol			U	ND	ug/kg						
2,4-Dimethylphenol			U	ND	ug/kg						
2,4-Dinitrophenol			U	ND	ug/kg						
2,4-Dinitrotoluene			U	ND	ug/kg						
2,6-Dinitrotoluene			U	ND	ug/kg						
2-Chloronaphthalene			U	ND	ug/kg						
2-Chlorophenol			U	ND	ug/kg						
2-Methyl-4,6-dinitrophenol			U	ND	ug/kg						
2-Methylnaphthalene			U	ND	ug/kg						

## QC Summary

Workorder: 67158

Page 2 of 4

Parname	NOM	Sample	Qual	QC	Units	RPD%	REC%	Range	Analst	Date	Time
Semi-Volatiles-GC/MS Federal											
Batch 201961											
2-Nitrophenol			U	ND	ug/kg						
3,3'-Dichlorobenzidine			U	ND	ug/kg						
4-Bromophenylphenylether			U	ND	ug/kg						
4-Chloro-3-methylphenol			U	ND	ug/kg						
4-Chloroaniline			U	ND	ug/kg						
4-Chlorophenylphenylether			U	ND	ug/kg						
4-Nitrophenol			U	ND	ug/kg						
Acenaphthene			U	ND	ug/kg						
Acenaphthylene			U	ND	ug/kg						
Anthracene			U	ND	ug/kg						
Benzo(a)anthracene			U	ND	ug/kg						
Benzo(a)pyrene			U	ND	ug/kg						
Benzo(b)fluoranthene			U	ND	ug/kg						
Benzo(ghi)perylene			U	ND	ug/kg						
Benzo(k)fluoranthene			U	ND	ug/kg						
Butylbenzylphthalate			U	ND	ug/kg						
Carbazole			U	ND	ug/kg						
Chrysene			U	ND	ug/kg						
Di-n-butylphthalate			U	ND	ug/kg						
Di-n-octylphthalate			U	ND	ug/kg						
Dibenzo(a,h)anthracene			U	ND	ug/kg						
Dibenzofuran			U	ND	ug/kg						
Diethylphthalate			U	ND	ug/kg						
Dimethylphthalate			U	ND	ug/kg						
Diphenylamine			U	ND	ug/kg						
Fluoranthene			U	ND	ug/kg						
Fluorene			U	ND	ug/kg						
Hexachlorobenzene			U	ND	ug/kg						
Hexachlorobutadiene			U	ND	ug/kg						
Hexachlorocyclopentadiene			U	ND	ug/kg						
Hexachloroethane			U	ND	ug/kg						
Indeno(1,2,3-cd)pyrene			U	ND	ug/kg						
Isophorone			U	ND	ug/kg						
N-Nitrosodipropylamine			U	ND	ug/kg						
Naphthalene			U	ND	ug/kg						
Nitrobenzene			U	ND	ug/kg						
Pentachlorophenol			U	ND	ug/kg						
Phenanthrene			U	ND	ug/kg						
Phenol			U	ND	ug/kg						
Pyrene			U	ND	ug/kg						
bis(2-Chloroethoxy)methane			U	ND	ug/kg						
bis(2-Chloroethyl) ether			U	ND	ug/kg						
bis(2-Chloroisopropyl)ether			U	ND	ug/kg						
bis(2-Ethylhexyl)phthalate			J	105	ug/kg						
m,p-Cresols			U	ND	ug/kg						
m-Nitroaniline			U	ND	ug/kg						
o-Cresol			U	ND	ug/kg						
o-Nitroaniline			U	ND	ug/kg						

## QC Summary

Workorder: 67158

Page 3 of 4

Parmaame	NOM	Sample	Qual	QC	Units	RPD%	REC%	Range	Anist	Date	Time
Semi-Volatiles-GC/MS Federal											
Batch 201961											
p-Nitroaniline				U	ND						
*2,4,6-Tribromophenol	3330				2100		63	(23%-111%)			
*2-Fluorobiphenyl	1670				1110		67	(21%-104%)			
*2-Fluorophenol	3330				2350		70	(22%-93%)			
*Nitrobenzene-d5	1670				1180		71	(24%-97%)			
*Phenol-d5	3330				2300		69	(22%-99%)			
*p-Terphenyl-d14	1670				1350		81	(30%-133%)			
QC1200301452 67158020 MSD											
Pyridine	1670				0.00	ug/kg					09/18/02 17:30
1,2,4-Trichlorobenzene	1670	U	ND		1010	ug/kg	61	(15%-112%)			
1,4-Dichlorobenzene	1670	U	ND		923	ug/kg	55	(19%-89%)			
2,4,5-Trichlorophenol	3330	U	ND		2300	ug/kg	69				
2,4,6-Trichlorophenol	3330	U	ND		2020	ug/kg	61				
2,4-Dinitrotoluene	1670	U	ND		1230	ug/kg	74	(32%-117%)			
2-Chlorophenol	3330	U	ND		1940	ug/kg	58	(13%-101%)			
4-Chloro-3-methylphenol	3330	U	ND		2460	ug/kg	74	(23%-114%)			
4-Nitrophenol	3330	U	ND		2300	ug/kg	69	(20%-126%)			
Acenaphthene	1670	U	ND		1010	ug/kg	61	(15%-114%)			
Hexachlorobenzene	1670	U	ND		1220	ug/kg	73				
Hexachlorobutadiene	1670	U	ND		928	ug/kg	56				
Hexachloroethane	1670	U	ND		940	ug/kg	56				
N-Nitrosodipropylamine	1670	U	ND		986	ug/kg	59	(18%-106%)			
Nitrobenzene	1670	U	ND		1010	ug/kg	61				
Pentachlorophenol	3330	U	ND		1640	ug/kg	49	(34%-110%)			
Phenol	3330	U	ND		2010	ug/kg	60	(17%-104%)			
Pyrene	1670	U	ND		1180	ug/kg	71	(26%-130%)			
m,p-Cresols	3330	U	ND		2060	ug/kg	62				
o-Cresol	3330	U	ND		1990	ug/kg	60				
*2,4,6-Tribromophenol	3330		2030		2310	ug/kg	69	(23%-111%)			
*2-Fluorobiphenyl	1670		983		947	ug/kg	57	(21%-104%)			
*2-Fluorophenol	3330		2140		1980	ug/kg	59	(22%-93%)			
*Nitrobenzene-d5	1670		1090		992	ug/kg	60	(24%-97%)			
*Phenol-d5	3330		2050		2020	ug/kg	61	(22%-99%)			
*p-Terphenyl-d14	1670		1360		1390	ug/kg	84	(30%-133%)			
QC1200301453 67158020 MSD											
Pyridine	1670				0.00	ug/kg					09/18/02 17:51
1,2,4-Trichlorobenzene	1670	U	ND		1080	ug/kg	6	(0%-31%)			
1,4-Dichlorobenzene	1670	U	ND		1030	ug/kg	11	(0%-36%)			
2,4,5-Trichlorophenol	3330	U	ND		2680	ug/kg	15				
2,4,6-Trichlorophenol	3330	U	ND		2220	ug/kg	10				
2,4-Dinitrotoluene	1670	U	ND		1380	ug/kg	12	(0%-37%)			
2-Chlorophenol	3330	U	ND		2180	ug/kg	12	(0%-34%)			
4-Chloro-3-methylphenol	3330	U	ND		2710	ug/kg	10	(0%-34%)			
4-Nitrophenol	3330	U	ND		2550	ug/kg	10	(0%-35%)			
Acenaphthene	1670	U	ND		1140	ug/kg	12	(0%-33%)			
Hexachlorobenzene	1670	U	ND		1420	ug/kg	15				
Hexachlorobutadiene	1670	U	ND		996	ug/kg	7				
Hexachloroethane	1670	U	ND		1010	ug/kg	7				

## QC Summary

Workorder: 67158

Page 4 of 4

Parname	NOM	Sample	Qual	QC	Units	RPD%	REC%	Range	Anlst	Date	Time
Semi-Volatiles-GC/MS Federal											
Batch 201961											
N-Nitrosodipropylamine	1670	U	ND	1090	ug/kg	10	66	(0%-29%)			
Nitrobenzene	1670	U	ND	1080	ug/kg	6	65				
Pentachlorophenol	3330	U	ND	1800	ug/kg	9	54	(0%-40%)			
Phenol	3330	U	ND	2260	ug/kg	12	68	(0%-37%)			
Pyrene	1670	U	ND	1230	ug/kg	5	74	(0%-39%)			
m,p-Cresols	3330	U	ND	2400	ug/kg	15	72				
o-Cresol	3330	U	ND	2270	ug/kg	13	68				
*2,4,6-Tribromophenol	3330		2030	2610	ug/kg		78	(23%-111%)			
*2-Fluorobiphenyl	1670		983	1000	ug/kg		60	(21%-104%)			
*2-Fluorophenol	3330		2140	2120	ug/kg		64	(22%-93%)			
*Nitrobenzene-d5	1670		1090	983	ug/kg		59	(24%-97%)			
*Phenol-d5	3330		2050	2220	ug/kg		67	(22%-99%)			
*p-Terphenyl-d14	1670		1360	1370	ug/kg		83	(30%-133%)			

**Notes.**

RER is calculated at the 95% confidence level (2-sigma).

The Qualifiers in this report are defined as follows:

- \* Recovery or %RPD not within acceptance limits and/or spike amount not compatible with the sample or the duplicate RPD's are not applicable where th
- \*\* Indicates analyte is a surrogate compound.
- B The analyte was found in the blank above the effective MDL.
- H Holding time was exceeded
- J Estimated value, the analyte concentration fell above the effective MDL and below the effective PQL
- P The response between the confirmation column and the primary column is >40% $\Delta$
- U The analyte was analyzed for but not detected below this concentration. For Organic and Inorganic analytes the result is less than the effective MDL. F
- X Presumptive evidence that the analyte is not present. Please see narrative for further information.
- X Presumptive evidence that the analyte is not present. Please see narrative for further information.
- X Uncertain identification for gamma spectroscopy.

N/A indicates that spike recovery limits do not apply when sample concentration exceeds spike conc. by a factor of 4 or more.

^ The Relative Percent Difference (RPD) obtained from the sample duplicate (DUP) is evaluated against the acceptance criteria when the sample is greater than five times (5X) the contract required detection limit (RL). In cases where either the sample or duplicate value is less than 5X the RL, a control limit of +/- the RL is used to evaluate the DUP result.

For PS, PSD, and SDILT results, the values listed are the measured amounts, not final concentrations.

Where the analytical method has been performed under NELAP certification, the analysis has met all of the requirements of the NELAC standard unless qualified on the QC Summary.

PCB Case Narrative  
Sandia National Labs (SNLS)  
SDG# 67158

Method/Analysis Information

Procedure: Polychlorinated Biphenyls by Method 8082  
Analytical Method: SW846 8082  
Prep Method: SW846 3550B  
Analytical Batch Number: 201940  
Prep Batch Number: 201939

Sample Analysis

The following samples were analyzed using the analytical protocol as established in SW846 8082:

Sample ID	Client ID
67158020	059820-002
67158021	059821-002
67158022	059822-002
67158023	059823-002
67158024	059824-002
67158025	059825-002
67158026	059828-002
67158027	059829-002
67158028	059836-002
67158029	059837-002
67158030	059838-002
67158031	059839-002
67158032	059841-002
67158033	059842-002
67158034	059843-002

SNLS SDG#67158 - PCB

67158035	059844-002
67158036	059846-001
67158037	059847-002
67158038	059848-002
1200301403	PBLK01(Method Blank)
1200301404	PBLK01LCS(Laboratory Control Sample)
1200301405	059820-002MS(Matrix Spike)
1200301406	059820-002MSD(Matrix Spike Duplicate)

### System Configuration

#### Chromatographic Columns

Column ID	Column Description
J&W1	DB-5(5%-Phenyl)-methylsiloxane 30m x 0.53mm x 1.5um DB-608 Durabond stationary phase* 30m x 0.53mm x 0.5um
J&W2	DB-5(5%-Phenyl)-methylsiloxane 30m x 0.32mm x 1.0um DB-1701 Durabond stationary phase* 30m x 0.32mm x 0.5um
J&W3	DB-5(5%-Phenyl)-methylsiloxane 30m x 0.53mm x 1.5um DB-1701(14% Cyanopropylphenyl)-methylsiloxane 30m x 0.53mm x 0.5um
J&W4	DB-608 Durabond stationary phase* 30m x 0.53mm x .83um DB-XLB* 30m x 0.53mm x 1.5um
J&W5	DB-XLB* 30m x 0.25mm x 0.25um DB-17MS(50%-Phenyl)-methylsiloxane 30m x 0.25mm x 0.25um
J&W6	DB-5(5%-Phenyl)-methylsiloxane 30m x 0.25mm x 0.25um DB-17MS(50%-Phenyl)-methylsiloxane 30m x 0.25mm x 0.25um
RESTEK	Rtx-CLPesticides 30m x 0.25mm x 0.25um Rtx-CLPesticides II 30m x 0.25mm x 0.20um

\* Durabond and DB-XLB are trademarks of J & W.



## **Instrument Configuration**

The samples reported in this SDG were analyzed on one or more of the following instrument systems. Instrument systems are referenced in the raw data and individual form headers by the Instrument ID designations listed below.

<b>Instrument ID</b>	<b>System Configuration</b>	<b>Chromatographic Column</b>
ECD1	HP 6890 Series GC ECD/ECD	RESTEK
ECD2	HP 6890 Series GC ECD/ECD	RESTEK
ECD3	HP 6890 Series GC ECD/ECD	RESTEK
ECD4	HP 5890 Series II Plus GC ECD/ECD	J&W5
ECD5	HP 6890 Series GC ECD/ECD	J&W5
ECD7	HP 6890 Series GC ECD/ECD	J&W5
ECD8	HP 6890 Series GC ECD/ECD	RESTEK

## **Preparation/Analytical Method Verification**

Procedures for preparation, analysis, and reporting of analytical data are documented by General Engineering Laboratories, Inc. (GEL) as Standard Operating Procedures (SOP).

## **Calibration Information**

### **Initial Calibration**

All initial calibration requirements have been met for this SDG.

### **CCV Requirements**

All calibration verification standard(s) (CVS, ICV or CCV) requirements have been met for this SDG.

## **Quality Control (QC) Information**

### **Surrogate Recoveries**

All the surrogate recoveries were within the established acceptance criteria for this SDG.

### **Blank Acceptance**

The blank(s) analyzed with this SDG met the established acceptance criteria.

### **LCS Recovery Statement**

The laboratory Control Sample (LCS) spike recoveries for this SDG were within the established acceptance limits.

### **QC Sample Designation**

The following sample was selected for the PCB method QC:

<u>Client Sample ID#</u>	<u>Laboratory Sample ID#</u>
059820-002	67158020

The method QC included a Matrix Spike (MS) and Matrix Spike Duplicate (MSD).

### **MS Recovery Statement**

The matrix spike recoveries for this SDG were within the established acceptance limits.

### **MSD Recovery Statement**

The matrix spike duplicate recoveries for this SDG were within the established acceptance limits.

### **MS/MSD RPD Statement**

The relative percent differences (RPD) between each MS and MSD were within the required acceptance limits.

### **Technical Information**

#### **Holding Time Specifications**

GEL assigns holding times based on the associated methodology which assigns the date and time from sample collection or sample receipt. Those holding times expressed in hours are calculated in the AlphaLIMS system. Those holding times expressed as days expire at midnight on the day of expiration. All samples in this SDG met the specified holding time requirements.

#### **Preparation/Analytical Method Verification**

All procedures were performed as stated in the SOP. All samples underwent sulfur and alumina cleanup procedure.

#### **Sample Dilutions**

None of the samples in this SDG were required dilutions.

#### **Sample Re-prep/Re-analysis**

None of the samples in this sample group were repped or reanalyzed.

### **Miscellaneous Information**

#### **Nonconformance (NCR) Documentation**

No nonconformance reports (NCRs) have been generated for this SDG.

### Manual Integrations

Due to software limitations, some manual integrations were performed on standards or samples in order for the integration of some analytes to match their integration in the calibration used. Certain standards and QC samples may have required manual integrations to correctly position the baseline as set in the calibration standard injections. If manual integrations were performed, copies of all manual integration peak profiles are included in the raw data section of this PCB fraction.

### Additional Comments

The additional comments field is used to address special issues associated with each analysis, clarify method/contractual issues pertaining to the analysis and to list any report documents generated as a result of sample analysis or review. The following additional comments were required for this sample set:

Aroclors quantitated on the raw data report by the Target data system do not necessarily represent positive aroclor identification. In order for positive identification to be made, the aroclor must match in pattern and retention time; as well as quantitate relatively close between the primary and confirmation columns, as specified in SW846 method 8000. When these conditions are not met, the aroclor is reported as a non-detect on the data report. These situations will be noted on the raw data as DMP, representing "does not match pattern", or DNC "does not confirm".

### Certification Statement

\* Where the analytical method has been performed under NELAP certification, the analysis has met all of the requirements of the NELAC standard unless otherwise noted in the analytical case narrative.

### Review Validation:

GEL requires all analytical data to be verified by a qualified data validator. In addition, all data designated for CLP or CLP-like packaging will receive a third level validation upon completion of the data package.

The following data validator verified the information presented in this case narrative:

Reviewer: Junie Cao Date: 10/11/02

## QC Summary

Workorder: 67158

Page 2 of 2

<u>Paramname</u>	<u>NOM</u>	<u>Sample</u>	<u>Qual</u>	<u>QC</u>	<u>Units</u>	<u>RPD%</u>	<u>REC%</u>	<u>Range</u>	<u>Anist</u>	<u>Date</u>	<u>Time</u>
------------------	------------	---------------	-------------	-----------	--------------	-------------	-------------	--------------	--------------	-------------	-------------

N/A indicates that spike recovery limits do not apply when sample concentration exceeds spike conc. by a factor of 4 or more.

^ The Relative Percent Difference (RPD) obtained from the sample duplicate (DUP) is evaluated against the acceptance criteria when the sample is greater than five times (5X) the contract required detection limit (RL). In cases where either the sample or duplicate value is less than 5X the RL, a control limit of +/- the RL is used to evaluate the DUP result.

For PS, PSD, and SDILT results, the values listed are the measured amounts, not final concentrations.

Where the analytical method has been performed under NELAP certification, the analysis has met all of the requirements of the NELAC standard unless qualified on the QC Summary.

## QC Summary

Report Date: October 10, 2002  
Page 1 of 2

Client : Sandia National Laboratories  
MS-0756  
P.O. Box 5800  
Albuquerque, New Mexico  
Contact: Pamela M. Puissant  
Workorder: 67158

Partname	NOM	Sample	Qual	QC	Units	RPD%	REC%	Range	Anlst	Date	Time
Semi-Volatiles-PCB Federal											
Batch 201940											
QC1200301404	LCS										
Aroclor-1260	33.3			29.0	ug/kg		87	(48%-116%)	GH1	09/25/02	17:05
**4cmx	6.67			171	ug/kg		86	(31%-120%)			
**Decachlorobiphenyl	6.67			187	ug/kg		93	(54%-115%)			
QC1200301403	MB										
Aroclor-1016			U	ND	ug/kg					09/25/02	16:53
Aroclor-1221			U	ND	ug/kg						
Aroclor-1232			U	ND	ug/kg						
Aroclor-1242			U	ND	ug/kg						
Aroclor-1248			U	ND	ug/kg						
Aroclor-1254			U	ND	ug/kg						
Aroclor-1260			U	ND	ug/kg						
**4cmx	6.67			170	ug/kg		85	(31%-120%)			
**Decachlorobiphenyl	6.67			183	ug/kg		91	(34%-115%)			
QC1200301405	67158020	MS									
Aroclor-1260	33.3	10.9		37.2	ug/kg		79	(36%-134%)		09/25/02	17:29
**4cmx	6.67	5.06		151	ug/kg		75	(31%-120%)			
**Decachlorobiphenyl	6.67	5.24		147	ug/kg		74	(34%-115%)			
QC1200301406	67158020	MSD									
Aroclor-1260	33.3	10.9		37.8	ug/kg	2	81	(0%-30%)		09/25/02	17:42
**4cmx	6.67	5.06		140	ug/kg		70	(31%-120%)			
**Decachlorobiphenyl	6.67	5.24		151	ug/kg		75	(34%-115%)			

**Notes:**

RER is calculated at the 95% confidence level (2-sigma).

The Qualifiers in this report are defined as follows:

- \* Recovery or %RPD not within acceptance limits and/or spike amount not compatible with the sample or the duplicate RPD's are not applicable where t
- \*\* Indicates analyte is a surrogate compound.
- B The analyte was found in the blank above the effective MDL.
- H Holding time was exceeded
- J Estimated value, the analytic concentration fell above the effective MDL and below the effective PQL
- P The response between the confirmation column and the primary column is >40%D
- U The analyte was analyzed for but not detected below this concentration. For Organic and Inorganic analytes the result is less than the effective MDL. J
- X Presumptive evidence that the analyte is not present. Please see narrative for further information.
- X Presumptive evidence that the analyte is not present. Please see narrative for further information.
- X Uncertain identification for gamma spectroscopy.

PCB Case Narrative  
Sandia National Labs (SNLS)  
SDG# 67158-1

Method/Analysis Information

Procedure: Polychlorinated Biphenyls by Method 8082  
Analytical Method: SW846 8082  
Prep Method: SW846 3510C  
Analytical Batch Number: 202231  
Prep Batch Number: 202230

Sample Analysis

The following samples were analyzed using the analytical protocol as established in SW846 8082:

Sample ID	Client ID
67169006	059826-003
1200302125	PBLK01(Method Blank)
1200302128	PBLK01LCS(Laboratory Control Sample)

System Configuration

Chromatographic Columns

Column ID	Column Description
J&W1	DB-5(5%-Phenyl)-methylsiloxane 30m x 0.53mm x 1.5um DB-608 Durabond stationary phase* 30m x 0.53mm x 0.5um
J&W2	DB-5(5%-Phenyl)-methylsiloxane 30m x 0.32mm x 1.0um DB-1701 Durabond stationary phase* 30m x 0.32mm x 0.5um
J&W3	DB-5(5%-Phenyl)-methylsiloxane 30m x 0.53mm x 1.5um DB-1701(14% Cyanopropylphenyl)-methylsiloxane 30m x 0.53mm x 0.5um
J&W4	DB-608 Durabond stationary phase* 30m x 0.53mm x .83um DB-XLB* 30m x 0.53mm x 1.5um
J&W5	DB-XLB* 30m x 0.25mm x 0.25um DB-17MS(50%-Phenyl)-methylsiloxane 30m x 0.25mm x 0.25um

SNLS SDG# 67158-1 - PCB

Page 1 of 4

J&W6 DB-5(5%-Phenyl)-methylsiloxane 30m x 0.25mm x 0.25um  
 DB-17MS(50%-Phenyl)-methylsiloxane 30m x 0.25mm x 0.25um

RESTEK Rtx-CLPesticides 30m x 0.25mm x 0.25um  
 Rtx-CLPesticides II 30m x 0.25mm x 0.20um

\* Durabond and DB-XLB are trademarks of J & W.

**Instrument Configuration**

The samples reported in this SDG were analyzed on one or more of the following instrument systems. Instrument systems are referenced in the raw data and individual form headers by the Instrument ID designations listed below.

Instrument ID	System Configuration	Chromatographic Column
ECD1	HP 6890 Series GC ECD/ECD	RESTEK
ECD2	HP 6890 Series GC ECD/ECD	RESTEK
ECD3	HP 6890 Series GC ECD/ECD	RESTEK
ECD4	HP 5890 Series II Plus GC ECD/ECD	J&W5
ECD5	HP 6890 Series GC ECD/ECD	J&W5
ECD7	HP 6890 Series GC ECD/ECD	J&W5
ECD8	HP 6890 Series GC ECD/ECD	RESTEK

**Preparation/Analytical Method Verification**

Procedures for preparation, analysis, and reporting of analytical data are documented by General Engineering Laboratories, Inc. (GEL) as Standard Operating Procedures (SOP).

**Calibration Information**

**Initial Calibration**

All initial calibration requirements have been met for this SDG.

**CCV Requirements**

All calibration verification standard(s) (CVS, ICV or CCV) requirements have been met for this SDG.

**Quality Control (QC) Information**

**Surrogate Recoveries**

All the surrogate recoveries were within the established acceptance criteria for this SDG.

**Blank Acceptance**

The blank(s) analyzed with this SDG met the established acceptance criteria.

**LCS Recovery Statement**

The laboratory Control Sample (LCS) spike recoveries for this SDG were within the established acceptance limits.

**QC Sample Designation**

The MS and MSD were analyzed on a sample contained in a non-client's SDG.

**MS Recovery Statement**

The matrix spike recoveries for this SDG were within the established acceptance limits.

**MSD Recovery Statement**

The matrix spike duplicate recoveries for this SDG were within the established acceptance limits.

**MS/MSD RPD Statement**

The relative percent differences (RPD) between each MS and MSD were within the required acceptance limits.

**Technical Information****Holding Time Specifications**

GEL assigns holding times based on the associated methodology which assigns the date and time from sample collection or sample receipt. Those holding times expressed in hours are calculated in the AlphaLIMS system. Those holding times expressed as days expire at midnight on the day of expiration. All samples in this SDG met the specified holding time requirements.

**Preparation/Analytical Method Verification**

All procedures were performed as stated in the SOP. All samples underwent sulfur and alumina cleanup procedure.

**Sample Dilutions**

None of the samples in this SDG were required dilutions.

**Sample Re-prep/Re-analysis**

None of the samples in this sample group were repped or reanalyzed.



**Miscellaneous Information**

**Nonconformance (NCR) Documentation**

No nonconformance reports (NCRs) have been generated for this SDG.

**Manual Integrations**

Due to software limitations, some manual integrations were performed on standards or samples in order for the integration of some analytes to match their integration in the calibration used. Certain standards and QC samples may have required manual integrations to correctly position the baseline as set in the calibration standard injections. If manual integrations were performed, copies of all manual integration peak profiles are included in the raw data section of this PCB fraction.

**Additional Comments**

The additional comments field is used to address special issues associated with each analysis, clarify method/contractual issues pertaining to the analysis and to list any report documents generated as a result of sample analysis or review. The following additional comments were required for this sample set:

Aroclors quantitated on the raw data report by the Target data system do not necessarily represent positive aroclor identification. In order for positive identification to be made, the aroclor must match in pattern and retention time; as well as quantitate relatively close between the primary and confirmation columns, as specified in SW846 method 8000. When these conditions are not met, the aroclor is reported as a non-detect on the data report. These situations will be noted on the raw data as DMP, representing "does not match pattern", or DNC "does not confirm".

**Certification Statement**

\* Where the analytical method has been performed under NELAP certification, the analysis has met all of the requirements of the NELAC standard unless otherwise noted in the analytical case narrative.

**Review Validation:**

GEL requires all analytical data to be verified by a qualified data validator. In addition, all data designated for CLP or CLP-like packaging will receive a third level validation upon completion of the data package.

The following data validator verified the information presented in this case narrative:

Reviewer:         Jimmy Cao         Date:         10/11/02

## QC Summary

Report Date: October 11, 2002  
Page 1 of 1

Client: Sandia National Laboratories  
MS-0756  
P.O. Box 5800  
Albuquerque, New Mexico  
Contact: Pamela M. Puissant  
Workorder: 67169

Parname	NOM	Sample Qual	QC	Units	RPD%	REC%	Range	Anlst	Date Time
Semi-Volatiles-PCB Federal									
Batch	202231								
QC1200302128	LCS								
Aroclor-1260	1.00		0.840	ug/L	84	(47%-131%)		GH1	09/23/02 11:39
**4cmx	0.200		154	ug/L	77	(34%-116%)			
**Decachlorobiphenyl	0.200		123	ug/L	62	(21%-122%)			
QC1200302125	MB								
Aroclor-1016		U	ND	ug/L					09/23/02 11:27
Aroclor-1221		U	ND	ug/L					
Aroclor-1232		U	ND	ug/L					
Aroclor-1242		U	ND	ug/L					
Aroclor-1248		U	ND	ug/L					
Aroclor-1254		U	ND	ug/L					
Aroclor-1260		U	ND	ug/L					
**4cmx	0.200		162	ug/L	81	(34%-116%)			
**Decachlorobiphenyl	0.200		136	ug/L	68	(21%-122%)			

**Notes:**

RER is calculated at the 95% confidence level (2-sigma).

The Qualifiers in this report are defined as follows:

- \* Recovery or %RPD not within acceptance limits and/or spike amount not compatible with the sample or the duplicate RPD's are not applicable where B
- \*\* Indicates analyte is a surrogate compound.
- B The analyte was found in the blank above the effective MDL.
- H Holding time was exceeded
- J Estimated value, the analyte concentration fell above the effective MDL and below the effective PQL
- P The response between the confirmation column and the primary column is >40%D
- U The analyte was analyzed for but not detected below this concentration. For Organic and Inorganic analytes the result is less than the effective MDL. )
- X Presumptive evidence that the analyte is not present. Please see narrative for further information.
- X Presumptive evidence that the analyte is not present. Please see narrative for further information.
- X Uncertain identification for gamma spectroscopy.

N/A indicates that spike recovery limits do not apply when sample concentration exceeds spike conc. by a factor of 4 or more.

^ The Relative Percent Difference (RPD) obtained from the sample duplicate (DUP) is evaluated against the acceptance criteria when the sample is greater than five times (5X) the contract required detection limit (RL). In cases where either the sample or duplicate value is less than 5X the RL, a control limit of +/- the RL is used to evaluate the DUP result.

For PS, PSD, and SDILT results, the values listed are the measured amounts, not final concentrations.

Where the analytical method has been performed under NELAP certification, the analysis has met all of the requirements of the NELAC standard unless qualified on the QC Summary.

67158030	059838-002
67158031	059839-002
67158032	059841-002
67158033	059842-002
67158034	059843-002
67158035	059844-002
67158036	059846-001
67158037	059847-002
67158038	059848-002
1200301707	XBLK01 (Blank)
1200301708	XBLK01LCS (Laboratory Control Sample)
1200301709	059846-001MS (Matrix Spike)
1200301710	059846-001MSD (Matrix Spike Duplicate)

### System Configuration

The laboratory utilizes a high performance liquid chromatography (HPLC) instrument configuration for explosives analyses. The chromatographic hardware system consists of an HP Model 1050 HPLC or HP Model 1100 HPLC with programmable gradient pumping and a 100 ul loop injector for the primary system and a 100 ul loop injector for the confirmation system. The HPLC 1050 is coupled to a HP Model G1306A Diode Array UV detector, and the HPLC 1100 is coupled to a HP Model G1315A Diode Array UV detector which monitor absorbance at the following five wavelengths: 1) 214 nm; 2) 224 nm; 3) 235 nm; 4) 254 nm; 5) 264 nm.

The primary HPLC system is usually identified with either a designation of HPLC #2, or hplcb in the raw data printouts. The confirmation HPLC system is usually identified with a designation of HPLC #1, or hplca in the raw data printouts. The HP 1100 HPLC system is identified as HPLC #3, or hplcc in the raw data printouts. The HP 1100 HPLC has a Column Switching Valve which enables this system to be used for primary analysis or confirmation analysis.

### **Chromatographic Columns**

Chromatographic separation of nitroaromatic and nitramine components is accomplished through analysis on the following reversed phase columns:

HP: Hypersil BDS-C18, 250 mm x 4 mm O.D. containing 5 um particle size.

Confirmation of nitroaromatic and nitramine components, initially identified on one of the above columns, is accomplished through analysis on the following column:

PH: Develosil CN-UG5-5, 250 mm x 4.6 mm ID.

The primary column is used for quantitation while the confirmation column is for qualitative purposes only.

### **Preparation/Analytical Method Verification**

Procedures for preparation, analysis, and reporting of analytical data are documented by General Engineering Laboratories, Inc. (GEL) as Standard Operating Procedures (SOP).

### **Calibration Information**

#### **Initial Calibration**

All initial calibration requirements have been met for this SDG.

#### **CCV Requirements**

All calibration verification standard(s) (CVS, ICV or CCV) requirements have been met for this SDG.

### **Quality Control (QC) Information**

#### **Surrogate Recoveries**

All the surrogate recoveries were within the established acceptance criteria for this SDG.

#### **Blank Acceptance**

The blank(s) analyzed with this SDG met the established acceptance criteria.

#### **LCS Recovery Statement**

All the LCS spike recoveries were within the established acceptance limits.

#### **QC Sample Designation**

The following sample analyzed with this SDG was chosen for matrix spike analysis:  
67158036 (059846-001).

#### **MS Recovery Statement**

One or more of the required spiking analytes were not within the acceptance limits in the matrix spike (MS). The matrix spike duplicate (MSD) also failed recoveries. The failing recoveries are attributed to matrix interference.

### **MSD Recovery Statement**

One or more of the required spiking analytes were not within the acceptance limits in the matrix spike duplicate (MSD). The matrix spike (MS) also failed recoveries. The failing recoveries are attributed to matrix interference.

### **MS/MSD RPD Statement**

The relative percent differences (RPD) between the MS and MSD were not within the required acceptance limits.

### **Technical Information**

#### **Holding Time Specifications**

All samples in this SDG met the specified holding time requirements. GEL assigns holding times based on the associated methodology that assigns the date and time from sample collection or sample receipt. Those holding times expressed in hours are calculated in the AlphaLIMS system. Those holding times expressed as days expire at midnight on the day of expiration.

#### **Preparation/Analytical Method Verification**

All procedures were performed as stated in the SOP.

#### **Sample Dilutions**

None of the samples in this SDG required dilutions.

### **Miscellaneous Information**

#### **Nonconformance (NCR) Documentation**

No nonconformance report (NCR) has been generated for this SDG.

#### **Manual Integration**

Some initial calibration standards, continuing calibration standards, and/or samples required manual integrations due to software limitations. All samples.

#### **Additional Comments**

Confirmation analysis was performed on some of the samples in this batch. The values reported are from the primary analysis. The confirmation analysis is used for qualitative purposes only.

The following analytes coelute on the cyano column: a.) 2,4,6-Trinitrotoluene, 2,4-Dinitrotoluene, and 2,6-Dinitrotoluene b.) 1,3,5-Trinitrotoluene and 1,3-Dinitrobenzene c.) m-Nitrotoluene, p-Nitrotoluene and o-Nitrotoluene. As a result some of these analytes may be flagged with a P qualifier. The coelution from the cyano column should be considered and the values as suspect to the sample.

The Form 8 uses the retention time of the surrogate as a measure of how close the retention time of the samples and QC are to a standard component. The Instrument Blank does not contain the surrogate.

The samples were concentrated prior to analysis to achieve the required detection limit.

**Certification Statement**

\* Where the analytical method has been performed under NELAP certification, the analysis has met all of the requirements of the NELAC standard unless otherwise noted in the analytical case narrative.

**Review Validation:**

GEL requires all analytical data to be verified by a qualified data validator. In addition, all data designated for CLP or CLP-like packaging will receive a third level validation upon completion of the data package.

Reviewer: Deborah Mace Date: 10/14/02

## QC Summary

Report Date: October 14, 2002  
Page 1 of 2

Client : Sandia National Laboratories  
MS-0756  
P.O. Box 5800  
Albuquerque, New Mexico  
Contact: Pamela M. Puissant  
Workorder: 67158

Parmaane	NOM	Sample	Qual	QC	Units	RPD%	REC%	Range	Anlst	Date	Time
HPLC Explosives Federal											
Batch 202056											
QC1200301708 LCS											
1,3,5-Trinitrobenzene	800			766	ug/kg		96	(77%-124%)	JLW	09/29/02	14:21
2,4,6-Trinitrotoluene	800			766	ug/kg		96	(80%-120%)			
2,4-Dinitrotoluene	800			739	ug/kg		92	(77%-122%)			
2,6-Dinitrotoluene	800			765	ug/kg		96	(74%-121%)			
2-Amino-4,6-dinitrotoluene	800			775	ug/kg		97	(81%-125%)			
4-Amino-2,6-dinitrotoluene	800			656	ug/kg		82	(79%-123%)			
HMX	800			777	ug/kg		97	(84%-131%)			
Nitrobenzene	800			709	ug/kg		89	(75%-125%)			
RDX	800			798	ug/kg		100	(80%-123%)			
Tetryl	800			644	ug/kg		81	(65%-124%)			
m-Dinitrobenzene	800			754	ug/kg		94	(77%-124%)			
m-Nitrotoluene	800			719	ug/kg		90	(77%-117%)			
o-Nitrotoluene	800			704	ug/kg		88	(75%-119%)			
p-Nitrotoluene	800			711	ug/kg		89	(76%-121%)			
**1,2-dinitrobenzene	400			370	ug/kg		92	(71%-118%)			
QC1200301707 MB											
1,3,5-Trinitrobenzene			U	ND	ug/kg					09/29/02	15:05
2,4,6-Trinitrotoluene			U	ND	ug/kg						
2,4-Dinitrotoluene			U	ND	ug/kg						
2,6-Dinitrotoluene			U	ND	ug/kg						
2-Amino-4,6-dinitrotoluene			U	ND	ug/kg						
4-Amino-2,6-dinitrotoluene			U	ND	ug/kg						
HMX			U	ND	ug/kg						
Nitrobenzene			U	ND	ug/kg						
RDX			U	ND	ug/kg						
Tetryl			U	ND	ug/kg						
m-Dinitrobenzene			U	ND	ug/kg						
m-Nitrotoluene			U	ND	ug/kg						
o-Nitrotoluene			U	ND	ug/kg						
p-Nitrotoluene			U	ND	ug/kg						
**1,2-dinitrobenzene	400			352	ug/kg		88	(71%-118%)			
QC1200301709 67158036 MS											
1,3,5-Trinitrobenzene	800	U	ND	776	ug/kg		97	(66%-133%)		09/29/02	13:39
2,4,6-Trinitrotoluene	800	U	ND	864	ug/kg		108	(77%-132%)			
2,4-Dinitrotoluene	800	U	ND	776	ug/kg		97	(61%-134%)			
2,6-Dinitrotoluene	800	U	ND	835	ug/kg		104	(70%-121%)			
2-Amino-4,6-dinitrotoluene	800	U	ND	720	ug/kg		90	(79%-124%)			
4-Amino-2,6-dinitrotoluene	800	U	ND	467	ug/kg		58*	(71%-120%)			
HMX	800	U	ND	783	ug/kg		98	(75%-138%)			
Nitrobenzene	800	U	ND	749	ug/kg		94	(72%-120%)			
RDX	800	U	ND	778	ug/kg		97	(61%-136%)			
Tetryl	800	U	ND	256	ug/kg		32*	(65%-135%)			

## QC Summary

Workorder: 67158

Page 2 of 2

Parname	NOM	Sample	Qual	QC	Units	RPD%	REC%	Range	Anlst	Date	Time
HPLC Explosives Federal											
Batch 202056											
m-Dinitrobenzene	800	U	ND	788	ug/kg		99	(75%-125%)			
m-Nitrotoluene	800	U	ND	776	ug/kg		97	(73%-116%)			
o-Nitrotoluene	800	U	ND	746	ug/kg		93	(68%-122%)			
p-Nitrotoluene	800	U	ND	757	ug/kg		95	(67%-125%)			
**1,2-dinitrobenzene	400		372	383	ug/kg		96	(71%-118%)			
QC1200301710 67158036 MSD											
1,3,5-Trinitrobenzene	800	U	ND	822	ug/kg	6	105	(0%-20%)		09/28/02	17:49
2,4,6-Trinitrotoluene	800	U	ND	922	ug/kg	7	115	(0%-20%)			
2,4-Dinitrotoluene	800	U	ND	782	ug/kg	1	98	(0%-24%)			
2,6-Dinitrotoluene	800	U	ND	847	ug/kg	1	106	(0%-21%)			
2-Amino-4,6-dinitrotoluene	800	U	ND	824	ug/kg	13	103	(0%-20%)			
4-Amino-2,6-dinitrotoluene	800	U	ND	733	ug/kg	44*	92	(0%-20%)			
HMX	800	U	ND	843	ug/kg	7	105	(0%-38%)			
Nitrobenzene	800	U	ND	771	ug/kg	3	96	(0%-21%)			
RDX	800	U	ND	797	ug/kg	2	100	(0%-35%)			
Tetryl	800	U	ND	141	ug/kg	58*	18	(0%-30%)			
m-Dinitrobenzene	800	U	ND	828	ug/kg	5	104	(0%-23%)			
m-Nitrotoluene	800	U	ND	775	ug/kg	0	97	(0%-20%)			
o-Nitrotoluene	800	U	ND	776	ug/kg	4	97	(0%-23%)			
p-Nitrotoluene	800	U	ND	798	ug/kg	5	100	(0%-22%)			
**1,2-dinitrobenzene	400		372	397	ug/kg		99	(71%-118%)			

**Notes:**

REC is calculated at the 95% confidence level (2-sigma).

The Qualifiers in this report are defined as follows:

- \* Recovery or %RPD not within acceptance limits and/or spike amount not compatible with the sample or the duplicate RPD's are not applicable where it
- \*\* Indicates analyte is a surrogate compound.
- B The analyte was found in the blank above the effective MDL.
- H Holding time was exceeded
- J Estimated value, the analyte concentration fell above the effective MDL and below the effective PQL
- P The response between the confirmation column and the primary column is >40%D
- U The analyte was analyzed for but not detected below this concentration. For Organic and Inorganic analytes the result is less than the effective MDL. 1
- X Presumptive evidence that the analyte is not present. Please see narrative for further information.
- X Presumptive evidence that the analyte is not present. Please see narrative for further information.
- X Uncertain identification for gamma spectroscopy.

N/A indicates that spike recovery limits do not apply when sample concentration exceeds spike conc. by a factor of 4 or more.

^ The Relative Percent Difference (RPD) obtained from the sample duplicate (DUP) is evaluated against the acceptance criteria when the sample is greater than five times (5X) the contract required detection limit (RL). In cases where either the sample or duplicate value is less than 5X the RL, a control limit of +/- the RL is used to evaluate the DUP result.

For PS, PSD, and SDLT results, the values listed are the measured amounts, not final concentrations.

Where the analytical method has been performed under NELAP certification, the analysis has met all of the requirements of the NELAC standard unless qualified on the QC Summary.



HPLC Narrative  
Sandia National Labs (SNLS)  
SDG 67158-1

Method/Analysis Information

Procedure: Nitroaromatics and Nitramines by High Performance Liquid Chromatography (HPLC)  
Analytical Method: SW846 8330  
Prep Method: SW846 8330 PREP  
Analytical Batch Number: 202049  
Prep Batch Number: 202046

Sample Analysis

The following samples were analyzed using the analytical protocol as established in SW846 8330:

Sample ID	Client ID
67169007	059826-004
1200301687	XBLK01 (Blank)
1200301688	XBLK01 LCS (Laboratory Control Sample)
1200301689	XBLK01LCSD (Laboratory Control Sample Duplicate)

System Configuration

The laboratory utilizes a high performance liquid chromatography (HPLC) instrument configuration for explosives analyses. The chromatographic hardware system consists of an HP Model 1050 HPLC or HP Model 1100 HPLC with programmable gradient pumping and a 100 ul loop injector for the primary system and a 100 ul loop injector for the confirmation system. The HPLC 1050 is coupled to a HP Model G1306A Diode Array UV detector, and the HPLC 1100 is coupled to a HP Model G1315A Diode Array UV detector which monitor absorbance at the following five wavelengths: 1) 214 nm; 2) 224 nm; 3) 235 nm; 4) 254 nm; 5) 264 nm.

The primary HPLC system is usually identified with either a designation of HPLC #2, or hplcb in the raw data printouts. The confirmation HPLC system is usually identified with a designation of HPLC #1, or hplca in the raw data printouts. The HP 1100 HPLC system is identified as HPLC #3, or hplcc in the raw data printouts. The HP 1100 HPLC has a Column Switching Valve which enables this system to be used for primary analysis or confirmation analysis.

### **Chromatographic Columns**

Chromatographic separation of nitroaromatic and nitramine components is accomplished through analysis on the following reversed phase columns:

HP: Hypersil BDS-C18, 250 mm x 4 mm O.D. containing 5 um particle size.

Confirmation of nitroaromatic and nitramine components, initially identified on one of the above columns, is accomplished through analysis on the following column:

PH: Develosil CN-UG5-5, 250 mm x 4.6 mm I.D.

The primary column is used for quantitation while the confirmation column is for qualitative purposes only.

### **Preparation/Analytical Method Verification**

Procedures for preparation, analysis, and reporting of analytical data are documented by General Engineering Laboratories, Inc. (GEL) as Standard Operating Procedures (SOP).

### **Calibration Information**

#### **Initial Calibration**

All initial calibration requirements have been met for this SDG.

#### **CCV Requirements**

All calibration verification standard(s) (CVS, ICV or CCV) requirements have been met for this SDG.

### **Quality Control (QC) Information**

#### **Surrogate Recoveries**

All the surrogate recoveries were within the established acceptance criteria for this SDG.

#### **Blank Acceptance**

The blank(s) analyzed with this SDG met the established acceptance criteria.

### **LCS Recovery Statement**

Two of the required spiking analytes were not within the SNLS 80-120% acceptance limits in the laboratory control sample (LCS). All the LCS recoveries were within the GEL SPC limits. The GEL SPC limits are on the Certificate of Analysis. Please see the emails in the Miscellaneous Section.

### **LCSD Recovery Statement**

Two of the required spiking analytes were not within the SNLS 80-120% acceptance limits in the laboratory control sample duplicate (LCSD). All the LCSD recoveries were within the GEL SPC limits. The GEL SPC limits are on the Certificate of Analysis. Please see the emails in the Miscellaneous Section.

### **LCS/LCSD RPD Statement**

All the relative percent differences (RPD) between each LCS and LCSD were within the required acceptance limits.

### **QC Sample Designation**

A matrix spike/matrix spike duplicate was not performed with this batch due to limited sample.

### **Technical Information**

#### **Holding Time Specifications**

All samples in this SDG met the specified holding time requirements. GEL assigns holding times based on the associated methodology that assigns the date and time from sample collection or sample receipt. Those holding times expressed in hours are calculated in the AlphaLIMS system. Those holding times expressed as days expire at midnight on the day of expiration.

#### **Preparation/Analytical Method Verification**

All procedures were performed as stated in the SOP.

#### **Sample Dilutions**

None of the samples in this SDG required dilutions.

### **Miscellaneous Information**

#### **Nonconformance (NCR) Documentation**

No nonconformance report (NCR) has been generated for this SDG.

#### **Manual Integration**

No manual integrations were required for any data file in this SDG.

#### **Additional Comments**

Confirmation analysis was performed on some of the samples in this batch. The values reported are from the primary analysis. The confirmation analysis is used for qualitative purposes only.

The samples were concentrated prior to analysis to achieve the required detection limit.

The Form 8 uses the retention time of the surrogate as a measure of how close the retention time of the samples and QC are to a standard component. The Instrument Blank does not contain the surrogate.

The following analytes coelute on the cyano column: a.) 2,4,6-Trinitrotoluene, 2,4-Dinitrotoluene, and 2,6-Dinitrotoluene b.) 1,3,5-Trinitrotoluene and 1,3-Dinitrobenzene c.) m-Nitrotoluene, p-Nitrotoluene and o-Nitrotoluene. As a result some of these analytes may be flagged with a P qualifier. The coelution from the cyano column should be considered and the values as suspect to the sample.

**Certification Statement**

\* Where the analytical method has been performed under NELAP certification, the analysis has met all of the requirements of the NELAC standard unless otherwise noted in the analytical case narrative.

**Review Validation:**

GEL requires all analytical data to be verified by a qualified data validator. In addition, all data designated for CLP or CLP-like packaging will receive a third level validation upon completion of the data package.

Reviewer: Robert M. Moore Date: 10/14/02

## QC Summary

Report Date: October 14, 2002  
Page 1 of 2

Client : Sandia National Laboratories  
MS-0756  
P.O. Box 5800  
Albuquerque, New Mexico  
Contact: Pamela M. Puissant  
Workorder: 67169

Parname	NOM	Sample	Qual	QC	Units	RPD%	REC%	Range	Analst	Date	Time
<b>HPLC Explosives Federal</b>											
Batch	202049										
QC1200301688	LCS										
1,3,5-Trinitrobenzene	1.04			0.956	ug/L		92	(84%-110%)	JLW	09/19/02	10:36
2,4,6-Trinitrotoluene	1.04			0.965	ug/L		93	(85%-110%)			
2,4-Dinitrotoluene	1.04			0.863	ug/L		83	(78%-110%)			
2,6-Dinitrotoluene	1.04			0.915	ug/L		88	(79%-110%)			
2-Amino-4,6-dinitrotoluene	1.04			0.967	ug/L		93	(77%-110%)			
4-Amino-2,6-dinitrotoluene	1.04			0.909	ug/L		88	(59%-110%)			
HMX	1.04			0.975	ug/L		94	(86%-110%)			
Nitrobenzene	1.04			0.770	ug/L		74	(68%-110%)			
RDX	1.04			0.932	ug/L		90	(76%-110%)			
Tetryl	1.04			1.01	ug/L		97	(73%-110%)			
m-Dinitrobenzene	1.04			0.868	ug/L		84	(76%-110%)			
m-Nitrotoluene	1.04			0.829	ug/L		80	(73%-110%)			
o-Nitrotoluene	1.04			0.830	ug/L		80	(69%-110%)			
p-Nitrotoluene	1.04			0.854	ug/L		82	(73%-110%)			
**1,2-dinitrobenzene	0.519			0.442	ug/L		85	(59%-118%)			
QC1200301689	LCS										
1,3,5-Trinitrobenzene	1.04			0.960	ug/L	0	92	(0%-20%)		09/19/02	11:19
2,4,6-Trinitrotoluene	1.04			0.966	ug/L	0	93	(0%-20%)			
2,4-Dinitrotoluene	1.04			0.848	ug/L	2	82	(0%-20%)			
2,6-Dinitrotoluene	1.04			0.876	ug/L	4	84	(0%-20%)			
2-Amino-4,6-dinitrotoluene	1.04			0.969	ug/L	0	93	(0%-20%)			
4-Amino-2,6-dinitrotoluene	1.04			0.909	ug/L	0	88	(0%-24%)			
HMX	1.04			0.974	ug/L	0	94	(0%-20%)			
Nitrobenzene	1.04			0.762	ug/L	1	73	(0%-20%)			
RDX	1.04			0.928	ug/L	0	89	(0%-20%)			
Tetryl	1.04			1.01	ug/L	0	97	(0%-20%)			
m-Dinitrobenzene	1.04			0.849	ug/L	2	82	(0%-20%)			
m-Nitrotoluene	1.04			0.819	ug/L	1	79	(0%-20%)			
o-Nitrotoluene	1.04			0.814	ug/L	2	78	(0%-23%)			
p-Nitrotoluene	1.04			0.855	ug/L	0	82	(0%-20%)			
**1,2-dinitrobenzene	0.519			0.437	ug/L		84	(59%-118%)			
QC1200301687	MB										
1,3,5-Trinitrobenzene			U	ND	ug/L					09/19/02	09:54
2,4,6-Trinitrotoluene			U	ND	ug/L						
2,4-Dinitrotoluene			U	ND	ug/L						
2,6-Dinitrotoluene			U	ND	ug/L						
2-Amino-4,6-dinitrotoluene			U	ND	ug/L						
4-Amino-2,6-dinitrotoluene			U	ND	ug/L						
HMX			U	ND	ug/L						
Nitrobenzene			U	ND	ug/L						
RDX			U	ND	ug/L						
Tetryl			U	ND	ug/L						

## QC Summary

Workorder: 67169

Page 2 of 2

Parameter	NOM	Sample	Qual	QC	Units	RPD%	REC%	Range	Anst	Date	Time
HPLC Explosives Federal											
Batch	202049										
m-Dinitrobenzene			U	ND	ug/L						
m-Nitrotoluene			U	ND	ug/L						
o-Nitrotoluene			U	ND	ug/L						
p-Nitrotoluene			U	ND	ug/L						
**1,2-dinitrobenzene	0.519			0.474	ug/L		91	(59%-118%)			

**Notes:**

RER is calculated at the 95% confidence level (2-sigma).

The Qualifiers in this report are defined as follows:

- \* Recovery or %RPD not within acceptance limits and/or spike amount not compatible with the sample or the duplicate RPD's are not applicable where it
- \*\* Indicates analyte is a surrogate compound.
- B The analyte was found in the blank above the effective MDL.
- H Holding time was exceeded
- J Estimated value, the analyte concentration fell above the effective MDL and below the effective PQL
- P The response between the confirmation column and the primary column is >40%D
- U The analyte was analyzed for but not detected below this concentration. For Organic and Inorganic analytes the result is less than the effective MDL. J
- X Presumptive evidence that the analyte is not present. Please see narrative for further information.
- X Presumptive evidence that the analyte is not present. Please see narrative for further information.
- X Uncertain identification for gamma spectroscopy.

N/A indicates that spike recovery limits do not apply when sample concentration exceeds spike conc. by a factor of 4 or more.

^ The Relative Percent Difference (RPD) obtained from the sample duplicate (DUP) is evaluated against the acceptance criteria when the sample is greater than five times (5X) the contract required detection limit (RL). In cases where either the sample or duplicate value is less than 5X the RL, a control limit of +/- the RL is used to evaluate the DUP result.

For PS, PSD, and SDILT results, the values listed are the measured amounts, not final concentrations.

Where the analytical method has been performed under NELAP certification, the analysis has met all of the requirements of the NELAC standard unless qualified on the QC Summary.

**Inorganic Case Narrative for  
Sandia National Laboratory  
SDG# 67158**

**Sample Analysis:**

The following samples were prepared and analyzed using the methods referenced in the "Method/Analysis Information" section of this narrative:

<b>Sample ID</b>	<b>Client ID</b>
67158020	059820-002
67158021	059821-002
67158022	059822-002
67158023	059823-002
67158024	059824-002
67158025	059825-002
67158026	059828-002
67158027	059829-002
67158028	059836-002
67158029	059837-002
67158030	059838-002
67158031	059839-002
67158032	059841-002
67158033	059842-002
67158034	059843-002
67158035	059844-002
67158036	059846-001
67158037	059847-002
67158038	059848-002
1200303449	Method Blank (MB) ICP-202762/202760
1200303453	Laboratory Control Sample (LCS)
1200303451	059846-001L (67158036) Serial Dilution (SD)
1200303450	059846-001D (67158036) Sample Duplicate (DUP)
1200303452	059846-001S (67158036) Matrix Spike (MS)
1200303376	Method Blank (MB) CVAA-202730/202729
1200303379	Laboratory Control Sample (LCS)
1200303377	059846-001D (67158036) Sample Duplicate (DUP)
1200303378	059846-001S (67158036) Matrix Spike (MS)

**Method/Analysis Information:**

<b>Analytical Batch #:</b>	202762, 202730
<b>Prep Batch #:</b>	202760, 202729
<b>Standard Operating Procedure:</b>	GL-MA-E-013 REV.6; GL-MA-E-010 REV.10
<b>Analytical Method:</b>	SW846 6010B; SW846 7471A
<b>Prep Method:</b>	SW846 3050B; SW846 7471A

**System Configuration**

The ICP analysis was performed on a Thermo Jarrell Ash 61E Trace axial-viewing inductively coupled plasma atomic emission spectrometer. The instrument is equipped with a Meinhardt nebulizer, cyclonic spray chamber, and yttrium internal standard. Operating conditions for the Trace ICP are set at a power level of 950 watts. The instrument has a peristaltic pump flow rate of 140 RPM (2.0 mL/min sample uptake rate), argon gas flows of 15 L/min and 0.5 L/min for the torch and auxiliary gases, and a pressure setting of 26 PSI for the nebulizer.

Mercury analysis was performed on a Perkin-Elmer Flow Injection Mercury System (FIMS-400) automated mercury analyzer. The instrument consists of a cold vapor atomic absorption spectrometer set to detect mercury at a wavelength of 254 nm. Sample introduction through the flow injection system is performed via a peristaltic pump at 9 mL/min and nitrogen carrier gas rate of 5 L/min.

#### **Sample Preparation**

All samples were prepared in accordance with the referenced SW-846 procedures.

#### **Calibration Information:**

##### **Initial Calibration**

Instrument calibrations are conducted using method and instrument manufacturer's specifications. All initial calibration requirements have been met for this analysis.

##### **CRDL Requirements**

All CRDL standards met the referenced advisory control limits.

##### **Continuing Calibration (CCV) Requirements**

All CCV standards bracketing this SDG met the established recovery acceptance criteria.

##### **Continuing Calibration Blanks (CCB) Requirements**

All continuing calibration blanks (CCB) bracketing this SDG met the established acceptance criteria.

##### **ICSA/ICSAB Requirements**

All interference check standard (ICSA and ICSAB) elements associated with this SDG met the established acceptance criteria.

#### **Quality Control (QC) Information:**

##### **Method Blank Acceptance**

The preparation blanks analyzed with this SDG did not contain analytes of interest at concentrations greater than the required detection limits (RDL).

##### **LCS Recovery Statement**

All LCS spike recoveries for this SDG were within the established acceptance limits.

##### **QC Sample Designation**

Sample 059846-001 (67158036) was designated as the quality control sample for the ICP and CVAA batches. Each batch included a sample duplicate (DUP) and a matrix spike (MS). The ICP batch included a serial dilution (SD).

##### **MS Recovery Statement**

The percent recoveries (%R) obtained from the MS analyses are evaluated when the sample concentration is less than four times (4X) the spike concentration added. All qualifying elements met the established acceptance limits for percent recovery.

##### **RPD Statement**

The relative percent difference (RPD) obtained from the sample duplicate (DUP) is evaluated against the acceptance criteria of 20% when the sample is greater than five times (5X) the contract required detection limit (RDL). In cases where either the sample or duplicate value is less than 5X the RDL, a control limit



of +/- the RDL is used to evaluate the DUP results. All applicable elements met the DUP acceptance criteria except arsenic, as indicated by the "\*" qualifier on the QC summary.

**Serial Dilution % Difference Statement**

The serial dilution is used to assess interference caused by matrix suppression or enhancement. Raw element concentrations that are at least 50X the instrument detection limit (IDL) for ICP analyses are applicable for serial dilution assessment. All applicable analytes met the acceptance criteria.

**Technical Information:**

**Holding Time Specifications**

All samples were analyzed within the specified holding times.

**Sample Dilutions**

Dilutions are performed to minimize matrix interference resulting from elevated mineral element concentrations and/or to bring over range target analyte concentrations into the linear calibration range of the instruments. The samples were diluted the standard 2x for soils on the ICP. No dilutions were required for the CVAA analysis.

**Miscellaneous Information:**

**NCR Documentation**

Nonconformance reports are generated to document procedural anomalies that may deviate from referenced SOP or contractual documents. No NCR's were issued for this SDG.

**Additional Comments**

The additional comments field is used to address special issues associated with each analysis, clarify method/contractual issues pertaining to the analysis and to list any report documents generated as a result of sample analysis or review. Additional comments were not required for this SDG.

**Review/Validation:**

GEL requires all analytical data to be verified by a qualified data validator.

The following data validator verified the data presented in this SDG:

Reviewer:           ADDISON          

Date:           10/9/02

## QC Summary

Report Date: October 8, 2002  
Page 1 of 2

Client : Sandia National Laboratories  
MS-0756  
P.O. Box 5800  
Albuquerque, New Mexico  
Contact: Pamela M. Puissant  
Workorder: 67158

Param Name	NOM	Sample	Qual	QC	Units	RPD%	REC%	Range	Anlst	Date	Time
<b>Metals Analysis-ICP Federal</b>											
Batch 202762											
QC1200303450 67158036 DUP											
Arsenic		4.96		3.18	mg/kg	44*		(0%-20%)	HSC	10/03/02	23:13
Barium		228		216	mg/kg	5		(0%-20%)			
Cadmium	J	0.194	J	0.211	mg/kg	N/A	^	(+/-0.490)			
Chromium		9.50		9.61	mg/kg	1		(0%-20%)			
Lead		5.47		5.14	mg/kg	6		(0%-20%)			
Selenium	BU	ND	BU	ND	mg/kg	N/A		(+/-0.490)			
Silver	J	0.441	J	0.089	mg/kg	N/A	^	(+/-0.490)			
QC1200303453 LCS											
Arsenic	192			205	mg/kg		107	(79%-121%)		10/03/02	20:56
Barium	417			462	mg/kg		111	(80%-120%)			
Cadmium	125			137	mg/kg		110	(81%-119%)			
Chromium	133			144	mg/kg		108	(77%-123%)			
Lead	160			175	mg/kg		109	(78%-123%)			
Selenium	97.0		B	103	mg/kg		106	(72%-128%)			
Silver	115			135	mg/kg		118	(55%-145%)			
QC1200303449 MB											
Arsenic			U	ND	mg/kg					10/03/02	20:50
Barium			U	ND	mg/kg						
Cadmium			U	ND	mg/kg						
Chromium			U	ND	mg/kg						
Lead			U	ND	mg/kg						
Selenium			J	0.201	mg/kg						
Silver			U	ND	mg/kg						
QC1200303452 67158036 MS											
Arsenic	23.6	4.96		24.7	mg/kg		84	(75%-125%)		10/03/02	23:19
Barium	23.6	228		264	mg/kg		N/A	(75%-125%)			
Cadmium	23.6	J 0.194		22.0	mg/kg		92	(75%-125%)			
Chromium	23.6	9.50		33.3	mg/kg		101	(75%-125%)			
Lead	23.6	5.47		27.5	mg/kg		93	(75%-125%)			
Selenium	23.5	BU ND	B	20.9	mg/kg		88	(75%-125%)			
Silver	23.6	J 0.441		23.0	mg/kg		96	(75%-125%)			
QC1200303451 67158036 SDLT											
Arsenic		50.6		9.65	ug/L	4.75				10/03/02	23:07
Barium		2320		466	ug/L	226					
Cadmium	J	1.98	U	ND	ug/L	N/A					
Chromium		96.9		19.6	ug/L	1					
Lead		55.8		11.4	ug/L	1.86					
Selenium	BU	ND	BU	ND	ug/L	N/A					
Silver	J	4.50	J	1.10	ug/L	21.9					
<b>Metals Analysis-Mercury Federal</b>											
Batch 202730											
QC1200303377 67158036 DUP											

## QC Summary

Workorder: 67158

Page 2 of 2

Parameter	NOM	Sample	Qual	QC	Units	RPD%	REC%	Range	Analst	Date	Time
Metals Analysis-Mercury Federal											
Batch 202730											
Mercury		J	0.00718	J	0.00775	mg/kg	N/A	(+/-0.00965)	NOR1	10/07/02	11:10
QC1200303379	LCS										
Mercury	23.6				26.2	mg/kg	111	(66%-134%)		10/07/02	10:30
QC1200303376	MB										
Mercury				U	ND	mg/kg				10/07/02	10:26
QC1200303378	67158036 MS										
Mercury	0.089	J	0.00718		0.0995	mg/kg	104	(75%-125%)		10/07/02	11:16

**Notes:**

RER is calculated at the 95% confidence level (2-sigma).

The Qualifiers in this report are defined as follows:

- \* Recovery or %RPD not within acceptance limits and/or spike amount not compatible with the sample or the duplicate RPD's are not applicable where d
- \*\* Indicates analyte is a surrogate compound.
- B The analyte was found in the blank above the effective MDL.
- H Holding time was exceeded
- J Estimated value, the analyte concentration fell above the effective MDL and below the effective PQL
- P The response between the confirmation column and the primary column is >40%D
- U The analyte was analyzed for but not detected below this concentration. For Organic and Inorganic analytes the result is less than the effective MDL.
- X Presumptive evidence that the analyte is not present. Please see narrative for further information.
- X Presumptive evidence that the analyte is not present. Please see narrative for further information.
- X Uncertain identification for gamma spectroscopy.

N/A indicates that spike recovery limits do not apply when sample concentration exceeds spike conc. by a factor of 4 or more.

^ The Relative Percent Difference (RPD) obtained from the sample duplicate (DUP) is evaluated against the acceptance criteria when the sample is greater than five times (5X) the contract required detection limit (RL). In cases where either the sample or duplicate value is less than 5X the RL, a control limit of +/- the RL is used to evaluate the DUP result.

For PS, PSD, and SDLT results, the values listed are the measured amounts, not final concentrations.

Where the analytical method has been performed under NELAP certification, the analysis has met all of the requirements of the NELAC standard unless qualified on the QC Summary.

**Metals Case Narrative for  
Sandia National Labs (SNLS)  
SDG# 67158-1**

**Sample Analysis:**

The following samples first extracted by SW 846 method 1311, then prepared and analyzed using the methods referenced in the "Method/Analysis Information" section of this narrative:

<b>Sample ID</b>	<b>Client ID</b>
67169010	059826-007
1200307728	Methods Blank (MB) ICP-204455/204453
1200307729	Laboratory Control Sample (LCS)
1200307666	Methods Blank (MB) CVAA-204420/204419
1200307669	Laboratory Control Sample (LCS)

**Method/Analysis Information:**

<b>Analytical Batch #:</b>	204455, 204420
<b>Prep Batch #:</b>	204453, 204419
<b>Analytical Method:</b>	SW846 6010B, SW846 7470A
<b>Prep Method:</b>	SW846 3010, SW846 7470A
<b>Standard Operating Procedure:</b>	GL-MA-E-013 REV.6, GL-MA-E-010 REV.10

**System Configuration**

The ICP analysis was performed on a Thermo Jarrell Ash 61E Trace axial-viewing inductively coupled plasma atomic emission spectrometer. The instrument is equipped with a Meinhardt nebulizer, cyclonic spray chamber, and yttrium internal standard. Operating conditions for the Trace ICP are set at a power level of 950 watts. The instrument has a peristaltic pump flow rate of 140 RPM (2.0 mL/min sample uptake rate), argon gas flows of 15 L/min and 0.5 L/min for the torch and auxiliary gases, and a pressure setting of 26 PSI for the nebulizer.

Mercury analysis was performed on a Perkin-Elmer Flow Injection Mercury System (FIMS-400) automated mercury analyzer. The instrument consists of a cold vapor atomic absorption spectrometer set to detect mercury at a wavelength of 254 nm. Sample introduction through the flow injection system is performed via a peristaltic pump at 9 mL/min and nitrogen carrier gas rate of 5 L/min.

**Sample Preparation**

All samples were prepared in accordance with the referenced SW-846 procedures.

**Calibration Information:**

**Initial Calibration**

Instrument calibrations are conducted using method and instrument manufacturer's specifications. All initial calibration requirements have been met for the analyses.

**CRDL Requirements**

All element recoveries in the CRDL standards met the advisory control limits (70% - 130).

**ICSA/ICSAB Requirements**

All interference check standard (ICSA and ICSAB) elements associated with this SDG met the established acceptance criteria.

### **Continuing Calibration (CCV) Requirements**

All CCV standards bracketing samples from this SDG met the established recovery acceptance criteria.

### **Continuing Calibration Blanks (CCB) Requirements**

All continuing calibration blanks (CCB) bracketing samples from this SDG met the established acceptance criteria.

### **Quality Control (QC) Information:**

#### **Method Blank Acceptance**

The preparation blanks analyzed with this SDG did not contain analytes of interest at concentrations greater than the client required detection limits (CRDL).

#### **LCS Recovery Statement**

All LCS spike recoveries for this SDG were within the required acceptance limits.

#### **QC Sample Statement**

Sample 060043-003 (67821004) from SNLS SDG 67821 was designated as the quality control sample for the ICP batch. Sample 059582-007 (67354008) from SNLS SDG 67354 was designated as the quality control sample for the CVAA batch. A matrix spike (MS) and a sample duplicate (DUP) were analyzed in each batch. A serial dilution (SD) was analyzed in the ICP batch.

#### **MS Recovery Statement**

The percent recoveries (%R) obtained from the MS analyses are evaluated when the sample concentration is less than four times (4X) the spike concentration added. The MS analyses met the recommended quality control acceptance criteria for percent recovery (75%-125%) for all applicable analytes.

#### **DUP RPD Statement**

The relative percent difference (RPD) obtained from the sample duplicate (DUP) is evaluated against the acceptance criteria of 20% when the sample is greater than five times (5X) the contract required detection limit (RDL). In cases where either the sample or duplicate value is less than 5X the RDL, a control limit of +/- the RDL is used to evaluate the DUP results. All applicable elements met the DUP acceptance criteria.

#### **Serial Dilution % Difference Statement**

The serial dilution is used to assess interference caused by matrix suppression or enhancement. Raw element concentrations that are at least 50X the MDL for ICP analyses are applicable for serial dilution assessment. All applicable analytes met the acceptance criteria.

### **Technical Information:**

#### **Holding Time Specifications**

All samples in this SDG met the specified holding time requirements.

#### **Sample Dilutions**

Dilutions are performed to minimize matrix interferences (e.g., those resulting from elevated mineral element concentrations) present in the sample and/or to bring over range target analyte concentrations into the linear calibration range of the instruments. No dilution was necessary.

### **Miscellaneous Information:**

**NCR Documentation**

Nonconformance reports (NCR) are generated to document procedural anomalies that may deviate from referenced SOP or contractual documents. No NCR was generated with this SDG.

**Additional Comments**

The additional comments field is used to address special issues associated with each analysis, clarify method/contractual issues pertaining to the analysis and to list any report documents generated as a result of sample analysis or review. Additional comments were not required for this SDG.

**Review/Validation:**

GEL requires all analytical data to be verified by a qualified data validator.

The following data validator verified the data presented in this SDG:

Reviewer:     Allison M. S.    

Date:     10/3/02

## QC Summary

Client : Sandia National Laboratories  
 MS-0756  
 P.O. Box 5800  
 Albuquerque, New Mexico  
 Contact: Pamela M. Puissant  
 Workorder: 67169

Report Date: October 3, 2002  
 Page 1 of 2

Paramname	NOM	Sample	Qual	QC	Units	RPD%	REC%	Range	Anlst	Date	Time
Metals Analysis-ICP Federal											
Batch 204453											
QC1200307730 67821004 DUP											
Arsenic		U	ND	U	ND	mg/L	N/A	(+/-0.005)	HSC	10/01/02	23:30
Barium				J	3.81	ug/L	N/A ^	(+/-5.00)			
Cadmium		J	0.00473	J	0.00469	mg/L	N/A ^	(+/-0.005)			
Chromium		BJ	0.00101	BJ	0.000999	mg/L	N/A ^	(+/-0.005)			
Lead		J	0.00387	J	0.00421	mg/L	N/A ^	(+/-0.005)			
Selenium		U	ND	U	ND	mg/L	N/A	(+/-0.005)			
Silver		U	ND	U	ND	mg/L	N/A	(+/-0.005)			
QC1200307729 LCS											
Arsenic	0.500				0.504	mg/L		101 (80%-120%)		10/01/02	22:54
Barium	500				516	ug/L		103 (80%-120%)			
Cadmium	0.500				0.510	mg/L		102 (80%-120%)			
Chromium	0.500			B	0.513	mg/L		103 (80%-120%)			
Lead	0.500				0.520	mg/L		104 (80%-120%)			
Selenium	0.500				0.495	mg/L		99 (80%-120%)			
Silver	0.500				0.491	mg/L		98 (80%-120%)			
QC1200307728 MB											
Arsenic				U	ND	mg/L				10/01/02	22:48
Barium				U	ND	ug/L					
Cadmium				U	ND	mg/L					
Chromium				J	0.000567	mg/L					
Lead				U	ND	mg/L					
Selenium				U	ND	mg/L					
Silver				U	ND	mg/L					
QC1200307731 67821004 MS											
Arsenic	0.500	U	ND		0.504	mg/L		101 (75%-125%)		10/01/02	23:36
Barium	500				523	ug/L		104 (75%-125%)			
Cadmium	0.500	J	0.00473		0.514	mg/L		102 (75%-125%)			
Chromium	0.500	BJ	0.00101	B	0.518	mg/L		103 (75%-125%)			
Lead	0.500	J	0.00387		0.525	mg/L		104 (75%-125%)			
Selenium	0.500	U	ND		0.503	mg/L		101 (75%-125%)			
Silver	0.500	U	ND		0.491	mg/L		98 (75%-125%)			
QC1200307732 67821004 SDILT											
Arsenic		U	ND	J	2.65	ug/L	N/A			10/01/02	23:24
Barium				J	0.888	ug/L	N/A				
Cadmium		J	4.73	J	0.787	ug/L	16.8				
Chromium		BJ	1.01	BJ	0.917	ug/L	352				
Lead		J	3.87	J	1.91	ug/L	146				
Selenium		U	ND	U	ND	ug/L	N/A				
Silver		U	ND	U	ND	ug/L	N/A				
Metals Analysis-Mercury Federal											
Batch 204420											
QC1200307667 67354008 DUP											

## QC Summary

Workorder: 67169

Page 2 of 2

Paramname	NOM	Sample	Qual	QC	Units	RPD%	REC%	Range	Anist	Date	Time
Metals Analysis-Mercury Federal											
Batch 204420											
Mercury		U	ND	U	ND	mg/L	N/A	(+/-0.0002)	NOR1	10/01/02	11:27
QC1200307669	LCS										
Mercury	0.002				0.00213	mg/L	106	(80%-120%)		10/01/02	11:17
QC1200307666	MB										
Mercury			U		ND	mg/L				10/01/02	11:15
QC1200307668	67154008	MS									
Mercury	0.002	U	ND		0.0021	mg/L	104	(75%-125%)		10/01/02	11:29

**Notes:**

RER is calculated at the 95% confidence level (2-sigma).

The Qualifiers in this report are defined as follows:

- \* Recovery or %RPD not within acceptance limits and/or spike amount not compatible with the sample or the duplicate RPD's are not applicable where t
- \*\* Indicates analyte is a surrogate compound.
- B The analyte was found in the blank above the effective MDL.
- H Holding time was exceeded
- J Estimated value, the analyte concentration fell above the effective MDL and below the effective PQL
- P The response between the confirmation column and the primary column is >40%D
- U The analyte was analyzed for but not detected below this concentration. For Organic and Inorganic analytes the result is less than the effective MDL. |
- X Presumptive evidence that the analyte is not present. Please see narrative for further information.
- X Presumptive evidence that the analyte is not present. Please see narrative for further information.
- X Uncertain identification for gamma spectroscopy.

N/A indicates that spike recovery limits do not apply when sample concentration exceeds spike conc. by a factor of 4 or more.

^ The Relative Percent Difference (RPD) obtained from the sample duplicate (DUP) is evaluated against the acceptance criteria when the sample is greater than five times (5X) the contract required detection limit (RL). In cases where either the sample or duplicate value is less than 5X the RL, a control limit of +/- the RL is used to evaluate the DUP result.

For PS, PSD, and SDILT results, the values listed are the measured amounts, not final concentrations.

Where the analytical method has been performed under NELAP certification, the analysis has met all of the requirements of the NELAC standard unless qualified on the QC Summary.



**Method/Analysis Information**

**Procedure:** Hexavalent Chromium  
**Analytical Method:** SW846 7196A  
**Prep Method:** SW846 3060A  
**Analytical Batch Number:** 203661  
**Prep Batch Number:** 203660

**Sample Analysis**

The following samples were analyzed using the analytical protocol as established in SW846 7196A:

<b>Sample ID</b>	<b>Client ID</b>
67158020	059820-002
67158021	059821-002
67158022	059822-002
67158023	059823-002
67158024	059824-002
67158025	059825-002
67158026	059828-002
67158027	059829-002
67158028	059836-002
67158029	059837-002
67158030	059838-002
67158031	059839-002
67158032	059841-002
67158033	059842-002
67158034	059843-002
1200305731	MB for batch 203661

1200305732	DUP of 67099003
1200305733	DUP of 67158024
1200305734	MS of 67099003
1200305735	MS of 67158024
1200305736	LCS for batch 203661

### **SOP Reference**

Procedure(s) for preparation, analysis and reporting of analytical data are controlled by General Engineering Laboratories, Inc. as Standard Operating Procedure(s) (SOP). The data discussed in this narrative has been analyzed in accordance with GL-GC-E-044 REV.4.

### **Preparation/Analytical Method Verification**

The SOP stated above has been prepared based on technical research and testing conducted by General Engineering Laboratories, Inc. and with guidance from the regulatory documents listed in this "Method/Analysis Information" section.

### **Calibration Information:**

The instrument used in this analysis was the following: Milton Roy Spectrophotometer 200

#### **Initial Calibration**

The instrument was properly calibrated.

#### **Calibration Verification Information**

All calibration verification standards were within the required limits.

### **Quality Control (QC) Information:**

#### **Blank Acceptance**

The method and calibration blanks associated with this data were within the required acceptance limits.

#### **Laboratory Control Sample Recovery**

The recovery for the laboratory control sample was within the required acceptance limits.

#### **Quality Control**

Samples 67099003 and 67158024 were designated for Quality Control.

**Sample Spike Recovery**

The matrix spike for SNLS sample 67099003 (1200305734) falls within GEL's acceptance limits, but outside the client's acceptance limits of 75%-125%. Per client, the batch is reported as is, since another SNLS sample in this batch passed their QC criteria.

**Sample Duplicate Acceptance**

The values for the samples and duplicates for this sample group are less than the Practical Quantitation Limit (PQL); therefore, the RPDs are not applicable.

**Technical Information:**

GEL assigns holding times based on the date and time of sample collection. Those holding times expressed in hours are calculated in the AlphaLims system by hours. Those holding times expressed as days expire at midnight on the day of expiration.

**Holding Times**

All samples from this sample group were analyzed within the required holding time for this method.

**Preparation/Analytical Method Verification**

All procedures were performed as stated in the SOP.

**Sample Dilutions**

No samples in this sample group required dilutions.

**Sample Reanalysis**

The samples in this batch were repped and reanalyzed due to batch failure. When reagents were added, the samples had a massive reaction. The LCS and matrix spikes did not change color; therefore, they did not have acceptable recoveries. The analyst added spiking reagents to post prep to verify a mistake occurred in the prep process.

**Miscellaneous Information:****Nonconformance Reports**

No Nonconformance Reports (NCR) were required for any of the samples in this sample group for this analysis.

**General Chemistry Narrative  
Sandia National Labs (SNLS)  
SDG 67158**

**Method/Analysis Information**

<b>Procedure:</b>	<b>Total Cyanide</b>
<b>Analytical Method:</b>	<b>SW846 9012A</b>
<b>Prep Method:</b>	<b>SW846 9010B Prep</b>
<b>Analytical Batch Number:</b>	<b>202749</b>
<b>Prep Batch Number:</b>	<b>202748</b>

**Sample Analysis**

The following samples were analyzed using the analytical protocol as established in SW846 9012A:

<b>Sample ID</b>	<b>Client ID</b>
67158020	059820-002
67158021	059821-002
67158022	059822-002
67158023	059823-002
67158024	059824-002
67158025	059825-002
67158026	059828-002
67158027	059829-002
67158028	059836-002
67158029	059837-002
67158030	059838-002

67158031	059839-002
67158032	059841-002
67158033	059842-002
67158034	059843-002
67158035	059844-002
67158036	059846-001
67158037	059847-002
67158038	059848-002
1200303418	MB for batch 202749
1200303419	DUP of 67158020
1200303420	DUP of 67158036
1200303421	MS of 67158020
1200303422	MS of 67158036
1200303423	LCS for batch 202749
1200303424	LCS for batch 202749

**SOP Reference**

Procedure(s) for preparation, analysis and reporting of analytical data are controlled by General Engineering Laboratories, Inc. as Standard Operating Procedure(s) (SOP). The data discussed in this narrative has been analyzed in accordance with GL-GC-E-095 Rev. 1.

**Preparation/Analytical Method Verification**

The SOP stated above has been prepared based on technical research and testing conducted by General Engineering Laboratories, Inc. and with guidance from the regulatory documents listed in this "Method/Analysis Information" section.

**Calibration Information:**

The instrument used in this analysis was the following: Lachat QuickChem FIA+

**Initial Calibration**

The instrument was properly calibrated.

**Calibration Verification Information**

All calibration verification standards were within the required limits.

**Quality Control (QC) Information:****Blank Acceptance**

The method and calibration blanks associated with this data were within the required acceptance limits.

**Laboratory Control Sample Recovery**

The recovery for the laboratory control sample was within the required acceptance limits.

**Quality Control**

Samples 67158020 and 67158036 were designated for Quality Control.

**Sample Spike Recovery**

The spike recoveries for this sample set were within the required acceptance limits.

**Sample Duplicate Acceptance**

The values for the samples and duplicates for this sample group are less than the Practical Quantitation Limit (PQL); therefore, the RPDs are not applicable.

**Technical Information:**

GEL assigns holding times based on the date and time of sample collection. Those holding times expressed in hours are calculated in the AlphaLims system by hours. Those holding times expressed as days expire at midnight on the day of expiration.

**Holding Times**

All samples from this sample group were analyzed within the required holding time for this method.

**Preparation/Analytical Method Verification**

All procedures were performed as stated in the SOP.

**Sample Dilutions**

The following QC sample in this sample group was diluted 1:50 due to high concentration for this analysis: 1200303424.

**Miscellaneous Information:**

**Nonconformance Reports**

No Nonconformance Reports (NCR) were required for any of the samples in this sample group for this analysis.

**Method/Analysis Information**

**Procedure:** Hexavalent Chromium  
**Analytical Method:** SW846 7196A  
**Prep Method:** SW846 3060A  
**Analytical Batch Number:** 203665  
**Prep Batch Number:** 203662

**Sample Analysis**

The following samples were analyzed using the analytical protocol as established in SW846 7196A:

<b>Sample ID</b>	<b>Client ID</b>
67158035	059844-002
67158036	059846-001
67158037	059847-002
67158038	059848-002
1200305737	MB for batch 203665
1200305738	DUP of 67158036
1200305739	MS of 67158036
1200305740	LCS for batch 203665

**SOP Reference**

Procedure(s) for preparation, analysis and reporting of analytical data are controlled by General Engineering Laboratories, Inc. as Standard Operating Procedure(s) (SOP). The data discussed in this narrative has been analyzed in accordance with GL-GC-E-044 REV.4.

**Preparation/Analytical Method Verification**

The SOP stated above has been prepared based on technical research and testing conducted by General Engineering Laboratories, Inc. and with guidance from the regulatory documents listed in this "Method/Analysis Information" section.



**Calibration Information:**

The instrument used in this analysis was the following: Milton Roy Spectrophotometer 200

**Initial Calibration**

The instrument was properly calibrated.

**Calibration Verification Information**

All calibration verification standards were within the required limits.

**Quality Control (QC) Information:**

**Blank Acceptance**

The method and calibration blanks associated with this data were within the required acceptance limits.

**Laboratory Control Sample Recovery**

The recovery for the laboratory control sample was within the required acceptance limits.

**Quality Control**

Sample 67158036 was designated for Quality Control.

**Sample Spike Recovery**

The spike recovery for this sample set was within the required acceptance limits.

**Sample Duplicate Acceptance**

The values for the sample and duplicate for this sample group are less than the Practical Quantitation Limit (PQL); therefore, the RPD is not applicable.

**Technical Information:**

GEL assigns holding times based on the date and time of sample collection. Those holding times expressed in hours are calculated in the AlphaLims system by hours. Those holding times expressed as days expire at midnight on the day of expiration.

**Holding Times**

All samples from this sample group were analyzed within the required holding time for this method.

**Preparation/Analytical Method Verification**

All procedures were performed as stated in the SOP.

**Sample Dilutions**

No samples in this sample group required dilutions.

**Miscellaneous Information:**

**Nonconformance Reports**

No Nonconformance Reports (NCR) were required for any of the samples in this sample group for this analysis.

**Certification Statement**

\* Where the analytical method has been performed under NELAP certification, the analysis has met all of the requirements of the NELAC standard unless otherwise noted in the analytical case narrative.

**Review Validation:**

GEL requires all analytical data to be verified by a qualified data validator. In addition, all data designated for CLP or CLP-like packaging will receive a third level validation upon completion of the data package.

**The following data validator verified the information presented in this case narrative:**

Reviewer: \_\_\_\_\_



Date: \_\_\_\_\_

10/09/02

## QC Summary

Report Date: October 9, 2002

Page 1 of 2

Client : Sandia National Laboratories  
 MS-0756  
 P.O. Box 5800  
 Albuquerque, New Mexico  
 Contact: Pamela M. Puiasant  
 Workorder: 67158

Parmaame	NOM	Sample	Qual	QC	Units	RPD%	REC%	Range	Anist	Date	Time
<b>Rapid Flow Analysis Federal</b>											
Batch	202749										
QC1200303419	67158020	DUP									
Cyanide, Total			BJ	0.110	BJ	0.077	mg/kg	N/A ^	(+/-0.227)	ADF	09/23/02 16:05
QC1200303420	67158036	DUP									
Cyanide, Total			BJ	0.117	BJ	0.0523	mg/kg	N/A ^	(+/-0.227)		09/23/02 16:24
QC1200303423	LCS										
Cyanide, Total	2.50			B		2.43	mg/kg		97 (62%-138%)		09/23/02 16:01
QC1200303424	LCS										
Cyanide, Total	275			B		242	mg/kg		88 (62%-138%)		09/23/02 16:04
QC1200303418	MB										
Cyanide, Total				J		0.048	mg/kg				09/23/02 16:00
QC1200303421	67158020	MS									
Cyanide, Total	4.55		BJ	0.110	B	5.32	mg/kg		115 (55%-145%)		09/23/02 16:06
QC1200303422	67158036	MS									
Cyanide, Total	4.55		BJ	0.117	B	4.55	mg/kg		98 (55%-145%)		09/23/02 16:24
<b>Spectrometric Analysis Federal</b>											
Batch	203661										
QC1200305732	67099003	DUP									
Hexavalent Chromium			J	0.0704	U	ND	mg/kg	N/A ^	(+/-0.0985)	BEP2	10/02/02 07:00
QC1200305733	67158024	DUP									
Hexavalent Chromium			U	ND	U	ND	mg/kg	N/A	(+/-0.0995)		
QC1200305736	LCS										
Hexavalent Chromium	0.998					1.02	mg/kg		102 (72%-121%)		
QC1200305731	MB										
Hexavalent Chromium				U		ND	mg/kg				
QC1200305734	67099003	MS									
Hexavalent Chromium	0.959		J	0.0704		0.700	mg/kg		66 (49%-130%)		
QC1200305735	67158024	MS									
Hexavalent Chromium	0.988		U	ND		0.909	mg/kg		92 (49%-130%)		
Batch	203665										
QC1200305738	67158036	DUP									
Hexavalent Chromium			U	ND	U	ND	mg/kg	N/A	(+/-0.0971)	BEP2	10/02/02 06:30
QC1200305740	LCS										
Hexavalent Chromium	0.993					1.05	mg/kg		106 (72%-121%)		
QC1200305737	MB										
Hexavalent Chromium				U		ND	mg/kg				
QC1200305739	67158036	MS									
Hexavalent Chromium	0.964		U	ND		0.790	mg/kg		82 (49%-130%)		

**Notes:**

RER is calculated at the 95% confidence level (2-sigma).

The Qualifiers in this report are defined as follows:

- \* Recovery or %RPD not within acceptance limits and/or spike amount not compatible with the sample or the duplicate RPD's are not applicable where it
- \*\* Indicates analyte is a surrogate compound.
- B The analyte was found in the blank above the effective MDL.

## QC Summary

Workorder: 67158

Page 2 of 2

Paramname	NOM	Sample Qual	QC	Units	RPD%	REC%	Range	Anlst	Date	Time
H										
Holding time was exceeded										
J										
Estimated value, the analyte concentration fell above the effective MDL and below the effective PQL										
P										
The response between the confirmation column and the primary column is >40%D										
U										
The analyte was analyzed for but not detected below this concentration. For Organic and Inorganic analytes the result is less than the effective MDL. 1										
X										
Presumptive evidence that the analyte is not present. Please see narrative for further information.										
X										
Presumptive evidence that the analyte is not present. Please see narrative for further information.										
X										
Uncertain identification for gamma spectroscopy.										

N/A indicates that spike recovery limits do not apply when sample concentration exceeds spike conc. by a factor of 4 or more.

^ The Relative Percent Difference (RPD) obtained from the sample duplicate (DUP) is evaluated against the acceptance criteria when the sample is greater than five times (5X) the contract required detection limit (RL). In cases where either the sample or duplicate value is less than 5X the RL, a control limit of +/- the RL is used to evaluate the DUP result.

For PS, PSD, and SDILT results, the values listed are the measured amounts, not final concentrations.

Where the analytical method has been performed under NELAP certification, the analysis has met all of the requirements of the NELAC standard unless qualified on the QC Summary.

**General Chemistry Narrative  
Sandia National Labs (SNLS)  
SDG 67158-1**

**Method/Analysis Information**

**Procedure:** Hexavalent Chromium  
**Analytical Method:** SW846 7196A  
**Analytical Batch Number:** 201822

**Sample Analysis**

The following samples were analyzed using the analytical protocol as established in SW846 7196A:

<b>Sample ID</b>	<b>Client ID</b>
67169009	059826-006
1200301230	MB for batch 201822
1200301231	DUP of 67169009
1200301232	PS of 67169009
1200301233	LCS for batch 201822

**SOP Reference**

Procedure(s) for preparation, analysis and reporting of analytical data are controlled by General Engineering Laboratories, Inc. as Standard Operating Procedure(s) (SOP). The data discussed in this narrative has been analyzed in accordance with *GL-GC-E-044 REV.4*.

**Preparation/Analytical Method Verification**

The SOP stated above has been prepared based on technical research and testing conducted by General Engineering Laboratories, Inc. and with guidance from the regulatory documents listed in this "Method/Analysis Information" section.

**Calibration Information:**

The instrument used in this analysis was the following: Milton Roy Spectrophotometer 200

**Initial Calibration**

The instrument was properly calibrated.

**Calibration Verification Information**

All calibration verification standards were within the required limits.

**Quality Control (QC) Information:**

**Blank Acceptance**

The method and calibration blanks associated with this data were within the required acceptance limits.

**Laboratory Control Sample Recovery**

The recovery for the laboratory control sample was within the required acceptance limits.

**Quality Control**

The following sample was designated for Quality Control: 67169009.

**Sample Spike Recovery**

The spike recovery for this sample set was within the required acceptance limits.

**Sample Duplicate Acceptance**

The values for the sample and duplicate for this sample group are less than the Practical Quantitation Limit (PQL); therefore, the RPD is not applicable.

**Technical Information:**

GEL assigns holding times based on the date and time of sample collection. Those holding times expressed in hours are calculated in the AlphaLims system by hours. Those holding times expressed as days expire at midnight on the day of expiration.

**Holding Times**

The samples from this sample group were received by the lab outside of the method specified holding time.

**Preparation/Analytical Method Verification**

All procedures were performed as stated in the SOP.

**Sample Dilutions**

No samples in this sample group required dilutions.

**Miscellaneous Information:**

**Nonconformance Reports**

Nonconformance Report(NCR) 4012 was submitted by the PM for sample 67169009 in this sample group because the sample was received beyond the recommended holding time for this analysis.

**Method/Analysis Information**

**Procedure:** Total Cyanide  
**Analytical Method:** SW846 9012A  
**Prep Method:** SW846 9010B Prep  
**Analytical Batch Number:** 202747  
**Prep Batch Number:** 202746

**Sample Analysis**

The following samples were analyzed using the analytical protocol as established in SW846 9012A:

<b>Sample ID</b>	<b>Client ID</b>
67169008	059826-005
1200303412	MB for batch 202746
1200303413	DUP of 67082013
1200303414	DUP of 67082014
1200303415	MS of 67082013
1200303416	MS of 67082014
1200303417	LCS for batch 202746

**SOP Reference**

Procedure(s) for preparation, analysis and reporting of analytical data are controlled by General Engineering Laboratories, Inc. as Standard Operating Procedure(s) (SOP). The data discussed in this narrative has been analyzed in accordance with GL-GC-E-095 Rev. 1.

**Preparation/Analytical Method Verification**

The SOP stated above has been prepared based on technical research and testing conducted by General Engineering Laboratories, Inc. and with guidance from the regulatory documents listed in this "Method/Analysis Information" section.



**Calibration Information:**

The instrument used in this analysis was the following: Lachat QuickChem FIA+

**Initial Calibration**

The instrument was properly calibrated.

**Calibration Verification Information**

All calibration verification standards were within the required limits.

**Quality Control (QC) Information:**

**Blank Acceptance**

The method and calibration blanks associated with this data were within the required acceptance limits.

**Laboratory Control Sample Recovery**

The recovery for the laboratory control sample was within the required acceptance limits.

**Quality Control**

The following SNLS samples were designated for Quality Control: 67082013, 67082014.

**Sample Spike Recovery**

The spike recoveries for this sample set were within the required acceptance limits.

**Sample Duplicate Acceptance**

The Relative Percent Differences between the samples and duplicates for this SDG were within the required acceptance limits.

**Technical Information:**

GEL assigns holding times based on the date and time of sample collection. Those holding times expressed in hours are calculated in the AlphaLims system by hours. Those holding times expressed as days expire at midnight on the day of expiration.

**Holding Times**

All samples from this sample group were analyzed within the required holding time for this method.

**Preparation/Analytical Method Verification**

All procedures were performed as stated in the SOP.

**Sample Dilutions**

No samples in this sample group required dilutions.

**Miscellaneous Information:**

**Nonconformance Reports**

No Nonconformance Reports (NCR) were required for any of the samples in this sample group for this analysis.


**Certification Statement**

\* Where the analytical method has been performed under NELAP certification, the analysis has met all of the requirements of the NELAC standard unless otherwise noted in the analytical case narrative.

**Review Validation:**

GEL requires all analytical data to be verified by a qualified data validator. In addition, all data designated for CLP or CLP-like packaging will receive a third level validation upon completion of the data package.

The following data validator verified the information presented in this case narrative:

Reviewer:  Date: 10/02/02

## QC Summary

Report Date: September 27, 2002  
Page 1 of 2

Client : Sandia National Laboratories  
MS-0756  
P.O. Box 5800  
Albuquerque, New Mexico  
Contact: Pamela M. Puissant  
Workorder: 67169

Parname	NOM	Sample	Qual	QC	Units	RPD%	REC%	Range	Anlst	Date	Time
<b>Rapid Flow Analysis Federal</b>											
Batch	202747										
QC1200303413	67082013	DUP									
Cyanide, Total		U	ND	U	ND	mg/L	N/A	(+/-0.005)	ADF	09/23/02	15:51
QC1200303414	67082014	DUP									
Cyanide, Total		J	0.00469	J	0.00428	mg/L	N/A ^	(+/-0.005)		09/23/02	15:53
QC1200303417	LCS										
Cyanide, Total	0.050				0.0475	mg/L		95 (90%-110%)		09/23/02	15:38
QC1200303412	MB										
Cyanide, Total				U	ND	mg/L					
QC1200303415	67082013	MS									
Cyanide, Total	0.100	U	ND		0.0927	mg/L		91 (72%-133%)		09/23/02	15:52
QC1200303416	67082014	MS									
Cyanide, Total	0.100	J	0.00469		0.101	mg/L		96 (72%-133%)		09/23/02	15:54
<b>Spectrometric Analysis Federal</b>											
Batch	201822										
QC1200301231	67169009	DUP									
Hexavalent Chromium		HU	ND	HU	ND	mg/L	N/A	(+/-0.010)	VH1	09/18/02	12:45
QC1200301233	LCS										
Hexavalent Chromium	0.100				0.101	mg/L		101 (89%-110%)			
QC1200301230	MB										
Hexavalent Chromium				U	ND	mg/L					
QC1200301232	67169009	PS									
Hexavalent Chromium	0.100	HU	ND	H	0.087	mg/L		87 (80%-122%)			

**Notes:**

RER is calculated at the 95% confidence level (2-sigma).

The Qualifiers in this report are defined as follows:

- \* Recovery or %RPD not within acceptance limits and/or spike amount not compatible with the sample or the duplicate RPD's are not applicable where ti
- \*\* Indicates analyte is a surrogate compound.
- B The analyte was found in the blank above the effective MDL.
- H Holding time was exceeded
- J Estimated value, the analyte concentration fell above the effective MDL and below the effective PQL
- P The response between the confirmation column and the primary column is >40%D
- U The analyte was analyzed for but not detected below this concentration. For Organic and Inorganic analytes the result is less than the effective MDL. I
- X Presumptive evidence that the analyte is not present. Please see narrative for further information.
- X Presumptive evidence that the analyte is not present. Please see narrative for further information.
- X Uncertain identification for gamma spectroscopy.

## QC Summary

Workorder: 67169

Page 2 of 2

Parmname	NOM	Sample	Qual	QC	Units	RPD%	REC%	Range	Anlst	Date	Time
----------	-----	--------	------	----	-------	------	------	-------	-------	------	------

N/A indicates that spike recovery limits do not apply when sample concentration exceeds spike conc. by a factor of 4 or more.

^ The Relative Percent Difference (RPD) obtained from the sample duplicate (DUP) is evaluated against the acceptance criteria when the sample is greater than five times (5X) the contract required detection limit (RL). In cases where either the sample or duplicate value is less than 5X the RL, a control limit of +/- the RL is used to evaluate the DUP result.

For PS, PSD, and SDILT results, the values listed are the measured amounts, not final concentrations.

Where the analytical method has been performed under NELAP certification, the analysis has met all of the requirements of the NELAC standard unless qualified on the QC Summary.

**Radiochemistry Case Narrative  
Sandia National Labs (SNLS)  
SDG 67158-1**

**Method/Analysis Information**

Batch Number: 204950  
Procedure: Determination of Gross Alpha And Gross Non-Volatile Beta in Water  
Analytical Method: EPA 900.0

Sample ID	Client ID
67169011	059826-008
1200308804	MB for batch 204950
1200308805	059826-008(67169011DUP)
1200308806	059826-008(67169011MS)
1200308807	059826-008(67169011MSD)
1200308808	LCS for batch 204950

**SOP Reference**

Procedure(s) for preparation, analysis and reporting of analytical data are controlled by General Engineering Laboratories, Inc. as Standard Operating Procedure(s) (SOP). The data discussed in this narrative has been analyzed in accordance with GL-RAD-A-001 REV.6.

**Calibration Information:**

**Calibration Information**

All initial and continuing calibration requirements have been met. The initial calibration was performed on June 12, 2002.

**Standards Information**

Standard solution(s) for these analyses are NIST traceable and used before the expiration date(s).

**Sample Geometry**

All counting sources were prepared in the same geometry as the calibration standards.

**Quality Control (QC) Information:**

**Blank Information**

The blank volume is representative of the sample volume(s) in this batch.

**Designated QC**

The following sample was used for QC: 67169011.

**QC Information**

All of the QC samples met the required acceptance limits.

**Technical Information:**

**Holding Time**

All sample procedures for this sample set were performed within the required holding time.

**Preparation Information**

All preparation criteria have been met for these analyses.

**Sample Re-prep/Re-analysis**

None of the samples in this sample set required reprep or reanalysis.

**Gross Alpha/Beta Preparation Information**

High hygroscopic salt content in evaporated samples can cause the sample mass to fluctuate due to moisture absorption. To minimize this interference, the salts are converted to oxides by heating the sample under a flame until a dull red color is obtained. The conversion to oxides stabilizes the sample weight and ensures that proper alpha/beta efficiencies are assigned for each sample. Volatile radioisotopes of carbon, hydrogen, technetium, polonium and cesium may be lost during sample heating, especially to a dull red heat. For this sample set, the prepared planchet was counted for beta activity before being flamed. After flaming, the planchet was counted for alpha activity. This sequence causes the alpha count run data to record over the beta count run data in AlphaLims, therefore only the alpha count data will appear on the instrument runlog.

**Miscellaneous Information:**

**NCR Documentation**

No NCR were generated for the preparation or analysis of this sample set.

**Certification Statement**

Where the analytical method has been performed under NELAP certification, the analysis has met all of the requirements of the NELAC standard unless otherwise noted in the analytical case narrative.

**Review Validation:**

GEL requires all analytical data to be verified by a qualified data validator. In addition, all data designated for CLP or CLP-like packaging will receive a third level validation upon completion of the data package. The following data validator verified the information presented in this case narrative:

Reviewer:                         *D. Brown*   Date:                         11 Oct 2002



# GENERAL ENGINEERING LABORATORIES

Meeting today's needs with a vision for tomorrow.

## QC Summary

Report Date: October 11, 2002  
Page 1 of 2

Client : Sandia National Laboratories  
MS-0756  
P.O. Box 5800  
Albuquerque, New Mexico  
Contact: Pamela M. Puissant  
Workorder: 67169

Paramname	NOM	Sample	Qual	QC	Units	RER	REC%	Range	Anlst	Date	Time
Rad Gas Flow											
Batch 204950											
QC1200308805 67169011 DUP											
Alpha		U	-0.293	U	-0.582	pCi/L	0.389 ^	(+/-1.00)	HOB1	10/08/02	05:44
		Uncert:	+/-0.333		+/-0.403						
		TPU:	0.334		0.408						
Beta		U	-0.0536	U	0.077	pCi/L	0.188 ^	(+/-1.00)			
		Uncert:	+/-0.341		+/-0.354						
		TPU:	0.341		0.354						
QC1200308808 LCS											
Alpha	9.89				10.9	pCi/L		110 (75%-125%)		10/07/02	21:03
		Uncert:			+/-1.84						
		TPU:			2.18						
Beta	39.7				44.1	pCi/L		111 (75%-125%)			
		Uncert:			+/-2.45						
		TPU:			2.52						
QC1200308804 MB											
Alpha				U	0.0431	pCi/L				10/08/02	05:44
		Uncert:			+/-0.0745						
		TPU:			0.0746						
Beta				U	0.126	pCi/L					
		Uncert:			+/-0.162						
		TPU:			0.162						
QC1200308806 67169011 MS											
Alpha	49.4	U	-0.293		56.9	pCi/L		116 (75%-125%)		10/07/02	21:03
		Uncert:	+/-0.333		+/-9.21						
		TPU:	0.334		12.7						
Beta	199	U	-0.0536		227	pCi/L		114 (75%-125%)			
		Uncert:	+/-0.341		+/-12.3						
		TPU:	0.341		12.4						
QC1200308807 67169011 MSD											
Alpha	49.4	U	-0.293		55.3	pCi/L		113 (75%-125%)			
		Uncert:	+/-0.333		+/-9.67						
		TPU:	0.334		11.9						
Beta	199	U	-0.0536		214	pCi/L		108 (75%-125%)			
		Uncert:	+/-0.341		+/-12.3						
		TPU:	0.341		12.9						

Notes:

The Qualifiers in this report are defined as follows:

- \* Recovery or %RPD not within acceptance limits and/or spike amount not compatible with the sample or the duplicate RPD's are not applicable where the concentration falls below the effective PQL.
- \*\* Indicates analyte is a surrogate compound.
- B The analyte was found in the blank above the effective MDL.

P O Box 30712 • Charleston, SC 29417 • 2040 Savage Road • 29407  
(843) 556-8171 • Fax (843) 766-1178



Printed on Recycled Paper.



# GENERAL ENGINEERING LABORATORIES

Meeting today's needs with a vision for tomorrow.

## QC Summary

Workorder: 67169

Page 2 of 2

Paramname	NOM	Sample Qual	QC	Units	RER	REC%	Range	Anst	Date	Time
H	Holding time was exceeded									
J	Estimated value, the analyte concentration fell above the effective MDL and below the effective PQL									
P	The response between the confirmation column and the primary column is >40%D									
U	The analyte was analyzed for but not detected below this concentration. For Organic and Inorganic analytes the result is less than the effective MDL. For radiochemical analytes the result is less than the Decision Level									
X	Presumptive evidence that the analyte is not present. Please see narrative for further information.									
X	Presumptive evidence that the analyte is not present. Please see narrative for further information.									
X	Uncertain identification for gamma spectroscopy.									

N/A indicates that spike recovery limits do not apply when sample concentration exceeds spike conc. by a factor of 4 or more.

^ The Relative Percent Difference (RPD) obtained from the sample duplicate (DUP) is evaluated against the acceptance criteria when the sample is greater than five times (5X) the contract required detection limit (RL). In cases where either the sample or duplicate value is less than 5X the RL, a control limit of +/- the RL is used to evaluate the DUP result.

For PS, PSD, and SDILT results, the values listed are the measured amounts, not final concentrations.

Where the analytical method has been performed under NELAP certification, the analysis has met all of the requirements of the NELAC standard unless qualified on the QC Summary.

P O Box 30712 • Charleston, SC 29417 • 2040 Savage Road • 29407

(843) 556-8171 • Fax (843) 766-1178

 Printed on Recycled Paper.



Radiochemistry Case Narrative  
Sandia National Labs (SNLS)  
Workorder 67158

**Method/Analysis Information**

Batch Number: 203325  
Procedure: Determination of Gross Alpha And Gross Non-Volatile Beta in Water  
Analytical Method: EPA 900.0

Sample ID	Client ID
67158020	059820-002
67158021	059821-002
67158022	059822-002
67158023	059823-002
67158024	059824-002
67158025	059825-002
67158026	059828-002
67158027	059829-002
67158028	059836-002
67158029	059837-002
67158030	059838-002
67158031	059839-002
67158032	059841-002
67158033	059842-002
67158034	059843-002
67158035	059844-002
67158036	059846-001
67158037	059847-002
67158038	059848-002
1200304874	MB for batch 203325
1200304875	059846-001(67158036DUP)
1200304876	059846-001(67158036MS)
1200304877	059846-001(67158036MSD)
1200304878	LCS for batch 203325

**SOP Reference**

Procedure(s) for preparation, analysis and reporting of analytical data are controlled by General Engineering Laboratories, Inc. as Standard Operating Procedure(s) (SOP). The data discussed in this narrative has been analyzed in accordance with GL-RAD-A-001 REV.6.

**Calibration Information:**

**Calibration Information**

All initial and continuing calibration requirements have been met. The initial calibration was performed on June 13, 2002.

**Standards Information**

Standard solution(s) for these analyses are NIST traceable and used before the expiration date(s).

**Sample Geometry**

All counting sources were prepared in the same geometry as the calibration standards.

**Quality Control (QC) Information:**

**Blank Information**

The blank volume is representative of the sample volume(s) in this batch.

**Designated QC**

The following sample was used for QC: 67158036.

**QC Information**

All of the QC samples met the required acceptance limits.

**Technical Information:****Holding Time**

All sample procedures for this sample set were performed within the required holding time.

**Preparation Information**

All preparation criteria have been met for these analyses.

**Sample Re-prep/Re-analysis**

None of the samples in this sample set required reprep or reanalysis.

**Gross Alpha/Beta Preparation Information**

High hygroscopic salt content in evaporated samples can cause the sample mass to fluctuate due to moisture absorption. To minimize this interference, the salts are converted to oxides by heating the sample under a flame until a dull red color is obtained. The conversion to oxides stabilizes the sample weight and ensures that proper alpha/beta efficiencies are assigned for each sample. Volatile radioisotopes of carbon, hydrogen, technetium, polonium and cesium may be lost during sample heating, especially to a dull red heat. For this sample set, the prepared planchet was counted for beta activity before being flamed. After flaming, the planchet was counted for alpha activity. This sequence causes the alpha count run data to record over the beta count run data in AlphaLims, therefore only the alpha count data will appear on the instrument analog.

**Miscellaneous Information:****NCR Documentation**

No NCR were generated for the preparation or analysis of this sample set.

**Certification Statement**

Where the analytical method has been performed under NELAP certification, the analysis has met all of the requirements of the NELAC standard unless otherwise noted in the analytical case narrative.

**Review Validation:**

GEL requires all analytical data to be verified by a qualified data validator. In addition, all data designated for CLP or CLP-like packaging will receive a third level validation upon completion of the data package.

The following data validator verified the information presented in this case narrative:

Reviewer: M. Nune Date: 11 Oct 2008



# GENERAL ENGINEERING LABORATORIES

Meeting today's needs with a vision for tomorrow.


## QC Summary


Report Date: October 11, 2002  
Page 1 of 2

Client : Sandia National Laboratories  
MS-0756  
P.O. Box 5800  
Albuquerque, New Mexico  
Contact: Pamela M. Puissant  
Workorder: 67158

Parname	NOM	Sample Qual	QC	Units	RER	REC%	Range	Analst	Date Time
<b>Gravimetric Solids</b>									
Batch 201819									
QC1200301124	67158020	DUP							
Moisture		2.08	1.89	percent	10		(0%-24%) AWB		09/17/02 15:04
<b>Rad Gas Flow</b>									
Batch 203325									
QC1200304875	67158036	DUP							
Alpha		10.5	8.80	pCi/g	0.318		(0%-20%) HOB1		10/07/02 12:34
		Uncert: +/-2.49	+/-2.60						
		TPU: 2.67	2.64						
Beta		17.3	16.1	pCi/g	0.326		(0%-20%)		
		Uncert: +/-1.73	+/-1.91						
		TPU: 1.78	2.02						
QC1200304878	LCS								
Alpha	9.89		9.64	pCi/g		98	(75%-125%)		10/07/02 13:17
		Uncert: +/-1.49							
		TPU: 1.69							
Beta	39.7		42.1	pCi/g		106	(75%-125%)		
		Uncert: +/-1.79							
		TPU: 2.35							
QC1200304874	MB								
Alpha		U	-0.0264	pCi/g					10/07/02 12:33
		Uncert: +/-0.079							
		TPU: 0.079							
Beta		U	0.165	pCi/g					
		Uncert: +/-0.348							
		TPU: 0.348							
QC1200304876	67158036	MS							
Alpha	94.2	10.5	105	pCi/g		100	(75%-125%)		10/07/02 12:34
		Uncert: +/-2.49	+/-7.11						
		TPU: 2.67	18.0						
Beta	378	17.3	402	pCi/g		102	(75%-125%)		
		Uncert: +/-1.73	+/-24.2						
		TPU: 1.78	29.1						
QC1200304877	67158036	MSD							
Alpha	96.9	10.5	103	pCi/g		96			
		Uncert: +/-2.49	+/-7.28						
		TPU: 2.67	14.3						
Beta	389	17.3	422	pCi/g		104			
		Uncert: +/-1.73	+/-25.1						
		TPU: 1.78	29.9						

P O Box 30712 • Charleston, SC 29417 • 2040 Savage Road • 29407  
(843) 556-8171 • Fax (843) 766-1178





# GENERAL ENGINEERING LABORATORIES

Meeting today's needs with a vision for tomorrow.

## QC Summary

Workorder: 67158

Page 2 of 2

Parname	NOM	Sample Qual	QC	Units	RER	REC%	Range	Ankt	Date	Time
---------	-----	-------------	----	-------	-----	------	-------	------	------	------

Notes:

The Qualifiers in this report are defined as follows:

- \* Recovery or %RPD not within acceptance limits and/or spike amount not compatible with the sample or the duplicate RPD's are not applicable where the concentration falls below the effective PQL.
- \*\* Indicates analyte is a surrogate compound.
- B The analyte was found in the blank above the effective MDL.
- H Holding time was exceeded
- J Estimated value, the analyte concentration fell above the effective MDL and below the effective PQL.
- P The response between the confirmation column and the primary column is >40%D
- U The analyte was analyzed for but not detected below this concentration. For Organic and Inorganic analytes the result is less than the effective MDL. For radiochemical analytes the result is less than the Decision Level
- X Presumptive evidence that the analyte is not present. Please see narrative for further information.
- X Presumptive evidence that the analyte is not present. Please see narrative for further information.
- X Uncertain identification for gamma spectroscopy.

N/A indicates that spike recovery limits do not apply when sample concentration exceeds spike conc. by a factor of 4 or more.

^ The Relative Percent Difference (RPD) obtained from the sample duplicate (DUP) is evaluated against the acceptance criteria when the sample is greater than five times (5X) the contract required detection limit (RL). In cases where either the sample or duplicate value is less than 5X the RL, a control limit of +/- the RL is used to evaluate the DUP result.

For PS, PSD, and SDILT results, the values listed are the measured amounts, not final concentrations.

Where the analytical method has been performed under NELAP certification, the analysis has met all of the requirements of the NELAC standard unless qualified on the QC Summary.

P O Box 30712 • Charleston, SC 29417 • 2040 Savage Road • 29407

(843) 556-8171 • Fax (843) 766-1178



Printed on Recycled Paper.

COC

\*\*\*\*\*  
 \* Sandia National Laboratories \*  
 \* Radiation Protection Sample Diagnostics Program \*  
 \* 9/20/02 9:31:31 AM \*  
 \*\*\*\*\*

\* Analyzed by: *he 9/20/02* Reviewed by: *K 9/20/02* \*

Customer : SANDERS, M (6135)  
 Customer Sample ID : 059828-003  
 Lab Sample ID : 20131501

Sample Description : 6536HP/1110-DF1-BH1-15-S  
 Sample Quantity : 753.000 gram  
 Sample Date/Time : 9/10/02 11:25:00 AM  
 Acquire Start Date/Time : 9/19/02 9:53:11 PM  
 Detector Name : LAB01  
 Elapsed Live/Real Time : 6000 / 6002 seconds

Comments:  
 U-235/Ra-226 peaks not resolved. Either isotope may be overestimated.  
 \*\*\*\*\*

Nuclide Name	Activity (pCi/gram)	2-sigma Error	MDA (pCi/gram)
U-238	Not Detected	-----	5.00E-001
RA-226	1.32E+000	5.03E-001	7.10E-001
PB-214	6.75E-001	1.05E-001	6.41E-002
BI-214	5.96E-001	1.02E-001	5.84E-002
PB-210	Not Detected	-----	8.77E+000
TH-232	6.57E-001	3.21E-001	2.03E-001
RA-228	6.02E-001	1.37E-001	1.53E-001
AC-228	6.76E-001	1.42E-001	1.04E-001
TH-228	8.53E-001	2.44E-001	4.30E-001
RA-224	8.85E-001	2.17E-001	1.01E-001
PB-212	7.00E-001	1.05E-001	3.86E-002
BI-212	7.10E-001	2.67E-001	3.38E-001
TL-208	5.92E-001	1.11E-001	8.65E-002
U-235	1.37E-001	1.67E-001	1.96E-001
TH-231	Not Detected	-----	6.51E+000
PA-231	Not Detected	-----	1.42E+000
TH-227	Not Detected	-----	3.17E-001
RA-223	Not Detected	-----	1.95E-001
RN-219	Not Detected	-----	3.92E-001
PB-211	Not Detected	-----	8.82E-001
TL-207	Not Detected	-----	1.55E+001
AM-241	Not Detected	-----	1.75E-001
PU-239	Not Detected	-----	3.44E+002
NP-237	Not Detected	-----	1.90E+000
PA-233	Not Detected	-----	5.62E-002
TH-229	Not Detected	-----	1.87E-001

[Summary Report] - Sample ID: : 20131501

Slide me	Activity (pCi/gram )	2-sigma Error	MDA (pCi/gram )
AG-108m	Not Detected	-----	4.34E-002
AG-110m	Not Detected	-----	2.91E-002
BA-133	Not Detected	-----	4.52E-002
BE-7	Not Detected	-----	2.83E-001
CD-115	Not Detected	-----	1.24E+000
CE-139	Not Detected	-----	2.58E-002
CE-141	Not Detected	-----	5.12E-002
CE-144	Not Detected	-----	1.96E-001
CM-243	Not Detected	-----	1.71E-001
CO-56	Not Detected	-----	3.73E-002
CO-57	Not Detected	-----	2.48E-002
CO-58	Not Detected	-----	3.50E-002
CO-60	Not Detected	-----	4.04E-002
CR-51	Not Detected	-----	2.90E-001
CS-134	Not Detected	-----	4.37E-002
CS-137	Not Detected	-----	3.10E-002
EU-152	Not Detected	-----	7.31E-002
EU-154	Not Detected	-----	2.02E-001
EU-155	Not Detected	-----	1.09E-001
FE-59	Not Detected	-----	8.73E-002
GD-153	Not Detected	-----	6.44E-002
HG-203	Not Detected	-----	3.58E-002
I-131	Not Detected	-----	6.29E-002
IR-192	Not Detected	-----	2.94E-002
IR-40	1.49E+001	2.07E+000	3.59E-001
I-52	Not Detected	-----	1.12E-001
IN-54	Not Detected	-----	3.62E-002
MO-99	Not Detected	-----	2.68E+000
NA-22	Not Detected	-----	5.08E-002
NA-24	Not Detected	-----	1.31E+003
ND-147	Not Detected	-----	3.61E-001
NI-57	Not Detected	-----	4.44E+000
RU-103	Not Detected	-----	3.56E-002
RU-106	Not Detected	-----	3.00E-001
SB-122	Not Detected	-----	4.57E-001
SB-124	Not Detected	-----	3.08E-002
SB-125	Not Detected	-----	8.37E-002
SN-113	Not Detected	-----	3.90E-002
SR-85	Not Detected	-----	3.90E-002
TA-182	Not Detected	-----	1.82E-001
TA-183	Not Detected	-----	5.47E-001
TL-201	Not Detected	-----	6.85E-001
Y-88	Not Detected	-----	3.23E-002
ZN-65	Not Detected	-----	1.20E-001
ZR-95	Not Detected	-----	6.48E-002

\*\*\*\*\*  
 \* Sandia National Laboratories \*  
 \* Radiation Protection Sample Diagnostics Program \*  
 \* 9/20/02 9:33:09 AM \*  
 \*\*\*\*\*

\* Analyzed by: *L. 9/20/02* Reviewed by: *K. 9/20/02* \*  
 \*\*\*\*\*

Customer : SANDERS, M (6135)  
 Customer Sample ID : 059829-003  
 Lab Sample ID : 20131502

Sample Description : 6536HP/1110-DF1-BH1-20-S  
 Sample Quantity : 773.000 gram  
 Sample Date/Time : 9/10/02 11:55:00 AM  
 Acquire Start Date/Time : 9/19/02 11:35:31 PM  
 Detector Name : LAB01  
 Elapsed Live/Real Time : 6000 / 6002 seconds

Comments:  
 U-235/Ra-226 peaks not resolved. Either isotope may be overestimated.  
 \*\*\*\*\*

Nuclide Name	Activity (pCi/gram)	2-sigma Error	MDA (pCi/gram)
U-238	Not Detected	-----	4.98E-001
RA-226	1.75E+000	5.54E-001	7.46E-001
PB-214	6.67E-001	1.04E-001	6.37E-002
BI-214	6.29E-001	1.05E-001	5.45E-002
PB-210	Not Detected	-----	8.54E+000
H-232	5.50E-001	2.76E-001	1.91E-001
RA-228	6.55E-001	1.41E-001	1.31E-001
AC-228	7.10E-001	1.46E-001	1.05E-001
TH-228	6.30E-001	2.15E-001	4.18E-001
RA-224	7.18E-001	1.84E-001	9.39E-002
PB-212	6.91E-001	1.03E-001	3.79E-002
BI-212	5.87E-001	2.99E-001	4.29E-001
TL-208	5.88E-001	1.12E-001	9.16E-002
U-235	Not Detected	-----	1.95E-001
TH-231	Not Detected	-----	6.50E+000
PA-231	Not Detected	-----	1.35E+000
TH-227	Not Detected	-----	3.11E-001
RA-223	Not Detected	-----	1.85E-001
RN-219	Not Detected	-----	3.81E-001
PB-211	Not Detected	-----	8.95E-001
TL-207	Not Detected	-----	1.60E+001
AM-241	Not Detected	-----	1.65E-001
FU-239	Not Detected	-----	3.45E+002
NP-237	Not Detected	-----	1.81E+000
PA-233	Not Detected	-----	5.80E-002
TH-229	Not Detected	-----	1.93E-001



Nuclide Name	Activity (pCi/gram )	2-sigma Error	MDA (pCi/gram )
AG-108m	Not Detected	-----	3.95E-002
AG-110m	Not Detected	-----	3.10E-002
BA-133	Not Detected	-----	4.36E-002
BE-7	Not Detected	-----	2.69E-001
CD-115	Not Detected	-----	1.22E+000
CE-139	Not Detected	-----	2.54E-002
CE-141	Not Detected	-----	5.25E-002
CE-144	Not Detected	-----	1.92E-001
CM-243	Not Detected	-----	1.64E-001
CO-56	Not Detected	-----	3.59E-002
CO-57	Not Detected	-----	2.52E-002
CO-58	Not Detected	-----	3.90E-002
CO-60	Not Detected	-----	4.18E-002
CR-51	Not Detected	-----	2.78E-001
CS-134	Not Detected	-----	4.06E-002
CS-137	Not Detected	-----	3.23E-002
EU-152	Not Detected	-----	7.41E-002
EU-154	Not Detected	-----	1.86E-001
EU-155	Not Detected	-----	1.10E-001
FE-59	Not Detected	-----	9.64E-002
GD-153	Not Detected	-----	6.62E-002
HG-203	Not Detected	-----	3.38E-002
I-131	Not Detected	-----	6.05E-002
IR-192	Not Detected	-----	2.93E-002
K-40	1.72E+001	2.36E+000	2.60E-001
LN-52	Not Detected	-----	1.06E-001
LN-54	Not Detected	-----	3.86E-002
MO-99	Not Detected	-----	2.79E+000
NA-22	Not Detected	-----	4.32E-002
NA-24	Not Detected	-----	1.19E+003
ND-147	Not Detected	-----	3.66E-001
NI-57	Not Detected	-----	4.62E+000
RU-103	Not Detected	-----	3.14E-002
RU-106	Not Detected	-----	2.88E-001
SB-122	Not Detected	-----	4.42E-001
SB-124	Not Detected	-----	3.10E-002
SB-125	Not Detected	-----	8.57E-002
SN-113	Not Detected	-----	4.10E-002
SR-85	Not Detected	-----	3.91E-002
TA-182	Not Detected	-----	1.79E-001
TA-183	Not Detected	-----	5.16E-001
TL-201	Not Detected	-----	6.59E-001
Y-88	Not Detected	-----	3.62E-002
ZN-65	Not Detected	-----	1.19E-001
ZR-95	Not Detected	-----	6.65E-002

\*\*\*\*\*  
 \* Sandia National Laboratories \*  
 \* Radiation Protection Sample Diagnostics Program \*  
 \* 9/20/02 2:58:05 AM \*  
 \*\*\*\*\*

analyzed by: *lu g/20/02* Reviewed by: *[Signature] 9/20/02*

Customer : SANDERS, M (6135)  
 Customer Sample ID : 059836-003  
 Lab Sample ID : 20131503

Sample Description : 6536HP/1110-DF1-BH2-10-S  
 Sample Quantity : 646.000 gram  
 Sample Date/Time : 9/13/02 9:05:00 AM  
 Acquire Start Date/Time : 9/20/02 1:17:51 AM  
 Detector Name : LAB01  
 Elapsed Live/Real Time : 6000 / 6002 seconds

Comments:  
 U-235/Ra-226 peaks not resolved. Either isotope may be overestimated.  
 \*\*\*\*\*

Nuclide Name	Activity (pCi/gram)	2-sigma Error	MDA (pCi/gram)
U-238	Not Detected	-----	5.70E-001
RA-226	1.59E+000	5.53E-001	7.59E-001
PB-214	7.65E-001	1.20E-001	7.51E-002
BI-214	7.11E-001	1.19E-001	6.07E-002
PB-210	Not Detected	-----	9.75E+000
H-232	8.50E-001	4.10E-001	2.43E-001
LA-228	9.58E-001	1.91E-001	1.61E-001
AC-228	9.44E-001	1.88E-001	1.24E-001
TH-228	7.14E-001	2.52E-001	5.14E-001
RA-224	9.75E-001	2.41E-001	1.11E-001
PB-212	8.69E-001	1.29E-001	4.21E-002
BI-212	9.41E-001	2.98E-001	3.33E-001
TL-208	8.02E-001	1.45E-001	1.11E-001
U-235	Not Detected	-----	2.23E-001
TH-231	Not Detected	-----	7.62E+000
PA-231	Not Detected	-----	1.58E+000
TH-227	Not Detected	-----	3.74E-001
RA-223	Not Detected	-----	1.92E-001
RN-219	Not Detected	-----	4.48E-001
PB-211	Not Detected	-----	9.75E-001
TL-207	Not Detected	-----	1.69E+001
AM-241	Not Detected	-----	1.90E-001
PU-239	Not Detected	-----	4.00E+002
NP-237	Not Detected	-----	2.07E+000
PA-233	Not Detected	-----	6.52E-002
TH-229	Not Detected	-----	2.20E-001

Nuclide Name	Activity (pCi/gram )	2-sigma Error	MDA (pCi/gram )
.G-108m	Not Detected	-----	4.97E-002
AG-110m	Not Detected	-----	3.67E-002
BA-133	Not Detected	-----	5.05E-002
BE-7	Not Detected	-----	2.95E-001
CD-115	Not Detected	-----	6.12E-001
CE-139	Not Detected	-----	2.82E-002
CE-141	Not Detected	-----	5.67E-002
CE-144	Not Detected	-----	2.16E-001
CM-243	Not Detected	-----	1.96E-001
CO-56	Not Detected	-----	3.95E-002
CO-57	Not Detected	-----	2.78E-002
CO-58	Not Detected	-----	4.01E-002
CO-60	Not Detected	-----	4.34E-002
CR-51	Not Detected	-----	3.03E-001
CS-134	Not Detected	-----	4.95E-002
CS-137	Not Detected	-----	3.74E-002
EU-152	Not Detected	-----	8.25E-002
EU-154	Not Detected	-----	2.34E-001
EU-155	Not Detected	-----	1.20E-001
FE-59	Not Detected	-----	1.05E-001
GD-153	Not Detected	-----	7.23E-002
HG-203	Not Detected	-----	3.87E-002
I-131	Not Detected	-----	5.54E-002
IR-192	Not Detected	-----	3.32E-002
K-40	1.48E+001	2.08E+000	3.82E-001
MN-52	Not Detected	-----	9.45E-002
N-54	Not Detected	-----	4.08E-002
MO-99	Not Detected	-----	1.54E+000
NA-22	Not Detected	-----	5.34E-002
NA-24	Not Detected	-----	6.68E+001
ND-147	Not Detected	-----	3.69E-001
NI-57	Not Detected	-----	1.44E+000
RU-103	Not Detected	-----	3.77E-002
RU-106	Not Detected	-----	3.47E-001
SB-122	Not Detected	-----	2.44E-001
SB-124	Not Detected	-----	3.55E-002
SB-125	Not Detected	-----	1.00E-001
SN-113	Not Detected	-----	4.63E-002
SR-85	Not Detected	-----	4.39E-002
TA-182	Not Detected	-----	1.95E-001
TA-183	Not Detected	-----	4.04E-001
TL-201	Not Detected	-----	4.18E-001
Y-88	Not Detected	-----	4.26E-002
ZN-65	Not Detected	-----	1.29E-001
ZR-95	Not Detected	-----	6.98E-002

\*\*\*\*\*  
 \* Sandia National Laboratories \*  
 \* Radiation Protection Sample Diagnostics Program \*  
 \* 9/20/02 4:40:24 AM \*  
 \*\*\*\*\*

\* Analyzed by: *[Signature]* 9/20/02 Reviewed by: *[Signature]* 9/20/02 \*  
 \*\*\*\*\*

Customer : SANDERS, M (6135)  
 Customer Sample ID : 059837-003  
 Lab Sample ID : 20131504

Sample Description : 6536HP/1110-DF1-BH2-15-S  
 Sample Quantity : 689.000 gram  
 Sample Date/Time : 9/13/02 9:20:00 AM  
 Acquire Start Date/Time : 9/20/02 3:00:10 AM  
 Detector Name : LAB01  
 Elapsed Live/Real Time : 6000 / 6002 seconds

Comments:  
 U-235/Ra-226 peaks not resolved. Either isotope may be overestimated.  
 \*\*\*\*\*

Nuclide Name	Activity (pCi/gram)	2-sigma Error	MDA (pCi/gram)
U-238	Not Detected	-----	5.40E-001
RA-226	1.87E+000	5.95E-001	8.00E-001
PB-214	7.05E-001	1.12E-001	7.53E-002
BI-214	6.66E-001	1.12E-001	5.83E-002
PB-210	Not Detected	-----	9.43E+000
TH-232	6.17E-001	3.18E-001	2.46E-001
RA-228	6.71E-001	1.82E-001	1.98E-001
AC-228	7.63E-001	1.61E-001	1.22E-001
TH-228	8.56E-001	2.58E-001	4.62E-001
RA-224	7.77E-001	2.08E-001	1.35E-001
PB-212	8.09E-001	1.20E-001	4.30E-002
BI-212	6.56E-001	2.88E-001	3.89E-001
TL-208	7.73E-001	1.36E-001	9.38E-002
U-235	Not Detected	-----	2.12E-001
TH-231	Not Detected	-----	6.93E+000
PA-231	Not Detected	-----	1.52E+000
TH-227	Not Detected	-----	3.54E-001
RA-223	Not Detected	-----	1.76E-001
RN-219	Not Detected	-----	4.47E-001
PB-211	Not Detected	-----	9.92E-001
TL-207	Not Detected	-----	1.67E+001
AM-241	Not Detected	-----	1.86E-001
PU-239	Not Detected	-----	3.84E+002
NP-237	Not Detected	-----	1.94E+000
PA-233	Not Detected	-----	6.34E-002
TH-229	Not Detected	-----	2.03E-001

Nuclide Name	Activity (pCi/gram )	2-sigma Error	MDA (pCi/gram )
AG-108m	Not Detected	-----	4.68E-002
AG-110m	Not Detected	-----	3.16E-002
BA-133	Not Detected	-----	4.96E-002
BE-7	Not Detected	-----	2.79E-001
CD-115	Not Detected	-----	5.83E-001
CE-139	Not Detected	-----	2.70E-002
CE-141	Not Detected	-----	5.32E-002
CE-144	Not Detected	-----	2.02E-001
CM-243	Not Detected	-----	1.83E-001
CO-56	Not Detected	-----	4.04E-002
CO-57	Not Detected	-----	2.59E-002
CO-58	Not Detected	-----	3.99E-002
CO-60	Not Detected	-----	4.45E-002
CR-51	Not Detected	-----	2.72E-001
CS-134	Not Detected	-----	4.75E-002
CS-137	Not Detected	-----	3.58E-002
EU-152	Not Detected	-----	7.66E-002
EU-154	Not Detected	-----	2.21E-001
EU-155	Not Detected	-----	1.17E-001
FE-59	Not Detected	-----	9.03E-002
GD-153	Not Detected	-----	6.78E-002
HG-203	Not Detected	-----	3.69E-002
I-131	Not Detected	-----	5.22E-002
IR-192	Not Detected	-----	2.88E-002
K-40	1.53E+001	2.13E+000	3.03E-001
MN-52	Not Detected	-----	8.93E-002
NI-54	Not Detected	-----	3.93E-002
PO-99	Not Detected	-----	1.50E+000
NA-22	Not Detected	-----	5.18E-002
NA-24	Not Detected	-----	7.10E+001
ND-147	Not Detected	-----	3.36E-001
NI-57	Not Detected	-----	1.39E+000
RU-103	Not Detected	-----	3.40E-002
RU-106	Not Detected	-----	3.19E-001
SB-122	Not Detected	-----	2.34E-001
SB-124	Not Detected	-----	3.34E-002
SB-125	Not Detected	-----	9.01E-002
SN-113	Not Detected	-----	4.09E-002
SR-85	Not Detected	-----	4.13E-002
TA-182	Not Detected	-----	1.80E-001
TA-183	Not Detected	-----	3.94E-001
TL-201	Not Detected	-----	3.85E-001
Y-88	Not Detected	-----	3.36E-002
ZN-65	Not Detected	-----	1.18E-001
ZR-95	Not Detected	-----	6.87E-002

\*\*\*\*\*  
 \* Sandia National Laboratories \*  
 \* Radiation Protection Sample Diagnostics Program \*  
 \* 9/20/02 6:22:43 AM \*  
 \*\*\*\*\*

- Analyzed by: *h* 9/20/02 Reviewed by: *K* 9/20/02  
 \*\*\*\*\*

Customer : SANDERS, M (6135)  
 Customer Sample ID : 059838-003  
 Lab Sample ID : 20131505  
 Sample Description : 6715/1035-SP1-BH1-11-S  
 Sample Quantity : 775.000 gram  
 Sample Date/Time : 9/12/02 2:20:00 PM  
 Acquire Start Date/Time : 9/20/02 4:42:29 AM  
 Detector Name : LAB01  
 Elapsed Live/Real Time : 6000 / 6002 seconds

Comments:  
 U-235/Ra-226 peaks not resolved. Either isotope may be overestimated.  
 \*\*\*\*\*

Nuclide Name	Activity (pCi/gram)	2-sigma Error	MDA (pCi/gram)
U-238	Not Detected	-----	4.87E-001
RA-226	1.73E+000	5.44E-001	7.28E-001
PB-214	7.07E-001	1.06E-001	5.52E-002
BI-214	6.06E-001	1.02E-001	5.58E-002
PB-210	Not Detected	-----	8.45E+000
H-232	6.96E-001	3.38E-001	2.09E-001
RA-228	7.28E-001	1.51E-001	1.41E-001
AC-228	7.76E-001	1.57E-001	1.10E-001
TH-228	7.06E-001	2.22E-001	4.06E-001
RA-224	9.06E-001	2.17E-001	8.79E-002
PB-212	7.33E-001	1.09E-001	3.73E-002
BI-212	6.73E-001	4.82E-001	7.46E-001
TL-208	6.35E-001	1.16E-001	8.93E-002
U-235	9.48E-002	1.69E-001	1.98E-001
TH-231	Not Detected	-----	6.32E+000
PA-231	Not Detected	-----	1.36E+000
TH-227	Not Detected	-----	3.15E-001
RA-223	Not Detected	-----	1.70E-001
RN-219	Not Detected	-----	3.72E-001
PB-211	Not Detected	-----	8.25E-001
TL-207	Not Detected	-----	1.47E+001
AM-241	Not Detected	-----	1.65E-001
PU-239	Not Detected	-----	3.56E+002
NP-237	Not Detected	-----	1.89E+000
PA-233	Not Detected	-----	5.52E-002
TH-229	Not Detected	-----	1.88E-001

[Summary Report] - Sample ID: : 20131505

Nuclide Name	Activity (pCi/gram )	2-sigma Error	MDA (pCi/gram )
AG-108m	Not Detected	-----	4.12E-002
AG-110m	Not Detected	-----	2.88E-002
BA-133	Not Detected	-----	4.22E-002
BE-7	Not Detected	-----	2.69E-001
CD-115	Not Detected	-----	7.04E-001
CE-139	Not Detected	-----	2.44E-002
CE-141	Not Detected	-----	5.09E-002
CE-144	Not Detected	-----	1.93E-001
CM-243	Not Detected	-----	1.69E-001
CO-56	Not Detected	-----	3.81E-002
CO-57	Not Detected	-----	2.50E-002
CO-58	Not Detected	-----	3.53E-002
CO-60	Not Detected	-----	3.81E-002
CR-51	Not Detected	-----	2.63E-001
CS-134	Not Detected	-----	4.10E-002
CS-137	Not Detected	-----	3.19E-002
EU-152	Not Detected	-----	7.38E-002
EU-154	Not Detected	-----	1.92E-001
EU-155	Not Detected	-----	1.09E-001
FE-59	Not Detected	-----	8.82E-002
GD-153	Not Detected	-----	6.33E-002
HG-203	Not Detected	-----	3.42E-002
I-131	Not Detected	-----	5.08E-002
IR-192	Not Detected	-----	2.70E-002
K-40	1.51E+001	2.09E+000	3.48E-001
MN-52	Not Detected	-----	8.55E-002
MN-54	Not Detected	-----	3.79E-002
MO-99	Not Detected	-----	1.78E+000
NA-22	Not Detected	-----	4.83E-002
NA-24	Not Detected	-----	1.57E+002
ND-147	Not Detected	-----	3.29E-001
NI-57	Not Detected	-----	1.77E+000
RU-103	Not Detected	-----	3.21E-002
RU-106	Not Detected	-----	2.91E-001
SB-122	Not Detected	-----	2.75E-001
SB-124	Not Detected	-----	2.98E-002
SB-125	Not Detected	-----	8.33E-002
SN-113	Not Detected	-----	3.87E-002
SR-85	Not Detected	-----	3.87E-002
TA-182	Not Detected	-----	1.70E-001
TA-183	Not Detected	-----	4.01E-001
TL-201	Not Detected	-----	4.44E-001
Y-88	Not Detected	-----	3.19E-002
ZN-65	Not Detected	-----	1.12E-001
ZR-95	Not Detected	-----	6.54E-002

\*\*\*\*\*  
 \* Sandia National Laboratories \*  
 \* Radiation Protection Sample Diagnostics Program \*  
 \* 9/20/02 9:20:40 AM \*  
 \*\*\*\*\*

\* Analyzed by: *me 9/20/02* Reviewed by: *[Signature] 9/20/02* \*

Customer : SANDERS, M (6135)  
 Customer Sample ID : 059839-003  
 Lab Sample ID : 20131506

Sample Description : 6715/1035-SP1-BH1-16-S  
 Sample Quantity : 736.000 gram  
 Sample Date/Time : 9/12/02 2:40:00 PM  
 Acquire Start Date/Time : 9/20/02 6:24:48 AM  
 Detector Name : LAB01  
 Elapsed Live/Real Time : 6000 / 6002 seconds

Comments:  
 U-235/Ra-226 peaks not resolved. Either isotope may be overestimated.  
 \*\*\*\*\*

Nuclide Name	Activity (pCi/gram)	2-sigma Error	MDA (pCi/gram)
U-238	Not Detected	-----	5.16E-001
RA-226	1.63E+000	5.09E-001	6.74E-001
PB-214	7.48E-001	1.13E-001	5.86E-002
BI-214	6.59E-001	1.11E-001	6.12E-002
PB-210	Not Detected	-----	8.96E+000
TH-232	7.94E-001	3.81E-001	2.17E-001
RA-228	6.41E-001	1.44E-001	1.61E-001
AC-228	6.76E-001	1.52E-001	1.36E-001
TH-228	7.96E-001	2.47E-001	4.88E-001
RA-224	9.45E-001	2.29E-001	1.07E-001
PB-212	7.87E-001	1.17E-001	3.83E-002
BI-212	8.21E-001	3.08E-001	3.99E-001
TL-208	6.26E-001	1.17E-001	9.08E-002
U-235	Not Detected	-----	1.99E-001
TH-231	Not Detected	-----	6.66E+000
PA-231	Not Detected	-----	1.37E+000
TH-227	Not Detected	-----	3.38E-001
RA-223	Not Detected	-----	1.75E-001
RN-219	Not Detected	-----	3.91E-001
PB-211	Not Detected	-----	8.74E-001
TL-207	Not Detected	-----	1.54E+001
AM-241	Not Detected	-----	1.75E-001
PU-239	Not Detected	-----	3.68E+002
NP-237	Not Detected	-----	1.94E+000
PA-233	Not Detected	-----	5.68E-002
TH-229	Not Detected	-----	1.94E-001



[Summary Report] - Sample ID: : 20131506

Nuclide Name	Activity (pCi/gram )	2-sigma Error	MDA (pCi/gram )
AG-108m	Not Detected	-----	4.53E-002
AG-110m	Not Detected	-----	3.09E-002
BA-133	Not Detected	-----	4.53E-002
BE-7	Not Detected	-----	2.75E-001
CD-115	Not Detected	-----	7.50E-001
CE-139	Not Detected	-----	2.63E-002
CE-141	Not Detected	-----	5.09E-002
CE-144	Not Detected	-----	1.98E-001
CM-243	Not Detected	-----	1.76E-001
CO-56	Not Detected	-----	3.64E-002
CO-57	Not Detected	-----	2.47E-002
CO-58	Not Detected	-----	3.58E-002
CO-60	Not Detected	-----	4.03E-002
CR-51	Not Detected	-----	2.62E-001
CS-134	Not Detected	-----	4.63E-002
CS-137	Not Detected	-----	3.44E-002
EU-152	Not Detected	-----	7.29E-002
EU-154	Not Detected	-----	2.12E-001
EU-155	Not Detected	-----	1.12E-001
FE-59	Not Detected	-----	9.44E-002
GD-153	Not Detected	-----	6.56E-002
HG-203	Not Detected	-----	3.51E-002
I-131	Not Detected	-----	5.39E-002
IR-192	Not Detected	-----	2.89E-002
K-40	1.52E+001	2.11E+000	3.08E-001
IN-52	Not Detected	-----	7.95E-002
IN-54	Not Detected	-----	3.71E-002
MO-99	Not Detected	-----	1.80E+000
NA-22	Not Detected	-----	4.62E-002
NA-24	Not Detected	-----	1.85E+002
ND-147	Not Detected	-----	3.38E-001
NI-57	Not Detected	-----	2.13E+000
RU-103	Not Detected	-----	3.05E-002
RU-106	Not Detected	-----	2.92E-001
SB-122	Not Detected	-----	2.96E-001
SB-124	Not Detected	-----	3.33E-002
SB-125	Not Detected	-----	8.97E-002
SN-113	Not Detected	-----	3.74E-002
SR-85	Not Detected	-----	3.87E-002
TA-182	Not Detected	-----	1.86E-001
TA-183	Not Detected	-----	4.19E-001
TL-201	Not Detected	-----	4.74E-001
Y-88	Not Detected	-----	3.16E-002
ZN-65	Not Detected	-----	1.25E-001
ZR-95	Not Detected	-----	7.00E-002

\*\*\*\*\*  
 \* Sandia National Laboratories \*  
 \* Radiation Protection Sample Diagnostics Program \*  
 \* 9/20/02 9:47:23 AM \*  
 \*\*\*\*\*

\* Analyzed by: *su* 9/20/02 Reviewed by: *K 9/20/02* \*  
 \*\*\*\*\*

Customer : SANDERS, M (6135)  
 Customer Sample ID : 059841-003  
 Lab Sample ID : 20131507

Sample Description : 6721/1090-DF1-BH1-4-S  
 Sample Quantity : 808.000 gram  
 Sample Date/Time : 9/13/02 9:35:00 AM  
 Acquire Start Date/Time : 9/20/02 8:07:08 AM  
 Detector Name : LAB01  
 Elapsed Live/Real Time : 6000 / 6002 seconds

Comments:  
 U-235/Ra-226 peaks not resolved. Either isotope may be overestimated.  
 \*\*\*\*\*

Nuclide Name	Activity (pCi/gram)	2-sigma Error	MDA (pCi/gram)
U-238	Not Detected	-----	4.50E-001
RA-226	1.55E+000	7.51E-001	1.13E+000
PB-214	6.57E-001	9.99E-002	5.49E-002
BI-214	5.98E-001	9.91E-002	4.76E-002
PB-210	Not Detected	-----	8.39E+000
TH-232	6.71E-001	3.24E-001	1.92E-001
RA-228	6.38E-001	1.40E-001	1.50E-001
AC-228	6.87E-001	1.44E-001	1.12E-001
TH-228	8.03E-001	2.35E-001	4.36E-001
RA-224	7.25E-001	1.82E-001	8.18E-002
PB-212	6.75E-001	1.01E-001	3.41E-002
BI-212	7.08E-001	2.66E-001	3.40E-001
TL-208	6.15E-001	1.11E-001	8.24E-002
U-235	2.29E-001	1.54E-001	1.84E-001
TH-231	Not Detected	-----	6.04E+000
PA-231	Not Detected	-----	1.29E+000
TH-227	Not Detected	-----	2.97E-001
RA-223	Not Detected	-----	1.56E-001
RN-219	Not Detected	-----	3.51E-001
PB-211	Not Detected	-----	7.90E-001
TL-207	Not Detected	-----	1.31E+001
AM-241	Not Detected	-----	1.56E-001
PU-239	Not Detected	-----	3.34E+002
NP-237	Not Detected	-----	1.76E+000
PA-233	Not Detected	-----	5.45E-002
TH-229	Not Detected	-----	1.81E-001

[Summary Report] - Sample ID: : 20131507

Nuclide Name	Activity (pCi/gram )	2-sigma Error	MDA (pCi/gram )
.G-108m	Not Detected	-----	4.09E-002
AG-110m	Not Detected	-----	3.00E-002
BA-133	Not Detected	-----	3.91E-002
BE-7	Not Detected	-----	2.38E-001
CD-115	Not Detected	-----	5.33E-001
CE-139	Not Detected	-----	2.42E-002
CE-141	Not Detected	-----	4.60E-002
CE-144	Not Detected	-----	1.82E-001
CM-243	Not Detected	-----	1.62E-001
CO-56	Not Detected	-----	3.27E-002
CO-57	Not Detected	-----	2.31E-002
CO-58	Not Detected	-----	3.42E-002
CO-60	Not Detected	-----	3.75E-002
CR-51	Not Detected	-----	2.56E-001
CS-134	Not Detected	-----	4.13E-002
CS-137	Not Detected	-----	3.17E-002
EU-152	Not Detected	-----	6.85E-002
EU-154	Not Detected	-----	1.91E-001
EU-155	Not Detected	-----	1.05E-001
FE-59	Not Detected	-----	8.16E-002
GD-153	Not Detected	-----	5.96E-002
HG-203	Not Detected	-----	3.21E-002
I-131	Not Detected	-----	4.49E-002
IR-192	Not Detected	-----	2.64E-002
K-40	1.46E+001	2.02E+000	2.83E-001
MN-52	Not Detected	-----	8.38E-002
MN-54	Not Detected	-----	3.43E-002
MO-99	Not Detected	-----	1.29E+000
NA-22	Not Detected	-----	4.49E-002
NA-24	Not Detected	-----	7.87E+001
ND-147	Not Detected	-----	2.90E-001
NI-57	Not Detected	-----	1.37E+000
RU-103	Not Detected	-----	3.09E-002
RU-106	Not Detected	-----	2.69E-001
SB-122	Not Detected	-----	2.34E-001
SB-124	Not Detected	-----	2.78E-002
SB-125	Not Detected	-----	7.82E-002
SN-113	Not Detected	-----	3.57E-002
SR-85	Not Detected	-----	3.56E-002
TA-182	Not Detected	-----	1.66E-001
TA-183	Not Detected	-----	3.40E-001
TL-201	Not Detected	-----	3.71E-001
Y-88	Not Detected	-----	2.68E-002
ZN-65	Not Detected	-----	1.11E-001
ZR-95	Not Detected	-----	5.95E-002

\*\*\*\*\*  
 \* Sandia National Laboratories \*  
 \* Radiation Protection Sample Diagnostics Program \*  
 \* 9/20/02 11:29:48 AM \*  
 \*\*\*\*\*

Analyzed by: *lm 9/20/02* Reviewed by: *K 9/20/02*  
 \*\*\*\*\*

Customer : SANDERS, M (6135)  
 Customer Sample ID : 059842-003  
 Lab Sample ID : 20131508

Sample Description : 6721/1090-DF1-BH1-9-S  
 Sample Quantity : 807.000 gram  
 Sample Date/Time : 9/13/02 9:50:00 AM  
 Acquire Start Date/Time : 9/20/02 9:49:28 AM  
 Detector Name : LAB01  
 Elapsed Live/Real Time : 6000 / 6002 seconds

Comments:  
 U-235/Ra-226 peaks not resolved. Either isotope may be overestimated.  
 \*\*\*\*\*

Nuclide Name	Activity (pCi/gram)	2-sigma Error	MDA (pCi/gram)
U-238	Not Detected	-----	4.74E-001
RA-226	1.32E+000	5.09E-001	7.25E-001
PB-214	7.10E-001	1.07E-001	5.70E-002
BI-214	5.64E-001	9.43E-002	4.67E-002
PB-210	Not Detected	-----	8.36E+000
TH-232	6.21E-001	3.04E-001	1.91E-001
RA-228	5.68E-001	1.30E-001	1.43E-001
AC-228	4.51E-001	1.11E-001	1.06E-001
TH-228	8.60E-001	2.35E-001	4.04E-001
RA-224	6.94E-001	1.75E-001	6.92E-002
PB-212	6.39E-001	9.58E-002	3.58E-002
BI-212	9.18E-001	3.25E-001	4.17E-001
TL-208	6.08E-001	1.10E-001	7.94E-002
U-235	Not Detected	-----	1.91E-001
TH-231	Not Detected	-----	6.26E+000
PA-231	Not Detected	-----	1.35E+000
TH-227	Not Detected	-----	2.98E-001
RA-223	Not Detected	-----	1.62E-001
RN-219	Not Detected	-----	3.63E-001
PB-211	Not Detected	-----	7.99E-001
TL-207	Not Detected	-----	1.50E+001
AM-241	Not Detected	-----	1.64E-001
PU-239	Not Detected	-----	3.39E+002
NP-237	Not Detected	-----	1.75E+000
PA-233	Not Detected	-----	5.52E-002
TH-229	Not Detected	-----	1.80E-001

Nuclide Name	Activity (pCi/gram )	2-sigma Error	MDA (pCi/gram )
J-108m	Not Detected	-----	4.09E-002
AG-110m	Not Detected	-----	2.97E-002
BA-133	Not Detected	-----	4.32E-002
BE-7	Not Detected	-----	2.51E-001
CD-115	Not Detected	-----	5.52E-001
CE-139	Not Detected	-----	2.43E-002
CE-141	Not Detected	-----	4.79E-002
CE-144	Not Detected	-----	1.86E-001
CM-243	Not Detected	-----	1.65E-001
CO-56	Not Detected	-----	3.57E-002
CO-57	Not Detected	-----	2.36E-002
CO-58	Not Detected	-----	3.53E-002
CO-60	Not Detected	-----	3.71E-002
CR-51	Not Detected	-----	2.55E-001
CS-134	Not Detected	-----	4.01E-002
CS-137	Not Detected	-----	3.14E-002
EU-152	Not Detected	-----	6.98E-002
EU-154	Not Detected	-----	1.93E-001
EU-155	Not Detected	-----	1.03E-001
FE-59	Not Detected	-----	8.80E-002
GD-153	Not Detected	-----	6.09E-002
HG-203	Not Detected	-----	3.27E-002
I-131	Not Detected	-----	4.81E-002
IR-192	Not Detected	-----	2.72E-002
K-40	1.62E+001	2.23E+000	3.30E-001
LN-52	Not Detected	-----	7.77E-002
LN-54	Not Detected	-----	3.32E-002
MO-99	Not Detected	-----	1.40E+000
NA-22	Not Detected	-----	4.57E-002
NA-24	Not Detected	-----	8.97E+001
ND-147	Not Detected	-----	2.92E-001
NI-57	Not Detected	-----	1.46E+000
RU-103	Not Detected	-----	3.20E-002
RU-106	Not Detected	-----	2.72E-001
SB-122	Not Detected	-----	2.27E-001
SB-124	Not Detected	-----	2.94E-002
SB-125	Not Detected	-----	8.14E-002
SN-113	Not Detected	-----	3.87E-002
SR-85	Not Detected	-----	3.67E-002
TA-182	Not Detected	-----	1.74E-001
TA-183	Not Detected	-----	3.59E-001
TL-201	Not Detected	-----	3.68E-001
Y-88	Not Detected	-----	3.18E-002
ZN-65	Not Detected	-----	1.16E-001
ZR-95	Not Detected	-----	6.28E-002

\*\*\*\*\*  
 \* Sandia National Laboratories \*  
 \* Radiation Protection Sample Diagnostics Program \*  
 \* 9/19/02 5:22:21 PM \*  
 \*\*\*\*\*

Analyzed by: *he 9/20/02* Reviewed by: *KA 9/20/02*

Customer : SANDERS, M (6135)  
 Customer Sample ID : 059843-003  
 Lab Sample ID : 20131509

Sample Description : 6721/1090-DF1-BH2-4S  
 Sample Quantity : 684.000 gram  
 Sample Date/Time : 9/13/02 10:14:00 AM  
 Acquire Start Date/Time : 9/19/02 3:41:54 PM  
 Detector Name : LAB02  
 Elapsed Live/Real Time : 6000 / 6002 seconds

Comments:  
 U-235/Ra-226 peaks not resolved. Either isotope may be overestimated.  
 \*\*\*\*\*

Nuclide Name	Activity (pCi/gram)	2-sigma Error	MDA (pCi/gram)
U-238	Not Detected	-----	6.89E-001
RA-226	2.05E+000	5.30E-001	6.51E-001
PB-214	6.93E-001	1.05E-001	6.32E-002
BI-214	6.60E-001	1.06E-001	5.28E-002
PB-210	Not Detected	-----	2.66E+001
TH-232	7.29E-001	3.49E-001	2.01E-001
RA-228	7.33E-001	1.41E-001	1.24E-001
AC-228	6.78E-001	1.33E-001	9.16E-002
TH-228	4.72E-001	4.26E-001	6.73E-001
RA-224	7.59E-001	1.77E-001	8.20E-002
PB-212	7.38E-001	1.08E-001	3.60E-002
BI-212	7.10E-001	2.51E-001	3.20E-001
TL-208	6.42E-001	1.11E-001	7.80E-002
U-235	Not Detected	-----	2.20E-001
TH-231	Not Detected	-----	1.06E+001
PA-231	Not Detected	-----	1.34E+000
TH-227	Not Detected	-----	3.34E-001
RA-223	Not Detected	-----	2.43E-001
RN-219	Not Detected	-----	3.42E-001
PB-211	Not Detected	-----	7.56E-001
TL-207	Not Detected	-----	1.17E+001
AM-241	Not Detected	-----	4.13E-001
PU-239	Not Detected	-----	3.98E+002
NP-237	Not Detected	-----	2.10E+000
PA-233	Not Detected	-----	5.28E-002
TH-229	Not Detected	-----	2.22E-001

[Summary Report] - Sample ID: : 20131509

Nuclide Name	Activity (pCi/gram )	2-sigma Error	MDA (pCi/gram )
G-108m	Not Detected	-----	3.36E-002
AG-110m	Not Detected	-----	2.59E-002
BA-133	Not Detected	-----	4.81E-002
BE-7	Not Detected	-----	2.25E-001
CD-115	Not Detected	-----	4.26E-001
CE-139	Not Detected	-----	2.64E-002
CE-141	Not Detected	-----	5.41E-002
CE-144	Not Detected	-----	2.15E-001
CM-243	Not Detected	-----	1.58E-001
CO-56	Not Detected	-----	2.86E-002
CO-57	Not Detected	-----	2.86E-002
CO-58	Not Detected	-----	3.00E-002
CO-60	Not Detected	-----	3.20E-002
CR-51	Not Detected	-----	2.43E-001
CS-134	Not Detected	-----	3.91E-002
CS-137	Not Detected	-----	2.78E-002
EU-152	Not Detected	-----	8.42E-002
EU-154	Not Detected	-----	1.55E-001
EU-155	Not Detected	-----	1.25E-001
FE-59	Not Detected	-----	6.83E-002
GD-153	Not Detected	-----	9.17E-002
HG-203	Not Detected	-----	3.15E-002
I-131	Not Detected	-----	4.49E-002
IR-192	Not Detected	-----	2.63E-002
K-40	1.51E+001	2.06E+000	2.75E-001
MN-52	Not Detected	-----	5.31E-002
MO-99	Not Detected	-----	2.91E-002
MO-99	Not Detected	-----	9.87E-001
NA-22	Not Detected	-----	3.58E-002
NA-24	Not Detected	-----	2.79E+001
ND-147	Not Detected	-----	2.55E-001
NI-57	Not Detected	-----	7.88E-001
RU-103	Not Detected	-----	2.73E-002
RU-106	Not Detected	-----	2.42E-001
SB-122	Not Detected	-----	1.73E-001
SB-124	Not Detected	-----	2.74E-002
SB-125	Not Detected	-----	7.75E-002
SN-113	Not Detected	-----	3.36E-002
SR-85	Not Detected	-----	3.28E-002
TA-182	Not Detected	-----	1.42E-001
TA-183	Not Detected	-----	8.27E-001
TL-201	Not Detected	-----	6.23E-001
Y-88	Not Detected	-----	2.17E-002
ZN-65	Not Detected	-----	9.16E-002
ZR-95	Not Detected	-----	4.78E-002

\*\*\*\*\*  
 \* Sandia National Laboratories \*  
 \* Radiation Protection Sample Diagnostics Program \*  
 \* 9/19/02 7:22:22 PM \*  
 \*\*\*\*\*

Analyzed by: *[Signature]* 9/20/02 Reviewed by: *[Signature]* 9/20/02  
 \*\*\*\*\*

Customer : SANDERS, M (6135)  
 Customer Sample ID : 059844-003  
 Lab Sample ID : 20131510

Sample Description : 6721/1090-DF1-BH2-9-S  
 Sample Quantity : 785.000 gram  
 Sample Date/Time : 9/13/02 10:35:00 AM  
 Acquire Start Date/Time : 9/19/02 5:24:15 PM  
 Detector Name : LAB02  
 Elapsed Live/Real Time : 6000 / 6003 seconds

Comments:  
 U-235/Ra-226 peaks not resolved. Either isotope may be overestimated.  
 \*\*\*\*\*

Nuclide Name	Activity (pCi/gram)	2-sigma Error	MDA (pCi/gram)
U-238	Not Detected	-----	6.38E-001
RA-226	1.23E+000	4.43E-001	6.20E-001
PB-214	6.81E-001	1.02E-001	6.03E-002
BI-214	6.43E-001	1.02E-001	4.49E-002
PB-210	Not Detected	-----	2.53E+001
H-232	7.42E-001	3.52E-001	1.91E-001
RA-228	6.87E-001	1.31E-001	1.18E-001
AC-228	7.15E-001	1.36E-001	8.95E-002
TH-228	6.85E-001	4.04E-001	6.11E-001
RA-224	8.96E-001	1.94E-001	5.54E-002
PB-212	7.18E-001	1.05E-001	3.53E-002
BI-212	8.45E-001	2.71E-001	3.42E-001
TL-208	6.50E-001	1.10E-001	7.65E-002
U-235	1.44E-001	1.63E-001	2.08E-001
TH-231	Not Detected	-----	1.01E+001
PA-231	Not Detected	-----	1.25E+000
TH-227	Not Detected	-----	3.12E-001
RA-223	Not Detected	-----	2.32E-001
RN-219	Not Detected	-----	3.10E-001
PB-211	Not Detected	-----	6.67E-001
TL-207	Not Detected	-----	1.07E+001
AM-241	Not Detected	-----	3.88E-001
PU-239	Not Detected	-----	3.68E+002
NP-237	Not Detected	-----	1.99E+000
PA-233	Not Detected	-----	4.74E-002
TH-229	Not Detected	-----	2.05E-001



Nuclide Name	Activity (pCi/gram)	2-sigma Error	MDA (pCi/gram)
3-108m	Not Detected	-----	3.05E-002
AG-110m	Not Detected	-----	2.42E-002
BA-133	Not Detected	-----	4.25E-002
BE-7	Not Detected	-----	2.13E-001
CD-115	Not Detected	-----	4.04E-001
CE-139	Not Detected	-----	2.62E-002
CE-141	Not Detected	-----	5.14E-002
CE-144	Not Detected	-----	2.10E-001
CM-243	Not Detected	-----	1.47E-001
CO-56	Not Detected	-----	2.77E-002
CO-57	Not Detected	-----	2.74E-002
CO-58	Not Detected	-----	2.71E-002
CO-60	Not Detected	-----	2.94E-002
CR-51	Not Detected	-----	2.20E-001
CS-134	Not Detected	-----	3.49E-002
CS-137	Not Detected	-----	2.65E-002
EU-152	Not Detected	-----	8.12E-002
EU-154	Not Detected	-----	1.40E-001
EU-155	Not Detected	-----	1.22E-001
FE-59	Not Detected	-----	6.32E-002
GD-153	Not Detected	-----	8.71E-002
HG-203	Not Detected	-----	2.92E-002
I-131	Not Detected	-----	4.06E-002
IR-192	Not Detected	-----	2.36E-002
K-40	1.75E+001	2.35E+000	2.37E-001
MN-52	Not Detected	-----	5.19E-002
MN-54	Not Detected	-----	2.79E-002
MO-99	Not Detected	-----	9.46E-001
NA-22	Not Detected	-----	3.33E-002
NA-24	Not Detected	-----	2.74E+001
ND-147	Not Detected	-----	2.28E-001
NI-57	Not Detected	-----	7.91E-001
RU-103	Not Detected	-----	2.46E-002
RU-106	Not Detected	-----	2.27E-001
SB-122	Not Detected	-----	1.68E-001
SB-124	Not Detected	-----	2.47E-002
SB-125	Not Detected	-----	7.09E-002
SN-113	Not Detected	-----	3.31E-002
SR-85	Not Detected	-----	3.22E-002
TA-182	Not Detected	-----	1.31E-001
TA-183	Not Detected	-----	7.83E-001
TL-201	Not Detected	-----	5.95E-001
Y-88	Not Detected	-----	2.24E-002
ZN-65	Not Detected	-----	8.58E-002
ZR-95	Not Detected	-----	4.57E-002

Analyzed by: *h 9/20/02* Reviewed by: *K 9/20/02*

Customer : SANDERS, M (6135)  
 Customer Sample ID : 059847-003  
 Lab Sample ID : 20131512

Sample Description : 6721/1090-DF1-BH3-4-S  
 Sample Quantity : 822.000 gram  
 Sample Date/Time : 9/13/02 10:50:00 AM  
 Acquire Start Date/Time : 9/19/02 9:06:12 PM  
 Detector Name : LAB02  
 Elapsed Live/Real Time : 6000 / 6003 seconds

Comments:  
 U-235/Ra-226 peaks not resolved. Either isotope may be overestimated.  
 \*\*\*\*\*

Nuclide Name	Activity (pCi/gram)	2-sigma Error	MDA (pCi/gram)
U-238	Not Detected	-----	6.24E-001
RA-226	1.66E+000	4.66E-001	6.01E-001
PB-214	6.06E-001	9.08E-002	5.27E-002
BI-214	4.98E-001	8.25E-002	4.68E-002
PB-210	Not Detected	-----	2.35E+001
H-232	6.90E-001	3.28E-001	1.80E-001
RA-228	7.23E-001	1.32E-001	1.03E-001
AC-228	7.28E-001	1.35E-001	8.32E-002
TH-228	4.07E-001	3.63E-001	5.73E-001
RA-224	7.98E-001	1.76E-001	6.39E-002
PB-212	6.81E-001	9.94E-002	3.35E-002
BI-212	7.37E-001	2.22E-001	2.61E-001
TL-208	5.83E-001	9.82E-002	6.53E-002
U-235	Not Detected	-----	1.94E-001
TH-231	Not Detected	-----	9.38E+000
PA-231	Not Detected	-----	1.11E+000
TH-227	Not Detected	-----	2.96E-001
RA-223	Not Detected	-----	2.15E-001
RN-219	Not Detected	-----	2.88E-001
PB-211	Not Detected	-----	6.63E-001
TL-207	Not Detected	-----	1.03E+001
AM-241	Not Detected	-----	3.53E-001
PU-239	Not Detected	-----	3.48E+002
NP-237	Not Detected	-----	1.87E+000
PA-233	Not Detected	-----	4.57E-002
TH-229	Not Detected	-----	2.01E-001

Nuclide Name	Activity (pCi/gram )	2-sigma Error	MDA (pCi/gram )
AG-108m	Not Detected	-----	2.78E-002
AG-110m	Not Detected	-----	2.27E-002
BA-133	Not Detected	-----	4.00E-002
BE-7	Not Detected	-----	2.09E-001
CD-115	Not Detected	-----	4.02E-001
CE-139	Not Detected	-----	2.34E-002
CE-141	Not Detected	-----	4.84E-002
CE-144	Not Detected	-----	1.91E-001
CM-243	Not Detected	-----	1.39E-001
CO-56	Not Detected	-----	2.75E-002
CO-57	Not Detected	-----	2.54E-002
CO-58	Not Detected	-----	2.64E-002
CO-60	Not Detected	-----	2.80E-002
CR-51	Not Detected	-----	2.13E-001
CS-134	Not Detected	-----	3.27E-002
CS-137	Not Detected	-----	2.52E-002
EU-152	Not Detected	-----	7.53E-002
EU-154	Not Detected	-----	1.28E-001
EU-155	Not Detected	-----	1.14E-001
FE-59	Not Detected	-----	6.15E-002
GD-153	Not Detected	-----	8.35E-002
HG-203	Not Detected	-----	2.71E-002
I-131	Not Detected	-----	3.95E-002
IR-192	Not Detected	-----	2.29E-002
K-40	1.51E+001	2.04E+000	2.20E-001
MN-52	Not Detected	-----	5.53E-002
MN-54	Not Detected	-----	2.74E-002
IO-99	Not Detected	-----	8.59E-001
NA-22	Not Detected	-----	3.17E-002
NA-24	Not Detected	-----	3.15E+001
ND-147	Not Detected	-----	2.13E-001
NI-57	Not Detected	-----	7.50E-001
RU-103	Not Detected	-----	2.45E-002
RU-106	Not Detected	-----	2.08E-001
SB-122	Not Detected	-----	1.58E-001
SB-124	Not Detected	-----	2.47E-002
SB-125	Not Detected	-----	6.62E-002
SN-113	Not Detected	-----	3.08E-002
SR-85	Not Detected	-----	2.99E-002
TA-182	Not Detected	-----	1.23E-001
TA-183	Not Detected	-----	7.27E-001
TL-201	Not Detected	-----	5.72E-001
Y-88	Not Detected	-----	2.12E-002
ZN-65	Not Detected	-----	7.97E-002
ZR-95	Not Detected	-----	4.12E-002

\*\*\*\*\*  
 \* Sandia National Laboratories \*  
 \* Radiation Protection Sample Diagnostics Program \*  
 \* 9/20/02 12:28:33 AM \*  
 \*\*\*\*\*

< Analyzed by: *A 9/20/02* Reviewed by: *[Signature] 9/20/02*  
 \*\*\*\*\*

Customer : SANDERS, M (6135)  
 Customer Sample ID : 059848-003  
 Lab Sample ID : 20131513

Sample Description : 6721/1090-DF1-BH3-9-S  
 Sample Quantity : 744.000 gram  
 Sample Date/Time : 9/13/02 11:10:00 AM  
 Acquire Start Date/Time : 9/19/02 10:48:10 PM  
 Detector Name : LAB02  
 Elapsed Live/Real Time : 6000 / 6003 seconds

Comments:  
 U-235/Ra-226 peaks not resolved. Either isotope may be overestimated.  
 \*\*\*\*\*

Nuclide Name	Activity (pCi/gram)	2-sigma Error	MDA (pCi/gram)
U-238	Not Detected	-----	6.49E-001
RA-226	1.70E+000	4.98E-001	6.53E-001
PB-214	7.47E-001	1.08E-001	5.17E-002
BI-214	6.18E-001	9.90E-002	4.71E-002
PB-210	Not Detected	-----	2.50E+001
TH-232	5.68E-001	2.61E-001	1.24E-001
RA-228	6.87E-001	1.32E-001	1.13E-001
AC-228	6.08E-001	1.22E-001	9.02E-002
TH-228	1.03E+000	4.06E-001	5.65E-001
RA-224	7.82E-001	1.78E-001	7.53E-002
PB-212	6.58E-001	9.69E-002	3.53E-002
BI-212	8.44E-001	2.51E-001	2.95E-001
TL-208	5.89E-001	1.02E-001	7.08E-002
U-235	Not Detected	-----	2.03E-001
TH-231	Not Detected	-----	9.85E+000
PA-231	Not Detected	-----	1.22E+000
TH-227	Not Detected	-----	3.10E-001
RA-223	Not Detected	-----	2.28E-001
RN-219	Not Detected	-----	3.21E-001
PB-211	Not Detected	-----	7.17E-001
TL-207	Not Detected	-----	1.07E+001
AM-241	Not Detected	-----	3.87E-001
PU-239	Not Detected	-----	3.68E+002
NP-237	Not Detected	-----	2.01E+000
PA-233	Not Detected	-----	5.12E-002
TH-229	Not Detected	-----	2.10E-001

[Summary Report] - Sample ID: : 20131513

Nuclide Name	Activity (pCi/gram )	2-sigma Error	MDA (pCi/gram )
AG-108m	Not Detected	-----	2.99E-002
AG-110m	Not Detected	-----	2.37E-002
BA-133	Not Detected	-----	4.44E-002
BE-7	Not Detected	-----	2.16E-001
CD-115	Not Detected	-----	4.25E-001
CE-139	Not Detected	-----	2.63E-002
CE-141	Not Detected	-----	5.06E-002
CE-144	Not Detected	-----	2.04E-001
CM-243	Not Detected	-----	1.48E-001
CO-56	Not Detected	-----	2.89E-002
CO-57	Not Detected	-----	2.63E-002
CO-58	Not Detected	-----	2.66E-002
CO-60	Not Detected	-----	2.84E-002
CR-51	Not Detected	-----	2.24E-001
CS-134	Not Detected	-----	3.54E-002
CS-137	Not Detected	-----	2.51E-002
EU-152	Not Detected	-----	7.83E-002
EU-154	Not Detected	-----	1.38E-001
EU-155	Not Detected	-----	1.21E-001
FE-59	Not Detected	-----	6.66E-002
GD-153	Not Detected	-----	8.86E-002
HG-203	Not Detected	-----	2.96E-002
I-131	Not Detected	-----	4.13E-002
IR-192	Not Detected	-----	2.44E-002
K-40	1.66E+001	2.24E+000	2.63E-001
MN-52	Not Detected	-----	5.85E-002
MN-54	Not Detected	-----	2.91E-002
MO-99	Not Detected	-----	9.82E-001
NA-22	Not Detected	-----	3.18E-002
NA-24	Not Detected	-----	3.86E+001
ND-147	Not Detected	-----	2.29E-001
NI-57	Not Detected	-----	9.21E-001
RU-103	Not Detected	-----	2.62E-002
RU-106	Not Detected	-----	2.23E-001
SB-122	Not Detected	-----	1.69E-001
SB-124	Not Detected	-----	2.47E-002
SB-125	Not Detected	-----	7.23E-002
SN-113	Not Detected	-----	3.14E-002
SR-85	Not Detected	-----	3.22E-002
TA-182	Not Detected	-----	1.34E-001
TA-183	Not Detected	-----	8.03E-001
TL-201	Not Detected	-----	6.15E-001
Y-88	Not Detected	-----	2.15E-002
ZN-65	Not Detected	-----	8.75E-002
ZR-95	Not Detected	-----	4.55E-002

\*\*\*\*\*  
 \* Sandia National Laboratories \*  
 \* Radiation Protection Sample Diagnostics Program \*  
 \* 9/20/02 2:10:34 AM \*  
 \*\*\*\*\*

\* Analyzed by: *A 9/20/02* Reviewed by: *Ka 9/20/02*  
 \*\*\*\*\*

Customer : SANDERS, M (6135)  
 Customer Sample ID : 059850-003  
 Lab Sample ID : 20131514

Sample Description : 6720/1111-SP1-BH1-10-S  
 Sample Quantity : 738.000 gram  
 Sample Date/Time : 9/13/02 8:45:00 AM  
 Acquire Start Date/Time : 9/20/02 12:30:19 AM  
 Detector Name : LAB02  
 Elapsed Live/Real Time : 6000 / 6003 seconds

Comments:  
 U-235/Ra-226 peaks not resolved. Either isotope may be overestimated.  
 \*\*\*\*\*

Nuclide Name	Activity (pCi/gram)	2-sigma Error	MDA (pCi/gram)
U-238	Not Detected	-----	6.67E-001
RA-226	1.78E+000	4.95E-001	6.33E-001
PB-214	6.29E-001	9.56E-002	5.81E-002
BI-214	5.85E-001	9.54E-002	5.02E-002
PB-210	Not Detected	-----	2.54E+001
TH-232	6.20E-001	3.01E-001	1.86E-001
RA-228	8.04E-001	1.45E-001	1.04E-001
AC-228	6.83E-001	1.35E-001	9.86E-002
TH-228	5.72E-001	3.90E-001	6.00E-001
RA-224	7.72E-001	1.77E-001	8.18E-002
PB-212	6.70E-001	9.86E-002	3.61E-002
BI-212	7.94E-001	2.62E-001	3.30E-001
TL-208	6.77E-001	1.16E-001	8.36E-002
U-235	Not Detected	-----	2.05E-001
TH-231	Not Detected	-----	1.03E+001
PA-231	Not Detected	-----	1.24E+000
TH-227	Not Detected	-----	3.14E-001
RA-223	Not Detected	-----	2.41E-001
<del>RN-219</del>	<del>3.94E-001</del>	<del>2.79E-001</del>	<del>3.34E-001</del>
PB-211	Not Detected	-----	7.08E-001
TL-207	Not Detected	-----	1.05E+001
AM-241	Not Detected	-----	3.84E-001
PU-239	Not Detected	-----	3.81E+002
NP-237	Not Detected	-----	2.01E+000
PA-233	Not Detected	-----	4.91E-002
TH-229	Not Detected	-----	2.20E-001

*MS ID. TL 208 2615 KeV NOT DETECTED Ka 9/20/02*

Nuclide Name	Activity (pCi/gram)	2-sigma Error	MDA (pCi/gram)
J-108m	Not Detected	-----	3.10E-002
AG-110m	Not Detected	-----	2.38E-002
BA-133	Not Detected	-----	4.43E-002
BE-7	Not Detected	-----	2.21E-001
CD-115	Not Detected	-----	4.58E-001
CE-139	Not Detected	-----	2.63E-002
CE-141	Not Detected	-----	5.22E-002
CE-144	Not Detected	-----	2.08E-001
CM-243	Not Detected	-----	1.54E-001
CO-56	Not Detected	-----	2.83E-002
CO-57	Not Detected	-----	2.72E-002
CO-58	Not Detected	-----	2.80E-002
CO-60	Not Detected	-----	3.12E-002
CR-51	Not Detected	-----	2.37E-001
CS-134	Not Detected	-----	3.53E-002
CS-137	Not Detected	-----	2.49E-002
EU-152	Not Detected	-----	8.09E-002
EU-154	Not Detected	-----	1.43E-001
EU-155	Not Detected	-----	1.21E-001
FE-59	Not Detected	-----	6.41E-002
GD-153	Not Detected	-----	9.27E-002
HG-203	Not Detected	-----	3.08E-002
I-131	Not Detected	-----	4.47E-002
IR-192	Not Detected	-----	2.47E-002
K-40	1.58E+001	2.14E+000	2.52E-001
MN-52	Not Detected	-----	5.93E-002
N-54	Not Detected	-----	2.93E-002
IO-99	Not Detected	-----	1.01E+000
NA-22	Not Detected	-----	3.55E-002
NA-24	Not Detected	-----	4.38E+001
ND-147	Not Detected	-----	2.34E-001
NI-57	Not Detected	-----	9.69E-001
RU-103	Not Detected	-----	2.61E-002
RU-106	Not Detected	-----	2.20E-001
SB-122	Not Detected	-----	1.79E-001
SB-124	Not Detected	-----	2.41E-002
SB-125	Not Detected	-----	7.27E-002
SN-113	Not Detected	-----	3.17E-002
SR-85	Not Detected	-----	3.33E-002
TA-182	Not Detected	-----	1.33E-001
TA-183	Not Detected	-----	8.15E-001
TL-201	Not Detected	-----	6.35E-001
Y-88	Not Detected	-----	2.25E-002
ZN-65	Not Detected	-----	8.71E-002
ZR-95	Not Detected	-----	4.42E-002

\*\*\*\*\*  
 \* Sandia National Laboratories \*  
 \* Radiation Protection Sample Diagnostics Program \*  
 \* 9/20/02 3:51:31 AM \*  
 \*\*\*\*\*

Analyzed by: *[Signature]* 9/20/02 Reviewed by: *[Signature]* 9/20/02  
 \*\*\*\*\*

Customer : SANDERS, M (6135)  
 Customer Sample ID : 059851-003  
 Lab Sample ID : 20131515

Sample Description : 6720/1111-SP1-BH1-15-S  
 Sample Quantity : 805.000 gram  
 Sample Date/Time : 9/13/02 9:00:00 AM  
 Acquire Start Date/Time : 9/20/02 2:12:17 AM  
 Detector Name : LAB02  
 Elapsed Live/Real Time : 6000 / 6003 seconds

Comments:  
 U-235/Ra-226 peaks not resolved. Either isotope may be overestimated.  
 \*\*\*\*\*

Nuclide Name	Activity (pCi/gram)	2-sigma Error	MDA (pCi/gram)
U-238	Not Detected	-----	5.99E-001
RA-226	1.84E+000	4.81E-001	6.00E-001
PB-214	7.00E-001	1.03E-001	5.47E-002
BI-214	6.17E-001	9.83E-002	4.75E-002
PB-210	Not Detected	-----	2.38E+001
TH-232	4.67E-001	2.40E-001	1.87E-001
RA-228	6.49E-001	1.22E-001	9.50E-002
AC-228	6.04E-001	1.16E-001	7.46E-002
TH-228	3.14E-001	3.73E-001	5.99E-001
RA-224	7.44E-001	1.68E-001	6.77E-002
PB-212	6.23E-001	9.15E-002	3.27E-002
BI-212	7.33E-001	2.59E-001	3.39E-001
TL-208	5.45E-001	9.40E-002	6.58E-002
U-235	Not Detected	-----	2.01E-001
TH-231	Not Detected	-----	9.48E+000
PA-231	Not Detected	-----	1.12E+000
TH-227	Not Detected	-----	2.87E-001
RA-223	Not Detected	-----	2.26E-001
RN-219	Not Detected	-----	3.06E-001
PB-211	Not Detected	-----	6.81E-001
TL-207	Not Detected	-----	1.05E+001
AM-241	Not Detected	-----	3.69E-001
PU-239	Not Detected	-----	3.58E+002
NP-237	Not Detected	-----	1.89E+000
PA-233	Not Detected	-----	4.63E-002
TH-229	Not Detected	-----	1.99E-001



[Summary Report] - Sample ID: : 20131515

Nuclide Name	Activity (pCi/gram )	2-sigma Error	MDA (pCi/gram )
AG-108m	Not Detected	-----	2.87E-002
AG-110m	Not Detected	-----	2.28E-002
BA-133	Not Detected	-----	4.24E-002
BE-7	Not Detected	-----	2.06E-001
CD-115	Not Detected	-----	4.15E-001
CE-139	Not Detected	-----	2.48E-002
CE-141	Not Detected	-----	4.98E-002
CE-144	Not Detected	-----	1.97E-001
CM-243	Not Detected	-----	1.39E-001
CO-56	Not Detected	-----	2.79E-002
CO-57	Not Detected	-----	2.64E-002
CO-58	Not Detected	-----	2.63E-002
CO-60	Not Detected	-----	2.81E-002
CR-51	Not Detected	-----	2.14E-001
CS-134	Not Detected	-----	3.39E-002
CS-137	Not Detected	-----	2.50E-002
EU-152	Not Detected	-----	7.81E-002
EU-154	Not Detected	-----	1.32E-001
EU-155	Not Detected	-----	1.14E-001
FE-59	Not Detected	-----	5.70E-002
GD-153	Not Detected	-----	8.61E-002
HG-203	Not Detected	-----	2.73E-002
I-131	Not Detected	-----	4.06E-002
IR-192	Not Detected	-----	2.26E-002
K-40	1.42E+001	1.92E+000	2.28E-001
MN-52	Not Detected	-----	5.25E-002
MN-54	Not Detected	-----	2.75E-002
MO-99	Not Detected	-----	9.26E-001
NA-22	Not Detected	-----	3.37E-002
NA-24	Not Detected	-----	4.45E+001
ND-147	Not Detected	-----	2.33E-001
NI-57	Not Detected	-----	9.31E-001
RU-103	Not Detected	-----	2.41E-002
RU-106	Not Detected	-----	2.14E-001
SB-122	Not Detected	-----	1.77E-001
SB-124	Not Detected	-----	2.44E-002
SB-125	Not Detected	-----	6.66E-002
SN-113	Not Detected	-----	3.03E-002
SR-85	Not Detected	-----	2.89E-002
TA-182	Not Detected	-----	1.27E-001
TA-183	Not Detected	-----	7.90E-001
TL-201	Not Detected	-----	6.21E-001
Y-88	Not Detected	-----	2.02E-002
ZN-65	Not Detected	-----	8.18E-002
ZR-95	Not Detected	-----	4.45E-002

\*\*\*\*\*  
 \* Sandia National Laboratories \*  
 \* Radiation Protection Sample Diagnostics Program \*  
 \* 9/20/02 5:33:30 AM \*  
 \*\*\*\*\*

\* Analyzed by: *[Signature]* 9/20/02 Reviewed by: *[Signature]* 9/20/02 \*  
 \*\*\*\*\*

Customer : SANDERS, M (6135)  
 Customer Sample ID : 059852-003  
 Lab Sample ID : 20131516

Sample Description : 6743/1087-SP1-BH1-8-S  
 Sample Quantity : 832.000 gram  
 Sample Date/Time : 9/17/02 10:12:00 AM  
 Acquire Start Date/Time : 9/20/02 3:53:15 AM  
 Detector Name : LAB02  
 Elapsed Live/Real Time : 6000 / 6003 seconds

Comments:  
 U-235/Ra-226 peaks not resolved. Either isotope may be overestimated.  
 \*\*\*\*\*

Nuclide Name	Activity (pCi/gram)	2-sigma Error	MDA (pCi/gram)
U-238	Not Detected	-----	6.21E-001
RA-226	1.61E+000	4.74E-001	6.24E-001
PB-214	6.02E-001	9.15E-002	5.76E-002
BI-214	5.46E-001	8.83E-002	4.53E-002
PB-210	Not Detected	-----	2.35E+001
H-232	6.87E-001	3.23E-001	1.66E-001
RA-228	7.79E-001	1.38E-001	9.72E-002
AC-228	6.73E-001	1.28E-001	8.64E-002
TH-228	6.64E-001	3.60E-001	5.37E-001
RA-224	7.83E-001	1.72E-001	5.79E-002
PB-212	6.98E-001	1.02E-001	3.25E-002
BI-212	8.54E-001	2.54E-001	3.06E-001
TL-208	5.87E-001	9.87E-002	6.58E-002
U-235	7.83E-002	1.49E-001	1.90E-001
TH-231	Not Detected	-----	9.59E+000
PA-231	Not Detected	-----	1.16E+000
TH-227	Not Detected	-----	2.98E-001
RA-223	Not Detected	-----	1.43E-001
RN-219	Not Detected	-----	2.97E-001
PB-211	Not Detected	-----	6.82E-001
TL-207	Not Detected	-----	1.05E+001
AM-241	Not Detected	-----	3.53E-001
PU-239	Not Detected	-----	3.55E+002
NP-237	Not Detected	-----	1.90E+000
PA-233	Not Detected	-----	4.58E-002
TH-229	Not Detected	-----	2.01E-001

[Summary Report] - Sample ID: : 20131516

Nuclide Name	Activity (pCi/gram )	2-sigma Error	MDA (pCi/gram )
AG-108m	Not Detected	-----	2.81E-002
AG-110m	Not Detected	-----	2.20E-002
BA-133	Not Detected	-----	4.10E-002
BE-7	Not Detected	-----	1.81E-001
CD-115	Not Detected	-----	1.24E-001
CE-139	Not Detected	-----	2.35E-002
CE-141	Not Detected	-----	4.34E-002
CE-144	Not Detected	-----	1.91E-001
CM-243	Not Detected	-----	1.44E-001
CO-56	Not Detected	-----	2.47E-002
CO-57	Not Detected	-----	2.54E-002
CO-58	Not Detected	-----	2.33E-002
CO-60	Not Detected	-----	2.81E-002
CR-51	Not Detected	-----	1.98E-001
CS-134	Not Detected	-----	3.22E-002
CS-137	Not Detected	-----	2.39E-002
EU-152	Not Detected	-----	7.59E-002
EU-154	Not Detected	-----	1.29E-001
EU-155	Not Detected	-----	1.11E-001
FE-59	Not Detected	-----	5.32E-002
GD-153	Not Detected	-----	8.35E-002
HG-203	Not Detected	-----	2.69E-002
I-131	Not Detected	-----	2.72E-002
IR-192	Not Detected	-----	2.15E-002
K-40	1.45E+001	1.96E+000	2.39E-001
LN-52	Not Detected	-----	3.32E-002
LN-54	Not Detected	-----	1.33E-002
MO-99	Not Detected	-----	3.37E-001
NA-22	Not Detected	-----	3.17E-002
NA-24	Not Detected	-----	5.37E-001
ND-147	Not Detected	-----	1.68E-001
NI-57	Not Detected	-----	9.31E-002
RU-103	Not Detected	-----	2.30E-002
RU-106	Not Detected	-----	2.20E-001
SB-122	Not Detected	-----	6.01E-002
SB-124	Not Detected	-----	2.27E-002
SB-125	Not Detected	-----	6.58E-002
SN-113	Not Detected	-----	2.98E-002
SR-85	Not Detected	-----	2.89E-002
TA-182	Not Detected	-----	1.18E-001
TA-183	Not Detected	-----	4.40E-001
TL-201	Not Detected	-----	2.50E-001
Y-88	Not Detected	-----	2.17E-002
ZN-65	Not Detected	-----	7.72E-002
ZR-95	Not Detected	-----	4.29E-002

\*\*\*\*\*  
 \* Sandia National Laboratories \*  
 \* Radiation Protection Sample Diagnostics Program \*  
 \* 9/20/02 7:41:53 AM \*  
 \*\*\*\*\*

\* Analyzed by: *lr 9/20/02* Reviewed by: *K 9/20/02* \*  
 \*\*\*\*\*

Customer : SANDERS, M (6135)  
 Customer Sample ID : 059853-003  
 Lab Sample ID : 20131517

Sample Description : 6743/1087-SP1-BH1-13-S  
 Sample Quantity : 779.000 gram  
 Sample Date/Time : 9/17/02 10:42:00 AM  
 Acquire Start Date/Time : 9/20/02 5:35:13 AM  
 Detector Name : LAB02  
 Elapsed Live/Real Time : 6000 / 6003 seconds

Comments:  
 U-235/Ra-226 peaks not resolved. Either isotope may be overestimated.  
 \*\*\*\*\*

Nuclide Name	Activity (pCi/gram)	2-sigma Error	MDA (pCi/gram)
U-238	Not Detected	-----	6.29E-001
RA-226	1.70E+000	4.93E-001	6.46E-001
PB-214	7.12E-001	1.04E-001	5.22E-002
BI-214	5.75E-001	9.36E-002	4.99E-002
PB-210	Not Detected	-----	2.52E+001
TH-232	7.48E-001	3.55E-001	1.96E-001
RA-228	6.58E-001	1.26E-001	1.10E-001
AC-228	7.26E-001	1.33E-001	7.27E-002
TH-228	1.01E+000	4.00E-001	5.60E-001
RA-224	8.62E-001	1.88E-001	5.62E-002
PB-212	7.39E-001	1.08E-001	3.45E-002
BI-212	7.28E-001	2.77E-001	3.74E-001
TL-208	6.48E-001	1.08E-001	6.89E-002
U-235	Not Detected	-----	2.05E-001
TH-231	Not Detected	-----	1.01E+001
PA-231	Not Detected	-----	1.18E+000
TH-227	Not Detected	-----	3.15E-001
RA-223	Not Detected	-----	1.88E-001
RN-219	Not Detected	-----	3.12E-001
PB-211	Not Detected	-----	7.08E-001
TL-207	Not Detected	-----	1.06E+001
AM-241	Not Detected	-----	3.72E-001
PU-239	Not Detected	-----	3.64E+002
NP-237	Not Detected	-----	1.96E+000
PA-233	Not Detected	-----	4.88E-002
TH-229	Not Detected	-----	2.08E-001

[Summary Report] - Sample ID: : 20131517

Nuclide Name	Activity (pCi/gram )	2-sigma Error	MDA (pCi/gram )
AG-108m	Not Detected	-----	3.04E-002
AG-110m	Not Detected	-----	2.33E-002
BA-133	Not Detected	-----	4.31E-002
BE-7	8.77E-002	8.53E-002	1.34E-001
CD-115	Not Detected	-----	1.35E-001
CE-139	Not Detected	-----	2.51E-002
CE-141	Not Detected	-----	4.66E-002
CE-144	Not Detected	-----	2.00E-001
CM-243	Not Detected	-----	1.47E-001
CO-56	Not Detected	-----	2.81E-002
CO-57	Not Detected	-----	2.64E-002
CO-58	Not Detected	-----	2.70E-002
CO-60	Not Detected	-----	2.93E-002
CR-51	Not Detected	-----	1.98E-001
CS-134	Not Detected	-----	3.48E-002
CS-137	Not Detected	-----	2.53E-002
EU-152	Not Detected	-----	7.89E-002
EU-154	Not Detected	-----	1.40E-001
EU-155	Not Detected	-----	1.18E-001
FE-59	Not Detected	-----	5.74E-002
GD-153	Not Detected	-----	8.60E-002
HG-203	Not Detected	-----	2.74E-002
I-131	Not Detected	-----	2.86E-002
IR-192	Not Detected	-----	2.29E-002
K-40	1.42E+001	1.92E+000	2.19E-001
MN-52	Not Detected	-----	3.33E-002
MN-54	Not Detected	-----	2.73E-002
MO-99	Not Detected	-----	3.53E-001
NA-22	Not Detected	-----	3.22E-002
NA-24	Not Detected	-----	6.36E-001
ND-147	Not Detected	-----	1.84E-001
NI-57	Not Detected	-----	8.83E-002
RU-103	Not Detected	-----	2.29E-002
RU-106	Not Detected	-----	2.17E-001
SB-122	Not Detected	-----	6.34E-002
SB-124	Not Detected	-----	2.49E-002
SB-125	Not Detected	-----	6.89E-002
SN-113	Not Detected	-----	3.18E-002
SR-85	Not Detected	-----	3.04E-002
TA-182	Not Detected	-----	1.23E-001
TA-183	Not Detected	-----	4.67E-001
TL-201	Not Detected	-----	2.59E-001
Y-88	Not Detected	-----	2.08E-002
ZN-65	Not Detected	-----	8.09E-002
ZR-95	Not Detected	-----	4.23E-002

*art. font BCC*

\*\*\*\*\*  
 \* Sandia National Laboratories \*  
 \* Radiation Protection Sample Diagnostics Program \*  
 \* 9/20/02 9:26:50 AM \*  
 \*\*\*\*\*

\* Analyzed by: *[Signature]* 9/24/02 Reviewed by: *[Signature]* 9/20/02 \*  
 \*\*\*\*\*

Customer : SANDERS, M (6135)  
 Customer Sample ID : 059854-003  
 Lab Sample ID : 20131518

Sample Description : 6734/1089-SP1-BH1-9-S  
 Sample Quantity : 741.000 gram  
 Sample Date/Time : 9/17/02 12:40:00 PM  
 Acquire Start Date/Time : 9/20/02 7:54:59 AM  
 Detector Name : LAB02  
 Elapsed Live/Real Time : 6000 / 6002 seconds

Comments:  
 U-235/Ra-226 peaks not resolved. Either isotope may be overestimated.  
 \*\*\*\*\*

Nuclide Name	Activity (pCi/gram)	2-sigma Error	MDA (pCi/gram)
U-238	Not Detected	-----	5.38E-001
RA-226	1.26E+000	4.02E-001	5.37E-001
PB-214	4.05E-001	6.75E-002	5.00E-002
BI-214	3.81E-001	6.65E-002	4.04E-002
PB-210	Not Detected	-----	2.12E+001
H-232	4.69E-001	2.35E-001	1.65E-001
RA-228	3.07E-001	1.02E-001	1.25E-001
AC-228	Not Detected	-----	1.38E-001
TH-228	Not Detected	-----	5.48E-001
RA-224	4.79E-001	1.24E-001	7.66E-002
PB-212	4.37E-001	6.68E-002	3.03E-002
BI-212	5.20E-001	1.93E-001	2.44E-001
TL-208	3.98E-001	7.69E-002	6.41E-002
U-235	Not Detected	-----	1.77E-001
TH-231	Not Detected	-----	8.38E+000
PA-231	Not Detected	-----	1.12E+000
TH-227	Not Detected	-----	2.58E-001
RA-223	Not Detected	-----	1.56E-001
RN-219	Not Detected	-----	2.64E-001
PB-211	Not Detected	-----	6.13E-001
TL-207	Not Detected	-----	9.83E+000
AM-241	Not Detected	-----	3.22E-001
PU-239	Not Detected	-----	3.18E+002
NP-237	Not Detected	-----	1.70E+000
PA-233	Not Detected	-----	4.14E-002
TH-229	Not Detected	-----	1.78E-001

[Summary Report] - Sample ID: : 20131518

Nuclide Name	Activity (pCi/gram )	2-sigma Error	MDA (pCi/gram )
AG-108m	Not Detected	-----	2.58E-002
AG-110m	Not Detected	-----	2.05E-002
BA-133	Not Detected	-----	3.69E-002
BE-7	Not Detected	-----	1.73E-001
CD-115	Not Detected	-----	1.14E-001
CE-139	Not Detected	-----	2.20E-002
CE-141	Not Detected	-----	4.08E-002
CE-144	Not Detected	-----	1.71E-001
CM-243	Not Detected	-----	1.22E-001
CO-56	Not Detected	-----	2.50E-002
CO-57	Not Detected	-----	2.24E-002
CO-58	Not Detected	-----	2.54E-002
CO-60	Not Detected	-----	2.71E-002
CR-51	Not Detected	-----	1.75E-001
CS-134	Not Detected	-----	2.93E-002
CS-137	Not Detected	-----	2.17E-002
EU-152	Not Detected	-----	6.74E-002
EU-154	Not Detected	-----	1.19E-001
EU-155	Not Detected	-----	1.03E-001
FE-59	Not Detected	-----	5.34E-002
GD-153	Not Detected	-----	7.60E-002
HG-203	Not Detected	-----	2.40E-002
I-131	Not Detected	-----	2.63E-002
IR-192	Not Detected	-----	1.96E-002
K-40	1.35E+001	1.84E+000	2.27E-001
LN-52	Not Detected	-----	3.33E-002
LN-54	Not Detected	-----	2.42E-002
MO-99	Not Detected	-----	3.44E-001
NA-22	Not Detected	-----	3.21E-002
NA-24	Not Detected	-----	5.17E-001
ND-147	Not Detected	-----	1.72E-001
NI-57	Not Detected	-----	6.86E-002
RU-103	Not Detected	-----	2.06E-002
RU-106	Not Detected	-----	1.99E-001
SB-122	Not Detected	-----	5.72E-002
SB-124	Not Detected	-----	2.16E-002
SB-125	Not Detected	-----	5.94E-002
SN-113	Not Detected	-----	2.64E-002
SR-85	Not Detected	-----	2.79E-002
TA-182	Not Detected	-----	1.05E-001
TA-183	Not Detected	-----	4.04E-001
TL-201	Not Detected	-----	2.23E-001
Y-88	Not Detected	-----	2.11E-002
ZN-65	Not Detected	-----	7.17E-002
ZR-95	Not Detected	-----	3.96E-002

\*\*\*\*\*  
 \* Sandia National Laboratories \*  
 \* Radiation Protection Sample Diagnostics Program \*  
 \* 9/20/02 11:08:49 AM \*  
 \*\*\*\*\*

\* Analyzed by: *hr 9/20/02* Reviewed by: *K 9/20/02* \*  
 \*\*\*\*\*

Customer : SANDERS, M (6135)  
 Customer Sample ID : 059855-003  
 Lab Sample ID : 20131519

Sample Description : 6734/1089-SP1-BH1-14-S  
 Sample Quantity : 819.000 gram  
 Sample Date/Time : 9/17/02 12:45:00 PM  
 Acquire Start Date/Time : 9/20/02 9:28:34 AM  
 Detector Name : LAB02  
 Elapsed Live/Real Time : 6000 / 6002 seconds

Comments:  
 U-235/Ra-226 peaks not resolved. Either isotope may be overestimated.  
 \*\*\*\*\*

Nuclide Name	Activity (pCi/gram)	2-sigma Error	MDA (pCi/gram)
U-238	Not Detected	-----	5.31E-001
RA-226	8.15E-001	3.79E-001	5.60E-001
PB-214	4.44E-001	7.06E-002	4.77E-002
BI-214	3.63E-001	6.41E-002	4.26E-002
PB-210	Not Detected	-----	1.97E+001
H-232	5.04E-001	2.40E-001	1.29E-001
RA-228	4.16E-001	9.14E-002	9.89E-002
AC-228	4.70E-001	9.55E-002	6.69E-002
TH-228	3.50E-001	1.45E-001	2.78E-001
RA-224	5.38E-001	1.32E-001	7.45E-002
PB-212	4.82E-001	7.23E-002	2.80E-002
BI-212	4.94E-001	2.14E-001	2.96E-001
TL-208	4.15E-001	7.54E-002	5.62E-002
U-235	Not Detected	-----	1.72E-001
TH-231	Not Detected	-----	8.54E+000
PA-231	Not Detected	-----	1.03E+000
TH-227	Not Detected	-----	2.55E-001
RA-223	Not Detected	-----	1.58E-001
RN-219	Not Detected	-----	2.60E-001
PB-211	Not Detected	-----	6.04E-001
TL-207	Not Detected	-----	8.70E+000
AM-241	Not Detected	-----	3.07E-001
PU-239	Not Detected	-----	3.13E+002
NP-237	Not Detected	-----	1.68E+000
PA-233	Not Detected	-----	4.10E-002
TH-229	Not Detected	-----	1.82E-001



Nuclide Name	Activity (pCi/gram )	2-sigma Error	MDA (pCi/gram )
AG-108m	Not Detected	-----	2.56E-002
AG-110m	Not Detected	-----	2.04E-002
BA-133	Not Detected	-----	3.46E-002
BE-7	Not Detected	-----	1.82E-001
CD-115	Not Detected	-----	1.14E-001
CE-139	Not Detected	-----	2.09E-002
CE-141	Not Detected	-----	3.93E-002
CE-144	Not Detected	-----	1.67E-001
CM-243	Not Detected	-----	1.24E-001
CO-56	Not Detected	-----	2.34E-002
CO-57	Not Detected	-----	2.23E-002
CO-58	Not Detected	-----	2.32E-002
CO-60	Not Detected	-----	2.59E-002
CR-51	Not Detected	-----	1.80E-001
CS-134	Not Detected	-----	2.84E-002
CS-137	Not Detected	-----	2.22E-002
EU-152	Not Detected	-----	6.72E-002
EU-154	Not Detected	-----	1.18E-001
EU-155	Not Detected	-----	1.01E-001
FE-59	Not Detected	-----	5.22E-002
GD-153	Not Detected	-----	7.37E-002
HG-203	Not Detected	-----	2.35E-002
I-131	Not Detected	-----	2.49E-002
IR-192	Not Detected	-----	1.98E-002
K-40	1.38E+001	1.87E+000	2.01E-001
MN-52	Not Detected	-----	3.06E-002
MN-54	Not Detected	-----	2.37E-002
MO-99	Not Detected	-----	3.23E-001
NA-22	Not Detected	-----	2.89E-002
NA-24	Not Detected	-----	5.48E-001
ND-147	Not Detected	-----	1.63E-001
NI-57	Not Detected	-----	9.85E-002
RU-103	Not Detected	-----	2.09E-002
RU-106	Not Detected	-----	1.99E-001
SB-122	Not Detected	-----	6.01E-002
SB-124	Not Detected	-----	2.10E-002
SB-125	Not Detected	-----	6.04E-002
SN-113	Not Detected	-----	2.63E-002
SR-85	Not Detected	-----	2.59E-002
TA-182	Not Detected	-----	1.10E-001
TA-183	Not Detected	-----	3.89E-001
TL-201	Not Detected	-----	2.23E-001
Y-88	Not Detected	-----	1.75E-002
ZN-65	Not Detected	-----	6.98E-002
ZR-95	Not Detected	-----	3.96E-002

\*\*\*\*\*  
 \* Sandia National Laboratories \*  
 \* Radiation Protection Sample Diagnostics Program \*  
 \* 9/19/02 9:04:28 PM \*  
 \*\*\*\*\*

\* Analyzed by: *Ar 9/20/02* Reviewed by: *Ar 9/20/02* \*  
 \*\*\*\*\*

Customer : SANDERS, M (6135)  
 Customer Sample ID : 059859-001  
 Lab Sample ID : 20131511

Sample Description : 6721/1090-DF1-BH2-4-DU  
 Sample Quantity : 704.000 gram  
 Sample Date/Time : 9/13/02 10:16:00 AM  
 Acquire Start Date/Time : 9/19/02 7:24:13 PM  
 Detector Name : LAB02  
 Elapsed Live/Real Time : 6000 / 6002 seconds

Comments:  
 U-235/Ra-226 peaks not resolved. Either isotope may be overestimated.

\*\*\*\*\*

Nuclide Name	Activity (pCi/gram)	2-sigma Error	MDA (pCi/gram)
U-238	Not Detected	-----	6.52E-001
RA-226	1.88E+000	5.17E-001	6.59E-001
PB-214	6.94E-001	1.04E-001	5.98E-002
BI-214	5.82E-001	9.55E-002	5.14E-002
PB-210	Not Detected	-----	2.61E+001
TH-232	7.71E-001	3.63E-001	1.83E-001
RA-228	7.85E-001	1.44E-001	1.05E-001
AC-228	6.86E-001	1.39E-001	1.09E-001
TH-228	5.86E-001	3.95E-001	6.07E-001
RA-224	8.47E-001	1.89E-001	6.18E-002
PB-212	7.02E-001	1.03E-001	3.55E-002
BI-212	6.12E-001	2.63E-001	3.64E-001
TL-208	6.17E-001	1.07E-001	7.51E-002
U-235	Not Detected	-----	2.07E-001
TH-231	Not Detected	-----	1.05E+001
PA-231	Not Detected	-----	1.23E+000
TH-227	Not Detected	-----	3.20E-001
RA-223	Not Detected	-----	2.47E-001
RN-219	Not Detected	-----	3.40E-001
PB-211	Not Detected	-----	7.56E-001
TL-207	Not Detected	-----	1.18E+001
AM-241	Not Detected	-----	3.83E-001
PU-239	Not Detected	-----	3.87E+002
NP-237	Not Detected	-----	2.02E+000
PA-233	Not Detected	-----	5.24E-002
TH-229	Not Detected	-----	2.19E-001

[Summary Report] - Sample ID: : 20131511

Slide Name	Activity (pCi/gram )	2-sigma Error	MDA (pCi/gram )
AG-108m	Not Detected	-----	3.12E-002
AG-110m	Not Detected	-----	2.60E-002
BA-133	Not Detected	-----	4.68E-002
BE-7	Not Detected	-----	2.15E-001
CD-115	Not Detected	-----	4.26E-001
CE-139	Not Detected	-----	2.67E-002
CE-141	Not Detected	-----	5.18E-002
CE-144	Not Detected	-----	2.06E-001
CM-243	Not Detected	-----	1.54E-001
CO-56	Not Detected	-----	3.02E-002
CO-57	Not Detected	-----	2.77E-002
CO-58	Not Detected	-----	2.80E-002
CO-60	Not Detected	-----	3.08E-002
CR-51	Not Detected	-----	2.30E-001
CS-134	Not Detected	-----	3.68E-002
CS-137	Not Detected	-----	2.92E-002
EU-152	Not Detected	-----	8.25E-002
EU-154	Not Detected	-----	1.43E-001
EU-155	Not Detected	-----	1.23E-001
FE-59	Not Detected	-----	6.27E-002
GD-153	Not Detected	-----	9.16E-002
HG-203	Not Detected	-----	3.01E-002
I-131	Not Detected	-----	4.28E-002
IR-192	Not Detected	-----	2.51E-002
40	1.56E+001	2.12E+000	2.81E-001
N-52	Not Detected	-----	5.22E-002
N-54	Not Detected	-----	1.79E-002
MO-99	Not Detected	-----	1.02E+000
NA-22	Not Detected	-----	3.37E-002
NA-24	Not Detected	-----	3.44E+001
ND-147	Not Detected	-----	2.32E-001
NI-57	Not Detected	-----	8.57E-001
RU-103	Not Detected	-----	2.68E-002
RU-106	Not Detected	-----	2.37E-001
SB-122	Not Detected	-----	1.77E-001
SB-124	Not Detected	-----	2.64E-002
SB-125	Not Detected	-----	7.34E-002
SN-113	Not Detected	-----	3.40E-002
SR-85	Not Detected	-----	3.21E-002
TA-182	Not Detected	-----	1.36E-001
TA-183	Not Detected	-----	7.83E-001
TL-201	Not Detected	-----	6.14E-001
Y-88	Not Detected	-----	2.44E-002
ZN-65	Not Detected	-----	8.81E-002
ZR-95	Not Detected	-----	4.86E-002

\*\*\*\*\*  
 \* Sandia National Laboratories \*  
 \* Radiation Protection Sample Diagnostics Program \*  
 \* 9/20/02 1:05:56 PM \*  
 \*\*\*\*\*

\* Analyzed by: *me* 9/20/02 Reviewed by: *[Signature]* 9/20/02 \*  
 \*\*\*\*\*

Customer : SANDERS, M (6135)  
 Customer Sample ID : LAB\_CONTROL\_SAMPLE\_USING\_CG-134  
 Lab Sample ID : 20131520

Sample Description : MIXED GAMMA STANDARD\_CG-134  
 Sample Quantity : 1.000 Each  
 Sample Date/Time : 11/1/90 12:00:00 PM  
 Acquire Start Date/Time : 9/20/02 12:55:40 PM  
 Detector Name : LAB01  
 Elapsed Live/Real Time : 600 / 604 seconds

Comments:

\*\*\*\*\*

Nuclide Name	Activity (pCi/Each)	2-sigma Error	MDA (pCi/Each)
U-238	Not Detected	-----	2.58E+003
RA-226	Not Detected	-----	5.57E+003
PB-214	Not Detected	-----	6.83E+002
BI-214	Not Detected	-----	5.84E+002
PB-210	Not Detected	-----	9.61E+004
H-232	Not Detected	-----	2.14E+003
LA-228	Not Detected	-----	2.48E+003
AC-228	Not Detected	-----	1.51E+003
TH-228	Not Detected	-----	4.67E+005
RA-224	Not Detected	-----	2.33E+004
PB-212	Not Detected	-----	3.43E+004
BI-212	Not Detected	-----	3.03E+005
TL-208	Not Detected	-----	6.67E+004
U-235	Not Detected	-----	1.36E+003
TH-231	Not Detected	-----	4.04E+004
PA-231	Not Detected	-----	1.38E+004
TH-227	Not Detected	-----	2.59E+003
RA-223	Not Detected	-----	1.00E+026
RN-219	Not Detected	-----	6.60E+003
PB-211	Not Detected	-----	1.49E+004
TL-207	Not Detected	-----	2.30E+005
AM-241	8.99E+004	1.30E+004	1.88E+003
PU-239	Not Detected	-----	2.40E+006
NP-237	Not Detected	-----	1.24E+004
PA-233	Not Detected	-----	5.92E+002
TH-229	Not Detected	-----	1.29E+003

[Summary Report] - Sample ID: : 20131520

Nuclide Name	Activity (pCi/Each )	2-sigma Error	MDA (pCi/Each )
AG-108m	Not Detected	-----	3.10E+002
AG-110m	Not Detected	-----	2.72E+008
BA-133	Not Detected	-----	9.38E+002
BE-7	Not Detected	-----	1.00E+026
CD-115	Not Detected	-----	1.00E+026
CE-139	Not Detected	-----	5.53E+011
CE-141	Not Detected	-----	1.00E+026
CE-144	Not Detected	-----	5.21E+007
CM-243	Not Detected	-----	2.10E+003
CO-56	Not Detected	-----	2.89E+019
CO-57	Not Detected	-----	1.09E+007
CO-58	Not Detected	-----	7.73E+020
CO-60	7.81E+004	1.03E+004	8.15E+002
CR-51	Not Detected	-----	1.00E+026
CS-134	Not Detected	-----	1.53E+004
CS-137	6.88E+004	8.74E+003	3.92E+002
EU-152	Not Detected	-----	9.42E+002
EU-154	Not Detected	-----	3.52E+003
EU-155	Not Detected	-----	4.23E+003
FE-59	Not Detected	-----	1.00E+026
GD-153	Not Detected	-----	1.08E+008
HG-203	Not Detected	-----	1.00E+026
I-131	Not Detected	-----	1.00E+026
IR-192	Not Detected	-----	1.38E+020
K-40	Not Detected	-----	1.37E+003
LN-52	Not Detected	-----	1.00E+026
LN-54	Not Detected	-----	4.99E+006
MO-99	Not Detected	-----	1.00E+026
NA-22	Not Detected	-----	4.94E+003
NA-24	Not Detected	-----	1.00E+026
ND-147	Not Detected	-----	1.00E+026
NI-57	Not Detected	-----	1.00E+026
RU-103	Not Detected	-----	1.00E+026
RU-106	Not Detected	-----	9.18E+006
SB-122	Not Detected	-----	1.00E+026
SB-124	Not Detected	-----	1.00E+026
SB-125	Not Detected	-----	2.38E+004
SN-113	Not Detected	-----	1.03E+014
SR-85	Not Detected	-----	1.00E+026
TA-182	Not Detected	-----	2.57E+014
TA-183	Not Detected	-----	1.00E+026
TL-201	Not Detected	-----	1.00E+026
Y-88	Not Detected	-----	3.07E+014
ZN-65	Not Detected	-----	1.95E+008
ZR-95	Not Detected	-----	1.00E+026



\*\*\*\*\*  
 \* Sandia National Laboratories \*  
 \* Radiation Protection Sample Diagnostics Program \*  
 \* 9/20/02 12:39:50 PM \*  
 \*\*\*\*\*

\* Analyzed by: *h 9/20/02* Reviewed by: *K 9/20/02*  
 \*\*\*\*\*

Customer : SANDERS, M (6135)  
 Customer Sample ID : LAB\_CONTROL\_SAMPLE\_USING\_CG-134  
 Lab Sample ID : 20131521

Sample Description : MIXED\_GAMMA\_STANDARD\_CG-134  
 Sample Quantity : 1.000 Each  
 Sample Date/Time : 11/01/90 12:00:00 PM  
 Acquire Start Date/Time : 9/20/02 12:29:34 PM  
 Detector Name : LAB02  
 Elapsed Live/Real Time : 600 / 604 seconds

Comments:

\*\*\*\*\*

Nuclide Name	Activity (pCi/Each)	2-sigma Error	MDA (pCi/Each)
U-238	Not Detected	-----	3.92E+003
RA-226	Not Detected	-----	5.81E+003
PB-214	Not Detected	-----	5.77E+002
BI-214	Not Detected	-----	4.78E+002
PB-210	Not Detected	-----	2.63E+005
H-232	Not Detected	-----	1.83E+003
RA-228	Not Detected	-----	1.76E+003
AC-228	Not Detected	-----	1.04E+003
TH-228	Not Detected	-----	4.28E+005
RA-224	Not Detected	-----	1.70E+004
PB-212	Not Detected	-----	3.27E+004
BI-212	Not Detected	-----	2.28E+005
TL-208	Not Detected	-----	5.28E+004
U-235	Not Detected	-----	1.46E+003
TH-231	Not Detected	-----	7.07E+004
PA-231	Not Detected	-----	1.23E+004
TH-227	Not Detected	-----	2.50E+003
RA-223	Not Detected	-----	1.00E+026
RN-219	Not Detected	-----	5.58E+003
PB-211	Not Detected	-----	1.28E+004
TL-207	Not Detected	-----	1.69E+005
AM-241	8.08E+004	1.20E+004	4.04E+003
PU-239	Not Detected	-----	2.69E+006
NP-237	Not Detected	-----	1.44E+004
PA-233	Not Detected	-----	5.19E+002
TH-229	Not Detected	-----	1.49E+003

[Summary Report] - Sample ID: : 20131521

Nuclide Name	Activity (pCi/Each )	2-sigma Error	MDA (pCi/Each )
AG-108m	Not Detected	-----	2.37E+002
AG-110m	Not Detected	-----	2.21E+008
BA-133	Not Detected	-----	7.74E+002
BE-7	Not Detected	-----	1.00E+026
CD-115	Not Detected	-----	1.00E+026
CE-139	Not Detected	-----	6.05E+011
CE-141	Not Detected	-----	1.00E+026
CE-144	Not Detected	-----	5.68E+007
CM-243	Not Detected	-----	1.87E+003
CO-56	Not Detected	-----	2.22E+019
CO-57	Not Detected	-----	1.28E+007
CO-58	Not Detected	-----	6.15E+020
CO-60	8.10E+004	1.05E+004	6.23E+002
CR-51	Not Detected	-----	1.00E+026
CS-134	Not Detected	-----	1.19E+004
CS-137	7.06E+004	8.93E+003	3.16E+002
EU-152	Not Detected	-----	1.10E+003
EU-154	Not Detected	-----	2.66E+003
EU-155	Not Detected	-----	4.94E+003
FE-59	Not Detected	-----	1.00E+026
GD-153	Not Detected	-----	1.62E+008
HG-203	Not Detected	-----	1.00E+026
I-131	Not Detected	-----	1.00E+026
IR-192	Not Detected	-----	1.24E+020
K-40	Not Detected	-----	1.07E+003
IN-52	Not Detected	-----	1.00E+026
IN-54	Not Detected	-----	3.91E+006
MO-99	Not Detected	-----	1.00E+026
NA-22	Not Detected	-----	3.69E+003
NA-24	Not Detected	-----	1.00E+026
ND-147	Not Detected	-----	1.00E+026
NI-57	Not Detected	-----	1.00E+026
RU-103	Not Detected	-----	1.00E+026
RU-106	Not Detected	-----	7.76E+006
SB-122	Not Detected	-----	1.00E+026
SB-124	Not Detected	-----	1.00E+026
SB-125	Not Detected	-----	1.89E+004
SN-113	Not Detected	-----	8.24E+013
SR-85	Not Detected	-----	1.00E+026
TA-182	Not Detected	-----	1.78E+014
TA-183	Not Detected	-----	1.00E+026
TL-201	Not Detected	-----	1.00E+026
Y-88	Not Detected	-----	1.85E+014
ZN-65	Not Detected	-----	1.35E+008
ZR-95	Not Detected	-----	1.00E+026



\*\*\*\*\*  
 Sandia National Laboratories \*  
 Radiation Protection Sample Diagnostics Program \*  
 Quality Assurance Report \*  
 \*\*\*\*\*

Report Date : 9/20/02 12:39:57 PM  
 QA File : C:\GENIE2K\CAMPFILES\LCS2.QAF  
 Analyst : KRSANSO  
 Sample ID : 20131521  
 Sample Quantity : 1.00 Each  
 Sample Date : 11/01/90 12:00:00 PM  
 Measurement Date : 9/20/02 12:29:34 PM  
 Elapsed Live Time : 600 seconds  
 Elapsed Real Time : 604 seconds

Parameter	Mean	1S Error	New Value	< LU : SD : UD : BS >
AM-241 Activity	8.241E-002	3.925E-003	8.077E-002	< : ✓ : >
CS-137 Activity	7.182E-002	3.737E-003	7.064E-002	< : ✓ : >
CO-60 Activity	8.001E-002	5.100E-003	8.078E-002	< : ✓ : >

Flags Key: LU = Boundary Test (Ab = Above , Be = Below )  
 SD = Sample Driven N-Sigma Test (In = Investigate, Ac = Action)  
 UD = User Driven N-Sigma Test (In = Investigate, Ac = Action)  
 BS = Measurement Bias Test (In = Investigate, Ac = Action)

Reviewed by:                     KRS 9/20/02

COC 605732  
 BATCH NO. 201316

RPSD QC CROSS REFERENCE

Site #	Site Name	SAMPLE#	F#	ER SAMPLE ID	SAMPLE DATE	MATRIX	LAB TEST
1110	Bldg. 6536 Drain	059828	003	6536HP/1110-DF1-BH1-15-S	10-SEP-02	SOIL	GAMMA SPEC
1110	Bldg. 6536 Drain	059829	003	6536HP/1110-DF1-BH1-20-S	10-SEP-02	SOIL	GAMMA SPEC
1110	Bldg. 6536 Drain	059836	003	6536HP/1110-DF1-BH2-10-S	13-SEP-02	SOIL	GAMMA SPEC
1110	Bldg. 6536 Drain	059837	003	6536HP/1110-DF1-BH2-15-S	13-SEP-02	SOIL	GAMMA SPEC
1035	Bldg. 6715 SS	059838	003	6715/1035-SP1-BH1-11-S	12-SEP-02	SOIL	GAMMA SPEC
1035	Bldg. 6715 SS	059839	003	6715/1035-SP1-BH1-16-S	12-SEP-02	SOIL	GAMMA SPEC
1090	Bldg. 6721 SS	059841	003	6721/1090-DF1-BH1-4-S	13-SEP-02	SOIL	GAMMA SPEC
1090	Bldg. 6721 SS	059842	003	6721/1090-DF1-BH1-9-S	13-SEP-02	SOIL	GAMMA SPEC
1090	Bldg. 6721 SS	059843	003	6721/1090-DF1-BH2-4-S	13-SEP-02	SOIL	GAMMA SPEC
1090	Bldg. 6721 SS	059844	003	6721/1090-DF1-BH2-9-S	13-SEP-02	SOIL	GAMMA SPEC
1090	Bldg. 6721 SS	059847	003	6721/1090-DF1-BH3-4-S	13-SEP-02	SOIL	GAMMA SPEC
1090	Bldg. 6721 SS	059848	003	6721/1090-DF1-BH3-9-S	13-SEP-02	SOIL	GAMMA SPEC
1111	Bldg. 6720 SP	059850	003	6720/1111-SP1-BH1-10-S	13-SEP-02	SOIL	GAMMA SPEC
1111	Bldg. 6720 SP	059851	003	6720/1111-SP1-BH1-15-S	13-SEP-02	SOIL	GAMMA SPEC
1087	Bldg. 6743 SP	059852	003	6743/1087-SP1-BH1-8-S	17-SEP-02	SOIL	GAMMA SPEC
1087	Bldg. 6743 SP	059853	003	6743/1087-SP1-BH1-13-S	17-SEP-02	SOIL	GAMMA SPEC
1089	Bldg. 6734 SP	059854	003	6734/1089-SP1-BH1-9-S	17-SEP-02	SOIL	GAMMA SPEC
1089	Bldg. 6734 SP	059855	003	6734/1089-SP1-BH1-14-S	17-SEP-02	SOIL	GAMMA SPEC
1090	Bldg. 6721 SS	059859	001	6721/1090-DF1-BH2-4-DU	13-SEP-02	SOIL	GAMMA SPEC

\*\*\*\*\*  
 \* Sandia National Laboratories \*  
 \* Radiation Protection Sample Diagnostics Program \*  
 \* 9/20/02 9:31:31 AM \*  
 \*\*\*\*\*

\* Analyzed by: *lu 9/20/02* Reviewed by: *K. 9/20/02* \*  
 \*\*\*\*\*

Customer : SANDERS, M (6135)  
 Customer Sample ID : 059828-003  
 Lab Sample ID : 20131501

Sample Description : 6536HP/1110-DF1-BH1-15-S  
 Sample Quantity : 753.000 gram  
 Sample Date/Time : 9/10/02 11:25:00 AM  
 Acquire Start Date/Time : 9/19/02 9:53:11 PM  
 Detector Name : LAB01  
 Elapsed Live/Real Time : 6000 / 6002 seconds

Comments:  
 U-235/Ra-226 peaks not resolved. Either isotope may be overestimated.  
 \*\*\*\*\*

Nuclide Name	Activity (pCi/gram)	2-sigma Error	MDA (pCi/gram)
U-238	Not Detected	-----	5.00E-001
RA-226	1.32E+000	5.03E-001	7.10E-001
PB-214	6.75E-001	1.05E-001	6.41E-002
BI-214	5.96E-001	1.02E-001	5.84E-002
B-210	Not Detected	-----	8.77E+000
H-232	6.57E-001	3.21E-001	2.03E-001
RA-228	6.02E-001	1.37E-001	1.53E-001
AC-228	6.76E-001	1.42E-001	1.04E-001
TH-228	8.53E-001	2.44E-001	4.30E-001
RA-224	8.85E-001	2.17E-001	1.01E-001
PB-212	7.00E-001	1.05E-001	3.86E-002
BI-212	7.10E-001	2.67E-001	3.38E-001
TL-208	5.92E-001	1.11E-001	8.65E-002
U-235	1.37E-001	1.67E-001	1.96E-001
TH-231	Not Detected	-----	6.51E+000
PA-231	Not Detected	-----	1.42E+000
TH-227	Not Detected	-----	3.17E-001
RA-223	Not Detected	-----	1.95E-001
RN-219	Not Detected	-----	3.92E-001
PB-211	Not Detected	-----	8.82E-001
TL-207	Not Detected	-----	1.55E+001
AM-241	Not Detected	-----	1.75E-001
PU-239	Not Detected	-----	3.44E+002
NP-237	Not Detected	-----	1.90E+000
PA-233	Not Detected	-----	5.62E-002
TH-229	Not Detected	-----	1.87E-001

[Summary Report] - Sample ID: : 20131501

Slide Name	Activity (pCi/gram )	2-sigma Error	MDA (pCi/gram )
AG-108m	Not Detected	-----	4.34E-002
AG-110m	Not Detected	-----	2.91E-002
BA-133	Not Detected	-----	4.52E-002
BE-7	Not Detected	-----	2.83E-001
CD-115	Not Detected	-----	1.24E+000
CE-139	Not Detected	-----	2.58E-002
CE-141	Not Detected	-----	5.12E-002
CE-144	Not Detected	-----	1.96E-001
CM-243	Not Detected	-----	1.71E-001
CO-56	Not Detected	-----	3.73E-002
CO-57	Not Detected	-----	2.48E-002
CO-58	Not Detected	-----	3.50E-002
CO-60	Not Detected	-----	4.04E-002
CR-51	Not Detected	-----	2.90E-001
CS-134	Not Detected	-----	4.37E-002
CS-137	Not Detected	-----	3.10E-002
EU-152	Not Detected	-----	7.31E-002
EU-154	Not Detected	-----	2.02E-001
EU-155	Not Detected	-----	1.09E-001
FE-59	Not Detected	-----	8.73E-002
GD-153	Not Detected	-----	6.44E-002
HG-203	Not Detected	-----	3.58E-002
I-131	Not Detected	-----	6.29E-002
IR-192	Not Detected	-----	2.94E-002
-40	1.49E+001	2.07E+000	3.59E-001
N-52	Not Detected	-----	1.12E-001
N-54	Not Detected	-----	3.62E-002
MO-99	Not Detected	-----	2.68E+000
NA-22	Not Detected	-----	5.08E-002
NA-24	Not Detected	-----	1.31E+003
ND-147	Not Detected	-----	3.61E-001
NI-57	Not Detected	-----	4.44E+000
RU-103	Not Detected	-----	3.56E-002
RU-106	Not Detected	-----	3.00E-001
SB-122	Not Detected	-----	4.57E-001
SB-124	Not Detected	-----	3.08E-002
SB-125	Not Detected	-----	8.37E-002
SN-113	Not Detected	-----	3.90E-002
SR-85	Not Detected	-----	3.90E-002
TA-182	Not Detected	-----	1.82E-001
TA-183	Not Detected	-----	5.47E-001
TL-201	Not Detected	-----	6.85E-001
Y-88	Not Detected	-----	3.23E-002
ZN-65	Not Detected	-----	1.20E-001
ZR-95	Not Detected	-----	6.48E-002

\*\*\*\*\*  
 \* Sandia National Laboratories \*  
 \* Radiation Protection Sample Diagnostics Program \*  
 \* 9/20/02 9:33:09 AM \*  
 \*\*\*\*\*

\* Analyzed by: *K 9/20/02* Reviewed by: *K 9/20/02* \*

Customer : SANDERS, M (6135)  
 Customer Sample ID : 059829-003  
 Lab Sample ID : 20131502

Sample Description : 6536HP/1110-DF1-BH1-20-S  
 Sample Quantity : 773.000 gram  
 Sample Date/Time : 9/10/02 11:55:00 AM  
 Acquire Start Date/Time : 9/19/02 11:35:31 PM  
 Detector Name : LAB01  
 Elapsed Live/Real Time : 6000 / 6002 seconds

Comments:

U-235/Ra-226 peaks not resolved. Either isotope may be overestimated.

\*\*\*\*\*

Nuclide Name	Activity (pCi/gram)	2-sigma Error	MDA (pCi/gram)
U-238	Not Detected	-----	4.98E-001
RA-226	1.75E+000	5.54E-001	7.46E-001
PB-214	6.67E-001	1.04E-001	6.37E-002
BI-214	6.29E-001	1.05E-001	5.45E-002
PB-210	Not Detected	-----	8.54E+000
TH-232	5.50E-001	2.76E-001	1.91E-001
RA-228	6.55E-001	1.41E-001	1.31E-001
AC-228	7.10E-001	1.46E-001	1.05E-001
TH-228	6.30E-001	2.15E-001	4.18E-001
RA-224	7.18E-001	1.84E-001	9.39E-002
PB-212	6.91E-001	1.03E-001	3.79E-002
BI-212	5.87E-001	2.99E-001	4.29E-001
TL-208	5.88E-001	1.12E-001	9.16E-002
U-235	Not Detected	-----	1.95E-001
TH-231	Not Detected	-----	6.50E+000
PA-231	Not Detected	-----	1.35E+000
TH-227	Not Detected	-----	3.11E-001
RA-223	Not Detected	-----	1.85E-001
RN-219	Not Detected	-----	3.81E-001
PB-211	Not Detected	-----	8.95E-001
TL-207	Not Detected	-----	1.60E+001
AM-241	Not Detected	-----	1.65E-001
PU-239	Not Detected	-----	3.45E+002
NP-237	Not Detected	-----	1.81E+000
PA-233	Not Detected	-----	5.80E-002
TH-229	Not Detected	-----	1.93E-001

Slide Name	Activity (pCi/gram )	2-sigma Error	MDA (pCi/gram )
AG-108m	Not Detected	-----	3.95E-002
AG-110m	Not Detected	-----	3.10E-002
BA-133	Not Detected	-----	4.36E-002
BE-7	Not Detected	-----	2.69E-001
CD-115	Not Detected	-----	1.22E+000
CE-139	Not Detected	-----	2.54E-002
CE-141	Not Detected	-----	5.25E-002
CE-144	Not Detected	-----	1.92E-001
CM-243	Not Detected	-----	1.64E-001
CO-56	Not Detected	-----	3.59E-002
CO-57	Not Detected	-----	2.52E-002
CO-58	Not Detected	-----	3.90E-002
CO-60	Not Detected	-----	4.18E-002
CR-51	Not Detected	-----	2.78E-001
CS-134	Not Detected	-----	4.06E-002
CS-137	Not Detected	-----	3.23E-002
EU-152	Not Detected	-----	7.41E-002
EU-154	Not Detected	-----	1.86E-001
EU-155	Not Detected	-----	1.10E-001
FE-59	Not Detected	-----	9.64E-002
GD-153	Not Detected	-----	6.62E-002
HG-203	Not Detected	-----	3.38E-002
I-131	Not Detected	-----	6.05E-002
IR-192	Not Detected	-----	2.93E-002
K-40	1.72E+001	2.36E+000	2.60E-001
N-52	Not Detected	-----	1.06E-001
N-54	Not Detected	-----	3.86E-002
MO-99	Not Detected	-----	2.79E+000
NA-22	Not Detected	-----	4.32E-002
NA-24	Not Detected	-----	1.19E+003
ND-147	Not Detected	-----	3.66E-001
NI-57	Not Detected	-----	4.62E+000
RU-103	Not Detected	-----	3.14E-002
RU-106	Not Detected	-----	2.88E-001
SB-122	Not Detected	-----	4.42E-001
SB-124	Not Detected	-----	3.10E-002
SB-125	Not Detected	-----	8.57E-002
SN-113	Not Detected	-----	4.10E-002
SR-85	Not Detected	-----	3.91E-002
TA-182	Not Detected	-----	1.79E-001
TA-183	Not Detected	-----	5.16E-001
TL-201	Not Detected	-----	6.59E-001
Y-88	Not Detected	-----	3.62E-002
ZN-65	Not Detected	-----	1.19E-001
ZR-95	Not Detected	-----	6.65E-002

\*\*\*\*\*  
 \* Sandia National Laboratories \*  
 \* Radiation Protection Sample Diagnostics Program \*  
 \* 9/20/02 2:58:05 AM \*  
 \*\*\*\*\*

\* Analyzed by: *lu 9/20/02* Reviewed by: *K 9/20/02* \*  
 \*\*\*\*\*

Customer : SANDERS, M (6135)  
 Customer Sample ID : 059836-003  
 Lab Sample ID : 20131503

Sample Description : 6536HP/1110-DF1-BH2-10-S  
 Sample Quantity : 646.000 gram  
 Sample Date/Time : 9/13/02 9:05:00 AM  
 Acquire Start Date/Time : 9/20/02 1:17:51 AM  
 Detector Name : LAB01  
 Elapsed Live/Real Time : 6000 / 6002 seconds

Comments:  
 U-235/Ra-226 peaks not resolved. Either isotope may be overestimated.  
 \*\*\*\*\*

Nuclide Name	Activity (pCi/gram)	2-sigma Error	MDA (pCi/gram)
U-238	Not Detected	-----	5.70E-001
RA-226	1.59E+000	5.53E-001	7.59E-001
PB-214	7.65E-001	1.20E-001	7.51E-002
BI-214	7.11E-001	1.19E-001	6.07E-002
PB-210	Not Detected	-----	9.75E+000
H-232	8.50E-001	4.10E-001	2.43E-001
RA-228	9.58E-001	1.91E-001	1.61E-001
AC-228	9.44E-001	1.88E-001	1.24E-001
TH-228	7.14E-001	2.52E-001	5.14E-001
RA-224	9.75E-001	2.41E-001	1.11E-001
PB-212	8.69E-001	1.29E-001	4.21E-002
BI-212	9.41E-001	2.98E-001	3.33E-001
TL-208	8.02E-001	1.45E-001	1.11E-001
U-235	Not Detected	-----	2.23E-001
TH-231	Not Detected	-----	7.62E+000
PA-231	Not Detected	-----	1.58E+000
TH-227	Not Detected	-----	3.74E-001
RA-223	Not Detected	-----	1.92E-001
RN-219	Not Detected	-----	4.48E-001
PB-211	Not Detected	-----	9.75E-001
TL-207	Not Detected	-----	1.69E+001
AM-241	Not Detected	-----	1.90E-001
PU-239	Not Detected	-----	4.00E+002
NP-237	Not Detected	-----	2.07E+000
PA-233	Not Detected	-----	6.52E-002
TH-229	Not Detected	-----	2.20E-001

[Summary Report] - Sample ID: : 20131503

Slide Name	Activity (pCi/gram )	2-sigma Error	MDA (pCi/gram )
AG-108m	Not Detected	-----	4.97E-002
AG-110m	Not Detected	-----	3.67E-002
BA-133	Not Detected	-----	5.05E-002
BE-7	Not Detected	-----	2.95E-001
CD-115	Not Detected	-----	6.12E-001
CE-139	Not Detected	-----	2.82E-002
CE-141	Not Detected	-----	5.67E-002
CE-144	Not Detected	-----	2.16E-001
CM-243	Not Detected	-----	1.96E-001
CO-56	Not Detected	-----	3.95E-002
CO-57	Not Detected	-----	2.78E-002
CO-58	Not Detected	-----	4.01E-002
CO-60	Not Detected	-----	4.34E-002
CR-51	Not Detected	-----	3.03E-001
CS-134	Not Detected	-----	4.95E-002
CS-137	Not Detected	-----	3.74E-002
EU-152	Not Detected	-----	8.25E-002
EU-154	Not Detected	-----	2.34E-001
EU-155	Not Detected	-----	1.20E-001
FE-59	Not Detected	-----	1.05E-001
GD-153	Not Detected	-----	7.23E-002
HG-203	Not Detected	-----	3.87E-002
I-131	Not Detected	-----	5.54E-002
IR-192	Not Detected	-----	3.32E-002
K-40	1.48E+001	2.08E+000	3.82E-001
LN-52	Not Detected	-----	9.45E-002
LN-54	Not Detected	-----	4.08E-002
MO-99	Not Detected	-----	1.54E+000
NA-22	Not Detected	-----	5.34E-002
NA-24	Not Detected	-----	6.68E+001
ND-147	Not Detected	-----	3.69E-001
NI-57	Not Detected	-----	1.44E+000
RU-103	Not Detected	-----	3.77E-002
RU-106	Not Detected	-----	3.47E-001
SB-122	Not Detected	-----	2.44E-001
SB-124	Not Detected	-----	3.55E-002
SB-125	Not Detected	-----	1.00E-001
SN-113	Not Detected	-----	4.63E-002
SR-85	Not Detected	-----	4.39E-002
TA-182	Not Detected	-----	1.95E-001
TA-183	Not Detected	-----	4.04E-001
TL-201	Not Detected	-----	4.18E-001
Y-88	Not Detected	-----	4.26E-002
ZN-65	Not Detected	-----	1.29E-001
ZR-95	Not Detected	-----	6.98E-002



\*\*\*\*\*  
 \* Sandia National Laboratories \*  
 \* Radiation Protection Sample Diagnostics Program \*  
 \* 9/20/02 4:40:24 AM \*  
 \*\*\*\*\*

\* Analyzed by: *AW 9/20/02* Reviewed by: *KA 9/20/02* \*  
 \*\*\*\*\*

Customer : SANDERS, M (6135)  
 Customer Sample ID : 059837-003  
 Lab Sample ID : 20131504

Sample Description : 6536HP/1110-DF1-BH2-15-S  
 Sample Quantity : 689.000 gram  
 Sample Date/Time : 9/13/02 9:20:00 AM  
 Acquire Start Date/Time : 9/20/02 3:00:10 AM  
 Detector Name : LAB01  
 Elapsed Live/Real Time : 6000 / 6002 seconds

Comments:  
 U-235/Ra-226 peaks not resolved. Either isotope may be overestimated.  
 \*\*\*\*\*

Nuclide Name	Activity (pCi/gram)	2-sigma Error	MDA (pCi/gram)
U-238	Not Detected	-----	5.40E-001
RA-226	1.87E+000	5.95E-001	8.00E-001
PB-214	7.05E-001	1.12E-001	7.53E-002
BI-214	6.66E-001	1.12E-001	5.83E-002
PB-210	Not Detected	-----	9.43E+000
TH-232	6.17E-001	3.18E-001	2.46E-001
RA-228	6.71E-001	1.82E-001	1.98E-001
AC-228	7.63E-001	1.61E-001	1.22E-001
TH-228	8.56E-001	2.58E-001	4.62E-001
RA-224	7.77E-001	2.08E-001	1.35E-001
PB-212	8.09E-001	1.20E-001	4.30E-002
BI-212	6.56E-001	2.88E-001	3.89E-001
TL-208	7.73E-001	1.36E-001	9.38E-002
U-235	Not Detected	-----	2.12E-001
TH-231	Not Detected	-----	6.93E+000
PA-231	Not Detected	-----	1.52E+000
TH-227	Not Detected	-----	3.54E-001
RA-223	Not Detected	-----	1.76E-001
RN-219	Not Detected	-----	4.47E-001
PB-211	Not Detected	-----	9.92E-001
TL-207	Not Detected	-----	1.67E+001
AM-241	Not Detected	-----	1.86E-001
PU-239	Not Detected	-----	3.84E+002
NP-237	Not Detected	-----	1.94E+000
PA-233	Not Detected	-----	6.34E-002
TH-229	Not Detected	-----	2.03E-001

Isotope Name	Activity (pCi/gram)	2-sigma Error	MDA (pCi/gram)
AG-108m	Not Detected	-----	4.68E-002
AG-110m	Not Detected	-----	3.16E-002
BA-133	Not Detected	-----	4.96E-002
BE-7	Not Detected	-----	2.79E-001
CD-115	Not Detected	-----	5.83E-001
CE-139	Not Detected	-----	2.70E-002
CE-141	Not Detected	-----	5.32E-002
CE-144	Not Detected	-----	2.02E-001
CM-243	Not Detected	-----	1.83E-001
CO-56	Not Detected	-----	4.04E-002
CO-57	Not Detected	-----	2.59E-002
CO-58	Not Detected	-----	3.99E-002
CO-60	Not Detected	-----	4.45E-002
CR-51	Not Detected	-----	2.72E-001
CS-134	Not Detected	-----	4.75E-002
CS-137	Not Detected	-----	3.58E-002
EU-152	Not Detected	-----	7.66E-002
EU-154	Not Detected	-----	2.21E-001
EU-155	Not Detected	-----	1.17E-001
FE-59	Not Detected	-----	9.03E-002
GD-153	Not Detected	-----	6.78E-002
HG-203	Not Detected	-----	3.69E-002
I-131	Not Detected	-----	5.22E-002
IR-192	Not Detected	-----	2.88E-002
K-40	1.53E+001	2.13E+000	3.03E-001
MN-52	Not Detected	-----	8.93E-002
NI-54	Not Detected	-----	3.93E-002
MO-99	Not Detected	-----	1.50E+000
NA-22	Not Detected	-----	5.18E-002
NA-24	Not Detected	-----	7.10E+001
ND-147	Not Detected	-----	3.36E-001
NI-57	Not Detected	-----	1.39E+000
RU-103	Not Detected	-----	3.40E-002
RU-106	Not Detected	-----	3.19E-001
SB-122	Not Detected	-----	2.34E-001
SB-124	Not Detected	-----	3.34E-002
SB-125	Not Detected	-----	9.01E-002
SN-113	Not Detected	-----	4.09E-002
SR-85	Not Detected	-----	4.13E-002
TA-182	Not Detected	-----	1.80E-001
TA-183	Not Detected	-----	3.94E-001
TL-201	Not Detected	-----	3.85E-001
Y-88	Not Detected	-----	3.36E-002
ZN-65	Not Detected	-----	1.18E-001
ZR-95	Not Detected	-----	6.87E-002

\*\*\*\*\*  
 \* Sandia National Laboratories \*  
 \* Radiation Protection Sample Diagnostics Program \*  
 \* 9/20/02 6:22:43 AM \*  
 \*\*\*\*\*

\* Analyzed by: *h 9/20/02* Reviewed by: *K 9/20/02* \*  
 \*\*\*\*\*

Customer : SANDERS, M (6135)  
 Customer Sample ID : 059838-003  
 Lab Sample ID : 20131505

Sample Description : 6715/1035-SP1-BH1-11-S  
 Sample Quantity : 775.000 gram  
 Sample Date/Time : 9/12/02 2:20:00 PM  
 Acquire Start Date/Time : 9/20/02 4:42:29 AM  
 Detector Name : LAB01  
 Elapsed Live/Real Time : 6000 / 6002 seconds

Comments:  
 U-235/Ra-226 peaks not resolved. Either isotope may be overestimated.  
 \*\*\*\*\*

Nuclide Name	Activity (pCi/gram)	2-sigma Error	MDA (pCi/gram)
U-238	Not Detected	-----	4.87E-001
RA-226	1.73E+000	5.44E-001	7.28E-001
PB-214	7.07E-001	1.06E-001	5.52E-002
BI-214	6.06E-001	1.02E-001	5.58E-002
PB-210	Not Detected	-----	8.45E+000
H-232	6.96E-001	3.38E-001	2.09E-001
RA-228	7.28E-001	1.51E-001	1.41E-001
AC-228	7.76E-001	1.57E-001	1.10E-001
TH-228	7.06E-001	2.22E-001	4.06E-001
RA-224	9.06E-001	2.17E-001	8.79E-002
PB-212	7.33E-001	1.09E-001	3.73E-002
BI-212	6.73E-001	4.82E-001	7.46E-001
TL-208	6.35E-001	1.16E-001	8.93E-002
U-235	9.48E-002	1.69E-001	1.98E-001
TH-231	Not Detected	-----	6.32E+000
PA-231	Not Detected	-----	1.36E+000
TH-227	Not Detected	-----	3.15E-001
RA-223	Not Detected	-----	1.70E-001
RN-219	Not Detected	-----	3.72E-001
PB-211	Not Detected	-----	8.25E-001
TL-207	Not Detected	-----	1.47E+001
AM-241	Not Detected	-----	1.65E-001
PU-239	Not Detected	-----	3.56E+002
NP-237	Not Detected	-----	1.89E+000
PA-233	Not Detected	-----	5.52E-002
TH-229	Not Detected	-----	1.88E-001

[Summary Report] - Sample ID: : 20131505

Slide Name	Activity (pCi/gram )	2-sigma Error	MDA (pCi/gram )
AG-108m	Not Detected	-----	4.12E-002
AG-110m	Not Detected	-----	2.88E-002
BA-133	Not Detected	-----	4.22E-002
BE-7	Not Detected	-----	2.69E-001
CD-115	Not Detected	-----	7.04E-001
CE-139	Not Detected	-----	2.44E-002
CE-141	Not Detected	-----	5.09E-002
CE-144	Not Detected	-----	1.93E-001
CM-243	Not Detected	-----	1.69E-001
CO-56	Not Detected	-----	3.81E-002
CO-57	Not Detected	-----	2.50E-002
CO-58	Not Detected	-----	3.53E-002
CO-60	Not Detected	-----	3.81E-002
CR-51	Not Detected	-----	2.63E-001
CS-134	Not Detected	-----	4.10E-002
CS-137	Not Detected	-----	3.19E-002
EU-152	Not Detected	-----	7.38E-002
EU-154	Not Detected	-----	1.92E-001
EU-155	Not Detected	-----	1.09E-001
FE-59	Not Detected	-----	8.82E-002
GD-153	Not Detected	-----	6.33E-002
HG-203	Not Detected	-----	3.42E-002
I-131	Not Detected	-----	5.08E-002
IR-192	Not Detected	-----	2.70E-002
K-40	1.51E+001	2.09E+000	3.48E-001
MN-52	Not Detected	-----	8.55E-002
MN-54	Not Detected	-----	3.79E-002
MO-99	Not Detected	-----	1.78E+000
NA-22	Not Detected	-----	4.83E-002
NA-24	Not Detected	-----	1.57E+002
ND-147	Not Detected	-----	3.29E-001
NI-57	Not Detected	-----	1.77E+000
RU-103	Not Detected	-----	3.21E-002
RU-106	Not Detected	-----	2.91E-001
SB-122	Not Detected	-----	2.75E-001
SB-124	Not Detected	-----	2.98E-002
SB-125	Not Detected	-----	8.33E-002
SN-113	Not Detected	-----	3.87E-002
SR-85	Not Detected	-----	3.87E-002
TA-182	Not Detected	-----	1.70E-001
TA-183	Not Detected	-----	4.01E-001
TL-201	Not Detected	-----	4.44E-001
Y-88	Not Detected	-----	3.19E-002
ZN-65	Not Detected	-----	1.12E-001
ZR-95	Not Detected	-----	6.54E-002

\*\*\*\*\*  
 \* Sandia National Laboratories \*  
 \* Radiation Protection Sample Diagnostics Program \*  
 \* 9/20/02 9:20:40 AM \*  
 \*\*\*\*\*

\* Analyzed by: *me 9/20/02* Reviewed by: *[Signature] 9/20/02* \*

Customer : SANDERS, M (6135)  
 Customer Sample ID : 059839-003  
 Lab Sample ID : 20131506

Sample Description : 6715/1035-SP1-BH1-16-S  
 Sample Quantity : 736.000 gram  
 Sample Date/Time : 9/12/02 2:40:00 PM  
 Acquire Start Date/Time : 9/20/02 6:24:48 AM  
 Detector Name : LAB01  
 Elapsed Live/Real Time : 6000 / 6002 seconds

Comments:  
 U-235/Ra-226 peaks not resolved. Either isotope may be overestimated.  
 \*\*\*\*\*

Nuclide Name	Activity (pCi/gram)	2-sigma Error	MDA (pCi/gram)
U-238	Not Detected	-----	5.16E-001
RA-226	1.63E+000	5.09E-001	6.74E-001
PB-214	7.48E-001	1.13E-001	5.86E-002
BI-214	6.59E-001	1.11E-001	6.12E-002
B-210	Not Detected	-----	8.96E+000
TH-232	7.94E-001	3.81E-001	2.17E-001
RA-228	6.41E-001	1.44E-001	1.61E-001
AC-228	6.76E-001	1.52E-001	1.36E-001
TH-228	7.96E-001	2.47E-001	4.88E-001
RA-224	9.45E-001	2.29E-001	1.07E-001
PB-212	7.87E-001	1.17E-001	3.83E-002
BI-212	8.21E-001	3.08E-001	3.99E-001
TL-208	6.26E-001	1.17E-001	9.08E-002
U-235	Not Detected	-----	1.99E-001
TH-231	Not Detected	-----	6.66E+000
PA-231	Not Detected	-----	1.37E+000
TH-227	Not Detected	-----	3.38E-001
RA-223	Not Detected	-----	1.75E-001
RN-219	Not Detected	-----	3.91E-001
PB-211	Not Detected	-----	8.74E-001
TL-207	Not Detected	-----	1.54E+001
AM-241	Not Detected	-----	1.75E-001
PU-239	Not Detected	-----	3.68E+002
NP-237	Not Detected	-----	1.94E+000
PA-233	Not Detected	-----	5.68E-002
TH-229	Not Detected	-----	1.94E-001

[Summary Report] - Sample ID: : 20131506

Isotope Name	Activity (pCi/gram )	2-sigma Error	MDA (pCi/gram )
AG-108m	Not Detected	-----	4.53E-002
AG-110m	Not Detected	-----	3.09E-002
BA-133	Not Detected	-----	4.53E-002
BE-7	Not Detected	-----	2.75E-001
CD-115	Not Detected	-----	7.50E-001
CE-139	Not Detected	-----	2.63E-002
CE-141	Not Detected	-----	5.09E-002
CE-144	Not Detected	-----	1.98E-001
CM-243	Not Detected	-----	1.76E-001
CO-56	Not Detected	-----	3.64E-002
CO-57	Not Detected	-----	2.47E-002
CO-58	Not Detected	-----	3.58E-002
CO-60	Not Detected	-----	4.03E-002
CR-51	Not Detected	-----	2.62E-001
CS-134	Not Detected	-----	4.63E-002
CS-137	Not Detected	-----	3.44E-002
EU-152	Not Detected	-----	7.29E-002
EU-154	Not Detected	-----	2.12E-001
EU-155	Not Detected	-----	1.12E-001
FE-59	Not Detected	-----	9.44E-002
GD-153	Not Detected	-----	6.56E-002
HG-203	Not Detected	-----	3.51E-002
I-131	Not Detected	-----	5.39E-002
IR-192	Not Detected	-----	2.89E-002
K-40	1.52E+001	2.11E+000	3.08E-001
LN-52	Not Detected	-----	7.95E-002
LN-54	Not Detected	-----	3.71E-002
MO-99	Not Detected	-----	1.80E+000
NA-22	Not Detected	-----	4.62E-002
NA-24	Not Detected	-----	1.85E+002
ND-147	Not Detected	-----	3.38E-001
NI-57	Not Detected	-----	2.13E+000
RU-103	Not Detected	-----	3.05E-002
RU-106	Not Detected	-----	2.92E-001
SB-122	Not Detected	-----	2.96E-001
SB-124	Not Detected	-----	3.33E-002
SB-125	Not Detected	-----	8.97E-002
SN-113	Not Detected	-----	3.74E-002
SR-85	Not Detected	-----	3.87E-002
TA-182	Not Detected	-----	1.86E-001
TA-183	Not Detected	-----	4.19E-001
TL-201	Not Detected	-----	4.74E-001
Y-88	Not Detected	-----	3.16E-002
ZN-65	Not Detected	-----	1.25E-001
ZR-95	Not Detected	-----	7.00E-002

\*\*\*\*\*  
 \* Sandia National Laboratories \*  
 \* Radiation Protection Sample Diagnostics Program \*  
 \* 9/20/02 9:47:23 AM \*  
 \*\*\*\*\*

\* Analyzed by: *AS* 9/20/02 Reviewed by: *AS* 9/20/02 \*  
 \*\*\*\*\*

Customer : SANDERS, M (6135)  
 Customer Sample ID : 059841-003  
 Lab Sample ID : 20131507

Sample Description : 6721/1090-DF1-BH1-4-S  
 Sample Quantity : 808.000 gram  
 Sample Date/Time : 9/13/02 9:35:00 AM  
 Acquire Start Date/Time : 9/20/02 8:07:08 AM  
 Detector Name : LAB01  
 Elapsed Live/Real Time : 6000 / 6002 seconds

Comments:  
 U-235/Ra-226 peaks not resolved. Either isotope may be overestimated.  
 \*\*\*\*\*

Nuclide Name	Activity (pCi/gram)	2-sigma Error	MDA (pCi/gram)
U-238	Not Detected	-----	4.50E-001
RA-226	1.55E+000	7.51E-001	1.13E+000
PB-214	6.57E-001	9.99E-002	5.49E-002
BI-214	5.98E-001	9.91E-002	4.76E-002
-PB-210	Not Detected	-----	8.39E+000
H-232	6.71E-001	3.24E-001	1.92E-001
RA-228	6.38E-001	1.40E-001	1.50E-001
AC-228	6.87E-001	1.44E-001	1.12E-001
TH-228	8.03E-001	2.35E-001	4.36E-001
RA-224	7.25E-001	1.82E-001	8.18E-002
PB-212	6.75E-001	1.01E-001	3.41E-002
BI-212	7.08E-001	2.66E-001	3.40E-001
TL-208	6.15E-001	1.11E-001	8.24E-002
U-235	2.29E-001	1.54E-001	1.84E-001
TH-231	Not Detected	-----	6.04E+000
PA-231	Not Detected	-----	1.29E+000
TH-227	Not Detected	-----	2.97E-001
RA-223	Not Detected	-----	1.56E-001
RN-219	Not Detected	-----	3.51E-001
PB-211	Not Detected	-----	7.90E-001
TL-207	Not Detected	-----	1.31E+001
AM-241	Not Detected	-----	1.56E-001
PU-239	Not Detected	-----	3.34E+002
NP-237	Not Detected	-----	1.76E+000
PA-233	Not Detected	-----	5.45E-002
TH-229	Not Detected	-----	1.81E-001

[Summary Report] - Sample ID: : 20131507

Nuclide Name	Activity (pCi/gram )	2-sigma Error	MDA (pCi/gram )
AG-108m	Not Detected	-----	4.09E-002
AG-110m	Not Detected	-----	3.00E-002
BA-133	Not Detected	-----	3.91E-002
BE-7	Not Detected	-----	2.38E-001
CD-115	Not Detected	-----	5.33E-001
CE-139	Not Detected	-----	2.42E-002
CE-141	Not Detected	-----	4.60E-002
CE-144	Not Detected	-----	1.82E-001
CM-243	Not Detected	-----	1.62E-001
CO-56	Not Detected	-----	3.27E-002
CO-57	Not Detected	-----	2.31E-002
CO-58	Not Detected	-----	3.42E-002
CO-60	Not Detected	-----	3.75E-002
CR-51	Not Detected	-----	2.56E-001
CS-134	Not Detected	-----	4.13E-002
CS-137	Not Detected	-----	3.17E-002
EU-152	Not Detected	-----	6.85E-002
EU-154	Not Detected	-----	1.91E-001
EU-155	Not Detected	-----	1.05E-001
FE-59	Not Detected	-----	8.16E-002
GD-153	Not Detected	-----	5.96E-002
HG-203	Not Detected	-----	3.21E-002
I-131	Not Detected	-----	4.49E-002
IR-192	Not Detected	-----	2.64E-002
K-40	1.46E+001	2.02E+000	2.83E-001
TN-52	Not Detected	-----	8.38E-002
IN-54	Not Detected	-----	3.43E-002
MO-99	Not Detected	-----	1.29E+000
NA-22	Not Detected	-----	4.49E-002
NA-24	Not Detected	-----	7.87E+001
ND-147	Not Detected	-----	2.90E-001
NI-57	Not Detected	-----	1.37E+000
RU-103	Not Detected	-----	3.09E-002
RU-106	Not Detected	-----	2.69E-001
SB-122	Not Detected	-----	2.34E-001
SB-124	Not Detected	-----	2.78E-002
SB-125	Not Detected	-----	7.82E-002
SN-113	Not Detected	-----	3.57E-002
SR-85	Not Detected	-----	3.56E-002
TA-182	Not Detected	-----	1.66E-001
TA-183	Not Detected	-----	3.40E-001
TL-201	Not Detected	-----	3.71E-001
Y-88	Not Detected	-----	2.68E-002
ZN-65	Not Detected	-----	1.11E-001
ZR-95	Not Detected	-----	5.95E-002



\*\*\*\*\*  
 \* Sandia National Laboratories \*  
 \* Radiation Protection Sample Diagnostics Program \*  
 \* 9/20/02 11:29:48 AM \*  
 \*\*\*\*\*

\* Analyzed by: *ms 9/20/02* Reviewed by: *KS 9/20/02*  
 \*\*\*\*\*

Customer : SANDERS, M (6135)  
 Customer Sample ID : 059842-003  
 Lab Sample ID : 20131508

Sample Description : 6721/1090-DF1-BH1-9-S  
 Sample Quantity : 807.000 gram  
 Sample Date/Time : 9/13/02 9:50:00 AM  
 Acquire Start Date/Time : 9/20/02 9:49:28 AM  
 Detector Name : LAB01  
 Elapsed Live/Real Time : 6000 / 6002 seconds

Comments:  
 U-235/Ra-226 peaks not resolved. Either isotope may be overestimated.  
 \*\*\*\*\*

Nuclide Name	Activity (pCi/gram)	2-sigma Error	MDA (pCi/gram)
U-238	Not Detected	-----	4.74E-001
RA-226	1.32E+000	5.09E-001	7.25E-001
PB-214	7.10E-001	1.07E-001	5.70E-002
BI-214	5.64E-001	9.43E-002	4.67E-002
PB-210	Not Detected	-----	8.36E+000
TH-232	6.21E-001	3.04E-001	1.91E-001
RA-228	5.68E-001	1.30E-001	1.43E-001
AC-228	4.51E-001	1.11E-001	1.06E-001
TH-228	8.60E-001	2.35E-001	4.04E-001
RA-224	6.94E-001	1.75E-001	6.92E-002
PB-212	6.39E-001	9.58E-002	3.58E-002
BI-212	9.18E-001	3.25E-001	4.17E-001
TL-208	6.08E-001	1.10E-001	7.94E-002
U-235	Not Detected	-----	1.91E-001
TH-231	Not Detected	-----	6.26E+000
PA-231	Not Detected	-----	1.35E+000
TH-227	Not Detected	-----	2.98E-001
RA-223	Not Detected	-----	1.62E-001
RN-219	Not Detected	-----	3.63E-001
PB-211	Not Detected	-----	7.99E-001
TL-207	Not Detected	-----	1.50E+001
AM-241	Not Detected	-----	1.64E-001
PU-239	Not Detected	-----	3.39E+002
NP-237	Not Detected	-----	1.75E+000
PA-233	Not Detected	-----	5.52E-002
TH-229	Not Detected	-----	1.80E-001

Slide Name	Activity (pCi/gram )	2-sigma Error	MDA (pCi/gram )
AG-108m	Not Detected	-----	4.09E-002
AG-110m	Not Detected	-----	2.97E-002
BA-133	Not Detected	-----	4.32E-002
BE-7	Not Detected	-----	2.51E-001
CD-115	Not Detected	-----	5.52E-001
CE-139	Not Detected	-----	2.43E-002
CE-141	Not Detected	-----	4.79E-002
CE-144	Not Detected	-----	1.86E-001
CM-243	Not Detected	-----	1.65E-001
CO-56	Not Detected	-----	3.57E-002
CO-57	Not Detected	-----	2.36E-002
CO-58	Not Detected	-----	3.53E-002
CO-60	Not Detected	-----	3.71E-002
CR-51	Not Detected	-----	2.55E-001
CS-134	Not Detected	-----	4.01E-002
CS-137	Not Detected	-----	3.14E-002
EU-152	Not Detected	-----	6.98E-002
EU-154	Not Detected	-----	1.93E-001
EU-155	Not Detected	-----	1.03E-001
FE-59	Not Detected	-----	8.80E-002
GD-153	Not Detected	-----	6.09E-002
HG-203	Not Detected	-----	3.27E-002
I-131	Not Detected	-----	4.81E-002
IR-192	Not Detected	-----	2.72E-002
K-40	1.62E+001	2.23E+000	3.30E-001
LN-52	Not Detected	-----	7.77E-002
LN-54	Not Detected	-----	3.32E-002
MO-99	Not Detected	-----	1.40E+000
NA-22	Not Detected	-----	4.57E-002
NA-24	Not Detected	-----	8.97E+001
ND-147	Not Detected	-----	2.92E-001
NI-57	Not Detected	-----	1.46E+000
RU-103	Not Detected	-----	3.20E-002
RU-106	Not Detected	-----	2.72E-001
SB-122	Not Detected	-----	2.27E-001
SB-124	Not Detected	-----	2.94E-002
SB-125	Not Detected	-----	8.14E-002
SN-113	Not Detected	-----	3.87E-002
SR-85	Not Detected	-----	3.67E-002
TA-182	Not Detected	-----	1.74E-001
TA-183	Not Detected	-----	3.59E-001
TL-201	Not Detected	-----	3.68E-001
Y-88	Not Detected	-----	3.18E-002
ZN-65	Not Detected	-----	1.16E-001
ZR-95	Not Detected	-----	6.28E-002

\*\*\*\*\*  
 \* Sandia National Laboratories \*  
 \* Radiation Protection Sample Diagnostics Program \*  
 \* 9/19/02 5:22:21 PM \*  
 \*\*\*\*\*

\* Analyzed by: *he 9/20/02* Reviewed by: *KA 9/20/02*  
 \*\*\*\*\*

Customer : SANDERS, M (6135)  
 Customer Sample ID : 059843-003  
 Lab Sample ID : 20131509

Sample Description : 6721/1090-DF1-BH2-4S  
 Sample Quantity : 684.000 gram  
 Sample Date/Time : 9/13/02 10:14:00 AM  
 Acquire Start Date/Time : 9/19/02 3:41:54 PM  
 Detector Name : LAB02  
 Elapsed Live/Real Time : 6000 / 6002 seconds

Comments:  
 U-235/Ra-226 peaks not resolved. Either isotope may be overestimated.  
 \*\*\*\*\*

Nuclide Name	Activity (pCi/gram)	2-sigma Error	MDA (pCi/gram)
U-238	Not Detected	-----	6.89E-001
RA-226	2.05E+000	5.30E-001	6.51E-001
PB-214	6.93E-001	1.05E-001	6.32E-002
BI-214	6.60E-001	1.06E-001	5.28E-002
PB-210	Not Detected	-----	2.66E+001
TH-232	7.29E-001	3.49E-001	2.01E-001
RA-228	7.33E-001	1.41E-001	1.24E-001
AC-228	6.78E-001	1.33E-001	9.16E-002
TH-228	4.72E-001	4.26E-001	6.73E-001
RA-224	7.59E-001	1.77E-001	8.20E-002
PB-212	7.38E-001	1.08E-001	3.60E-002
BI-212	7.10E-001	2.51E-001	3.20E-001
TL-208	6.42E-001	1.11E-001	7.80E-002
U-235	Not Detected	-----	2.20E-001
TH-231	Not Detected	-----	1.06E+001
PA-231	Not Detected	-----	1.34E+000
TH-227	Not Detected	-----	3.34E-001
RA-223	Not Detected	-----	2.43E-001
RN-219	Not Detected	-----	3.42E-001
PB-211	Not Detected	-----	7.56E-001
TL-207	Not Detected	-----	1.17E+001
AM-241	Not Detected	-----	4.13E-001
PU-239	Not Detected	-----	3.98E+002
NP-237	Not Detected	-----	2.10E+000
PA-233	Not Detected	-----	5.28E-002
TH-229	Not Detected	-----	2.22E-001

[Summary Report] - Sample ID: : 20131509

Nuclide Name	Activity (pCi/gram )	2-sigma Error	MDA (pCi/gram )
AG-108m	Not Detected	-----	3.36E-002
AG-110m	Not Detected	-----	2.59E-002
BA-133	Not Detected	-----	4.81E-002
BE-7	Not Detected	-----	2.25E-001
CD-115	Not Detected	-----	4.26E-001
CE-139	Not Detected	-----	2.64E-002
CE-141	Not Detected	-----	5.41E-002
CE-144	Not Detected	-----	2.15E-001
CM-243	Not Detected	-----	1.58E-001
CO-56	Not Detected	-----	2.86E-002
CO-57	Not Detected	-----	2.86E-002
CO-58	Not Detected	-----	3.00E-002
CO-60	Not Detected	-----	3.20E-002
CR-51	Not Detected	-----	2.43E-001
CS-134	Not Detected	-----	3.91E-002
CS-137	Not Detected	-----	2.78E-002
EU-152	Not Detected	-----	8.42E-002
EU-154	Not Detected	-----	1.55E-001
EU-155	Not Detected	-----	1.25E-001
FE-59	Not Detected	-----	6.83E-002
GD-153	Not Detected	-----	9.17E-002
HG-203	Not Detected	-----	3.15E-002
I-131	Not Detected	-----	4.49E-002
IR-192	Not Detected	-----	2.63E-002
K-40	1.51E+001	2.06E+000	2.75E-001
IN-52	Not Detected	-----	5.31E-002
IN-54	Not Detected	-----	2.91E-002
MO-99	Not Detected	-----	9.87E-001
NA-22	Not Detected	-----	3.58E-002
NA-24	Not Detected	-----	2.79E+001
ND-147	Not Detected	-----	2.55E-001
NI-57	Not Detected	-----	7.88E-001
RU-103	Not Detected	-----	2.73E-002
RU-106	Not Detected	-----	2.42E-001
SB-122	Not Detected	-----	1.73E-001
SB-124	Not Detected	-----	2.74E-002
SB-125	Not Detected	-----	7.75E-002
SN-113	Not Detected	-----	3.36E-002
SR-85	Not Detected	-----	3.28E-002
TA-182	Not Detected	-----	1.42E-001
TA-183	Not Detected	-----	8.27E-001
TL-201	Not Detected	-----	6.23E-001
Y-88	Not Detected	-----	2.17E-002
ZN-65	Not Detected	-----	9.16E-002
ZR-95	Not Detected	-----	4.78E-002

\*\*\*\*\*  
 \* Sandia National Laboratories \*  
 \* Radiation Protection Sample Diagnostics Program \*  
 \* 9/19/02 7:22:22 PM \*  
 \*\*\*\*\*

\* Analyzed by: *[Signature]* 9/20/02 Reviewed by: *[Signature]* 9/20/02 \*  
 \*\*\*\*\*

Customer : SANDERS, M (6135)  
 Customer Sample ID : 059844-003  
 Lab Sample ID : 20131510

Sample Description : 6721/1090-DF1-BH2-9-S  
 Sample Quantity : 785.000 gram  
 Sample Date/Time : 9/13/02 10:35:00 AM  
 Acquire Start Date/Time : 9/19/02 5:24:15 PM  
 Detector Name : LAB02  
 Elapsed Live/Real Time : 6000 / 6003 seconds

Comments:  
 U-235/Ra-226 peaks not resolved. Either isotope may be overestimated.  
 \*\*\*\*\*

Nuclide Name	Activity (pCi/gram)	2-sigma Error	MDA (pCi/gram)
U-238	Not Detected	-----	6.38E-001
RA-226	1.23E+000	4.43E-001	6.20E-001
PB-214	6.81E-001	1.02E-001	6.03E-002
BI-214	6.43E-001	1.02E-001	4.49E-002
PB-210	Not Detected	-----	2.53E+001
TH-232	7.42E-001	3.52E-001	1.91E-001
RA-228	6.87E-001	1.31E-001	1.18E-001
AC-228	7.15E-001	1.36E-001	8.95E-002
TH-228	6.85E-001	4.04E-001	6.11E-001
RA-224	8.96E-001	1.94E-001	5.54E-002
PB-212	7.18E-001	1.05E-001	3.53E-002
BI-212	8.45E-001	2.71E-001	3.42E-001
TL-208	6.50E-001	1.10E-001	7.65E-002
U-235	1.44E-001	1.63E-001	2.08E-001
TH-231	Not Detected	-----	1.01E+001
PA-231	Not Detected	-----	1.25E+000
TH-227	Not Detected	-----	3.12E-001
RA-223	Not Detected	-----	2.32E-001
RN-219	Not Detected	-----	3.10E-001
PB-211	Not Detected	-----	6.67E-001
TL-207	Not Detected	-----	1.07E+001
AM-241	Not Detected	-----	3.88E-001
PU-239	Not Detected	-----	3.68E+002
NP-237	Not Detected	-----	1.99E+000
PA-233	Not Detected	-----	4.74E-002
TH-229	Not Detected	-----	2.05E-001

[Summary Report] - Sample ID: : 20131510

Nuclide Name	Activity (pCi/gram )	2-sigma Error	MDA (pCi/gram )
AG-108m	Not Detected	-----	3.05E-002
AG-110m	Not Detected	-----	2.42E-002
BA-133	Not Detected	-----	4.25E-002
BE-7	Not Detected	-----	2.13E-001
CD-115	Not Detected	-----	4.04E-001
CE-139	Not Detected	-----	2.62E-002
CE-141	Not Detected	-----	5.14E-002
CE-144	Not Detected	-----	2.10E-001
CM-243	Not Detected	-----	1.47E-001
CO-56	Not Detected	-----	2.77E-002
CO-57	Not Detected	-----	2.74E-002
CO-58	Not Detected	-----	2.71E-002
CO-60	Not Detected	-----	2.94E-002
CR-51	Not Detected	-----	2.20E-001
CS-134	Not Detected	-----	3.49E-002
CS-137	Not Detected	-----	2.65E-002
EU-152	Not Detected	-----	8.12E-002
EU-154	Not Detected	-----	1.40E-001
EU-155	Not Detected	-----	1.22E-001
FE-59	Not Detected	-----	6.32E-002
GD-153	Not Detected	-----	8.71E-002
HG-203	Not Detected	-----	2.92E-002
I-131	Not Detected	-----	4.06E-002
IR-192	Not Detected	-----	2.36E-002
K-40	1.75E+001	2.35E+000	2.37E-001
N-52	Not Detected	-----	5.19E-002
N-54	Not Detected	-----	2.79E-002
MO-99	Not Detected	-----	9.46E-001
NA-22	Not Detected	-----	3.33E-002
NA-24	Not Detected	-----	2.74E+001
ND-147	Not Detected	-----	2.28E-001
NI-57	Not Detected	-----	7.91E-001
RU-103	Not Detected	-----	2.46E-002
RU-106	Not Detected	-----	2.27E-001
SB-122	Not Detected	-----	1.68E-001
SB-124	Not Detected	-----	2.47E-002
SB-125	Not Detected	-----	7.09E-002
SN-113	Not Detected	-----	3.31E-002
SR-85	Not Detected	-----	3.22E-002
TA-182	Not Detected	-----	1.31E-001
TA-183	Not Detected	-----	7.83E-001
TL-201	Not Detected	-----	5.95E-001
Y-88	Not Detected	-----	2.24E-002
ZN-65	Not Detected	-----	8.58E-002
ZR-95	Not Detected	-----	4.57E-002

\*\*\*\*\*  
 \* Sandia National Laboratories \*  
 \* Radiation Protection Sample Diagnostics Program \*  
 \* 9/19/02 10:46:27 PM \*  
 \*\*\*\*\*

\* Analyzed by: *h 9/20/02* Reviewed by: *K 9/20/02*  
 \*\*\*\*\*

Customer : SANDERS, M (6135)  
 Customer Sample ID : 059847-003  
 Lab Sample ID : 20131512

Sample Description : 6721/1090-DF1-BH3-4-S  
 Sample Quantity : 822.000 gram  
 Sample Date/Time : 9/13/02 10:50:00 AM  
 Acquire Start Date/Time : 9/19/02 9:06:12 PM  
 Detector Name : LAB02  
 Elapsed Live/Real Time : 6000 / 6003 seconds

Comments:  
 U-235/Ra-226 peaks not resolved. Either isotope may be overestimated.  
 \*\*\*\*\*

Nuclide Name	Activity (pCi/gram )	2-sigma Error	MDA (pCi/gram )
U-238	Not Detected	-----	6.24E-001
RA-226	1.66E+000	4.66E-001	6.01E-001
PB-214	6.06E-001	9.08E-002	5.27E-002
BI-214	4.98E-001	8.25E-002	4.68E-002
PB-210	Not Detected	-----	2.35E+001
H-232	6.90E-001	3.28E-001	1.80E-001
RA-228	7.23E-001	1.32E-001	1.03E-001
AC-228	7.28E-001	1.35E-001	8.32E-002
TH-228	4.07E-001	3.63E-001	5.73E-001
RA-224	7.98E-001	1.76E-001	6.39E-002
PB-212	6.81E-001	9.94E-002	3.35E-002
BI-212	7.37E-001	2.22E-001	2.61E-001
TL-208	5.83E-001	9.82E-002	6.53E-002
U-235	Not Detected	-----	1.94E-001
TH-231	Not Detected	-----	9.38E+000
PA-231	Not Detected	-----	1.11E+000
TH-227	Not Detected	-----	2.96E-001
RA-223	Not Detected	-----	2.15E-001
RN-219	Not Detected	-----	2.88E-001
PB-211	Not Detected	-----	6.63E-001
TL-207	Not Detected	-----	1.03E+001
AM-241	Not Detected	-----	3.53E-001
PU-239	Not Detected	-----	3.48E+002
NP-237	Not Detected	-----	1.87E+000
PA-233	Not Detected	-----	4.57E-002
TH-229	Not Detected	-----	2.01E-001

[Summary Report] - Sample ID: : 20131512

Nuclide Name	Activity (pCi/gram )	2-sigma Error	MDA (pCi/gram )
AG-108m	Not Detected	-----	2.78E-002
AG-110m	Not Detected	-----	2.27E-002
BA-133	Not Detected	-----	4.00E-002
BE-7	Not Detected	-----	2.09E-001
CD-115	Not Detected	-----	4.02E-001
CE-139	Not Detected	-----	2.34E-002
CE-141	Not Detected	-----	4.84E-002
CE-144	Not Detected	-----	1.91E-001
CM-243	Not Detected	-----	1.39E-001
CO-56	Not Detected	-----	2.75E-002
CO-57	Not Detected	-----	2.54E-002
CO-58	Not Detected	-----	2.64E-002
CO-60	Not Detected	-----	2.80E-002
CR-51	Not Detected	-----	2.13E-001
CS-134	Not Detected	-----	3.27E-002
CS-137	Not Detected	-----	2.52E-002
EU-152	Not Detected	-----	7.53E-002
EU-154	Not Detected	-----	1.28E-001
EU-155	Not Detected	-----	1.14E-001
FE-59	Not Detected	-----	6.15E-002
GD-153	Not Detected	-----	8.35E-002
HG-203	Not Detected	-----	2.71E-002
I-131	Not Detected	-----	3.95E-002
IR-192	Not Detected	-----	2.29E-002
K-40	1.51E+001	2.04E+000	2.20E-001
IN-52	Not Detected	-----	5.53E-002
IN-54	Not Detected	-----	2.74E-002
MO-99	Not Detected	-----	8.59E-001
NA-22	Not Detected	-----	3.17E-002
NA-24	Not Detected	-----	3.15E+001
ND-147	Not Detected	-----	2.13E-001
NI-57	Not Detected	-----	7.50E-001
RU-103	Not Detected	-----	2.45E-002
RU-106	Not Detected	-----	2.08E-001
SB-122	Not Detected	-----	1.58E-001
SB-124	Not Detected	-----	2.47E-002
SB-125	Not Detected	-----	6.62E-002
SN-113	Not Detected	-----	3.08E-002
SR-85	Not Detected	-----	2.99E-002
TA-182	Not Detected	-----	1.23E-001
TA-183	Not Detected	-----	7.27E-001
TL-201	Not Detected	-----	5.72E-001
Y-88	Not Detected	-----	2.12E-002
ZN-65	Not Detected	-----	7.97E-002
ZR-95	Not Detected	-----	4.12E-002



\*\*\*\*\*  
 \* Sandia National Laboratories \*  
 \* Radiation Protection Sample Diagnostics Program \*  
 \* 9/20/02 12:28:33 AM \*  
 \*\*\*\*\*

\* Analyzed by: *A. 9/20/02* Reviewed by: *[Signature] 9/20/02* \*

Customer : SANDERS, M (6135)  
 Customer Sample ID : 059848-003  
 Lab Sample ID : 20131513

Sample Description : 6721/1090-DF1-BH3-9-S  
 Sample Quantity : 744.000 gram  
 Sample Date/Time : 9/13/02 11:10:00 AM  
 Acquire Start Date/Time : 9/19/02 10:48:10 PM  
 Detector Name : LAB02  
 Elapsed Live/Real Time : 6000 / 6003 seconds

Comments:  
 U-235/Ra-226 peaks not resolved. Either isotope may be overestimated.  
 \*\*\*\*\*

Nuclide Name	Activity (pCi/gram)	2-sigma Error	MDA (pCi/gram)
U-238	Not Detected	-----	6.49E-001
RA-226	1.70E+000	4.98E-001	6.53E-001
PB-214	7.47E-001	1.08E-001	5.17E-002
BI-214	6.18E-001	9.90E-002	4.71E-002
PB-210	Not Detected	-----	2.50E+001
TH-232	5.68E-001	2.61E-001	1.24E-001
RA-228	6.87E-001	1.32E-001	1.13E-001
AC-228	6.08E-001	1.22E-001	9.02E-002
TH-228	1.03E+000	4.06E-001	5.65E-001
RA-224	7.82E-001	1.78E-001	7.53E-002
PB-212	6.58E-001	9.69E-002	3.53E-002
BI-212	8.44E-001	2.51E-001	2.95E-001
TL-208	5.89E-001	1.02E-001	7.08E-002
U-235	Not Detected	-----	2.03E-001
TH-231	Not Detected	-----	9.85E+000
PA-231	Not Detected	-----	1.22E+000
TH-227	Not Detected	-----	3.10E-001
RA-223	Not Detected	-----	2.28E-001
RN-219	Not Detected	-----	3.21E-001
PB-211	Not Detected	-----	7.17E-001
TL-207	Not Detected	-----	1.07E+001
AM-241	Not Detected	-----	3.87E-001
PU-239	Not Detected	-----	3.68E+002
NP-237	Not Detected	-----	2.01E+000
PA-233	Not Detected	-----	5.12E-002
TH-229	Not Detected	-----	2.10E-001

[Summary Report] - Sample ID: : 20131513

Nuclide Name	Activity (pCi/gram )	2-sigma Error	MDA (pCi/gram )
AG-108m	Not Detected	-----	2.99E-002
AG-110m	Not Detected	-----	2.37E-002
BA-133	Not Detected	-----	4.44E-002
BE-7	Not Detected	-----	2.16E-001
CD-115	Not Detected	-----	4.25E-001
CE-139	Not Detected	-----	2.63E-002
CE-141	Not Detected	-----	5.06E-002
CE-144	Not Detected	-----	2.04E-001
CM-243	Not Detected	-----	1.48E-001
CO-56	Not Detected	-----	2.89E-002
CO-57	Not Detected	-----	2.63E-002
CO-58	Not Detected	-----	2.66E-002
CO-60	Not Detected	-----	2.84E-002
CR-51	Not Detected	-----	2.24E-001
CS-134	Not Detected	-----	3.54E-002
CS-137	Not Detected	-----	2.51E-002
EU-152	Not Detected	-----	7.83E-002
EU-154	Not Detected	-----	1.38E-001
EU-155	Not Detected	-----	1.21E-001
FE-59	Not Detected	-----	6.66E-002
GD-153	Not Detected	-----	8.86E-002
HG-203	Not Detected	-----	2.96E-002
I-131	Not Detected	-----	4.13E-002
IR-192	Not Detected	-----	2.44E-002
K-40	1.66E+001	2.24E+000	2.63E-001
MN-52	Not Detected	-----	5.85E-002
MN-54	Not Detected	-----	2.91E-002
MO-99	Not Detected	-----	9.82E-001
NA-22	Not Detected	-----	3.18E-002
NA-24	Not Detected	-----	3.86E+001
ND-147	Not Detected	-----	2.29E-001
NI-57	Not Detected	-----	9.21E-001
RU-103	Not Detected	-----	2.62E-002
RU-106	Not Detected	-----	2.23E-001
SB-122	Not Detected	-----	1.69E-001
SB-124	Not Detected	-----	2.47E-002
SB-125	Not Detected	-----	7.23E-002
SN-113	Not Detected	-----	3.14E-002
SR-85	Not Detected	-----	3.22E-002
TA-182	Not Detected	-----	1.34E-001
TA-183	Not Detected	-----	8.03E-001
TL-201	Not Detected	-----	6.15E-001
Y-88	Not Detected	-----	2.15E-002
ZN-65	Not Detected	-----	8.75E-002
ZR-95	Not Detected	-----	4.55E-002

\*\*\*\*\*  
 \* Sandia National Laboratories \*  
 \* Radiation Protection Sample Diagnostics Program \*  
 \* 9/20/02 2:10:34 AM \*  
 \*\*\*\*\*

\* Analyzed by: *A. Z/02/02* Reviewed by: *K. 9/20/02* \*  
 \*\*\*\*\*

Customer : SANDERS, M (6135)  
 Customer Sample ID : 059850-003  
 Lab Sample ID : 20131514

Sample Description : 6720/1111-SP1-BH1-10-S  
 Sample Quantity : 738.000 gram  
 Sample Date/Time : 9/13/02 8:45:00 AM  
 Acquire Start Date/Time : 9/20/02 12:30:19 AM  
 Detector Name : LAB02  
 Elapsed Live/Real Time : 6000 / 6003 seconds

Comments:  
 U-235/Ra-226 peaks not resolved. Either isotope may be overestimated.  
 \*\*\*\*\*

Nuclide Name	Activity (pCi/gram)	2-sigma Error	MDA (pCi/gram)
U-238	Not Detected	-----	6.67E-001
RA-226	1.78E+000	4.95E-001	6.33E-001
PB-214	6.29E-001	9.56E-002	5.81E-002
BI-214	5.85E-001	9.54E-002	5.02E-002
PB-210	Not Detected	-----	2.54E+001
TH-232	6.20E-001	3.01E-001	1.86E-001
RA-228	8.04E-001	1.45E-001	1.04E-001
AC-228	6.83E-001	1.35E-001	9.86E-002
TH-228	5.72E-001	3.90E-001	6.00E-001
RA-224	7.72E-001	1.77E-001	8.18E-002
PB-212	6.70E-001	9.86E-002	3.61E-002
BI-212	7.94E-001	2.62E-001	3.30E-001
TL-208	6.77E-001	1.16E-001	8.36E-002
U-235	Not Detected	-----	2.05E-001
TH-231	Not Detected	-----	1.03E+001
PA-231	Not Detected	-----	1.24E+000
TH-227	Not Detected	-----	3.14E-001
RA-223	Not Detected	-----	2.41E-001
<del>RN-219</del>	<del>3.94E-001</del>	<del>2.79E-001</del>	<del>3.34E-001</del>
PB-211	Not Detected	-----	7.08E-001
TL-207	Not Detected	-----	1.05E+001
AM-241	Not Detected	-----	3.84E-001
PU-239	Not Detected	-----	3.81E+002
NP-237	Not Detected	-----	2.01E+000
PA-233	Not Detected	-----	4.91E-002
TH-229	Not Detected	-----	2.20E-001

*MS ID. TL 208 2615 KeV NOT DETECTED K. 9/20/02*

Nuclide Name	Activity (pCi/gram)	2-sigma Error	MDA (pCi/gram)
AG-108m	Not Detected	-----	3.10E-002
AG-110m	Not Detected	-----	2.38E-002
BA-133	Not Detected	-----	4.43E-002
BE-7	Not Detected	-----	2.21E-001
CD-115	Not Detected	-----	4.58E-001
CE-139	Not Detected	-----	2.63E-002
CE-141	Not Detected	-----	5.22E-002
CE-144	Not Detected	-----	2.08E-001
CM-243	Not Detected	-----	1.54E-001
CO-56	Not Detected	-----	2.83E-002
CO-57	Not Detected	-----	2.72E-002
CO-58	Not Detected	-----	2.80E-002
CO-60	Not Detected	-----	3.12E-002
CR-51	Not Detected	-----	2.37E-001
CS-134	Not Detected	-----	3.53E-002
CS-137	Not Detected	-----	2.49E-002
EU-152	Not Detected	-----	8.09E-002
EU-154	Not Detected	-----	1.43E-001
EU-155	Not Detected	-----	1.21E-001
FE-59	Not Detected	-----	6.41E-002
GD-153	Not Detected	-----	9.27E-002
HG-203	Not Detected	-----	3.08E-002
I-131	Not Detected	-----	4.47E-002
IR-192	Not Detected	-----	2.47E-002
K-40	1.58E+001	2.14E+000	2.52E-001
IN-52	Not Detected	-----	5.93E-002
IN-54	Not Detected	-----	2.93E-002
MO-99	Not Detected	-----	1.01E+000
NA-22	Not Detected	-----	3.55E-002
NA-24	Not Detected	-----	4.38E+001
ND-147	Not Detected	-----	2.34E-001
NI-57	Not Detected	-----	9.69E-001
RU-103	Not Detected	-----	2.61E-002
RU-106	Not Detected	-----	2.20E-001
SB-122	Not Detected	-----	1.79E-001
SB-124	Not Detected	-----	2.41E-002
SB-125	Not Detected	-----	7.27E-002
SN-113	Not Detected	-----	3.17E-002
SR-85	Not Detected	-----	3.33E-002
TA-182	Not Detected	-----	1.33E-001
TA-183	Not Detected	-----	8.15E-001
TL-201	Not Detected	-----	6.35E-001
Y-88	Not Detected	-----	2.25E-002
ZN-65	Not Detected	-----	8.71E-002
ZR-95	Not Detected	-----	4.42E-002

\*\*\*\*\*  
 \* Sandia National Laboratories \*  
 \* Radiation Protection Sample Diagnostics Program \*  
 \* 9/20/02 3:51:31 AM \*  
 \*\*\*\*\*

Analyzed by: *mu* 9/20/02 Reviewed by: *Ka* 9/20/02  
 \*\*\*\*\*

Customer : SANDERS, M (6135)  
 Customer Sample ID : 059851-003  
 Lab Sample ID : 20131515  
 Sample Description : 6720/1111-SP1-BH1-15-S  
 Sample Quantity : 805.000 gram  
 Sample Date/Time : 9/13/02 9:00:00 AM  
 Acquire Start Date/Time : 9/20/02 2:12:17 AM  
 Detector Name : LAB02  
 Elapsed Live/Real Time : 6000 / 6003 seconds

Comments:  
 U-235/Ra-226 peaks not resolved. Either isotope may be overestimated.  
 \*\*\*\*\*

Nuclide Name	Activity (pCi/gram)	2-sigma Error	MDA (pCi/gram)
U-238	Not Detected	-----	5.99E-001
RA-226	1.84E+000	4.81E-001	6.00E-001
PB-214	7.00E-001	1.03E-001	5.47E-002
BI-214	6.17E-001	9.83E-002	4.75E-002
PB-210	Not Detected	-----	2.38E+001
TH-232	4.67E-001	2.40E-001	1.87E-001
RA-228	6.49E-001	1.22E-001	9.50E-002
AC-228	6.04E-001	1.16E-001	7.46E-002
TH-228	3.14E-001	3.73E-001	5.99E-001
RA-224	7.44E-001	1.68E-001	6.77E-002
PB-212	6.23E-001	9.15E-002	3.27E-002
BI-212	7.33E-001	2.59E-001	3.39E-001
TL-208	5.45E-001	9.40E-002	6.58E-002
U-235	Not Detected	-----	2.01E-001
TH-231	Not Detected	-----	9.48E+000
PA-231	Not Detected	-----	1.12E+000
TH-227	Not Detected	-----	2.87E-001
RA-223	Not Detected	-----	2.26E-001
RN-219	Not Detected	-----	3.06E-001
PB-211	Not Detected	-----	6.81E-001
TL-207	Not Detected	-----	1.05E+001
AM-241	Not Detected	-----	3.69E-001
PU-239	Not Detected	-----	3.58E+002
NP-237	Not Detected	-----	1.89E+000
PA-233	Not Detected	-----	4.63E-002
TH-229	Not Detected	-----	1.99E-001

Nuclide Name	Activity (pCi/gram )	2-sigma Error	MDA (pCi/gram )
AG-108m	Not Detected	-----	2.87E-002
AG-110m	Not Detected	-----	2.28E-002
BA-133	Not Detected	-----	4.24E-002
BE-7	Not Detected	-----	2.06E-001
CD-115	Not Detected	-----	4.15E-001
CE-139	Not Detected	-----	2.48E-002
CE-141	Not Detected	-----	4.98E-002
CE-144	Not Detected	-----	1.97E-001
CM-243	Not Detected	-----	1.39E-001
CO-56	Not Detected	-----	2.79E-002
CO-57	Not Detected	-----	2.64E-002
CO-58	Not Detected	-----	2.63E-002
CO-60	Not Detected	-----	2.81E-002
CR-51	Not Detected	-----	2.14E-001
CS-134	Not Detected	-----	3.39E-002
CS-137	Not Detected	-----	2.50E-002
EU-152	Not Detected	-----	7.81E-002
EU-154	Not Detected	-----	1.32E-001
EU-155	Not Detected	-----	1.14E-001
FE-59	Not Detected	-----	5.70E-002
GD-153	Not Detected	-----	8.61E-002
HG-203	Not Detected	-----	2.73E-002
I-131	Not Detected	-----	4.06E-002
IR-192	Not Detected	-----	2.26E-002
K-40	1.42E+001	1.92E+000	2.28E-001
MN-52	Not Detected	-----	5.25E-002
IN-54	Not Detected	-----	2.75E-002
MO-99	Not Detected	-----	9.26E-001
NA-22	Not Detected	-----	3.37E-002
NA-24	Not Detected	-----	4.45E+001
ND-147	Not Detected	-----	2.33E-001
NI-57	Not Detected	-----	9.31E-001
RU-103	Not Detected	-----	2.41E-002
RU-106	Not Detected	-----	2.14E-001
SB-122	Not Detected	-----	1.77E-001
SB-124	Not Detected	-----	2.44E-002
SB-125	Not Detected	-----	6.66E-002
SN-113	Not Detected	-----	3.03E-002
SR-85	Not Detected	-----	2.89E-002
TA-182	Not Detected	-----	1.27E-001
TA-183	Not Detected	-----	7.90E-001
TL-201	Not Detected	-----	6.21E-001
Y-88	Not Detected	-----	2.02E-002
ZN-65	Not Detected	-----	8.18E-002
ZR-95	Not Detected	-----	4.45E-002

\*\*\*\*\*  
 \* Sandia National Laboratories \*  
 \* Radiation Protection Sample Diagnostics Program \*  
 \* 9/20/02 5:33:30 AM \*  
 \*\*\*\*\*

\* Analyzed by: *[Signature]* 9/20/02 Reviewed by: *[Signature]* 9/20/02 \*  
 \*\*\*\*\*

Customer : SANDERS, M (6135)  
 Customer Sample ID : 059852-003  
 Lab Sample ID : 20131516

Sample Description : 6743/1087-SP1-BH1-8-S  
 Sample Quantity : 832.000 gram  
 Sample Date/Time : 9/17/02 10:12:00 AM  
 Acquire Start Date/Time : 9/20/02 3:53:15 AM  
 Detector Name : LAB02  
 Elapsed Live/Real Time : 6000 / 6003 seconds

Comments:  
 U-235/Ra-226 peaks not resolved. Either isotope may be overestimated.  
 \*\*\*\*\*

Nuclide Name	Activity (pCi/gram)	2-sigma Error	MDA (pCi/gram)
U-238	Not Detected	-----	6.21E-001
RA-226	1.61E+000	4.74E-001	6.24E-001
PB-214	6.02E-001	9.15E-002	5.76E-002
BI-214	5.46E-001	8.83E-002	4.53E-002
PB-210	Not Detected	-----	2.35E+001
H-232	6.87E-001	3.23E-001	1.66E-001
RA-228	7.79E-001	1.38E-001	9.72E-002
AC-228	6.73E-001	1.28E-001	8.64E-002
TH-228	6.64E-001	3.60E-001	5.37E-001
RA-224	7.83E-001	1.72E-001	5.79E-002
PB-212	6.98E-001	1.02E-001	3.25E-002
BI-212	8.54E-001	2.54E-001	3.06E-001
TL-208	5.87E-001	9.87E-002	6.58E-002
U-235	7.83E-002	1.49E-001	1.90E-001
TH-231	Not Detected	-----	9.59E+000
PA-231	Not Detected	-----	1.16E+000
TH-227	Not Detected	-----	2.98E-001
RA-223	Not Detected	-----	1.43E-001
RN-219	Not Detected	-----	2.97E-001
PB-211	Not Detected	-----	6.82E-001
TL-207	Not Detected	-----	1.05E+001
AM-241	Not Detected	-----	3.53E-001
PU-239	Not Detected	-----	3.55E+002
NP-237	Not Detected	-----	1.90E+000
PA-233	Not Detected	-----	4.58E-002
TH-229	Not Detected	-----	2.01E-001

Nuclide Name	Activity (pCi/gram )	2-sigma Error	MDA (pCi/gram )
AG-108m	Not Detected	-----	2.81E-002
AG-110m	Not Detected	-----	2.20E-002
BA-133	Not Detected	-----	4.10E-002
BE-7	Not Detected	-----	1.81E-001
CD-115	Not Detected	-----	1.24E-001
CE-139	Not Detected	-----	2.35E-002
CE-141	Not Detected	-----	4.34E-002
CE-144	Not Detected	-----	1.91E-001
CM-243	Not Detected	-----	1.44E-001
CO-56	Not Detected	-----	2.47E-002
CO-57	Not Detected	-----	2.54E-002
CO-58	Not Detected	-----	2.33E-002
CO-60	Not Detected	-----	2.81E-002
CR-51	Not Detected	-----	1.98E-001
CS-134	Not Detected	-----	3.22E-002
CS-137	Not Detected	-----	2.39E-002
EU-152	Not Detected	-----	7.59E-002
EU-154	Not Detected	-----	1.29E-001
EU-155	Not Detected	-----	1.11E-001
FE-59	Not Detected	-----	5.32E-002
GD-153	Not Detected	-----	8.35E-002
HG-203	Not Detected	-----	2.69E-002
I-131	Not Detected	-----	2.72E-002
IR-192	Not Detected	-----	2.15E-002
K-40	1.45E+001	1.96E+000	2.39E-001
LN-52	Not Detected	-----	3.32E-002
LN-54	Not Detected	-----	1.33E-002
MO-99	Not Detected	-----	3.37E-001
NA-22	Not Detected	-----	3.17E-002
NA-24	Not Detected	-----	5.37E-001
ND-147	Not Detected	-----	1.68E-001
NI-57	Not Detected	-----	9.31E-002
RU-103	Not Detected	-----	2.30E-002
RU-106	Not Detected	-----	2.20E-001
SB-122	Not Detected	-----	6.01E-002
SB-124	Not Detected	-----	2.27E-002
SB-125	Not Detected	-----	6.58E-002
SN-113	Not Detected	-----	2.98E-002
SR-85	Not Detected	-----	2.89E-002
TA-182	Not Detected	-----	1.18E-001
TA-183	Not Detected	-----	4.40E-001
TL-201	Not Detected	-----	2.50E-001
Y-88	Not Detected	-----	2.17E-002
ZN-65	Not Detected	-----	7.72E-002
ZR-95	Not Detected	-----	4.29E-002



\*\*\*\*\*  
 \* Sandia National Laboratories \*  
 \* Radiation Protection Sample Diagnostics Program \*  
 \* 9/20/02 7:41:53 AM \*  
 \*\*\*\*\*

Analyzed by: *lu 9/20/02* Reviewed by: *[Signature] 9/20/02*  
 \*\*\*\*\*

Customer : SANDERS, M (6135)  
 Customer Sample ID : 059853-003  
 Lab Sample ID : 20131517

Sample Description : 6743/1087-SP1-BH1-13-S  
 Sample Quantity : 779.000 gram  
 Sample Date/Time : 9/17/02 10:42:00 AM  
 Acquire Start Date/Time : 9/20/02 5:35:13 AM  
 Detector Name : LAB02  
 Elapsed Live/Real Time : 6000 / 6003 seconds

Comments:  
 U-235/Ra-226 peaks not resolved. Either isotope may be overestimated.  
 \*\*\*\*\*

Nuclide Name	Activity (pCi/gram)	2-sigma Error	MDA (pCi/gram)
U-238	Not Detected	-----	6.29E-001
RA-226	1.70E+000	4.93E-001	6.46E-001
PB-214	7.12E-001	1.04E-001	5.22E-002
BI-214	5.75E-001	9.36E-002	4.99E-002
PB-210	Not Detected	-----	2.52E+001
TH-232	7.48E-001	3.55E-001	1.96E-001
RA-228	6.58E-001	1.26E-001	1.10E-001
AC-228	7.26E-001	1.33E-001	7.27E-002
TH-228	1.01E+000	4.00E-001	5.60E-001
RA-224	8.62E-001	1.88E-001	5.62E-002
PB-212	7.39E-001	1.08E-001	3.45E-002
BI-212	7.28E-001	2.77E-001	3.74E-001
TL-208	6.48E-001	1.08E-001	6.89E-002
U-235	Not Detected	-----	2.05E-001
TH-231	Not Detected	-----	1.01E+001
PA-231	Not Detected	-----	1.18E+000
TH-227	Not Detected	-----	3.15E-001
RA-223	Not Detected	-----	1.88E-001
RN-219	Not Detected	-----	3.12E-001
PB-211	Not Detected	-----	7.08E-001
TL-207	Not Detected	-----	1.06E+001
AM-241	Not Detected	-----	3.72E-001
PU-239	Not Detected	-----	3.64E+002
NP-237	Not Detected	-----	1.96E+000
PA-233	Not Detected	-----	4.88E-002
TH-229	Not Detected	-----	2.08E-001

Nuclide Name	Activity (pCi/gram )	2-sigma Error	MDA (pCi/gram )
AG-108m	Not Detected	-----	3.04E-002
AG-110m	Not Detected	-----	2.33E-002
BA-133	Not Detected	-----	4.31E-002
BE-7	8.77E-002	8.53E-002	1.34E-001
CD-115	Not Detected	-----	1.35E-001
CE-139	Not Detected	-----	2.51E-002
CE-141	Not Detected	-----	4.66E-002
CE-144	Not Detected	-----	2.00E-001
CM-243	Not Detected	-----	1.47E-001
CO-56	Not Detected	-----	2.81E-002
CO-57	Not Detected	-----	2.64E-002
CO-58	Not Detected	-----	2.70E-002
CO-60	Not Detected	-----	2.93E-002
CR-51	Not Detected	-----	1.98E-001
CS-134	Not Detected	-----	3.48E-002
CS-137	Not Detected	-----	2.53E-002
EU-152	Not Detected	-----	7.89E-002
EU-154	Not Detected	-----	1.40E-001
EU-155	Not Detected	-----	1.18E-001
FE-59	Not Detected	-----	5.74E-002
GD-153	Not Detected	-----	8.60E-002
HG-203	Not Detected	-----	2.74E-002
I-131	Not Detected	-----	2.86E-002
IR-192	Not Detected	-----	2.29E-002
K-40	1.42E+001	1.92E+000	2.19E-001
MN-52	Not Detected	-----	3.33E-002
NI-54	Not Detected	-----	2.73E-002
NO-99	Not Detected	-----	3.53E-001
NA-22	Not Detected	-----	3.22E-002
NA-24	Not Detected	-----	6.36E-001
ND-147	Not Detected	-----	1.84E-001
NI-57	Not Detected	-----	8.83E-002
RU-103	Not Detected	-----	2.29E-002
RU-106	Not Detected	-----	2.17E-001
SB-122	Not Detected	-----	6.34E-002
SB-124	Not Detected	-----	2.49E-002
SB-125	Not Detected	-----	6.89E-002
SN-113	Not Detected	-----	3.18E-002
SR-85	Not Detected	-----	3.04E-002
TA-182	Not Detected	-----	1.23E-001
TA-183	Not Detected	-----	4.67E-001
TL-201	Not Detected	-----	2.59E-001
Y-88	Not Detected	-----	2.08E-002
ZN-65	Not Detected	-----	8.09E-002
ZR-95	Not Detected	-----	4.23E-002

at: 1.5m + 136

\*\*\*\*\*  
 \* Sandia National Laboratories \*  
 \* Radiation Protection Sample Diagnostics Program \*  
 \* 9/20/02 9:26:50 AM \*  
 \*\*\*\*\*

Analyzed by: *[Signature]* 9/20/02 Reviewed by: *[Signature]* 9/20/02  
 \*\*\*\*\*

Customer : SANDERS, M (6135)  
 Customer Sample ID : 059854-003  
 Lab Sample ID : 20131518

Sample Description : 6734/1089-SP1-BH1-9-S  
 Sample Quantity : 741.000 gram  
 Sample Date/Time : 9/17/02 12:40:00 PM  
 Acquire Start Date/Time : 9/20/02 7:54:59 AM  
 Detector Name : LAB02  
 Elapsed Live/Real Time : 6000 / 6002 seconds

Comments:  
 U-235/Ra-226 peaks not resolved. Either isotope may be overestimated.  
 \*\*\*\*\*

Nuclide Name	Activity (pCi/gram)	2-sigma Error	MDA (pCi/gram)
U-238	Not Detected	-----	5.38E-001
RA-226	1.26E+000	4.02E-001	5.37E-001
PB-214	4.05E-001	6.75E-002	5.00E-002
BI-214	3.81E-001	6.65E-002	4.04E-002
PB-210	Not Detected	-----	2.12E+001
H-232	4.69E-001	2.35E-001	1.65E-001
LA-228	3.07E-001	1.02E-001	1.25E-001
AC-228	Not Detected	-----	1.38E-001
TH-228	Not Detected	-----	5.48E-001
RA-224	4.79E-001	1.24E-001	7.66E-002
PB-212	4.37E-001	6.68E-002	3.03E-002
BI-212	5.20E-001	1.93E-001	2.44E-001
TL-208	3.98E-001	7.69E-002	6.41E-002
U-235	Not Detected	-----	1.77E-001
TH-231	Not Detected	-----	8.38E+000
PA-231	Not Detected	-----	1.12E+000
TH-227	Not Detected	-----	2.58E-001
RA-223	Not Detected	-----	1.56E-001
RN-219	Not Detected	-----	2.64E-001
PB-211	Not Detected	-----	6.13E-001
TL-207	Not Detected	-----	9.83E+000
AM-241	Not Detected	-----	3.22E-001
PU-239	Not Detected	-----	3.18E+002
NP-237	Not Detected	-----	1.70E+000
PA-233	Not Detected	-----	4.14E-002
TH-229	Not Detected	-----	1.78E-001

[Summary Report] - Sample ID: : 20131518

Nuclide Name	Activity (pCi/gram)	2-sigma Error	MDA (pCi/gram)
AG-108m	Not Detected	-----	2.58E-002
AG-110m	Not Detected	-----	2.05E-002
BA-133	Not Detected	-----	3.69E-002
BE-7	Not Detected	-----	1.73E-001
CD-115	Not Detected	-----	1.14E-001
CE-139	Not Detected	-----	2.20E-002
CE-141	Not Detected	-----	4.08E-002
CE-144	Not Detected	-----	1.71E-001
CM-243	Not Detected	-----	1.22E-001
CO-56	Not Detected	-----	2.50E-002
CO-57	Not Detected	-----	2.24E-002
CO-58	Not Detected	-----	2.54E-002
CO-60	Not Detected	-----	2.71E-002
CR-51	Not Detected	-----	1.75E-001
CS-134	Not Detected	-----	2.93E-002
CS-137	Not Detected	-----	2.17E-002
EU-152	Not Detected	-----	6.74E-002
EU-154	Not Detected	-----	1.19E-001
EU-155	Not Detected	-----	1.03E-001
FE-59	Not Detected	-----	5.34E-002
GD-153	Not Detected	-----	7.60E-002
HG-203	Not Detected	-----	2.40E-002
I-131	Not Detected	-----	2.63E-002
IR-192	Not Detected	-----	1.96E-002
K-40	1.35E+001	1.84E+000	2.27E-001
LN-52	Not Detected	-----	3.33E-002
LN-54	Not Detected	-----	2.42E-002
MO-99	Not Detected	-----	3.44E-001
NA-22	Not Detected	-----	3.21E-002
NA-24	Not Detected	-----	5.17E-001
ND-147	Not Detected	-----	1.72E-001
NI-57	Not Detected	-----	6.86E-002
RU-103	Not Detected	-----	2.06E-002
RU-106	Not Detected	-----	1.99E-001
SB-122	Not Detected	-----	5.72E-002
SB-124	Not Detected	-----	2.16E-002
SB-125	Not Detected	-----	5.94E-002
SN-113	Not Detected	-----	2.64E-002
SR-85	Not Detected	-----	2.79E-002
TA-182	Not Detected	-----	1.05E-001
TA-183	Not Detected	-----	4.04E-001
TL-201	Not Detected	-----	2.23E-001
Y-88	Not Detected	-----	2.11E-002
ZN-65	Not Detected	-----	7.17E-002
ZR-95	Not Detected	-----	3.96E-002

\*\*\*\*\*  
 \* Sandia National Laboratories \*  
 \* Radiation Protection Sample Diagnostics Program \*  
 \* 9/20/02 11:08:49 AM \*  
 \*\*\*\*\*

Analyzed by: *h 9/20/02* Reviewed by: *K 9/20/02*  
 \*\*\*\*\*

Customer : SANDERS, M (6135)  
 Customer Sample ID : 059855-003  
 Lab Sample ID : 20131519

Sample Description : 6734/1089-SP1-BH1-14-S  
 Sample Quantity : 819.000 gram  
 Sample Date/Time : 9/17/02 12:45:00 PM  
 Acquire Start Date/Time : 9/20/02 9:28:34 AM  
 Detector Name : LAB02  
 Elapsed Live/Real Time : 6000 / 6002 seconds

Comments:  
 U-235/Ra-226 peaks not resolved. Either isotope may be overestimated.  
 \*\*\*\*\*

Nuclide Name	Activity (pCi/gram)	2-sigma Error	MDA (pCi/gram)
U-238	Not Detected	-----	5.31E-001
RA-226	8.15E-001	3.79E-001	5.60E-001
PB-214	4.44E-001	7.06E-002	4.77E-002
BI-214	3.63E-001	6.41E-002	4.26E-002
PB-210	Not Detected	-----	1.97E+001
H-232	5.04E-001	2.40E-001	1.29E-001
RA-228	4.16E-001	9.14E-002	9.89E-002
AC-228	4.70E-001	9.55E-002	6.69E-002
TH-228	3.50E-001	1.45E-001	2.78E-001
RA-224	5.38E-001	1.32E-001	7.45E-002
PB-212	4.82E-001	7.23E-002	2.80E-002
BI-212	4.94E-001	2.14E-001	2.96E-001
TL-208	4.15E-001	7.54E-002	5.62E-002
U-235	Not Detected	-----	1.72E-001
TH-231	Not Detected	-----	8.54E+000
PA-231	Not Detected	-----	1.03E+000
TH-227	Not Detected	-----	2.55E-001
RA-223	Not Detected	-----	1.58E-001
RN-219	Not Detected	-----	2.60E-001
PB-211	Not Detected	-----	6.04E-001
TL-207	Not Detected	-----	8.70E+000
AM-241	Not Detected	-----	3.07E-001
PU-239	Not Detected	-----	3.13E+002
NP-237	Not Detected	-----	1.68E+000
PA-233	Not Detected	-----	4.10E-002
TH-229	Not Detected	-----	1.82E-001

[Summary Report] - Sample ID: : 20131519

Nuclide Name	Activity (pCi/gram )	2-sigma Error	MDA (pCi/gram )
AG-108m	Not Detected	-----	2.56E-002
AG-110m	Not Detected	-----	2.04E-002
BA-133	Not Detected	-----	3.46E-002
BE-7	Not Detected	-----	1.82E-001
CD-115	Not Detected	-----	1.14E-001
CE-139	Not Detected	-----	2.09E-002
CE-141	Not Detected	-----	3.93E-002
CE-144	Not Detected	-----	1.67E-001
CM-243	Not Detected	-----	1.24E-001
CO-56	Not Detected	-----	2.34E-002
CO-57	Not Detected	-----	2.23E-002
CO-58	Not Detected	-----	2.32E-002
CO-60	Not Detected	-----	2.59E-002
CR-51	Not Detected	-----	1.80E-001
CS-134	Not Detected	-----	2.84E-002
CS-137	Not Detected	-----	2.22E-002
EU-152	Not Detected	-----	6.72E-002
EU-154	Not Detected	-----	1.18E-001
EU-155	Not Detected	-----	1.01E-001
FE-59	Not Detected	-----	5.22E-002
GD-153	Not Detected	-----	7.37E-002
HG-203	Not Detected	-----	2.35E-002
I-131	Not Detected	-----	2.49E-002
IR-192	Not Detected	-----	1.98E-002
K-40	1.38E+001	1.87E+000	2.01E-001
MN-52	Not Detected	-----	3.06E-002
MN-54	Not Detected	-----	2.37E-002
MO-99	Not Detected	-----	3.23E-001
NA-22	Not Detected	-----	2.89E-002
NA-24	Not Detected	-----	5.48E-001
ND-147	Not Detected	-----	1.63E-001
NI-57	Not Detected	-----	9.85E-002
RU-103	Not Detected	-----	2.09E-002
RU-106	Not Detected	-----	1.99E-001
SB-122	Not Detected	-----	6.01E-002
SB-124	Not Detected	-----	2.10E-002
SB-125	Not Detected	-----	6.04E-002
SN-113	Not Detected	-----	2.63E-002
SR-85	Not Detected	-----	2.59E-002
TA-182	Not Detected	-----	1.10E-001
TA-183	Not Detected	-----	3.89E-001
TL-201	Not Detected	-----	2.23E-001
Y-88	Not Detected	-----	1.75E-002
ZN-65	Not Detected	-----	6.98E-002
ZR-95	Not Detected	-----	3.96E-002

\*\*\*\*\*  
 \* Sandia National Laboratories \*  
 \* Radiation Protection Sample Diagnostics Program \*  
 \* 9/19/02 9:04:28 PM \*  
 \*\*\*\*\*

Analyzed by: *AS 9/20/02* Reviewed by: *[Signature] 9/20/02*  
 \*\*\*\*\*

Customer : SANDERS, M (6135)  
 Customer Sample ID : 059859-001  
 Lab Sample ID : 20131511

Sample Description : 6721/1090-DF1-BH2-4-DU  
 Sample Quantity : 704.000 gram  
 Sample Date/Time : 9/13/02 10:16:00 AM  
 Acquire Start Date/Time : 9/19/02 7:24:13 PM  
 Detector Name : LAB02  
 Elapsed Live/Real Time : 6000 / 6002 seconds

Comments:  
 U-235/Ra-226 peaks not resolved. Either isotope may be overestimated.  
 \*\*\*\*\*

Nuclide Name	Activity (pCi/gram)	2-sigma Error	MDA (pCi/gram)
U-238	Not Detected	-----	6.52E-001
RA-226	1.88E+000	5.17E-001	6.59E-001
PB-214	6.94E-001	1.04E-001	5.98E-002
BI-214	5.82E-001	9.55E-002	5.14E-002
PB-210	Not Detected	-----	2.61E+001
H-232	7.71E-001	3.63E-001	1.83E-001
RA-228	7.85E-001	1.44E-001	1.05E-001
AC-228	6.86E-001	1.39E-001	1.09E-001
TH-228	5.86E-001	3.95E-001	6.07E-001
RA-224	8.47E-001	1.89E-001	6.18E-002
PB-212	7.02E-001	1.03E-001	3.55E-002
BI-212	6.12E-001	2.63E-001	3.64E-001
TL-208	6.17E-001	1.07E-001	7.51E-002
U-235	Not Detected	-----	2.07E-001
TH-231	Not Detected	-----	1.05E+001
PA-231	Not Detected	-----	1.23E+000
TH-227	Not Detected	-----	3.20E-001
RA-223	Not Detected	-----	2.47E-001
RN-219	Not Detected	-----	3.40E-001
PB-211	Not Detected	-----	7.56E-001
TL-207	Not Detected	-----	1.18E+001
AM-241	Not Detected	-----	3.83E-001
PU-239	Not Detected	-----	3.87E+002
NP-237	Not Detected	-----	2.02E+000
PA-233	Not Detected	-----	5.24E-002
TH-229	Not Detected	-----	2.19E-001

[Summary Report] - Sample ID: : 20131511

Nuclide Name	Activity (pCi/gram )	2-sigma Error	MDA (pCi/gram )
AG-108m	Not Detected	-----	3.12E-002
AG-110m	Not Detected	-----	2.60E-002
BA-133	Not Detected	-----	4.68E-002
BE-7	Not Detected	-----	2.15E-001
CD-115	Not Detected	-----	4.26E-001
CE-139	Not Detected	-----	2.67E-002
CE-141	Not Detected	-----	5.18E-002
CE-144	Not Detected	-----	2.06E-001
CM-243	Not Detected	-----	1.54E-001
CO-56	Not Detected	-----	3.02E-002
CO-57	Not Detected	-----	2.77E-002
CO-58	Not Detected	-----	2.80E-002
CO-60	Not Detected	-----	3.08E-002
CR-51	Not Detected	-----	2.30E-001
CS-134	Not Detected	-----	3.68E-002
CS-137	Not Detected	-----	2.92E-002
EU-152	Not Detected	-----	8.25E-002
EU-154	Not Detected	-----	1.43E-001
EU-155	Not Detected	-----	1.23E-001
FE-59	Not Detected	-----	6.27E-002
GD-153	Not Detected	-----	9.16E-002
HG-203	Not Detected	-----	3.01E-002
I-131	Not Detected	-----	4.28E-002
IR-192	Not Detected	-----	2.51E-002
K-40	1.56E+001	2.12E+000	2.81E-001
N-52	Not Detected	-----	5.22E-002
N-54	Not Detected	-----	1.79E-002
MO-99	Not Detected	-----	1.02E+000
NA-22	Not Detected	-----	3.37E-002
NA-24	Not Detected	-----	3.44E+001
ND-147	Not Detected	-----	2.32E-001
NI-57	Not Detected	-----	8.57E-001
RU-103	Not Detected	-----	2.68E-002
RU-106	Not Detected	-----	2.37E-001
SB-122	Not Detected	-----	1.77E-001
SB-124	Not Detected	-----	2.64E-002
SB-125	Not Detected	-----	7.34E-002
SN-113	Not Detected	-----	3.40E-002
SR-85	Not Detected	-----	3.21E-002
TA-182	Not Detected	-----	1.36E-001
TA-183	Not Detected	-----	7.83E-001
TL-201	Not Detected	-----	6.14E-001
Y-88	Not Detected	-----	2.44E-002
ZN-65	Not Detected	-----	8.81E-002
ZR-95	Not Detected	-----	4.86E-002



\*\*\*\*\*  
 \* Sandia National Laboratories \*  
 \* Radiation Protection Sample Diagnostics Program \*  
 \* 9/20/02 1:05:56 PM \*  
 \*\*\*\*\*

\* Analyzed by: *je 9/20/02* Reviewed by: *[Signature] 9/20/02*  
 \*\*\*\*\*

Customer : SANDERS, M (6135)  
 Customer Sample ID : LAB\_CONTROL\_SAMPLE\_USING\_CG-134  
 Lab Sample ID : 20131520

Sample Description : MIXED\_GAMMA\_STANDARD\_CG-134  
 Sample Quantity : 1.000 Each  
 Sample Date/Time : 11/1/90 12:00:00 PM  
 Acquire Start Date/Time : 9/20/02 12:55:40 PM  
 Detector Name : LAB01  
 Elapsed Live/Real Time : 600 / 604 seconds

Comments:

\*\*\*\*\*

Nuclide Name	Activity (pCi/Each)	2-sigma Error	MDA (pCi/Each)
U-238	Not Detected	-----	2.58E+003
RA-226	Not Detected	-----	5.57E+003
PB-214	Not Detected	-----	6.83E+002
BI-214	Not Detected	-----	5.84E+002
PB-210	Not Detected	-----	9.61E+004
H-232	Not Detected	-----	2.14E+003
LA-228	Not Detected	-----	2.48E+003
AC-228	Not Detected	-----	1.51E+003
TH-228	Not Detected	-----	4.67E+005
RA-224	Not Detected	-----	2.33E+004
PB-212	Not Detected	-----	3.43E+004
BI-212	Not Detected	-----	3.03E+005
TL-208	Not Detected	-----	6.67E+004
U-235	Not Detected	-----	1.36E+003
TH-231	Not Detected	-----	4.04E+004
PA-231	Not Detected	-----	1.38E+004
TH-227	Not Detected	-----	2.59E+003
RA-223	Not Detected	-----	1.00E+026
RN-219	Not Detected	-----	6.60E+003
PB-211	Not Detected	-----	1.49E+004
TL-207	Not Detected	-----	2.30E+005
AM-241	8.99E+004	1.30E+004	1.88E+003
PU-239	Not Detected	-----	2.40E+006
NP-237	Not Detected	-----	1.24E+004
PA-233	Not Detected	-----	5.92E+002
TH-229	Not Detected	-----	1.29E+003

[Summary Report] - Sample ID: : 20131520

Nuclide Name	Activity (pCi/Each )	2-sigma Error	MDA (pCi/Each )
AG-108m	Not Detected	-----	3.10E+002
AG-110m	Not Detected	-----	2.72E+008
BA-133	Not Detected	-----	9.38E+002
BE-7	Not Detected	-----	1.00E+026
CD-115	Not Detected	-----	1.00E+026
CE-139	Not Detected	-----	5.53E+011
CE-141	Not Detected	-----	1.00E+026
CE-144	Not Detected	-----	5.21E+007
CM-243	Not Detected	-----	2.10E+003
CO-56	Not Detected	-----	2.89E+019
CO-57	Not Detected	-----	1.09E+007
CO-58	Not Detected	-----	7.73E+020
CO-60	7.81E+004	1.03E+004	8.15E+002
CR-51	Not Detected	-----	1.00E+026
CS-134	Not Detected	-----	1.53E+004
CS-137	6.88E+004	8.74E+003	3.92E+002
EU-152	Not Detected	-----	9.42E+002
EU-154	Not Detected	-----	3.52E+003
EU-155	Not Detected	-----	4.23E+003
FE-59	Not Detected	-----	1.00E+026
GD-153	Not Detected	-----	1.08E+008
HG-203	Not Detected	-----	1.00E+026
I-131	Not Detected	-----	1.00E+026
IR-192	Not Detected	-----	1.38E+020
K-40	Not Detected	-----	1.37E+003
LN-52	Not Detected	-----	1.00E+026
LN-54	Not Detected	-----	4.99E+006
MO-99	Not Detected	-----	1.00E+026
NA-22	Not Detected	-----	4.94E+003
NA-24	Not Detected	-----	1.00E+026
ND-147	Not Detected	-----	1.00E+026
NI-57	Not Detected	-----	1.00E+026
RU-103	Not Detected	-----	1.00E+026
RU-106	Not Detected	-----	9.18E+006
SB-122	Not Detected	-----	1.00E+026
SB-124	Not Detected	-----	1.00E+026
SB-125	Not Detected	-----	2.38E+004
SN-113	Not Detected	-----	1.03E+014
SR-85	Not Detected	-----	1.00E+026
TA-182	Not Detected	-----	2.57E+014
TA-183	Not Detected	-----	1.00E+026
TL-201	Not Detected	-----	1.00E+026
Y-88	Not Detected	-----	3.07E+014
ZN-65	Not Detected	-----	1.95E+008
ZR-95	Not Detected	-----	1.00E+026

\*\*\*\*\*  
 \* Sandia National Laboratories \*  
 \* Radiation Protection Sample Diagnostics Program \*  
 \* 9/20/02 12:39:50 PM \*  
 \*\*\*\*\*

Analyzed by: *hm* 9/20/02 Reviewed by: *K* 9/20/02  
 \*\*\*\*\*

Customer : SANDERS, M (6135)  
 Customer Sample ID : LAB\_CONTROL\_SAMPLE\_USING\_CG-134  
 Lab Sample ID : 20131521

Sample Description : MIXED\_GAMMA\_STANDARD\_CG-134  
 Sample Quantity : 1.000 Each  
 Sample Date/Time : 11/01/90 12:00:00 PM  
 Acquire Start Date/Time : 9/20/02 12:29:34 PM  
 Detector Name : LAB02  
 Elapsed Live/Real Time : 600 / 604 seconds

Comments:  
 \*\*\*\*\*

Nuclide Name	Activity (pCi/Each)	2-sigma Error	MDA (pCi/Each)
U-238	Not Detected	-----	3.92E+003
RA-226	Not Detected	-----	5.81E+003
PB-214	Not Detected	-----	5.77E+002
BI-214	Not Detected	-----	4.78E+002
PB-210	Not Detected	-----	2.63E+005
TH-232	Not Detected	-----	1.83E+003
RA-228	Not Detected	-----	1.76E+003
AC-228	Not Detected	-----	1.04E+003
TH-228	Not Detected	-----	4.28E+005
RA-224	Not Detected	-----	1.70E+004
PB-212	Not Detected	-----	3.27E+004
BI-212	Not Detected	-----	2.28E+005
TL-208	Not Detected	-----	5.28E+004
U-235	Not Detected	-----	1.46E+003
TH-231	Not Detected	-----	7.07E+004
PA-231	Not Detected	-----	1.23E+004
TH-227	Not Detected	-----	2.50E+003
RA-223	Not Detected	-----	1.00E+026
RN-219	Not Detected	-----	5.58E+003
PB-211	Not Detected	-----	1.28E+004
TL-207	Not Detected	-----	1.69E+005
AM-241	8.08E+004	1.20E+004	4.04E+003
PU-239	Not Detected	-----	2.69E+006
NP-237	Not Detected	-----	1.44E+004
PA-233	Not Detected	-----	5.19E+002
TH-229	Not Detected	-----	1.49E+003

\*\*\*\*\*  
 \* Sandia National Laboratories \*  
 \* Radiation Protection Sample Diagnostics Program \*  
 \* Quality Assurance Report \*  
 \*\*\*\*\*

Report Date : 9/20/02 1:06:02 PM  
 QA File : C:\GENIE2K\CAMFILES\LCS1.QAF  
 Analyst : KRSANSO  
 Sample ID : 20131520  
 Sample Quantity : 1.00 Each  
 Sample Date : 11/1/90 12:00:00 PM  
 Measurement Date : 9/20/02 12:55:40 PM  
 Elapsed Live Time : 600 seconds  
 Elapsed Real Time : 604 seconds

Parameter	Mean	1S Error	New Value	< LU	: SD	: UD	: BS >
AM-241 ACTIVITY	8.573E-002	3.463E-003	8.985E-002	<	:	:	>
CS-137 Activity	6.836E-002	1.364E-003	6.883E-002	<	:	:	>
CO-60 Activity	7.658E-002	3.469E-003	7.757E-002	<	:	:	>

Flags Key: LU = Boundary Test (Ab = Above, Be = Below)  
 SD = Sample Driven N-Sigma Test (In = Investigate, Ac = Action)  
 UD = User Driven N-Sigma Test (In = Investigate, Ac = Action)  
 BS = Measurement Bias Test (In = Investigate, Ac = Action)

Reviewed by: K. 9/20/02

[Summary Report] - Sample ID: : 20131521

Nuclide Name	Activity (pCi/Each)	2-sigma Error	MDA (pCi/Each)
AG-108m	Not Detected	-----	2.37E+002
AG-110m	Not Detected	-----	2.21E+008
BA-133	Not Detected	-----	7.74E+002
BE-7	Not Detected	-----	1.00E+026
CD-115	Not Detected	-----	1.00E+026
CE-139	Not Detected	-----	6.05E+011
CE-141	Not Detected	-----	1.00E+026
CE-144	Not Detected	-----	5.68E+007
CM-243	Not Detected	-----	1.87E+003
CO-56	Not Detected	-----	2.22E+019
CO-57	Not Detected	-----	1.28E+007
CO-58	Not Detected	-----	6.15E+020
CO-60	8.10E+004	1.05E+004	6.23E+002
CR-51	Not Detected	-----	1.00E+026
CS-134	Not Detected	-----	1.19E+004
CS-137	7.06E+004	8.93E+003	3.16E+002
EU-152	Not Detected	-----	1.10E+003
EU-154	Not Detected	-----	2.66E+003
EU-155	Not Detected	-----	4.94E+003
FE-59	Not Detected	-----	1.00E+026
GD-153	Not Detected	-----	1.62E+008
HG-203	Not Detected	-----	1.00E+026
I-131	Not Detected	-----	1.00E+026
IR-192	Not Detected	-----	1.24E+020
K-40	Not Detected	-----	1.07E+003
MN-52	Not Detected	-----	1.00E+026
MN-54	Not Detected	-----	3.91E+006
MO-99	Not Detected	-----	1.00E+026
NA-22	Not Detected	-----	3.69E+003
NA-24	Not Detected	-----	1.00E+026
ND-147	Not Detected	-----	1.00E+026
NI-57	Not Detected	-----	1.00E+026
RU-103	Not Detected	-----	1.00E+026
RU-106	Not Detected	-----	1.00E+026
SB-122	Not Detected	-----	7.76E+006
SB-124	Not Detected	-----	1.00E+026
SB-125	Not Detected	-----	1.00E+026
SN-113	Not Detected	-----	1.89E+004
SR-85	Not Detected	-----	8.24E+013
TA-182	Not Detected	-----	1.00E+026
TA-183	Not Detected	-----	1.78E+014
TL-201	Not Detected	-----	1.00E+026
Y-88	Not Detected	-----	1.00E+026
ZN-65	Not Detected	-----	1.85E+014
ZR-95	Not Detected	-----	1.35E+008
			1.00E+026

\*\*\*\*\*  
\* Sandia National Laboratories \*  
\* Radiation Protection Sample Diagnostics Program \*  
\* Quality Assurance Report \*  
\*\*\*\*\*

Report Date : 9/20/02 12:39:57 PM  
QA File : C:\GENIE2K\CAMPFILES\LCS2.QAF  
Analyst : KRSANSO  
Sample ID : 20131521  
Sample Quantity : 1.00 Each  
Sample Date : 11/01/90 12:00:00 PM  
Measurement Date : 9/20/02 12:29:34 PM  
Elapsed Live Time : 600 seconds  
Elapsed Real Time : 604 seconds

Parameter	Mean	1S Error	New Value	<	LU	:	SD	:	UD	:	BS	>
AM-241 Activity	8.241E-002	3.925E-003	8.077E-002	<	:				:			>
CS-137 Activity	7.182E-002	3.737E-003	7.064E-002	<	:				:			>
CO-60 Activity	8.001E-002	5.100E-003	8.078E-002	<	:				:			>

Flags Key: LU = Boundary Test (Ab = Above, Be = Below)  
SD = Sample Driven N-Sigma Test (In = Investigate, Ac = Action)  
UD = User Driven N-Sigma Test (In = Investigate, Ac = Action)  
BS = Measurement Bias Test (In = Investigate, Ac = Action)

Reviewed by:           *KRS* 9/20/02